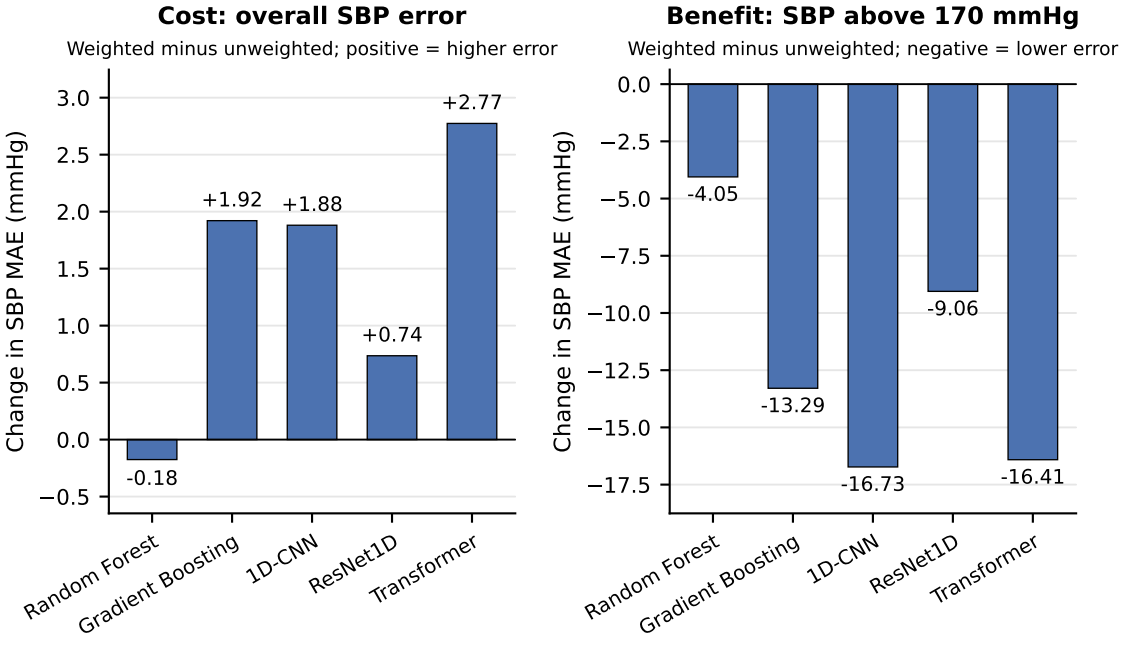
Cost: overall SBP error
Weighted minus unweighted; positive = higher error
Change in SBP MAE (mmHg)
3.0
2.5
2.0
1.5
1.0
0.5
0.0
−0.5
-0.18
+1.92
+1.88
+0.74
+2.77
Random Forest
Gradient Boosting
1D-CNN
ResNet1D
Transformer
Benefit: SBP above 170 mmHg
Weighted minus unweighted; negative = lower error
Change in SBP MAE (mmHg)
0.0
−2.5
−5.0
−7.5
−10.0
−12.5
−15.0
−17.5
-4.05
-13.29
-16.73
-9.06
-16.41
Random Forest
Gradient Boosting
1D-CNN
ResNet1D
Transformer