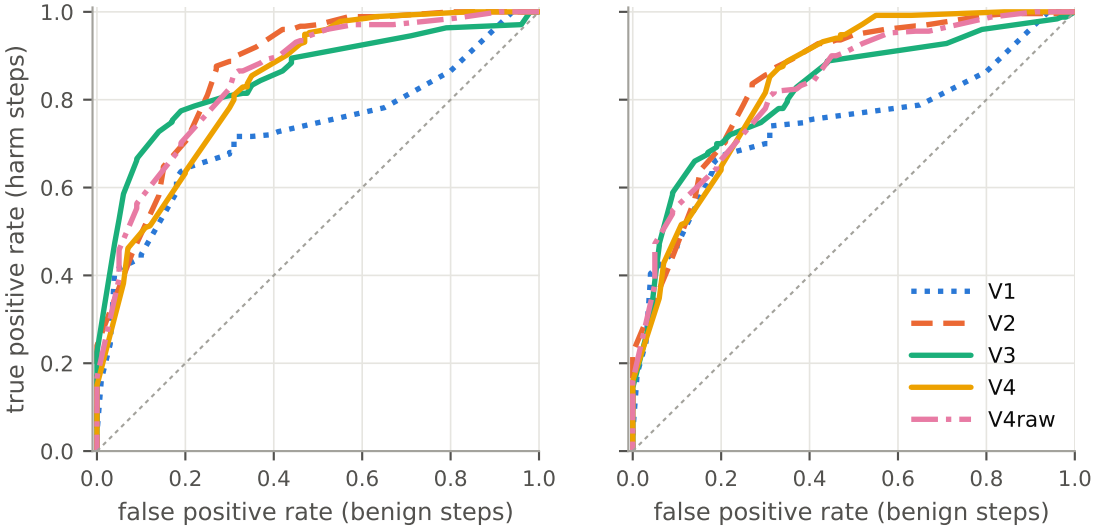
standard injection
monitor-aware injection
true positive rate (harm steps)
false positive rate (benign steps)
false positive rate (benign steps)
0.0
0.2
0.4
0.6
0.8
1.0
V1
V2
V3
V4
V4raw