Intended Use

The device is intended to secure a hemodialysis catheter to the patient's skin to reduce catheter movement and prevent accidental traction or dislodgement.

Indications for Use

The SureSet Dialysis Catheter Securement Device is indicated for use in adult patients with a compatible hemodialysis catheter with dimensions 12.5Fr to 13.5Fr. The device is intended for use in in-center dialysis units, hospital-based dialysis services or long-term assisted care facilities under the supervision of a clinician. Apply only to intact, clean, dry skin. Do not use on compromised skin, on skin with active exit-site infection, in environments with standing water exposure, or outside ambient indoor conditions.

Safety Considerations

- Single use only. Do not reuse or reapply.
- Discard if the package is damaged or the seal is broken.
- Inspect the application site and catheter exit site before each dialysis session in clinical settings for redness, swelling, drainage, tenderness, or skin breakdown.
- The device does not replace the primary catheter dressing. Apply per facility protocol for catheter exit-site dressing and securement.

Key Usage Points

- Prepare the skin. Cleanse with an antiseptic wipe and allow to dry completely before application.
- Affix the device per the application steps in this document, ensuring the catheter limbs are routed without kinking or tension.
- To access the catheter, place a finger under the clasp and lift to open the cover of the SureSet device.
- Replace the device if the adhesive pad lifts, becomes soiled, becomes wet, or loses contact with the skin.
- Replace the device if it shows blood or fluid contamination after a dialysis session.
- Remove any residue of the dressing pad adhesive with alcohol after removing the device.

Warnings, Precautions

Read and understand all warnings, precautions, and instructions for use prior to using the device.

Warnings

- Do not use the device where loss of adhesive could occur, such as on non-adherent skin, diaphoretic skin, or in patients who are confused or unable to cooperate with catheter site management.
- Do not apply the device over an exit site that shows signs of infection. Notify the dialysis care team and follow facility protocol.
- Use aseptic technique for application and removal of the device.
- The device does not replace the primary catheter exit-site dressing. Apply over or adjacent to the primary dressing per facility protocol.
- In case of device loosening, contamination, or malfunction, the device should be removed and replaced.
- Do not apply tension to the catheter limbs during application. Tension or kinking under the device cover can compromise blood flow during dialysis.

Precautions

- Do not use if the patient has known sensitivity to acrylate adhesives.
- Read all package insert warnings and instructions prior to use.
- The device, the catheter exit site, and the surrounding skin should be inspected before each dialysis session and at any point the device or dressing appears compromised.
- Minimize catheter manipulation during application and removal of the device to reduce the risk of dislodgement or exit-site disruption.
- Remove any oil, moisturizer, or residual antimicrobial ointment from the targeted skin area before application.
- Respect infection control guidelines during application and removal of the device. Perform hand hygiene before and after handling the device or the catheter site.
- This is a single use device. Do not reuse. If reused, the adhesive may not maintain its performance, causing the device to loosen from the skin and increasing the risk of catheter dislodgement.
- Replace the device if it shows blood or fluid contamination after a dialysis session.
- Position and route the catheter limbs so that connections to the dialysis circuit can be made without lifting or applying tension to the device.
- Incidents should be reported to the manufacturer.

alera TES

MD **SureSet**

Dialysis Catheter Securement Device

REF **SSD-30**

30 device(s) per box

UDI **00816022024012**

Alera TES
159 West Mason Avenue
Buckley, WA 98321
USA
+1(360) 829-0400
customerservice@aleramedtech.com
www.sureset-secure.com

Assembled in India
Mfg License Number:
MFG/MD/2023/001035

STERILE EO




IMPORTANT: Carefully read and understand all instructions, indications, warnings, precautions, and directions for use prior to using the SureSet Securement device. Failure to do so could result in compromised patient safety, patient complications, and/or insufficient treatment.

Visit our website to learn more


AT-100-L02-A Issue 2 Effective 01-Aug-2026

Device Overview

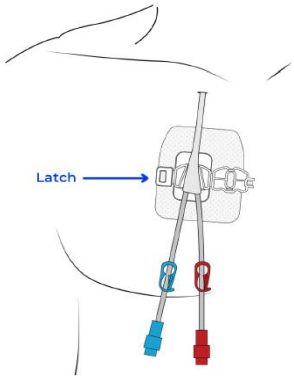

I


1




Place the protective dressing over the IV catheter hub. Do not cover the Luer connection with the

Peel off the adhesive cover to reveal adhesive strip on underside of SureSet.

2




3




Place the device over the protective dressing, ensuring it adheres securely.

Press and secure tubing into the side channel. (supported tubing size - 12.5Fr to 13.5Fr)

4



5



Close the device cover. Make sure it closes securely.

Device Removal

To remove, open the cover, gently remove tubing from the channel. While holding the catheter in place, peel the protective dressing off the skin. The catheter, protective dressing and SureSet device may then be removed in one motion. Dispose of device according to hospital protocol.

R

