# Technical data

## Oticon Reveal™ 1 | 2 | 3 | 4
## miniRITE R

Oticon Reveal miniRITE R features a discreet design with a single push-button and a rechargeable lithium-ion battery, compatible with the miniFit Detect speaker system. Built on the new Reveal AI™ platform, fueling the latest BrainHearing™ technologies, this miniRITE supports Bluetooth® LE Audio, Bluetooth® Low Energy, and Auracast™ broadcast. It also offers hands-free communication and direct streaming for iPhone®, iPad®, Apple Vision Pro™, Apple Watch®, Mac® and select Android™ devices.

| Speaker 60 | Speaker 85 | Speaker 100 | Speaker 105 |
|---|---|---|---|
|  |  |  |  |
| miniRITE R | miniRITE R | miniRITE R | miniRITE R |

### Technical Features

- Auracast™ broadcast
- Bluetooth® LE Audio
- Bluetooth® Low Energy
- Contact charging
- CROS compatible
- IP68 rated
- Fast Pair
- NFMI (Near-Field Magnetic Induction)
- Tap control

### Accessories

- Oticon Companion app
- ConnectClip
- EduMic
- TV Adapter 3.0
- Oticon Charger miniRITE
- miniFit Detect speakers

For information on compatibility, please visit www.oticon.com/support/compatibility-guide

**Operating and charging conditions**
Temperature: +5°C to +40°C (+41°F to +104°F)
Humidity: 5% to 93% relative humidity, non-condensing
Atmospheric pressure: 700 hPa to 1060 hPa

**Transportation and storage conditions**
Temperature and humidity shall not exceed the mentioned limits during transportation and storage.

**Transport**
Temperature: -20°C to +60°C (-4°F to +140°F)
Humidity: 5% to 93% relative humidity, non-condensing
Atmospheric pressure: 700 hPa to 1060 hPa


**Storage**
Temperature: -20°C to +30°C (-4°F to +86°F)
Humidity: 5% to 93% relative humidity, non-condensing
Atmospheric pressure: 700 hPa to 1060 hPa


**WARNING:** No modification of this equipment is allowed.


Apple, the Apple logo, iPhone®, iPad®, Apple Vision Pro™, Apple Watch®, Mac® and the Mac logo are trademarks of Apple Inc., registered in the U.S. and other countries. Use of the Made for Apple badge means that an accessory has been designed to connect specifically to the Apple product(s) identified in the badge and has been certified by the developer to meet Apple performance standards. Apple is not responsible for the operation of this device or its compliance with safety and regulatory standards. Android™ and Fast Pair are trademarks of Google LLC. The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The Auracast™ word mark and logos are trademarks owned by the Bluetooth SIG. Any use of such marks by Demant is under license. Other trademarks and trade names are those of their respective owners.


# Fitting ranges

## Oticon Reveal 1

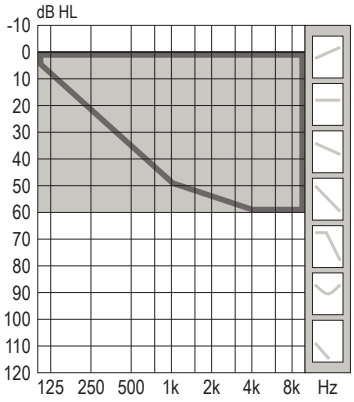


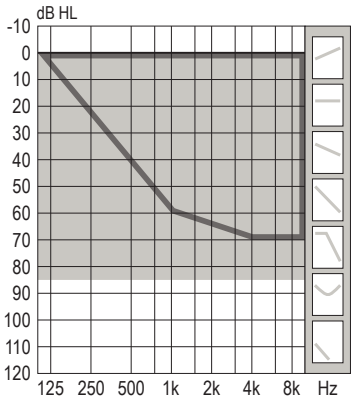


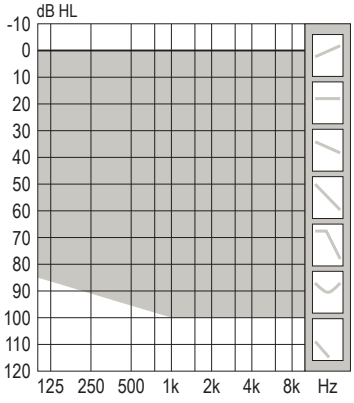
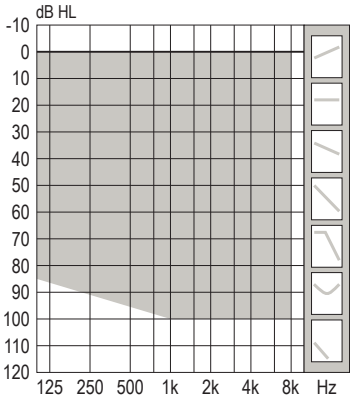


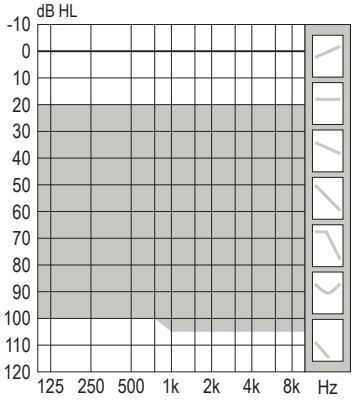
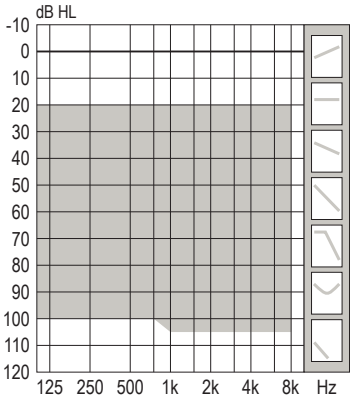


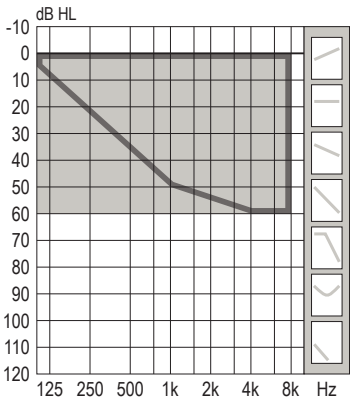

## Oticon Reveal 2 | 3 | 4

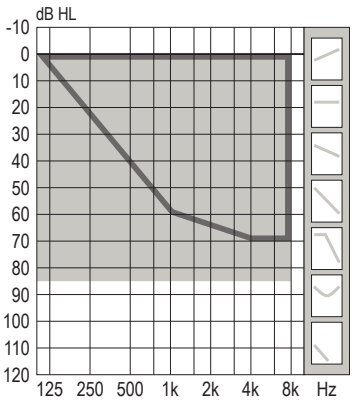


**60**

Mold, Bass & Power dome

OpenBass dome

**85**

Mold, Bass & Power dome

OpenBass dome

**100**

MicroShell Detect 100, Bass & Power dome

**105**

MicroShell Detect 105

# Feature overview

| | Reveal 1 | Reveal 2 | Reveal 3 | Reveal 4 |
|---|---|---|---|---|
| **Speech understanding & listening ease** | | | | |
| Reveal AI Clarifier™ | Level 1 | Level 2 | Level 3 | Level 4 |
| 4D Sensor technology | • | • | – | – |
| Environment classifier | 5 configurations | 5 configurations | 3 configurations | 1 configuration |
| AI Voice Clarifier | • | • | • | • |
| Operating area | 3 configurations | 2 configurations | 2 configurations | 1 configuration |
| Strength | 100% | 60% | 60% | 40% |
| Virtual Outer Ear | 3 configurations | 2 configurations | 2 configurations | 1 configuration |
| AI Noise Suppression Difficult/Easy | 12 dB / 6 dB | 10 dB / 4 dB | 8 dB / 2 dB | 6 dB / 0 dB |
| Sound Enhancer | 3 configurations | 2 configurations | 1 configuration | 1 configuration |
| Wind & Handling Stabilizer 2.0 | • | • | – | – |
| Wind & Handling Stabilizer | – | – | • | • |
| Reveal Amplifier™ | • | • | • | • |
| SuddenSound Stabilizer | 6 configurations | 5 configurations | 4 configurations | 2 configurations |
| Reveal Optimizer™ | • | • | • | • |
| Spatial Sound™ | 4 estimators | 4 estimators | 4 estimators | – |
| Soft Speech Booster | • | • | • | • |
| Frequency lowering, Speech Rescue™ | • | • | • | • |
| **Sound quality** | | | | |
| Clear Dynamics | • | • | – | – |
| Better-Ear Priority | • | • | • | – |
| Fitting Bandwidth[1] | 10 kHz | 8 kHz | 8 kHz | 8 kHz |
| Power Bass (streaming) | • | • | • | • |
| Processing Channels | 64 | 48 | 48 | 48 |
| **Personalization & optimized fitting** | | | | |
| Fitting Bands | 24 | 20 | 18 | 14 |
| Multiple Directionality options | • | • | • | • |
| Adaptation Management | • | • | • | • |
| Fitting Formulas | VAC+, NAL-NL1/NAL-NL2/NAL-NL3, DSL v5 | VAC+, NAL-NL1/NAL-NL2/NAL-NL3, DSL v5 | VAC+, NAL-NL1/NAL-NL2/NAL-NL3, DSL v5 | VAC+, NAL-NL1/NAL-NL2/NAL-NL3, DSL v5 |
| **Connecting to the world** | | | | |
| Oticon Companion app | • | • | • | • |
| Bluetooth® LE Audio[2] | • | • | • | • |
| Auracast™ broadcast[2] | • | • | • | • |
| Fast Pair | • | • | • | • |
| Hands-free communication[2] | • | • | • | • |
| Direct streaming[2] | • | • | • | • |
| Streaming comfort | • | • | • | • |
| ConnectClip | • | • | • | • |
| EduMic | • | • | • | • |
| Remote Control 3.0 | • | • | • | • |
| TV Adapter 3.0 | • | • | • | • |
| Tinnitus SoundSupport™ | • | • | • | • |
| CROS/BiCROS support | • | • | • | • |

1) Bandwidth accessible for gain adjustments during fitting
2) Available on select devices. For more information, please visit www.oticon.com/support/compatibility-guide

# Oticon Reveal 1 miniRITE R

# Ear Simulator

Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2022, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010





**Technical information**
Omnidirectional mode is used unless otherwise stated.

**Speaker 60 / 100**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m


**Speaker 85 / 105**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m

Speaker 60 — Speaker 85


OSPL90 (dB SPL)




Full-on gain (dB)





Frequency response (dB SPL)





Speaker 100 — Speaker 105


OSPL90 (dB SPL)




Full-on gain (dB)




Frequency response (dB SPL)




| | Speaker 60 | Speaker 85 | Speaker 100 | Speaker 105 |
|---|---|---|---|---|
| OSPL90, Peak (dB SPL) | 120 | 127 | 132 | 135 |
| OSPL90, 1600 Hz (dB SPL) | 113 | 121 | 130 | 133 |
| OSPL90, HFA (dB SPL) | 113 | 121 | 129 | 131 |
| Full-on gain, Peak (dB)[1] | 44 | 66 | 69 | 72 |
| Full-on gain, 1600 Hz (dB)[1] | 40 | 54 | 65 | 65 |
| Full-on gain, HFA (dB)[1] | 39 | 56 | 65 | 65 |
| Reference test gain (dB) | 33 | 46 | 54 | 57 |
| Frequency range (Hz) | <100-9400 | <100-9400 | <100-8800 | <100-8800 |
| Telecoil output, 1 mA/m field (1600 Hz) (dB SPL) | 71 | 85 | 97 | 97 |
| Telecoil output, 10 mA/m field (1600 Hz) (dB SPL) | 91 | 105 | 117 | 117 |
| Total harmonic distortion (Input 70 dB SPL), 500 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 70 dB SPL), 800 Hz (%) | <2 | <2 | <3 | <3 |
| Total harmonic distortion (Input 70 dB SPL), 1600 Hz (%) | <3 | <3 | <2 | <3 |
| Equivalent input noise level, Omni (dB SPL) | 17 | 22 | 16 | 17 |
| Battery | Lithium-ion | Lithium-ion | Lithium-ion | Lithium-ion |
| Expected operating time, hours[2] | 24 | 24 | 24 | 24 |

1) Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response but without influence of feedback.
2) Measurement is done in quiescent mode. Expected use time for rechargeable battery depends on use pattern, active feature set, hearing loss, sound environment, battery age and use of wireless accessories.

# Oticon Reveal 1 miniRITE R

# 2CC Coupler

Measured according to ANSI S3.22-2024,
IEC 60118-0:2022 and IEC 60318-5:2006





**Technical information**
Omnidirectional mode is used unless otherwise stated.

**Speaker 60 / 100**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m


**Speaker 85 / 105**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m

Speaker 60 — Speaker 85


OSPL90 (dB SPL)




Full-on gain (dB)





Frequency response (dB SPL)





Speaker 100 — Speaker 105


OSPL90 (dB SPL)




Full-on gain (dB)




Frequency response (dB SPL)




| | Speaker 60 | Speaker 85 | Speaker 100 | Speaker 105 |
|---|---|---|---|---|
| OSPL90, Peak (dB SPL) | 109 | 116 | 123 | 126 |
| OSPL90, HFA (dB SPL) | 105 | 113 | 121 | 123 |
| Full-on gain, Peak (dB)[1] | 34 | 55 | 59 | 63 |
| Full-on gain, HFA (dB)[1] | 31 | 47 | 57 | 57 |
| Reference test gain (dB) | 27 | 36 | 43 | 45 |
| Frequency range (Hz) | <100-8400 | <100-8500 | <100-7100 | <100-8200 |
| Telecoil output, HFA SPLITS L/R (dB SPL) | 87 | 96 | 103 | 105 |
| Telecoil output, Full-on HFA-SPLIV (dB SPL) | 82 | 99 | 108 | 108 |
| Total harmonic distortion (Input 70 dB SPL), 500 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 70 dB SPL), 800 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 65 dB SPL), 1600 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 60 dB SPL), 3200 Hz (%) | <2 | <2 | <2 | <2 |
| Equivalent input noise level, Omni (dB SPL) | 18 | 19 | 16 | 17 |
| Battery | Lithium-ion | Lithium-ion | Lithium-ion | Lithium-ion |
| Latency, (ms) | 8.1 | 8.1 | 8.1 | 8.1 |
| Expected operating time, hours[2] | 24 | 24 | 24 | 24 |

1) Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response but without influence of feedback.
2) Measurement is done in quiescent mode. Expected use time for rechargeable battery depends on use pattern, active feature set, hearing loss, sound environment, battery age and use of wireless accessories.

# Oticon Reveal 2 | 3 | 4 miniRITE R

# Ear Simulator

Measured according to IEC 60118-0:1983/AMD1:1994, IEC 60118-0:2022, IEC 60118-1:1995+AMD1:1998 CSV and IEC 60318-4:2010





**Technical information**
Omnidirectional mode is used unless otherwise stated.

**Speaker 60 / 100**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m


**Speaker 85 / 105**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m

Speaker 60 — Speaker 85


OSPL90 (dB SPL)




Full-on gain (dB)





Frequency response (dB SPL)





Speaker 100 — Speaker 105


OSPL90 (dB SPL)




Full-on gain (dB)




Frequency response (dB SPL)




| | Speaker 60 | Speaker 85 | Speaker 100 | Speaker 105 |
|---|---|---|---|---|
| OSPL90, Peak (dB SPL) | 120 | 127 | 132 | 135 |
| OSPL90, 1600 Hz (dB SPL) | 113 | 121 | 130 | 133 |
| OSPL90, HFA (dB SPL) | 113 | 121 | 129 | 131 |
| Full-on gain, Peak (dB)[1] | 44 | 66 | 69 | 72 |
| Full-on gain, 1600 Hz (dB)[1] | 40 | 54 | 65 | 65 |
| Full-on gain, HFA (dB)[1] | 39 | 56 | 65 | 65 |
| Reference test gain (dB) | 33 | 46 | 54 | 57 |
| Frequency range (Hz) | <100-7500 | <100-7500 | <100-7500 | <100-7500 |
| Telecoil output, 1 mA/m field (1600 Hz) (dB SPL) | 71 | 85 | 97 | 97 |
| Telecoil output, 10 mA/m field (1600 Hz) (dB SPL) | 91 | 105 | 117 | 117 |
| Total harmonic distortion (Input 70 dB SPL), 500 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 70 dB SPL), 800 Hz (%) | <2 | <2 | <3 | <3 |
| Total harmonic distortion (Input 70 dB SPL), 1600 Hz (%) | <3 | <3 | <2 | <3 |
| Equivalent input noise level, Omni (dB SPL) | 17 | 22 | 16 | 17 |
| Battery | Lithium-ion | Lithium-ion | Lithium-ion | Lithium-ion |
| Expected operating time, hours[2] | 24 | 24 | 24 | 24 |

1) Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response but without influence of feedback.
2) Measurement is done in quiescent mode. Expected use time for rechargeable battery depends on use pattern, active feature set, hearing loss, sound environment, battery age and use of wireless accessories.

# Oticon Reveal 2 | 3 | 4 miniRITE R

# 2CC Coupler

Measured according to ANSI S3.22-2024,
IEC 60118-0:2022 and IEC 60318-5:2006





**Technical information**
Omnidirectional mode is used unless otherwise stated.

**Speaker 60 / 100**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m


**Speaker 85 / 105**
Acoustic input: 60 dB SPL
Magnetic input: 31.6 mA/m

Speaker 60 — Speaker 85


OSPL90 (dB SPL)




Full-on gain (dB)





Frequency response (dB SPL)





Speaker 100 — Speaker 105


OSPL90 (dB SPL)




Full-on gain (dB)




Frequency response (dB SPL)




| | Speaker 60 | Speaker 85 | Speaker 100 | Speaker 105 |
|---|---|---|---|---|
| OSPL90, Peak (dB SPL) | 109 | 116 | 123 | 126 |
| OSPL90, HFA (dB SPL) | 105 | 113 | 121 | 123 |
| Full-on gain, Peak (dB)[1] | 34 | 55 | 59 | 63 |
| Full-on gain, HFA (dB)[1] | 31 | 47 | 57 | 57 |
| Reference test gain (dB) | 27 | 36 | 43 | 45 |
| Frequency range (Hz) | <100-7500 | <100-7500 | <100-7100 | <100-7500 |
| Telecoil output, HFA SPLITS L/R (dB SPL) | 87 | 96 | 103 | 105 |
| Telecoil output, Full-on HFA-SPLIV (dB SPL) | 82 | 99 | 108 | 108 |
| Total harmonic distortion (Input 70 dB SPL), 500 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 70 dB SPL), 800 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 65 dB SPL), 1600 Hz (%) | <2 | <2 | <2 | <2 |
| Total harmonic distortion (Input 60 dB SPL), 3200 Hz (%) | <2 | <2 | <2 | <2 |
| Equivalent input noise level, Omni (dB SPL) | 18 | 19 | 16 | 17 |
| Battery | Lithium-ion | Lithium-ion | Lithium-ion | Lithium-ion |
| Latency, (ms) | 8.1 | 8.1 | 8.1 | 8.1 |
| Expected operating time, hours[2] | 24 | 24 | 24 | 24 |

1) Measured with the gain control of the hearing aids set to their full-on position minus 20 dB and with an input SPL of 70 dB. This is to obtain a gain response equal to the full-on gain response but without influence of feedback.
2) Measurement is done in quiescent mode. Expected use time for rechargeable battery depends on use pattern, active feature set, hearing loss, sound environment, battery age and use of wireless accessories.

SBO Hearing A/S
Kongebakken 9
DK-2765 Smørum
Denmark

**Headquarters**
Oticon A/S
Kongebakken 9
DK-2765 Smørum
Denmark

300960US / 2026.05.07 / v1