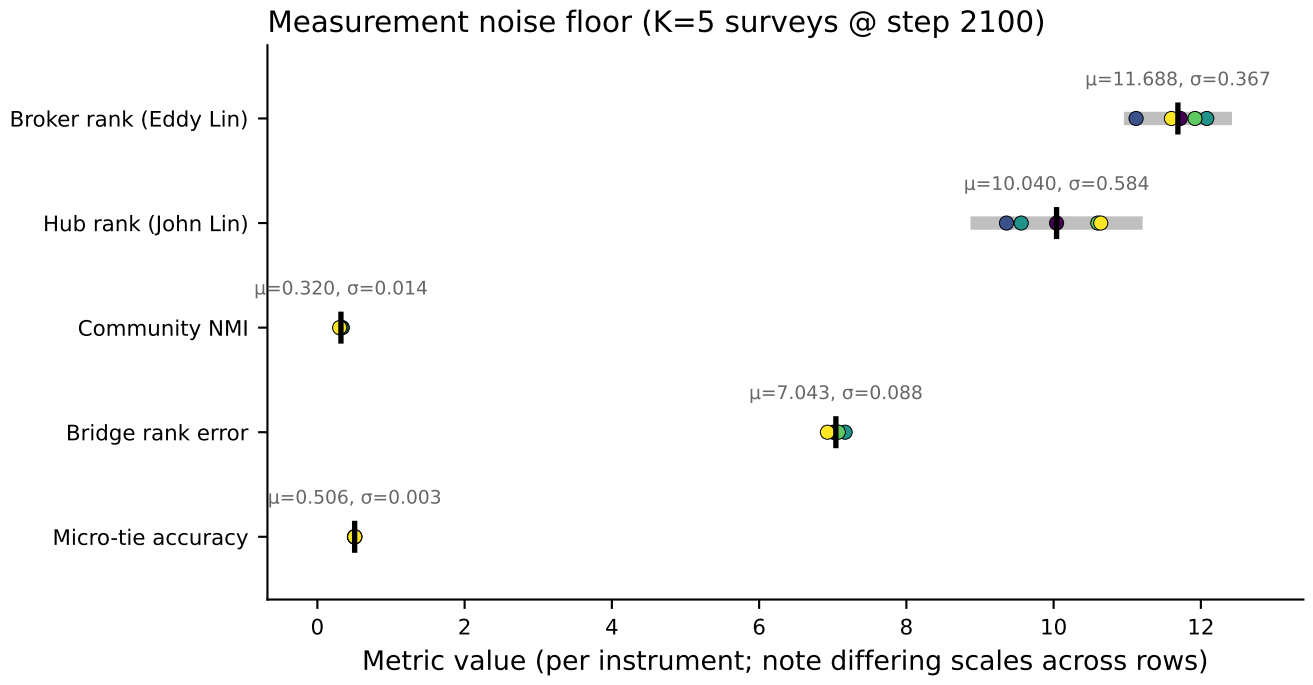
Measurement noise floor (K=5 surveys @ step 2100)
Broker rank (Eddy Lin)
μ=11.688, σ=0.367
Hub rank (John Lin)
μ=10.040, σ=0.584
Community NMI
μ=0.320, σ=0.014
Bridge rank error
μ=7.043, σ=0.088
Micro-tie accuracy
μ=0.506, σ=0.003
0
2
4
6
8
10
12
Metric value (per instrument; note differing scales across rows)