Maltose calibration curve · DNS assay

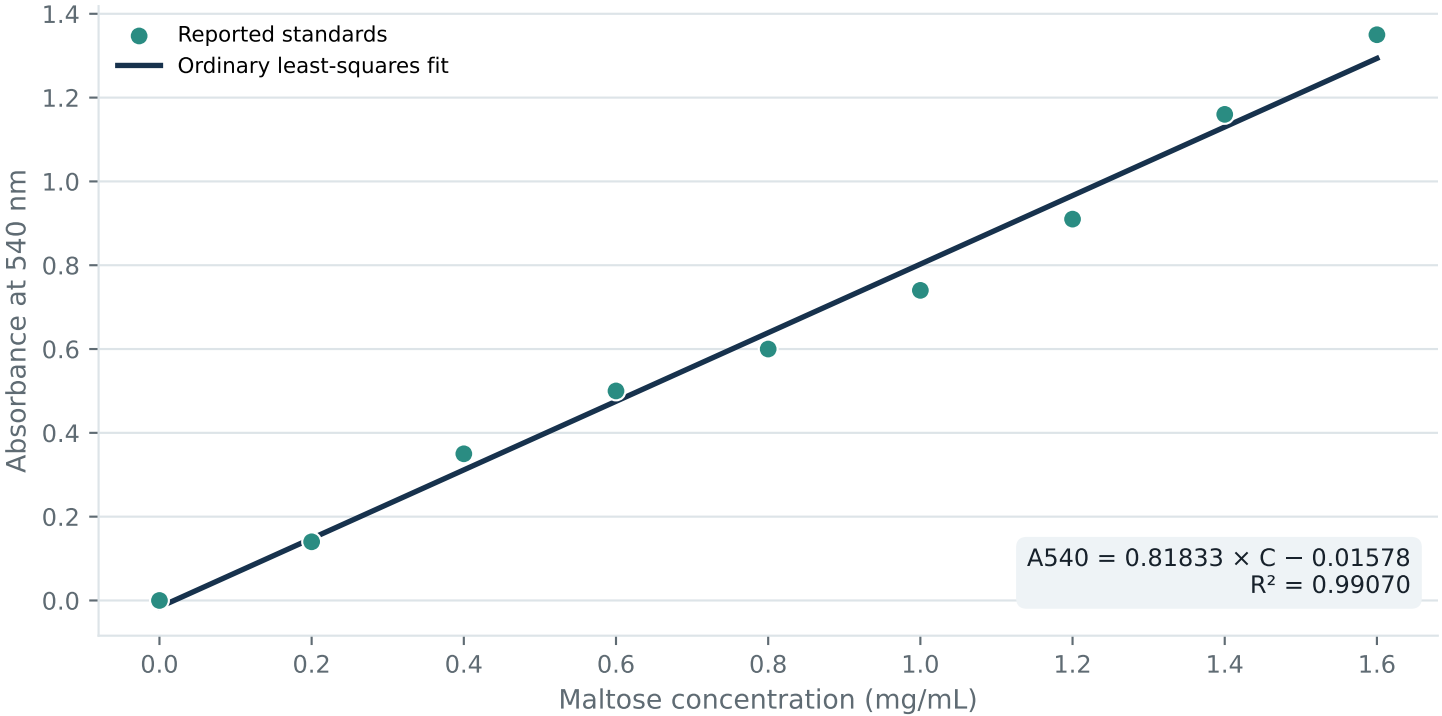

Fit recalculated from the nine tabulated standards; the source text contains an intercept-sign inconsistency.