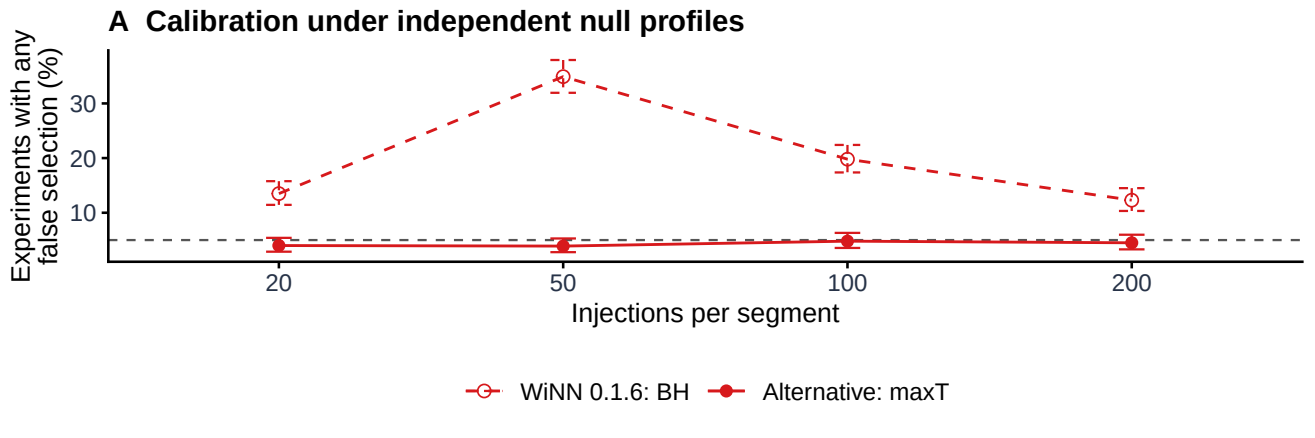
A Calibration under independent null profiles
Experiments with any false selection (%)
30
20
10
20
50
100
200
Injections per segment
WiNN 0.1.6: BH
Alternative: maxT