


DANTROLENE RECONSTITUTION


(HIGHEST PRIORITY)

MIXING DANTROLENE CAN BE TIME CONSUMING
USE AS MANY PEOPLE AS ARE AVAILABLE. HERE IS ONE
METHOD

12 AMPOULES WILL BE REQUIRED FOR EACH DOSE IN A
100KG PATIENT UP TO **EVERY 10-15 MINUTES**

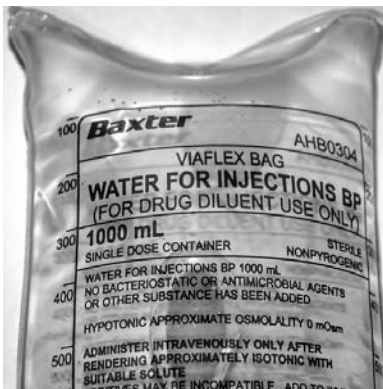

1) Dantrolene must be mixed **ONLY** with **STERILE WATER**

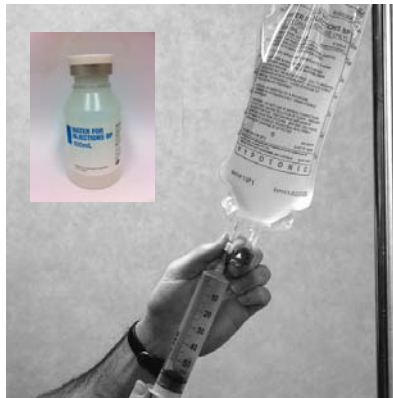


2) 60 mls water for each 20mg vial from bag or bottle




3) Remove metal vial cap or flip off cap



4) Inject 30ml of water

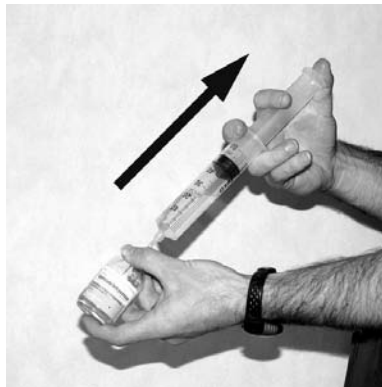

5) Hold syringe vertically, allow air in vial to escape, inject remaining 30mls water

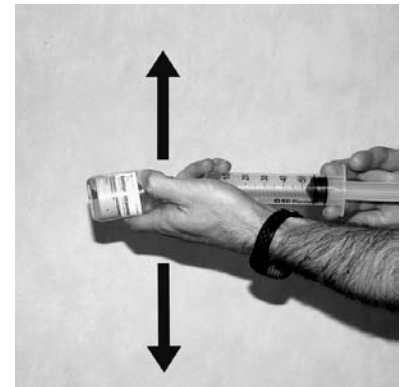

6) Hold together firmly or disconnect and shake to mix