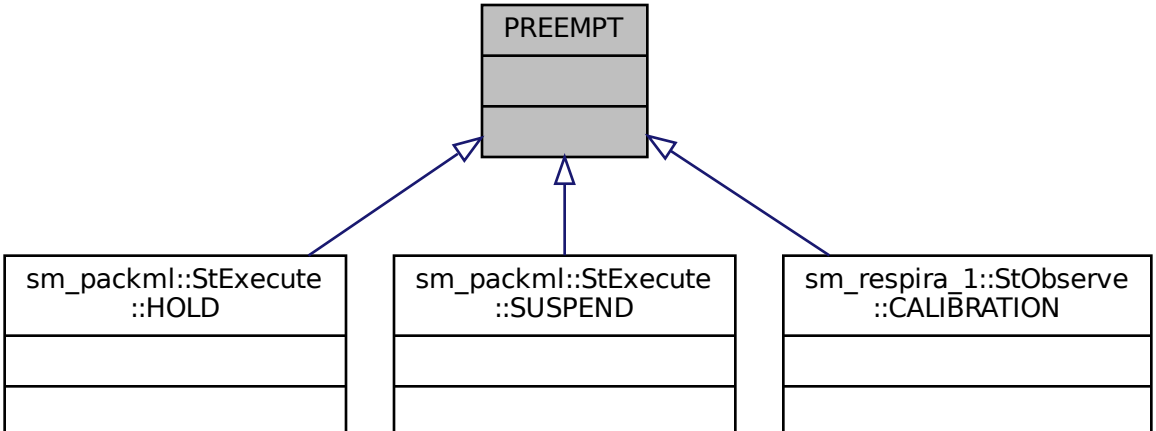
PREEMPT
sm_packml::StExecute
::HOLD
sm_packml::StExecute
::SUSPEND
sm_respira_1::StObserve
::CALIBRATION