


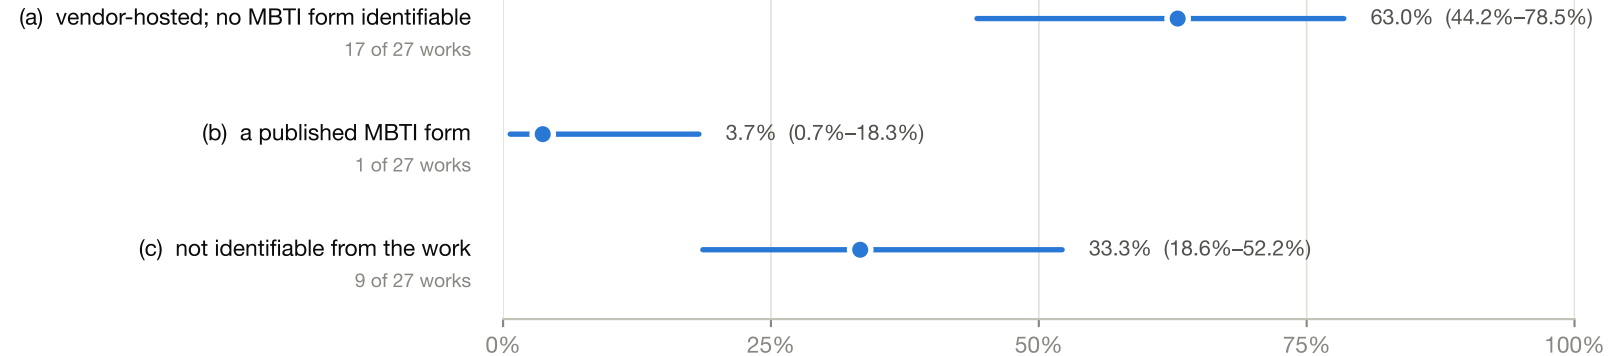

Share of the 27 works in the main analysis that administered an instrument, with model-based Wilson 95% intervals