

# A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in Telehealth System

Maurine C. Panergo  
 College of Engineering  
 Southern Luzon State University  
 Lucban, Quezon, Philippines  
 mpanergo@slsu.edu.ph

Febus Reidj G. Cruz  
 School of EECE  
 Mapua University  
 Intramuros, Manila, Philippines  
 frgcruz@mapua.edu.ph

Renato R. Maaliw III  
 College of Engineering  
 Southern Luzon State University  
 Lucban, Quezon, Philippines  
 rmaaliw@slsu.edu.ph

**Abstract**—Hypertension is one of the leading causes of mortality worldwide, increasing the likelihood of developing heart, renal, brain, and other illnesses. Reliable blood pressure measurement is critical because even minor errors can have severe effects on individuals. In this study, we developed a telehealth system that integrates an instrumentation amplifier and band-pass filter circuit to resolve dissipation losses and monitor such conditions, thus improving accurate health parameter measurements. Our prototype was tested on 30 subjects of varying ages for ten cross-validated trials. Quantitative results show that our amplified system was able to outperform high-end digital commercially available instruments with a mean precision of 96.67% (mean arterial pressure), 96.79% (pulse rate), and 99.13% (temperature).

**Keywords**—dissipation losses, e-health, hypertension, instrumentation amplifier, mean arterial pressure, monitoring

## I. INTRODUCTION

Society needs numerous healthcare solutions that deliver life-saving services. Electronic health (e-health) facilitates health and wellness benefits to patients remotely using telecommunication technologies. Aside from traditional methods, electronic devices can measure various bio-signals such as heart rate, pulse oximetry, temperatures, and other related health parameters. Blood pressure (BP) is a critical vital indicator that requires monitoring due to its link with various health problems, including hypertension [1 – 3]. It is a life-threatening medical condition that increases the chance of developing cardiovascular, renal, and cerebrovascular diseases, among other complications. Moreover, it is one of the leading causes of early mortality worldwide, affecting more than a billion people [4]. Statistics show that for an increase of 10mmHg (millimeter mercury) in systolic blood pressure, the relative risk of death rose by 28%, according to a 10-year study from different parts of the globe [5]. Medical professionals highlight the risks that even a slight change in blood pressure can have devastating repercussions.

Regrettably, the accuracy of BP measurement differs significantly amongst devices. The American Heart Association (AHA) advises using a manual mercury manometer for this measurement [6]. Even with a fully calibrated instrument, however, significant measurement error is inevitable [7]. With all of these potential impediments to reliable manual readings, one could conclude that an electronic device is preferable. However, it is not always the case as certifying authorities such as the Food and Drug Administration (FDA) rely on manufacturer's voluntary

compliance with requirements [8]. Companies seeking an easy profit are avoiding the procedure of equipment precision testing due to its high cost. These findings pertain to the non-certification of BP equipment sold to hospitals, clinics, and individuals. Additionally, the accuracy issues associated with low-cost and even high-end BP electronic monitors for home users are well known [9 – 11]. Hence, authorities must impose strict testing and mandatory certifications to mitigate and resolve these pressing issues.

Most modern electronic BP devices currently in the market are composed of a pressure sensor, processor, motor mechanism, and cuff. The cuff pressure of the BP sensor can directly measure the magnitude of these pressure pulses. As it reaches the maximum amplitude, the pulses become increasingly significant as soon as the pressure in the cuff is slowly exhausted. If the cuff pressure decreases, it minimizes the occlusion of the artery that causes the pulse amplitude to decay. According to different studies, this dissipating factor causes most electronic BP devices to provide inaccurate results [12], leading to the need to design an additional sensor amplifier [13 - 15]. The use of technology to create tailored interventions for people with hypertension is gaining popularity. In the study of [16], the efficiency of digital technology on hypertension management has a considerable positive influence on BP control. Considering the ubiquity of modern wireless communication devices such as smartphones has made it easier to manage chronic conditions. According to literature, a lot of organizations and researchers have focused on the improvement of these devices for hypertension control.

Telehealth (TH) is a word used to describe electronic applications that leverage information and communication technology (ICT) to provide remote support, flexible and convenient access, and individualized feedback to serve growing health demands [17]. Integration of these systems with pre-existing infrastructures is straightforward and accessible via personal computers, mobile phones, and tablets. Numerous studies have shown that it is a viable option for managing and changing hypertension self-care habits [18 - 22]. Furthermore, it encourages patients, particularly younger generations, who are less likely to undergo lifestyle modification therapy to sustain conscious health behaviors. As a result, the efficacy of existing TH interventions on hypertension self-care using modern technology has to be improved. The primary goal of this study was to design and develop a sensor amplifier for blood pressure sensors in improving the accuracy of critical BP measurements.

Moreover, a TH system was created with wireless transmission technologies such as a global system for mobile communication (GSM) and radio frequency (RF) for real-time data transmission. It also aims to compare the conventional way of monitoring health parameters between the developed systems.

The paper's main contribution was improving health monitoring in medicine through the design of an instrumentation amplifier as it is beneficial to the public, patients, and health practitioners.

## II. METHODOLOGY

### A. System Overview

The system primarily concentrates on designing the sensor amplifier of the BP measurement for the TH system. Input components are connected to the designed amplifier, such as pressure sensor, motor pump, and cuff. The process needs to have this crucial amplifier to magnify the signal from the band pass filter to eliminate substantial noises within the signal. A final stage amplifier connects to the output, which is the blood pressure sensor.

After the design of the circuit, the BP's amplifier is connected with other inputs such as the AC source, power supply, body temperature sensor, and pulse rate sensor. Such inputs are processed and read through the microcontroller serving as the heart of the system. The controller then sends the data to the GSM and Zigbee, reflecting the output through an LCD display.

### B. Methods and Procedures

This section presents the processes and methods adopted in gathering data needed for the research work. It includes hardware and software development, and other related methods to determine the effectiveness of the study. Figure 1 shows the block diagram of the methodologies used to design and implement the circuit amplifier design.

The process flow diagram consists of the sensor amplifier's design, the TH system's design and fabrication, simulation of the sensor amplifier, and the tests evaluation.

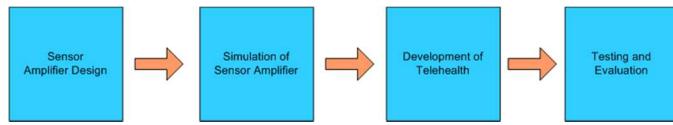


Fig. 1. Process flow diagram

### C. Sensor Amplifier Design

Figure 2 shows the schematic principle operation of the system initially based on Karplus and the Texas Instrument handbook using a Wheatstone bridge sensor [23]. The amplifiers consist of an instrumentation amplifier, a low-pass filter, and a final stage amplifier. These three additional electronic components are specifically designed to solve the occurrence of signal losses as observed for the wide array of electronic BP measuring devices available on the market. It is crucial to solve the dissipation losses encountered as observed on commercially available electronic measuring devices.

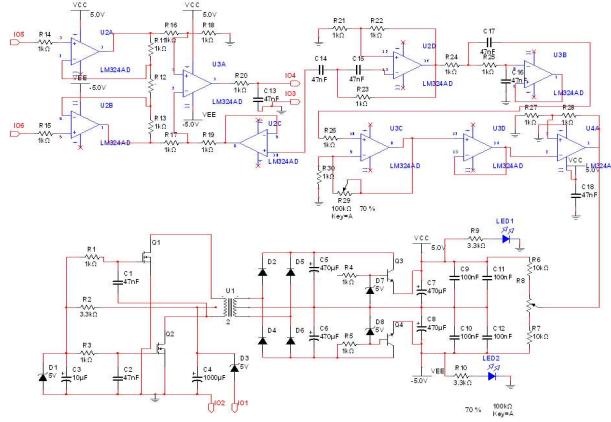


Fig. 2. Schematic diagram of the sensor amplifier

### D. Operational Amplifier Selection

A critical part of the design is the selection of operational amplifiers (op amps). Most op amps will work for the design but we intentionally selected the LM324 instrument amplifier (IA) [24] comprised of four operational amplifiers on a single chip to minimize the amount of wires to construct the circuit. It also has a proven track record in many complex electronics designs having a notable maximum gain and has a saturation level at  $V_{cc} - 1.5$  V. If the product of the input and the gain exceeds the threshold, the op-amp will enter saturation and provide an incorrect output. It is the primary reason for the selection of the component.

### E. Resistor Value Selection

A typical IA has seven resistors. Selection of resistor values is identified through using a transfer function using the equation of:

$$V_{out} = (V_1 - V_2)(R_2/R_1)(1 + (2R_5)/R_G) \quad (1)$$

This is true if  $R_5$  equaled  $R_6$ ,  $R_2$  matches  $R_4$ , and  $R_1$  equals  $R_3$ . However, if  $R_6 = R_5 = R_1 = R_4 = R_2 = R$ , this transfer function could be reduced further, Thus, the formula is:

$$V_{out} = (V_1 - V_2)(1 + 2R/R_G) \quad (2)$$

Based on the equation, we select the value of R ranging from 25KOhm to 1MOhm. Figure 3 shows the schematic diagram of IA.

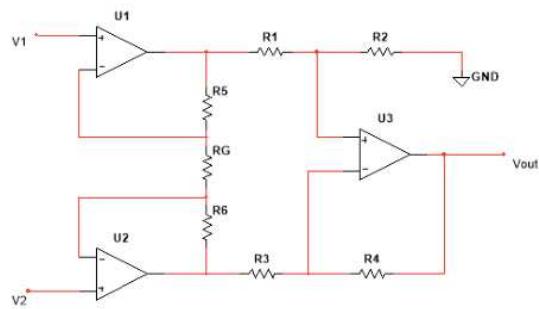


Fig. 3. Instrumentation amplifier (IA) circuit

#### F. Gain Calculation and Testing IA

A streamlined transfer function based on Equation 2 enables the overall gain to be determined by a single resistor ( $R_G$ ). A low value resistor for  $R_G$  results in a higher gain, whereas a bigger resistor leads in a lower gain.

We run the tests using MultiSim software to test the circuit to verify and characterize the design's performance by setting the function generator to 500m  $V_{PP}$  SIN wave at 1 kHz and inputting it to  $V_I$  (see Figure 3). To check the gain of an instrumentation amplifier, an oscilloscope probe must be placed on the function generator and another on the output amplifier.

Figure 4 shows the input and output simulation testing waveforms with an input offset equal to  $172.991\mu$  while the output offset is  $-172.934\mu$  with only 0.057 absolute difference.

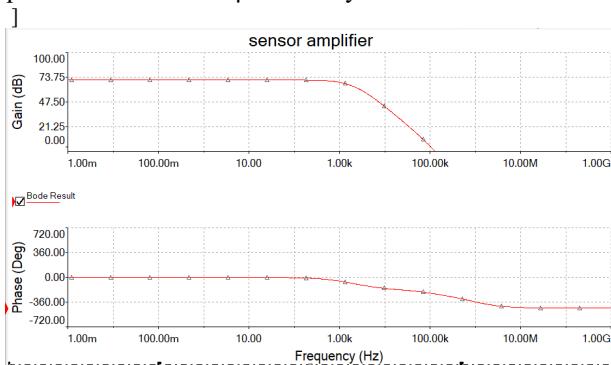


Fig. 4. Simulation of gain and phase

#### G. Band-Pass Filter Design

A band-pass filter was adapted to capture the cuff pressure and pulse wave signals from the noise signals. This design is adapted to adjust the appropriate signal levels and as an input to the analog-to-digital conversion circuits. The filter's circuitry is composed of 4-stage operational amplifier to properly detect pulse signals and remove further interferences. Figure 5 shows the band-pass filter (BPF) for the pulse wave signals processing.

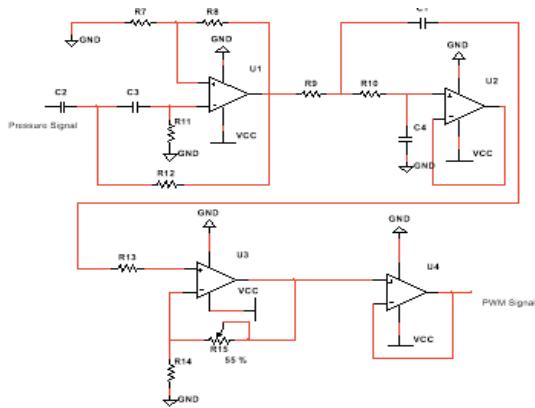


Fig. 5. Band-pass filter design

#### H. Final Stage Amplifier

A signal coming from a BPF is weak and needs amplification at the final stage to further avoid dissipation

losses. This is significant to attain accurate reading. Figure 6 illustrates the design of the final stage amplifier.

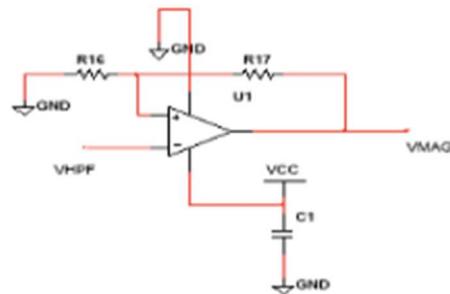


Fig. 6. Final stage amplifier design

#### I. Design and Development of Telehealth System

Figure 7 and Figure 8 show the diagram of the system's setup, including both hardware and software components. Two major components, such as the transmitting and receiving units, handle the system's essential operation. The transmitting unit serves as the input, which is composed of medical sensors that measure a person's specific health parameters. An Arduino microcontroller manages the sensors and data acquisitions are displayed on the liquid crystal display (LCD) and transmitted to the receiving unit. The two units in the system are the host computer and mobile phone.

Through Zigbee technology, the acquired data are accessed through wireless medium to the host computer for storage purposes. Furthermore, the data are received through a mobile phone using short-message sending (SMS). Moreover, the figure shows the system operation along with the interconnections of the components involved in the system. The body temperature sensor, pulse rate sensor, and blood pressure sensor served as the system's input while the LCD, computer, and mobile phone served as the output at which the acquired data are received and displayed.

We utilized a ZigBee router and a GSM module as transmitters for their known flexibility while the ZigBee coordinator connected to the computer through the Arduino and the mobile phone serves as the receivers.

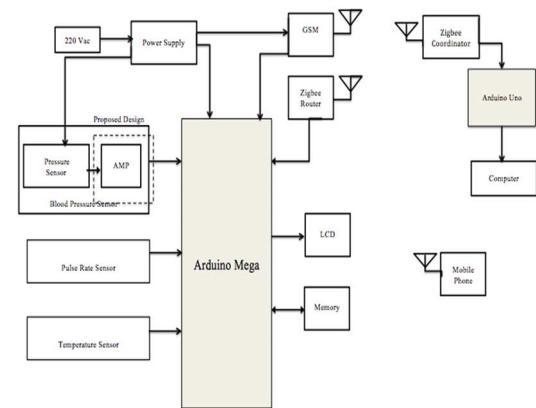


Fig. 7. Block diagram of the Telehealth system

### III. RESULTS

This section investigates and assesses the accuracy of health parameter data measured using conventional (C), digital (D), and our prototype (P) instruments using the amplifier design. The following subsections show the different results.

#### A. Mean Arterial Blood Pressure (MAP) Readings

Table 1 shows the comparative blood pressure measurements compiled from the conventional, commercial, and our developed prototype.

TABLE 1  
MEAN ARTERIAL PRESSURE COMPARATIVE TEST RESULTS

Trial	Age Brackets								
	8 - 16			17 - 29			30 and above		
	C	D	P	C	D	P	C	D	P
1	90	87.7	88.6	90	71	82.1	94.4	101.7	95.8
2	87.7	79.3	84.1	86.67	88.3	88.5	87.7	80.3	85.4
3	74.4	71.7	78.3	78.89	78.1	81.3	92.2	94.5	91.3
4	90	86.6	87.7	87.78	87.7	85.2	82.2	81.7	76.7
5	82.2	78.5	78.6	77.78	67	81.6	91.1	94.4	91.4
6	83.3	80.3	80.4	74.44	71.7	74.7	85.5	84.5	89
7	77.7	76	79.8	92.22	87.8	84.5	78.8	81.2	79.7
8	88.8	82.8	85.2	78.89	80.3	78.3	81.6	78.1	76.6
9	85.5	82.7	86.5	87.78	81.8	84.3	92.2	93.3	91.8
10	77.7	76.5	75.7	92.22	87.5	85.3	88.8	88.2	90
RMSE	4.06			2.81			7.53		
MAPE	4.14			3.18			6.01		
MBE	-3.52			-1.24			-4.54		

It demonstrates that our prototype produces an accurate measurement compared to a commercially available blood pressure device by obtaining lower RMSE outcomes for all age brackets of 2.81, 4.61, and 2.79. In addition, it achieved better MAPE values of 3.18, 4.27, and 2.52. MBE results show that our prototype, on average, underestimated the baseline readings by only -1.33.

#### B. Pulse Rate Readings

The comparison of pulse rate data taken from the conventional, digital, and our designed prototype is shown in Table 2. Our prototype beats a commercially available digital pulse rate monitoring instrument with reduced RMSE scores of 2.01, 6.54, and 2.31. The results indicated our amplifier's design capacity in achieving MAPE values of 2.15, 5.60, and 1.88. MBE records show that our prototype deprecated the baseline measurements by only -2.28.

TABLE 2  
PULSE RATE COMPARATIVE TEST RESULTS

Trial	Age Brackets								
	8 - 16			17 - 29			30 and above		
	C	D	P	C	D	P	C	D	P
1	82.6	87.6	83	72.6	88	70.3	101	104.6	100.6
2	75.6	76.3	76.1	67	89.6	69.3	72.6	77	74.3
3	77.3	75	76.3	77.3	82	74.6	80.3	85.3	83.6
4	82.3	79.6	79.6	93.3	98.3	90.6	84.8	84.4	84.4
5	72.3	69	68.6	83.3	80.3	81.3	91.3	93.3	90.6
6	67.3	64	66.3	98.3	93.67	88.3	101	105.3	101.3
7	79	74.6	76.6	103	93	92	74.6	76.6	73.6
8	77.6	75.3	75.4	102	127.3	94.6	75.3	75.3	74.1
9	71.3	70	71.2	92.6	95	91	94.3	90.6	88.3
10	80.6	76.3	78	101.6	101.6	90.6	71.6	70.6	70.6
RMSE	3.23			2.01			12.53		
MAPE	3.83			2.15			11.17		
MBE	-1.82			-1.48			-5.77		

#### C. Temperature Readings

The temperature measurements accumulated from the conventional, commercial, and our prototype are summarized

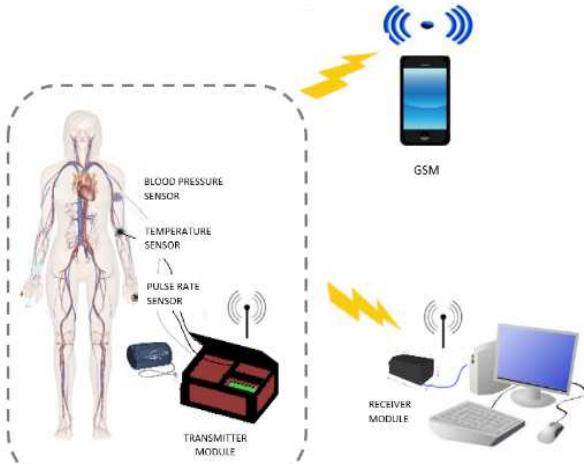


Fig. 8. Telehealth system's setup

#### J. Testing and Evaluation Metrics

To validate the measurement accuracy of the design, we performed cross-validated trials for three age brackets (8 – 16, 17 – 29 & 30 and above). We selected thirty respondents for each age bracket and recorded their average mean arterial pressure (MAP) [25], temperature, and pulse rate ten times on each trial using a conventional calibrated manual manometer conducted by trained professionals to set the unbiased baseline measurements. These results were then compared to commercially available high-end digital instruments and the records made by our enhanced prototype. Three standard-based evaluation metrics were used, such as root mean squared error (RMSE) [26], mean absolute percentage error (MAPE), and mean bias error (MBE) for results validation [27]. Equations 3, 4, and 5 express the details of the formula:

$$RMSE = \sqrt{\frac{\sum_{i=1}^N (t_i - p_i)^2}{N}} \quad (3)$$

$$MAPE = \frac{\sum_{i=1}^N \left| \frac{t_i - p_i}{p_i} \right| \times 100}{N} \quad (4)$$

$$MBE = \frac{\sum_{i=1}^N \left| \frac{t_i - p_i}{p_i} \right|}{N} \quad (5)$$

where  $t_i$  is the cross-validated health parameter measured values,  $p_i$  is the benchmarked results of a commercial digital instrument and the developed prototype, and  $N$  is the number of trials.

We have purposely selected the scaled-dependent RMSE as it is a remarkable all-purpose error statistics capable of examining error differences. MAPE is another error metrics that are not scale-dependent and compares results at various scales. Finally, the MBE primarily determined if the measurement results are underestimated or overestimated.

in Table 3. Our device surpasses a commercially available pulse rate apparatus in terms of performance and has a lesser RMSE evaluation of 0.23 and 0.51 except for age bracket 30 and above (0.48). The results revealed our design's advantages in achieving MAPE values of 0.54, 1.10, and 0.96. According to MBE results, our prototype underestimated the measurements by an average of -0.083.

TABLE 3  
TEMPERATURE COMPARATIVE TEST RESULTS

Trial	Age Brackets								
	8 - 16			17 - 29			30 and above		
	C	D	P	C	D	P	C	D	P
1	36.1	36.3	36	36.3	37	36.2	36.9	37	36.2
2	36.3	36.2	36.2	36.2	37	36.1	36.3	36.8	35.1
3	36.8	37	36.9	35.4	36.7	36.6	37	36.8	37
4	37	36.7	36.6	36	36.3	36.1	37.3	37.5	37
5	36.4	36.6	36.5	36.4	36.8	36.7	35.7	36.2	36.7
6	35.8	36	36.1	36.2	36.8	35.8	36.8	36.4	36.7
7	36.3	36.7	36.2	36.3	36.6	35.9	37	37.4	37
8	36.2	36.8	36	37.1	36.7	36.6	37.2	36.6	37.5
9	36.7	36.3	36.3	36.7	36.8	36	35.8	36	36
10	36.6	36.5	36.4	36.7	36.8	36.9	36	37	37
RMSE		0.30	0.23		0.60	0.51		0.48	0.49
MAPE		0.74	0.54		1.38	1.10		1.12	0.96
MBE		0.09	-0.01		0.42	-0.04		0.17	0.02

#### IV. DISCUSSIONS

This research demonstrated the advantages of the amplifier circuit design in improving the accuracy of health-related parameter measurements through extensive testing. The quantitative results show that our prototype using the amplifier circuit design outperforms high-end commercially available digital instruments with a precision of 96.67% (blood pressure), 96.79% (pulse rate), and 99.13% (temperature). Our findings clearly illustrate that integrating additional amplifiers to the test instruments coupled with circuit filter design significantly improves overall readings. It reduces error rates by a collective mean of 1.39%. Furthermore, it demonstrates that the dissipation losses in signals were intuitively compensated by the prototype. The study's findings are at par with the works of [28 – 34] in digital measurements of health parameters. Similar to any vital signs measuring device, improper connection of the sensors to the appropriate body parts can result to inaccurate readings. Also, unnecessary movements and action of an individual during testing specifically for the blood pressure and pulse rate sensor can greatly affect the quantitative results. Thus, standard operating procedures must also be considered in using our health measuring device.

#### V. CONCLUSIONS AND FUTURE WORKS

A sensor amplifier based on an instrumentation amplifier with a band-pass filter was designed and deployed in the TH system. The data gathered determined the prototype's accuracy compared to commercially available digital instruments. Quantitative results demonstrated its capabilities in measuring blood pressure and other health parameters significantly closer to traditional devices readings. It indicates that the amplification of the signal plays a crucial role in obtaining accurate results. Our research is far from perfect as a full-fledged system and more improvements can be done. As for the future direction of the research, the authors will expand the system's feature by adding more sensors to monitor health-

related parameters, such as oxygen saturation, glucose, electrocardiogram (ECG), electromyography (EMG), and galvanic skin response. In addition, a transformer-less power supply for weight reduction and a smaller-sized microcontroller and transmitting unit will be explored to make the system as portable as possible.

#### ACKNOWLEDGMENT

The researchers would like to express their sincere gratitude to the participants and Southern Luzon State University's Health Service Unit for allowing us to conduct the prototype's testing in the University clinic.

#### REFERENCES

- [1] K. Mills, A. Stefanescu and J. He, "The global epidemiology of hypertension", *Nature Reviews*, 16(4), pp. 223-237, 2020.
- [2] C. Cardoso and G. Salles, "Prognostic impact of home blood pressures for adverse cardiovascular outcomes and mortality in patients with resistant hypertension: A prospective cohort study", *Hypertension*, 2021.
- [3] C. Bartels, E. Ramly, H. Johnson, et al., "Connecting rheumatology patients to primary care for high blood pressure: Specialty clinic protocol improves follow-up and population blood pressures", *Arthritis care & research*, 71(4), pp. 461-470, 2019.
- [4] S. Kjeldsen, "Hypertension and cardiovascular risk: general aspects. *Pharmacological research*", 129(2), pp. 95-99, 2018.
- [5] D. Rabi, K. McBrien, R. Sapir-Pichhadze, et al. "Hypertension Canada's 2020 comprehensive guidelines for the prevention, diagnosis, risk assessment, and treatment of hypertension in adults and children", *Canadian Journal of Cardiology*, 36(4), pp. 596-624, 2020.
- [6] J. McEvoy, N. Daya, F. Rahman, et al., "Association of isolated diastolic hypertension as defined by the 2017 ACC/AHA blood pressure guideline with incident cardiovascular outcomes", *JAMA*, 323(4), 2020.
- [7] S. Seals, L. Colantino, J. Tingle, D. Shimbo, A. Correa, M. Griswold and P. Munter, "Calibration of blood pressure measurements in the Jackson Heart Study", *Blood Pressure Monitoring*, 24(3), pp. 130, 2019
- [8] J. Sharman, E. O'Brien, B. Alpert, Schutte, et al., "Lancet Commission on Hypertension group position statement on the global improvement of accuracy standards for devices that measure blood pressure", *Journal of Hypertension*, 38(1), p. 15-21, 2020.
- [9] J. Hodgkinson, M. Lee, S. Milner, P. Bradburn, et al., "Accuracy of blood-pressure monitors owned by patients with hypertension (ACCU-RATE study): a cross-sectional, observational study in central England", *British Journal of General Practice*, 70(697), pp. 548-554, 2020.
- [10] N. Bello, J. Woodley, K. Cleary, L. Falzon, et al., "Accuracy of blood pressure measurement devices in pregnancy: A systematic review of validation studies", *Hypertension*, 7(12), pp. 326-335, 2018.
- [11] R. Padwal, N. Campbell, M. Weber, D. Lackland, et al., "The accuracy in measurement of blood pressure (aim - bp) collaborative: Background and rationale", *The Journal of Clinical Hypertension*, 21(12), pp. 1780-1783, 2019.
- [12] M. Gotzmann, M. Hogeweg, F. Bauer, F. Seibert, et al., "The impact of calibration approaches on the accuracy of oscillometric central aortic blood pressure measurement", *Journal of Hypertension*, 38(11), pp. 2154-2160, 2020.
- [13] M. Rahman, M. Islam and M. Ahmad, "Design and implementation of a smart health band for the measurement of blood pressure, pulse rate and body temperature", 2018 4th International Conference on Electrical Engineering and Information & Communication Technology (iCEEiCT), pp. 156-161, 2018.
- [14] X. Sun, "Low noise, high accuracy analog electrocardiogram (ECG) signal front end amplifier for wearable equipment", 2021 International Conference on Electronics, Circuits and Information Engineering (ECIE), pp. 85-88, 2021.
- [15] M. Hoseinzadeh, A. Ekhlaei and H. Ahmadi, "Design and implementation of a blood pressure device with high sampling frequency

- to analyze cardiovascular diseases in LabVIEW”, 2020 6th Iranian Conference on Signal Processing and Intelligent Systems (ICSPIS), pp. 1-5. 2020.
- [16] M. Schultz, D. Picone, M. Armstrong, J. Black, N. Dwyer, P. Roberts-Thomson and J. Sharman, “Validation study to determine the accuracy of central blood pressure measurement using the Sphygmocor Xcel cuff device”, *Hypertension*, 76(1), pp. 244-250, 2020.
- [17] J. Wosik, M. Fudim, B. Cameron, Z. Gellad, A. Cho, et al., “Telehealth transformation: COVID-19 and the rise of virtual care”, *Journal of the American Medical Informatics Association*, 27(6), pp. 957-962, 2020.
- [18] K. Margolis, A. Crain, A. Bergdall, M. Beran, J. Anderson, et al., “Design of a pragmatic cluster-randomized trial comparing telehealth care and best practice clinic-based care for uncontrolled high blood pressure”, *Contemporary clinical trials* 92,105939, 2020.
- [19] A. Dansharif, N. Dlodlo and N. Angula, “A Mobile Telehealth Application for Rural Namibia”, 2018 IST-Africa Week Conference (IST-Africa), pp. 1-9, 2018.
- [20] C. Liu, C. Hsu, F. Yang, J. Wu, K. Kuo and P. Lai, “Population health management outcomes obtained through a hospital-based and telehealth informatics-enabled telecare service”, 2017 IEEE Biomedical Circuits and Systems Conference (BioCAS), pp. 1-4, 2017.
- [21] T. Pereira, G. Pires, D. Jorge and D. Santos, “Telehealth monitoring of a hypertensive elderly patient with the new VITASENIOR-MT system: a case study”, *Blood pressure monitoring*, 25(4), pp. 227-230, 2020.
- [22] B. Niu, N. Mukhtarova, O. Alagoz and K. Hoppe, “Cost-effectiveness of telehealth with remote patient monitoring for postpartum hypertension”, *The Journal of Maternal-Fetal & Neonatal Medicine*, pp. 1-7, 2021.
- [23] X. Tan, Y. Lv, X. Zhou, X. Song, Y. Wang, et al., “High performance AlGaN/GaN pressure sensor with a Wheatstone bridge circuit”, *Microelectronic Engineering*, 219, 111143, 2020.
- [24] B. Basumatary, R. Halder, and A. Sahani, “A Microcontroller based charge balanced trapezoidal stimulus generator for FES system”, 2021 IEEE International Instrumentation and Measurement Technology Conference (I2MTC) , pp. 1-4, 2021.
- [25] Y. Tang, S. M. Brown, J. Sorensen and J. B. Harley, “Physiology-informed real-time mean arterial blood pressure learning and prediction for septic patients receiving norepinephrine,” *IEEE Transactions on Biomedical Engineering*, 68(1), pp. 181-191, 2021.
- [26] R. Maaliw III, Z. Mabunga and F. Villa, “Time series forecasting of COVID-19 cases using stacked long short-term memory networks”, 2021 IEEE International Conference on Innovation and Intelligence for Informatics, Computing, and Technologies (3ICT), pp. 435-441, 2021.
- [27] R. Maaliw III, M. Ballera, Z. Mabunga, A. Mahusay, D. Dejelo and M. Seño, “An ensemble machine learning approach for time series forecasting of COVID-19 cases”, 2021 IEEE 12<sup>th</sup> Annual Information Technology, Electronics and Mobile Communication Conference (IEMCON), 2021.
- [28] Y. Kao, P. Chao, T. Tu, K. Chiang and C. Wey, “A new cuffless optical sensor for blood pressure measuring with self-adaptive signal processing”, 2016 IEEE Sensors, pp. 1-3, 2016.
- [29] K. Eker and M. K. Kiyimik, “Design of a functional medical device for home monitoring”, 2016 Medical Technologies National Congress (TIPTEKNO), pp. 1-4, 2016.
- [30] W. Singh, S. Deb and P. Bahubalindruni, “Low-noise energy efficient readout front-end for wearable continuous blood pressure monitoring systems.” *IEEE Transactions on Consumer Electronics*, 66(4), pp. 318-326, 2020.
- [31] A. Atef, M. Atef, E. E. M. Khaled and M. Abbas, “CMOS transimpedance amplifiers for biomedical applications: A comparative study,” *IEEE Circuits and Systems Magazine*, 20(1), pp. 12-31, 2020.
- [32] G. Wang, M. Atef and Y. Lian, “Towards a continuous non-invasive cuffless blood pressure monitoring system using PPG: Systems and circuits review”, *IEEE Circuits and Systems Magazine*, 18(3), pp. 6-26, 2018.
- [33] S. N. Mahmood and E. Ercelebi “Development of blood pressure monitor by using capacitive pressure sensor and microcontroller”, 2018 International Conference on Engineering Technology and their Applications (IICETA), pp. 96-100, 2018.
- [34] A. Rasool, M. Rafiq, A. Nasir and F. M. Kashif, “Continuous and Noninvasive Blood Pressure Estimation by Two-Sensor Measurement of Pulse Transit Time,” 2018 14th International Conference on Emerging Technologies (ICET), pp. 1-5, 2018.


**Scopus**

Search
Lists
Sources
SciVal
 
[Create account](#)
[Sign in](#)

Indexed keywords

1 SciVal Topics

 [Download](#)    [Print](#)    [Save to PDF](#)    [Add to List](#)    [Create bibliography](#)

Funding details

---

Document type  
Conference Paper

Source type  
Conference Proceedings

ISBN  
978-166540066-4

DOI  
10.1109/IEMCON53756.2021.9623070

[View more](#) 

2021 IEEE 12th Annual Information Technology, Electronics and Mobile Communication Conference, IEMCON 2021 • Pages 783 - 788 • 2021 • 12th IEEE Annual Information Technology, Electronics and Mobile Communication Conference, IEMCON 2021 • Vancouver • 27 October 2021 through 30 October 2021 • Code 17528

## A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in Telehealth System

Panergo, Maurine C.<sup>a</sup>  ; Cruz, Febus Reidj G.<sup>b</sup>  ; Maaliw, Renato R.<sup>a</sup>  

<sup>a</sup> College of Engineering, Southern Luzon State University, Quezon, Lucban, Philippines  
<sup>b</sup> School of EECE Mapua University, Intramuros, Manila, Philippines

1 60th percentile  
Citation in Scopus

0.58  
FWCI 

9  
Views count 

[View all metrics >](#)

[Full text options](#)    [Export](#) 

---

**Abstract**

Author keywords

Indexed keywords

SciVal Topics

Metrics

Funding details

SciVal topics

Metrics

Funding details

**Abstract**

Hypertension is one of the leading causes of mortality worldwide, increasing the likelihood of developing heart, renal, brain, and other illnesses. Reliable blood pressure measurement is critical because even minor errors can have severe effects on individuals. In this study, we developed a telehealth system that integrates an instrumentation amplifier and band-pass filter circuit to resolve dissipation losses and monitor such conditions, thus improving accurate health parameter measurements. Our prototype was tested on 30 subjects of varying ages for ten cross-validated trials. Quantitative results show that our amplified system was able to outperform high-end digital commercially available instruments with a mean precision of 96.67% (mean arterial pressure), 96.79% (pulse rate), and 99.13% (temperature). © 2021 IEEE.

**Author keywords**

dissipation losses; e-health; hypertension; instrumentation amplifier; mean arterial pressure; monitoring

**Indexed keywords**

**SciVal Topics** 

**Metrics**

**Funding details**

**Cited by 1 document**

A Low-Cost Highly Responsive Capacitive Control Switch for Lighting and Motor Control System  
Villaverde, E.D. , Maaliw, R.R. , Mahusay, A.T. (2022) 2022 IEEE 13th Annual Ubiquitous Computing, Electronics and Mobile Communication Conference, UEMCON 2022

[View details of this citation](#)

Inform me when this document is cited in Scopus:  
 [Set citation alert >](#)

---

**Related documents**

The Hypertension Canada blood pressure device recommendation listing: Empowering use of clinically validated devices in Canada  
Padwal, R. , Berg, A. , Gelfer, M. (2020) *Journal of Clinical Hypertension*

Accuracy of noninvasive central blood pressure estimation: Still a long 'wave' to go  
Pucci, G. , Vaudo, G. , Picone, D.S. (2020) *Journal of Hypertension*

Brief online certification course for measuring blood pressure with an automated blood pressure device. A free new resource to support World Hypertension Day Oct 17, 2020  
Campbell, N.R.C. , Khalsa, T. , Ordunez, P. (2020) *Journal of Clinical Hypertension*

[View all related documents based on references](#)

Find more related documents in Scopus based on:  
[Authors >](#) [Keywords >](#)

**References (34)** [View in search results format >](#)

All   [Export](#)    [Print](#)    [E-mail](#)    [Save to PDF](#)   [Create bibliography](#)

1 Mills, K.T., Stefanescu, A., He, J.  
**The global epidemiology of hypertension**  
(2020) *Nature Reviews Nephrology*, 16 (4), pp. 223-237. Cited 987 times.  
<http://www.nature.com/mapua.idm.oclc.org/nrneph/archive/index.html>  
doi: 10.1038/s41581-019-0244-2

[View at Publisher](#)

2 Cardoso, C.R.L., Salles, G.F.

All



ADVANCED SEARCH

Conferences &gt; 2021 IEEE 12th Annual Informa... ?

# A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in Telehealth System

Publisher: IEEE

Cite This

PDF

Maurine C. Panergo ; Febus Reidj G. Cruz ; Renato R. Maaliw All Authors

**1**  
Paper  
Citation

**118**  
Full  
Text Views



&lt; Previous | Back to Results | Next &gt;

## Need Full-Text

access to IEEE Xplore for your organization?

CONTACT IEEE TO SUBSCRIBE ➔

### More Like This

The System of Indicators of the Continuous Non-Invasive Blood Pressure Measurement

2021 IEEE Conference of Russian Young Researchers in Electrical and Electronic Engineering (ElConRus)

Published: 2021

Blood Pressure Measurement Using a Gaussian Curve Fitting Algorithm

2022 29th National and 7th International Iranian Conference on Biomedical Engineering (ICBME)

Published: 2022

Show More



IEEE Access is celebrating its 10 Year Publishing Anniversary!

View the top 10 articles published over the last decade based on downloads, citations, and overall impact in IEEE fields of interest.

View Articles

### Abstract

#### Document Sections

I. Introduction

II. Methodology

III. Results

IV. Discussions

V. Conclusions and Future Works

#### Authors

#### Figures

#### References

#### Citations

#### Keywords

#### Metrics

### Abstract:

Hypertension is one of the leading causes of mortality worldwide, increasing the likelihood of developing heart, renal, brain, and other illnesses. Reliable blood pressure measurement is critical because even minor errors can have severe effects on individuals. In this study, we developed a telehealth system that integrates an instrumentation amplifier and band-pass filter circuit to resolve dissipation losses and monitor such conditions, thus improving accurate health parameter measurements. Our prototype was tested on 30 subjects of varying ages for ten cross-validated trials. Quantitative results show that our amplified system was able to outperform high-end digital commercially available instruments with a mean precision of 96.67% (mean arterial pressure), 96.79% (pulse rate), and 99.13% (temperature).

**Published in:** 2021 IEEE 12th Annual Information Technology, Electronics and Mobile Communication Conference (IEMCON)

**Date of Conference:** 27-30 October 2021

**INSPEC Accession Number:** 21482738

**Date Added to IEEE Xplore:** 06 December

**DOI:** 10.1109/IEMCON53756.2021.9623070

2021

**Publisher:** IEEE

► **ISBN Information:**

**Conference Location:** Vancouver, BC, Canada

► **ISSN Information:**

#### I. Introduction

Society needs numerous healthcare solutions that deliver life-saving services. Electronic health (e-health) facilitates health and wellness benefits to patients remotely using telecommunication technologies. Aside from traditional methods, electronic devices can measure various bio-signals such as heart rate, pulse oximetry, temperatures, and other related health parameters. Blood pressure (BP) is a critical vital indicator that requires monitoring due to its link with various health problems, including hypertension, a medical condition that increases the chance of developing cardiovascular diseases, among other complications. Moreover, it is one of the leading causes of early mortality worldwide, affecting more than a billion people [4]. Statistics show that for an increase of 10mmHg (millimeter mercury) in systolic blood pressure, the relative risk of death rose by 28%, according

Sign in to Continue Reading

### Authors

Maurine C. Panergo

College of Engineering, Southern Luzon State University, Lucban, Quezon, Philippines

Febus Reidj G. Cruz

School of EEECE, Mapúa University, Intramuros, Manila, Philippines



[My...](#) »[My email messages](#) »

#112 (1570761738): A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in Telehealth System

## #112 (1570761738): A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in Telehealth System



Property	Change Add	Value	Affiliation			Country		
		Name	ID	Edit	Flag	(edit for paper)		
Conference and track		<b>2021 IEEE 12th Annual Information Technology, Electronics and Mobile Communication Conference (IEMCON)</b> - IEMCON Paper - Regular Research Paper						
Authors		Maurine C. Panergo	1900980	not creator		Southern Luzon State University, Philippines	mpanergo@slsu.edu.ph	Philippines
		Febus Reidj G. Cruz	491145	not creator		Mapua University, Philippines	frgcruz@mapua.edu.ph	Philippines
		Renato R. Maaliw III	1841045			Southern Luzon State University, Philippines	renatomaaliw3@gmail.com	Philippines
Title	Only the chairs (ieeiemcon2021-chairs@edas.info) can edit	A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in Telehealth System						
Abstract	Only the chairs (ieeiemcon2021-chairs@edas.info) can edit	Hypertension is one of the leading causes of mortality worldwide, increasing the likelihood of developing heart, renal, brain, and other illnesses. We developed a telehealth system that integrates an instrumentation amplifier and band-pass filter circuit to resolve dissipation losses to monitor such conditions, thus improving health parameter measurements accurately. Our prototype was tested on 30 subjects of varying ages for ten cross-validated trials. Quantitative results show that our amplified system was able to outperform high-end digital commercially available instruments with a mean precision of 96.67% (mean arterial pressure), 96.79% (pulse rate), and 99.13 (temperature).						
Keywords	Only the chairs (ieeiemcon2021-chairs@edas.info) can edit	dissipation losses; e-health; hypertension; instrumentation amplifier; mean arterial pressure; monitoring						
Topics	Only the chairs (ieeiemcon2021-chairs@edas.info) can edit	Electronic Instrumentations						
Presenter(s)		Maurine C. Panergo  and Renato R. Maaliw III (bio)						
Registration		Maurine C. Panergo has registered and paid for T:IEEENM						
DOI	Only the chairs (ieeiemcon2021-chairs@edas.info) can edit							
URL								
Status		Accepted						
Copyright form		IEEE; IEEE: Oct 1, 2021 23:39 Asia/Hong_Kong						
Review manuscript	However, authors cannot upload: paper status							
	Document (show)	Pages	File size	Changed				
		5	397,688	Sep 7, 2021 14:11 Asia/Hong_Kong				

	Could upload until <a href="#">Nov 11, 2021 07:59</a> <a href="#">Asia/Hong_Kong.</a>	<b>Document (show)</b>	<b>Pages</b>	<b>File size</b>	<b>Changed</b>
Final manuscript			6	419,499	<a href="#">Oct 12, 2021 17:26 Asia/Hong_Kong</a> 
However, authors cannot upload: final deadline					
Presentation	Could upload until <a href="#">Oct 29, 2021 07:22</a> <a href="#">Asia/Hong_Kong.</a>	<b>Document (show)</b>	<b>Pages</b>	<b>File size</b>	<b>Changed</b>
				178,826,952 (16 min 46 sec)	<a href="#">Oct 20, 2021 13:35 Asia/Hong_Kong</a> 
However, authors cannot upload: presentation deadline					

## Personal notes



You are the creator, an author and a reviewer for this paper. You have authored an accepted paper.

## Reviews

### 3 IEMCON 2021s

#### Review 1

None of the scores are visible for your roles.

#### Comments (Please write 100 words regarding this review report)

Improve the figure quality.  
Check for grammar and spellings  
Literature review part is required to be improved  
State the novelty of your work  
Author should cited the figure and table in your paper content  
Author research should follow the recent year and also compare your results with recent articles.  
More Number of References Should be added in your article

#### Review 2

None of the scores are visible for your roles.

#### Comments (Please write 100 words regarding this review report)

This paper presents a circuit design of a sensor amplifier for improving blood pressure measurement in telehealth system. I have some minor comments.

1. Some figures need to have large characters. It is difficult to recognize some of the letters in the figures.
2. In tables 1 to 3, it was observed that the commercial product (D) did not perform as good as the prototype. This is somewhat difficult to understand. For instance the heart pressure of the commercial product can be off by close to 20 from the ground truth. This is a poor product that should not be sold to the public. Can the authors use a different product?

#### Review 3

None of the scores are visible for your roles.

#### Comments (Please write 100 words regarding this review report)

- . The topic proposed by the authors is quite appreciable and the work has novelty.
- . The Conclusion section is not well explained.
- . The future prospect applications of this work not well explained.

## FACULTY POSITION RECLASSIFICATION FOR SUCS

(DBM-CHED Joint Circular No. 3, series of 2022)

## CERTIFICATION OF PERCENTAGE CONTRIBUTION

(Research Output with Multiple Authors)

**Title of Research:** A Circuit Design of a Sensor Amplifier for Improving Blood Pressure Measurement in TeleHealth System

**Type of Research Output:** Conference Paper (Scopus-Indexed, IEEE Paper)

**Instruction:** Supply ALL the names of the authors involved in the publication of Research output and indicate the contribution of each author in percentage. Each author shall sign the conforme column if he/she agrees with the distribution. The conforme should be signed by all the authors in order to be considered. Please prepare separate Certification for each output.

	Author Name	Percentage Contribution	Signature
1	Maurine C. Panergo (Lead Author)	80%	
2	Febus Reidj G. Cruz	10%	
3	Renato R. Maaliw III	10%	
	* Should have a total of 100%	100.00%	

Prepared by:

  
Renato R. Maaliw III, DIT  
(Name and Signature)  
Faculty

Certified by:

  
Nicanor L. Guinto, Ph.D  
(Name and Signature)  
Director, Office of Research Services