

# इंटरनेट

# मानक

## Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan


“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS/ISO 5356-1 (2004): Anaesthetic and Respiratory Equipment  
– Conical Connectors, Part 1 Cones and Sockets [MHD 11:  
Anaesthetic, Resuscitation and Allied Equipment]

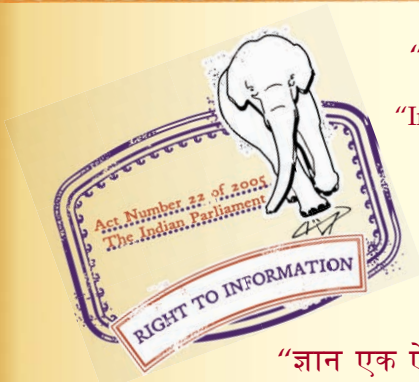

“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”



BLANK PAGE



भारतीय मानक  
एनिस्थिटिक एवं श्वसन उपस्कर — शंक्वाकार कनेक्टर्स  
भाग 1 शंकु और सॉकेट

*Indian Standard*  
**ANAESTHETIC AND RESPIRATORY EQUIPMENT —  
CONICAL CONNECTORS**  
**PART 1 CONES AND SOCKETS**

ICS 11.040.10

© BIS 2012  
**BUREAU OF INDIAN STANDARDS**  
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG  
NEW DELHI 110002

## NATIONAL FOREWORD

This Indian Standard (Part 1) which is identical with ISO 5356-1 : 2004 'Anaesthetic and respiratory equipment — Conical connectors — Part 1: Cones and sockets' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendation of the Anaesthetic, Resuscitation and Allied Equipment Sectional Committee and approval of the Medical Equipment and Hospital Planning Division Council.

This standard was first published in 1974 as IS 7409 and revised in 1985. Consequent upon the publication of ISO 5356-1 : 1987 the standard was revised as a dual number standard identical to ISO 5356-1 : 1987 to align its requirements with the latest international practices. Then after, based on the revision of ISO 5356-1 in 1996, the third revision of IS 7409 was undertaken. This standard is now being published in a single number as IS/ISO, based on ISO 5356-1 : 2004 and will supersede IS 7409 (Part 1) : 2003 'Anaesthetic and respiratory equipment — Conical connectors: Part 1 Cones and sockets (*third revision*)' and after the publication of this standard IS 7409 (Part 1) shall be treated as withdrawn.

In clinical practice, several breathing attachments used in anaesthetic and respiratory equipment may have to be joined together to provide a suitable breathing system. Items of medical equipment, such as, a humidifier or a spirometer, are often incorporated into the breathing system which may also be connected to an anaesthetic-gas scavenging system. Connections for these purposes are usually cone and socket joints, and a lack of standardization of these connections has given rise to problems of interchangeability when connecting equipment made by different manufacturers. This standard specifies the requirements and dimensions for conical connectors used in anaesthetic and respiratory equipment. This standard includes 8.5 mm size connectors.

An important consideration is that conical connections need to be secure but nevertheless disconnectable by the operator. The use of connectors meeting the requirements of this standard will not necessarily prevent them being disconnected accidentally. To minimize the risk of 22 mm connectors being accidentally disconnected, latching connectors can be used.

Annex A includes a figure and a table detailing plug and ring test gauges that are used to check conical connectors made of materials other than metal. Annexes B, C and D provide test methods for latching connectors, Annex E includes a figure and table detailing plug and ring test gauges that may be used to check metal conical connectors, and Annex F contains recommendations for testing security of latching connectors.

The text of ISO Standard has been approved as suitable for publication as an Indian Standard without deviations. Certain conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker while in Indian Standards, the current practice is to use a point (.) as the decimal marker.

*Indian Standard*

# ANAESTHETIC AND RESPIRATORY EQUIPMENT — CONICAL CONNECTORS

## PART 1 CONES AND SOCKETS

### 1 Scope

This part of ISO 5356 specifies dimensional and gauging requirements for cones and sockets intended for connecting anaesthetic and respiratory equipment, e.g. in breathing systems, anaesthetic-gas scavenging systems and vaporizers.

This part of ISO 5356 gives requirements for the following conical connectors:

- 8,5 mm size intended for use in paediatric breathing systems;
- 15 mm and 22 mm sizes intended for general use in breathing systems;
- 22 mm latching connectors (including performance requirements);
- 23 mm size intended for use with vaporizers, but not for use in breathing systems;
- 30 mm size intended for the connection of a breathing system to an anaesthetic gas scavenging system.

This part of ISO 5356 does not specify the medical devices and accessories on which these connections are to be provided.

Requirements for the application of conical connectors are not included in this part of ISO 5356, but are or will be given in the relevant International Standards for specific medical devices and accessories.

NOTE Requirements for screw-threaded weight-bearing conical connectors are specified in ISO 5356-2.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 4135, *Anaesthetic and respiratory equipment — Vocabulary*

ISO 5367, *Breathing tubes intended for use with anaesthetic apparatus and ventilators*

IEC 60601-1:1988, *Medical electrical equipment — Part 1: General requirements for safety*, including Amendment 1:1991 and Amendment 2:1995

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 4135 and the following apply.

**3.1**  
**22 mm latching connector**  
 female connector for engagement with a male conical connector of 22 mm size complying with this part of ISO 5356, and which has a feature to reduce the possibility of accidental disconnection

### 4 Conical connectors made of metal

#### 4.1 General requirements

The dimensions of conical connectors made of metal, including those made of composite materials in which the mating surfaces are metal, shall be as shown in Figures 1 and 2 and Table 1.


NOTE See Annex E for dimensions of plug and ring gauges for the connectors.

#### 4.2 Additional requirements for male conical connectors of 22 mm size

**4.2.1** Male conical connectors of 22 mm size, with the exception of those intended for connection to a face mask, shall incorporate the recess as shown in Figure 2 a).

**4.2.2** Male conical connectors of 22 mm size to which it is intended to attach a face mask shall incorporate a shoulder or equivalent construction as shown in Figure 2 b).

**4.2.3** If a circumferential groove or grooves are incorporated in the surface of a male conical connector of 22 mm size, the total width of the groove or grooves at the surface shall not exceed 8 mm.

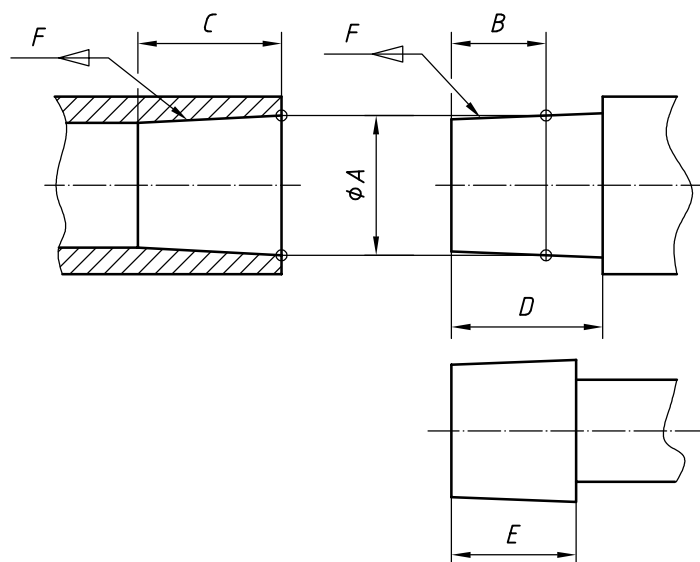

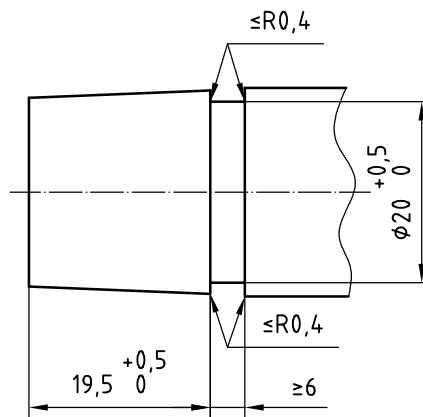
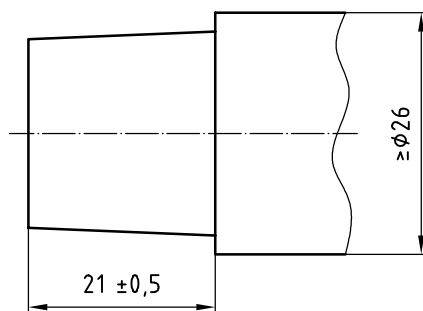
The radius on the entrance to the female connector and on the leading edge of the male cone should be not less than 0,5 mm and not more than 0,8 mm.

Figure 1 — Conical connectors made of metal

**Table 1 — Conical connectors made of metal — Dimensions** (see Figure 1)

Connector size mm	<i>A</i> mm	<i>B</i> mm	Taper length min. <i>C</i> mm	Clearance to shoulder (if present) <i>D</i> mm	Length to taper min. <i>E</i> mm	Taper ratio <i>F</i>
8,5	$8,45 \pm 0,04$	6	6,4	8,9 min.	8	1:19
15	$15,47 \pm 0,04$	10	16	16 min.	14,5	1:40
22	$22,37 \pm 0,04$	15	21	See Figure 2	See Figure 2	1:40
23	$23,175 \pm 0,02$	13	18	18 min.	15	1:36
30	$30,9 \pm 0,05$	14	18	18 min.	14	1:20

Dimensions in millimetres

**a) Connector intended for breathing attachment (with recess)****b) Connector intended for face mask (with shoulder)**

Circumferential grooves may be incorporated on the surface of the male cone, if required (see 4.2.3).

**Figure 2 — Conical connectors of 22 mm size made of metal — Supplementary dimensions**



### 4.3 Additional requirements for conical connectors of 8,5 mm size

The male conical connector shall have a minimum inside diameter of 6 mm extending inward for at least 6 mm from the end of the connector.

## 5 Conical connectors made of materials other than metal

### 5.1 General requirements

Conical connectors made of materials other than metal shall meet the following requirements when they are type-tested with gauges having dimensions as shown in Figure A.1 and Table A.1.

- a) Conical connectors made of materials other than metal shall meet the dimensional requirements in Figure 1 and Table 1, with the exception that dimensions *A* and *B* and ratio *F* may vary from those shown.
- b) When the connector is engaged in the appropriate plug or ring test gauge shown in Figure A.1 and Table A.1, by applying an axial force of  $(35 \pm 3,5)$  N for 8,5 mm and 15 mm connectors and  $(50 \pm 5)$  N for 22 mm and 30 mm connectors and, while maintaining the same force, rotating the connector up to  $20^\circ$ , its leading edge shall lie between the minimum and maximum diameter steps of the gauge. The connectors and gauges shall be maintained at a temperature of  $(20 \pm 3)$  °C during the test.

**NOTE** Because connectors made from plastics materials, for example polyamide, polyacetal, polycarbonate, polysulfone, etc., can vary greatly in their physical characteristics, it is not considered practicable to specify their dimensions; for this reason, gauging requirements have been included. It is also considered impracticable to generalize on matters such as cold flow and thermal instability, as well as possible changes in physical characteristics, contact with solvents, etc.

It is the responsibility of the manufacturer to ensure that adequate tests have been carried out to prove as far as possible that the particular materials chosen for the connectors are suitable.

### 5.2 Additional requirements for conical connectors of 22 mm size

The requirements given in 4.2 apply.

### 5.3 Additional requirements for conical connectors of 8,5 mm size

The requirements given in 4.3 apply.

## 6 22 mm latching connectors

**6.1** 22 mm latching connectors shall engage with the 22 mm male connector with a recess as specified in Figure 2 a).

**6.2** When tested in accordance with Annex B, the engaged connection shall not become disconnected.

**6.3** When tested in accordance with Annex C, the leakage rate from the engaged connectors shall not exceed 5 ml/min (corrected to 20 °C and 101,3 kPa).

**6.4** After being subjected to the procedure described in Annex D, the 22 mm latching connector shall still meet the requirements in 6.1, 6.2 and 6.3.


**6.5** 22 mm latching connectors intended for re-use shall meet the requirements in 6.1, 6.2, 6.3 and 6.4 after being subjected to the cleaning, disinfection or sterilization procedures specified in IEC 60601-1:1998, 44.7.

## Annex A (normative)

### Plug and ring test gauges for conical connectors made of materials other than metal

Figure A.1 and Table A.1 give details of plug and ring gauges for use in checking conical connectors made of materials other than metals.

Dimensions in millimetres  
Surface roughness values in micrometres

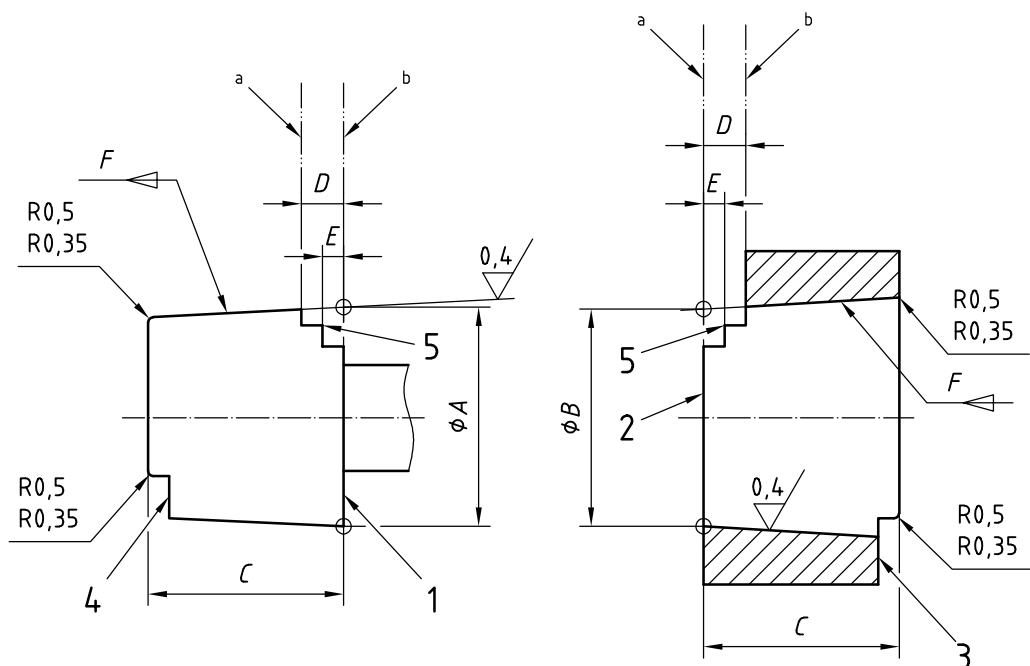

#### Key

- 1 face A
- 2 face B
- 3 step to check mating gauges ground flush to face A
- 4 step to check mating gauges ground flush to face B
- 5 basic steps

a Position max.

b Position min.

NOTE Basic and mating gauge steps are optional.

**Figure A.1 — Plug and ring test gauges for conical connectors made of materials other than metal**

**Table A.1 — Plug and ring test gauges for conical connectors made of materials other than metal — Dimensions** (see Figure A.1)

Dimensions in millimetres

Connector size	<i>A</i>	<i>B</i>	<i>C</i>	<i>D</i>	<i>E</i>	<i>F</i>	Tolerance on taper per unit of length on diameter
8,5	$8,50 \pm 0,005$	$8,09 \pm 0,005$	$8,4 \pm 0,005$	$1,31 \pm 0,005$	See NOTE	1:19	$0,053 \pm 0,000\ 2$
15	$15,525 \pm 0,005$	$15,165 \pm 0,005$	$14,5 \pm 0,005$	$4,3 \pm 0,005$	$2,2 \pm 0,005$	1:40	$0,025 \pm 0,000\ 2$
22	$22,425 \pm 0,005$	$21,94 \pm 0,005$	$19,5 \pm 0,005$	$5,2 \pm 0,005$	$2,2 \pm 0,005$	1:40	$0,025 \pm 0,000\ 2$
30	$30,98 \pm 0,005$	$30,12 \pm 0,005$	$17,2 \pm 0,005$	$3,1 \pm 0,005$	$1,6 \pm 0,005$	1:20	$0,050 \pm 0,000\ 2$
NOTE Gauge for 8,5 mm connector has only one mating step.							

## **Annex B**

(normative)

### **Test for security of engagement of 22 mm latching connector to male conical connector**

**B.1** Condition the male 22 mm conical connector complying with Figure 2 a) and the 22 mm latching connector for 1 h at a temperature of  $(35 \pm 3) ^\circ\text{C}$  and relative humidity of at least 80 %, and carry out the test under the same conditions.

**B.2** Engage the 22 mm latching connector with the male connector in accordance with the manufacturer's instructions.

**B.3** After 1 min of engagement without activation of any disengagement mechanism, apply for 10 s an axial separation force of  $(50 \pm 5) \text{ N}$  and, unless the 22 mm latching connector permits free radial rotation, also apply a torque of  $(25 \pm 5) \text{ N}\cdot\text{cm}$  at a rate not exceeding  $20 \text{ N}\cdot\text{s}^{-1}$ .

**B.4** Observe whether the assembled connectors become disconnected.

**NOTE** Examples of suitable apparatus that can be used to test security of engagement, together with a more detailed test procedure, are given for information in Annex F.

**Annex C**  
(normative)

**Test for leakage from 22 mm latching connectors**

**C.1** Take the engaged male conical connector and 22 mm latching connector that have been tested as described in Annex B and condition them at  $(35 \pm 3) ^\circ\text{C}$ .

**C.2** Using air, apply an internal static pressure of  $(8 \pm 0,5)$  kPa above ambient to the assembly and determine the leakage rate from the assembly, e.g. by pressure drop or volumetric method.

## **Annex D** (normative)

### **Drop procedure for 22 mm latching connectors**

**D.1** Condition a male conical connector complying with Figure 2 a) and the 22 mm latching connector for 1 h at a temperature of  $(20 \pm 3) ^\circ\text{C}$  and relative humidity of at least 80 %, and carry out the test under the same conditions.

**D.2** Engage the 22 mm latching connector with the male conical connector in accordance with the manufacturer's instructions. Attach the male conical connector to a breathing tube complying with ISO 5367 and having a length of 2 m.

**D.3** Attach the opposite end of the breathing tube to a point 1 m above a 50 mm thick hardwood board (e.g. hardwood having a density greater than  $700 \text{ kg/m}^3$ ) standing on a rigid base (e.g. a concrete block).

**D.4** Raise the engaged connectors to a point 1 m above the board and 2 m distant from the other end of the breathing tube and release them so that they fall onto the hardwood board. Repeat this five times.


**D.5** Proceed with desired test.

## Annex E (informative)

### Plug and ring test gauges for conical connectors made of metal

Figure E.1 and Table E.1 give, for information, details of plug and ring test gauges that may be used to check metal conical connectors.

Dimensions in millimetres  
Surface roughness values in micrometres

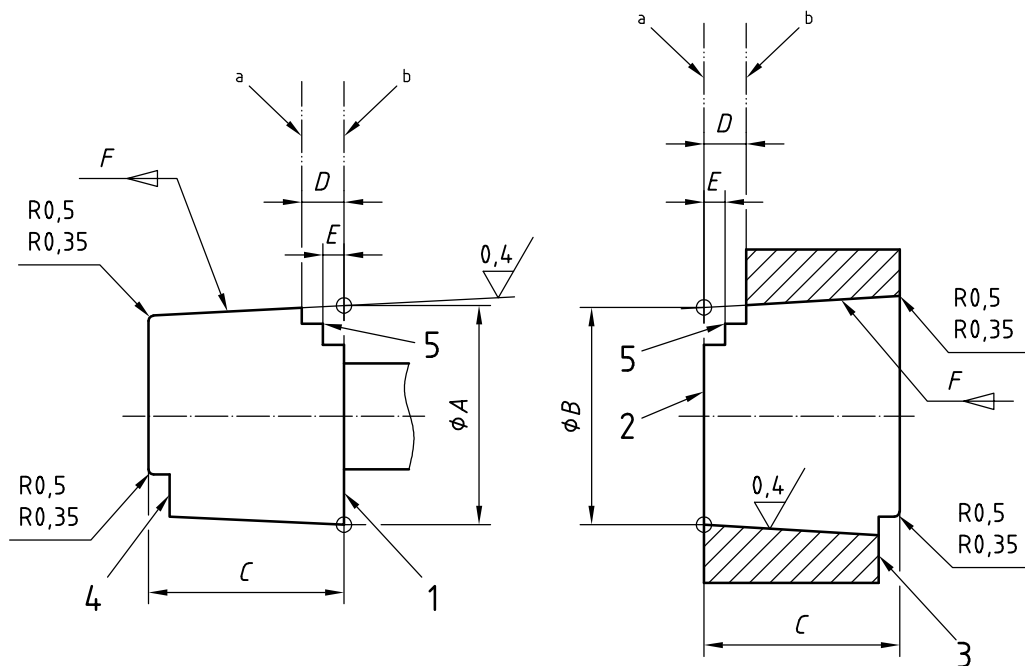

#### Key

- 1 face A
- 2 face B
- 3 step to check mating gauges ground flush to face A
- 4 step to check mating gauges ground flush to face B
- 5 basic steps
- a Position max.
- b Position min.

NOTE Basic and mating gauge steps are optional.

Figure E.1 — Plug and ring test gauges for conical connectors made of metal

**Table E.1 — Plug and ring test gauges for conical connectors made of metal —  
Dimensions (see Figure E.1)**

Dimensions in millimetres

Connector size	<i>A</i>	<i>B</i>	<i>C</i>	<i>D</i>	<i>E</i>	Taper ratio <i>F</i>	Tolerance on taper per unit of length on diameter
8,5	$8,49 \pm 0,005$	$8,094 \pm 0,005$	$8,4 \pm 0,005$	$1,52 \pm 0,005$	See NOTE	1:19	$0,053 \pm 0,000\ 2$
15	$15,51 \pm 0,005$	$15,18 \pm 0,005$	$14,5 \pm 0,005$	$3 \pm 0,005$	$1,6 \pm 0,005$	1:40	$0,025 \pm 0,000\ 2$
22	$22,41 \pm 0,005$	$21,955 \pm 0,005$	$19,5 \pm 0,005$	$3 \pm 0,005$	$1,6 \pm 0,005$	1:40	$0,025 \pm 0,000\ 2$
23	$23,195 \pm 0,003$	$22,794 \pm 0,003$	$16 \pm 0,005$	$1,33 \pm 0,005$	$0,72 \pm 0,005$	1:36	$0,0278 \pm 0,000\ 2$
30	$30,95 \pm 0,005$	$30,15 \pm 0,005$	$17 \pm 0,005$	$1,9 \pm 0,005$	$1 \pm 0,005$	1:20	$0,050 \pm 0,000\ 2$
NOTE Gauge for 8,5 mm connector has only one mating step.							



## **Annex F** (informative)

### **Suggested apparatus and methods for testing the security of engagement of 22 mm latching connectors**

#### **F.1 Method 1 — Bench-mounted test equipment**

##### **F.1.1 Apparatus**

A typical bench-mounted apparatus for testing the security of engagement of 22 mm latching connectors is shown in Figure F.1. The male test piece should be a 22 mm male conical connector dimensioned as shown in Figure 2 a) but with all the tolerances reduced to  $\pm 0,005$  mm and a surface finish of  $0,4 \mu\text{m}$ .

**NOTE** There are a number of methods for applying the test forces, and Figure F.1 is illustrative of only one approach. Other methods include the use of gravity loading by weights or liquid containers.

The essential features of the apparatus should ensure that the tensile force can be applied in a truly axial direction and that torque can be applied without changing the tensile force. To minimize the effects of friction of the apparatus, the tensile force should be measured directly between the 22 mm latching connector and the male test piece.

##### **F.1.2 Procedure**

**F.1.2.1** Secure the 22 mm latching connector to be tested in the self-centring holder of the apparatus (F.1.1), ensuring that the method of securing the 22 mm latching connector does not deform the section(s) that are intended to engage with the male test piece.

**F.1.2.2** Condition the 22 mm latching connector and the apparatus at a temperature of  $(35 \pm 3) ^\circ\text{C}$  and a relative humidity of at least 80 % for 1 h.

If a number of 22 mm latching connectors are to be tested, some may be conditioned at the required temperature and relative humidity without being secured to the apparatus, provided that they are conditioned again for at least 5 min after being secured to the apparatus.

**F.1.2.3** Engage the 22 mm latching connector with the male test piece in accordance with the manufacturer's instructions.

**F.1.2.4** After 1 min, attach the force-measuring device and apply an axial separation force at a rate not exceeding  $20 \text{ N}\cdot\text{s}^{-1}$  until a force of  $(50 \pm 5) \text{ N}$  is being applied. Maintain this force for 10 s without activating any disengagement mechanism, and observe whether the engaged 22 mm latching connector and male test piece become disconnected.

**F.1.2.5** Without reducing the tensile load and without activation of any disengagement mechanism, apply a torque of  $(25 \pm 5) \text{ N}\cdot\text{cm}$  or rotate the male test piece through an angle of  $20^\circ$ , whichever occurs first. Maintain this torque or position for 10 s and observe whether the engaged 22 mm latching connector and male test piece become disconnected.

## **F.2 Method 2 — Hand-held test equipment**

### **F.2.1 Apparatus**

A typical hand-held apparatus for testing the security of engagement of 22 mm latching connectors is shown in Figure F.2.


### **F.2.2 Procedure**

**F.2.2.1** Condition the 22 mm latching connector and the apparatus (F.2.1) at a temperature of  $(35 \pm 3) ^\circ\text{C}$  and a relative humidity of at least 80 % for 1 h.

**F.2.2.2** Engage the 22 mm latching connector with the male test piece on the apparatus.

**F.2.2.3** After 1 min, manually apply an axial separation force at a rate not exceeding  $20 \text{ N}\cdot\text{s}^{-1}$  until a force of  $(50 \pm 5) \text{ N}$  is applied. Maintain this force for 10 s without activation of any disengagement mechanism, and observe whether the engaged 22 mm latching connector and male test piece become disconnected.


**F.2.2.4** Without reducing the tensile load and without activation of any disengagement mechanism, apply a torque of  $(25 \pm 5) \text{ N}\cdot\text{cm}$  or rotate the male test piece through an angle of  $20^\circ$ , whichever occurs first. Maintain this torque or position for 10 s, and observe whether the engaged 22 mm latching connector and male test piece become disconnected.

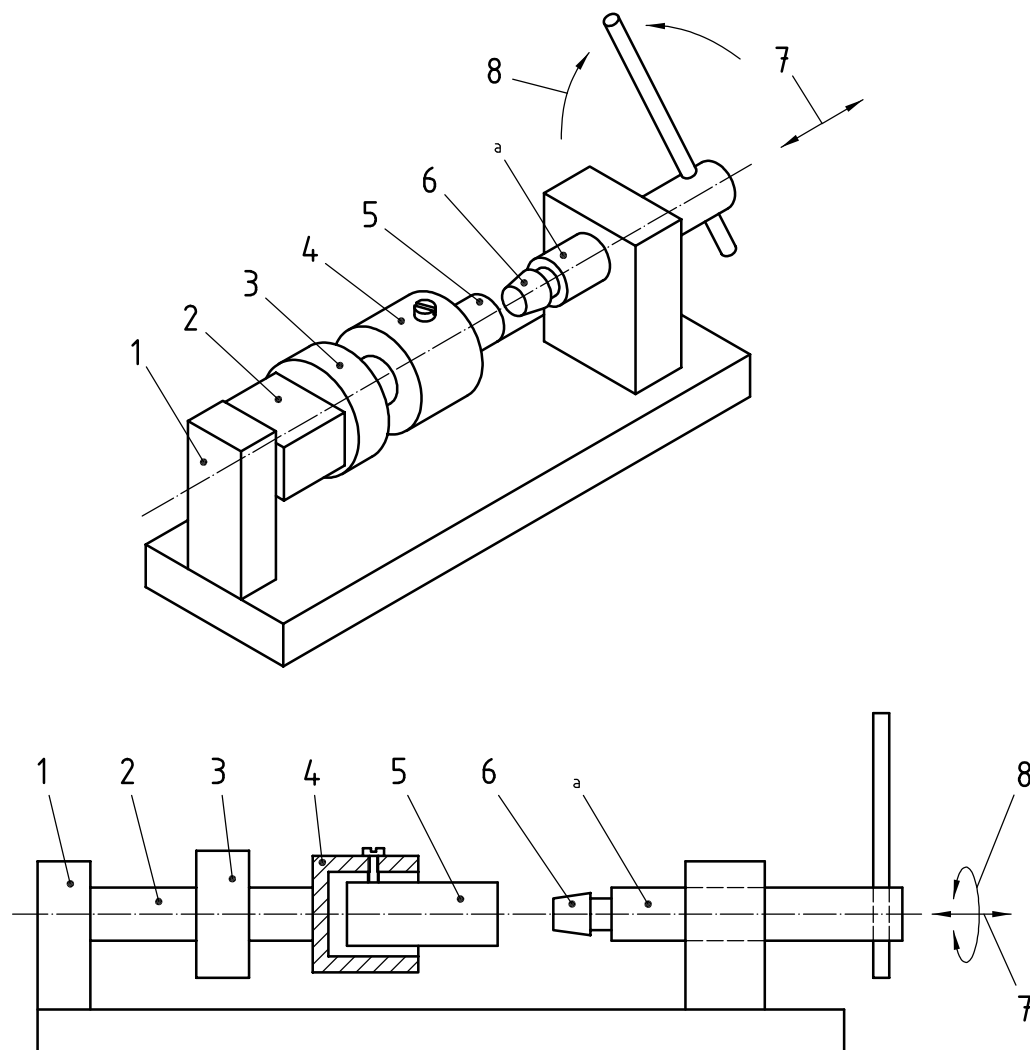

**Key**

- 1 rigid support
- 2 axial load meter
- 3 torque meter
- 4 holder
- 5 22 mm latching connector under test
- 6 22 mm male test piece
- 7 application of adjustable axial force
- 8 application of adjustable torque
- <sup>a</sup> Free to slide and rotate.

**Figure F.1 — Apparatus for testing the security of engagement of 22 mm latching connectors  
(Method 1 — Bench-mounted)**

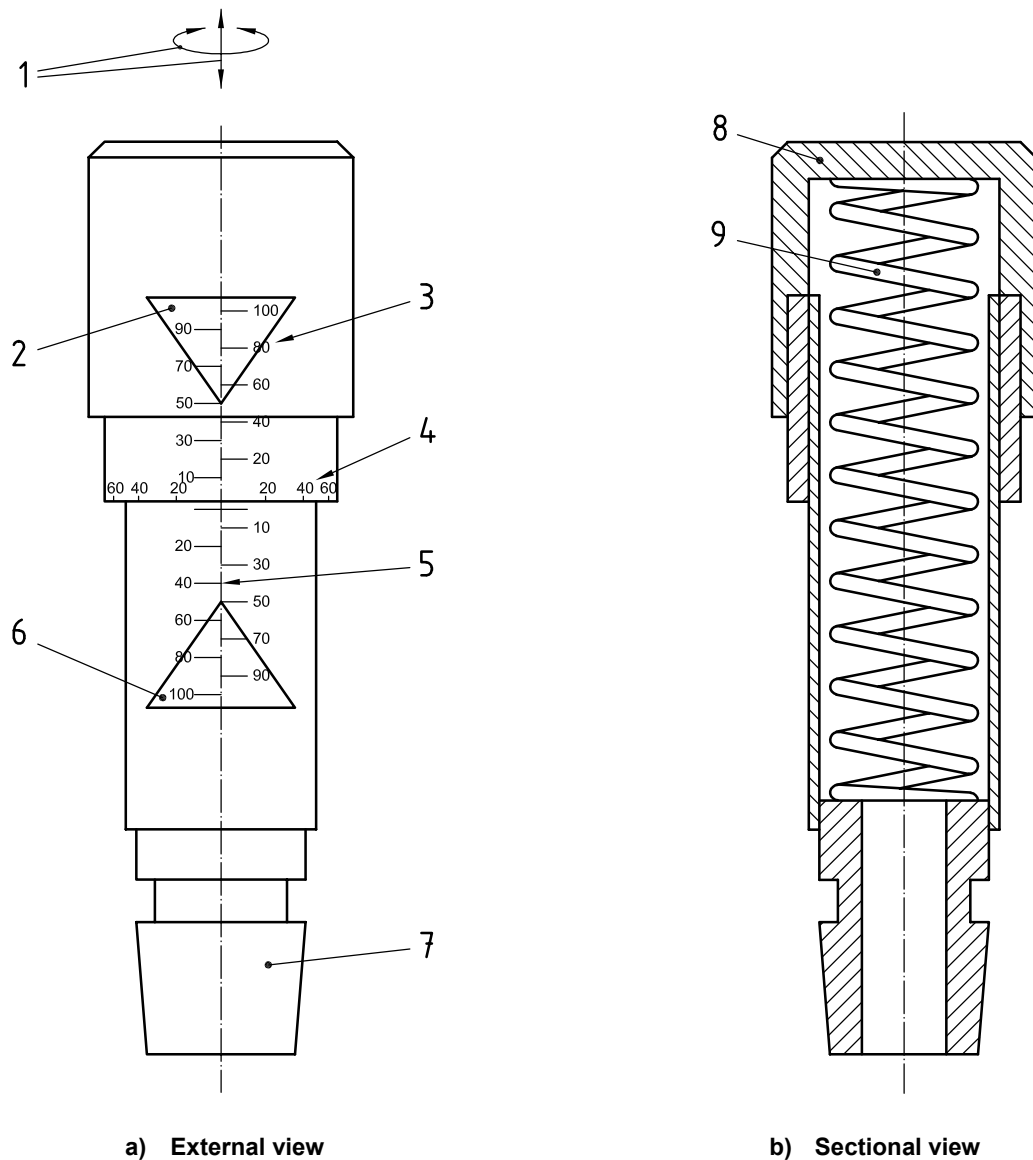**Key**

- |   |                                  |
|---|----------------------------------|
| 1 application of torque or push or pull by hand             | 8 knob                           |
| 2 area of scale indicating acceptable pull and twist forces | 9 coil spring fixed at both ends |
| 3 pull-force scale  |                                  |
| 4 torque scale  |                                  |
| 5 push-force scale  |                                  |
| 6 area of scale indicating acceptable push and twist forces |                                  |
| 7 22 mm male test piece                                     |                                  |

Torque and force scales should be precalibrated using apparatus in Figure F.1.

**Figure F.2 — Apparatus for testing the security of engagement of 22 mm latching connectors (Method 2 — Hand-held)**

## Bibliography

- [1] ISO 3040:1990, *Technical drawings — Dimensioning and tolerancing — Cones*

(Continued from second cover)

In this adopted standard, reference appears to certain International Standards for which Indian Standards also exist. The corresponding Indian Standards which are to be substituted in their respective places are listed below along with their degree of equivalence for the editions indicated:

<i>International Standard</i>	<i>Corresponding Indian Standard</i>	<i>Degree of Equivalence</i>
ISO 4135 : 2001 Anaesthetic and respiratory equipment – Vocabulary	IS 13200 : 1993 Anaesthesiology – Vocabulary	Technically Equivalent
ISO 5367 : 2000 Breathing tubes intended for use with anesthetic apparatus and ventilators	IS/ISO 5367 : 2000 Breathing tubes intended for use with anesthetic apparatus and ventilators	Identical
IEC 60601-1: 1988 Medical electrical equipment — Part 1: General requirements for safety	IS 13450 (Part 1) : 2008 Medical electrical equipment: Part 1 General requirements for basic safety and essential performance ( <i>first revision</i> )	Technically Equivalent

For the purpose of deciding whether a particular requirement of this standard is complied with, the final value, observed or calculated, expressing the result of a test, shall be rounded off in accordance with IS 2 : 1960 'Rules for rounding off numerical values (*revised*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard

## Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 1986* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

## Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

## Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc No.: MHD 11 (0094).

### Amendments Issued Since Publication

Amendment No.	Date of Issue	Text Affected

## BUREAU OF INDIAN STANDARDS

### Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110002

Telephones: 2323 0131, 2323 3375, 2323 9402

Website: [www.bis.org.in](http://www.bis.org.in)

### Regional Offices:

#### Telephones

Central	: Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110002	{ 2323 7617 2323 3841
Eastern	: 1/14, C.I.T. Scheme VII M, V.I.P. Road, Kankurgachi KOLKATA 700054	{ 2337 8499, 2337 8561 2337 8626, 2337 9120
Northern	: SCO 335-336, Sector 34-A, CHANDIGARH 160022	{ 260 3843 260 9285
Southern	: C.I.T. Campus, IV Cross Road, CHENNAI 600113	{ 2254 1216, 2254 1442 2254 2519, 2254 2315
Western	: Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400093	{ 2832 9295, 2832 7858 2832 7891, 2832 7892

**Branches:** AHMEDABAD. BANGALORE. BHOPAL. BHUBANESHWAR. COIMBATORE. DEHRADUN. FARIDABAD. GHAZIABAD. GUWAHATI. HYDERABAD. JAIPUR. KANPUR. LUCKNOW. NAGPUR. PARWANOO. PATNA. PUNE. RAJKOT. THIRUVANATHAPURAM. VISAKHAPATNAM.