




**XRD TEST REPORT**  
**INSTRUMENT: BRUKER D8 ADVANCE ECO**

Coupled TwoTheta/Theta 15.18.09 LYNXEYE\_XE\_T (1D mode): PSD counter

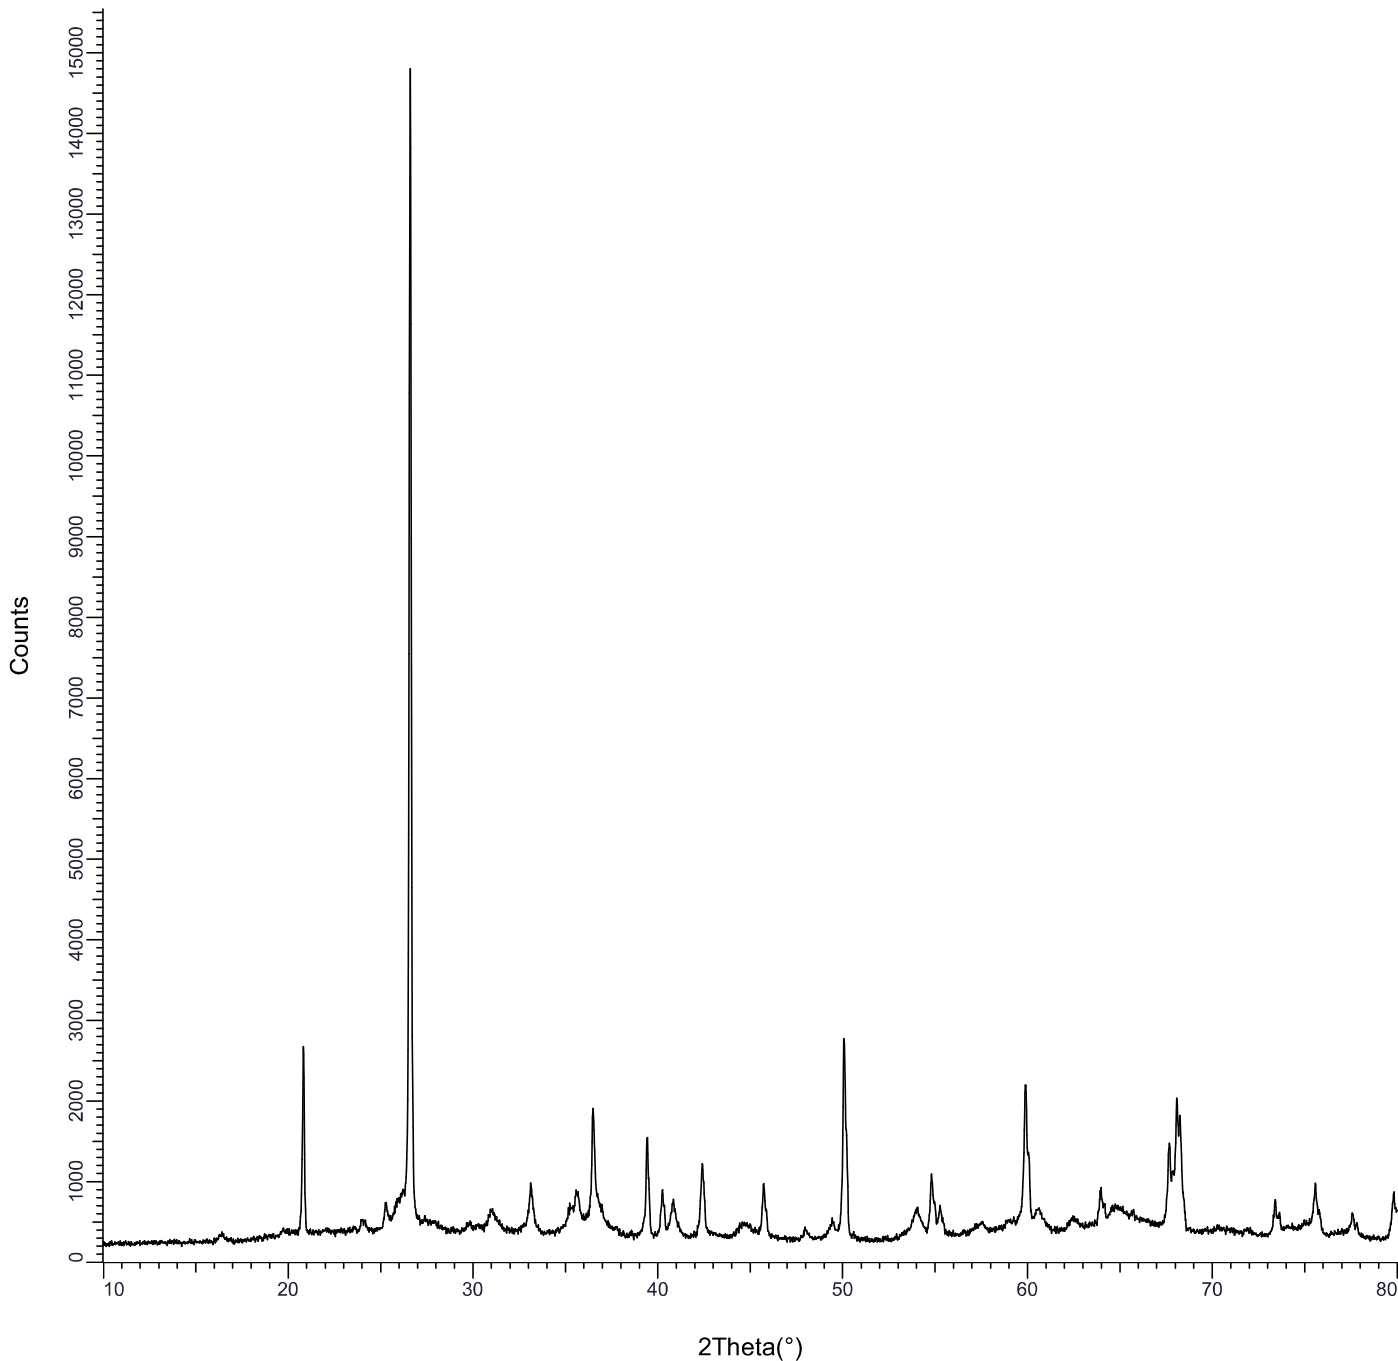

**Experiment**

User ID	213
Instrument	Gajah Mada University
Time	12/22/2023 3:42:22 PM
Sample ID	2882a CFA - Sodalite
Raw File ID	3245
Scan type	Coupled TwoTheta/Theta
Scan mode	PsdFastScan
2Theta	Start: 10 [°] Increment: 0.02045866002 [°] Stop: 80.0096 [°]
Theta	Start: 5 [°] Increment: 0.01022933001 [°] Stop: 40.0048 [°]