




XRD TEST REPORT
INSTRUMENT: BRUKER D8 ADVANCE ECO

Coupled TwoTheta/Theta 15.47.01 LYNXEYE_XE_T (1D mode): PSD counter

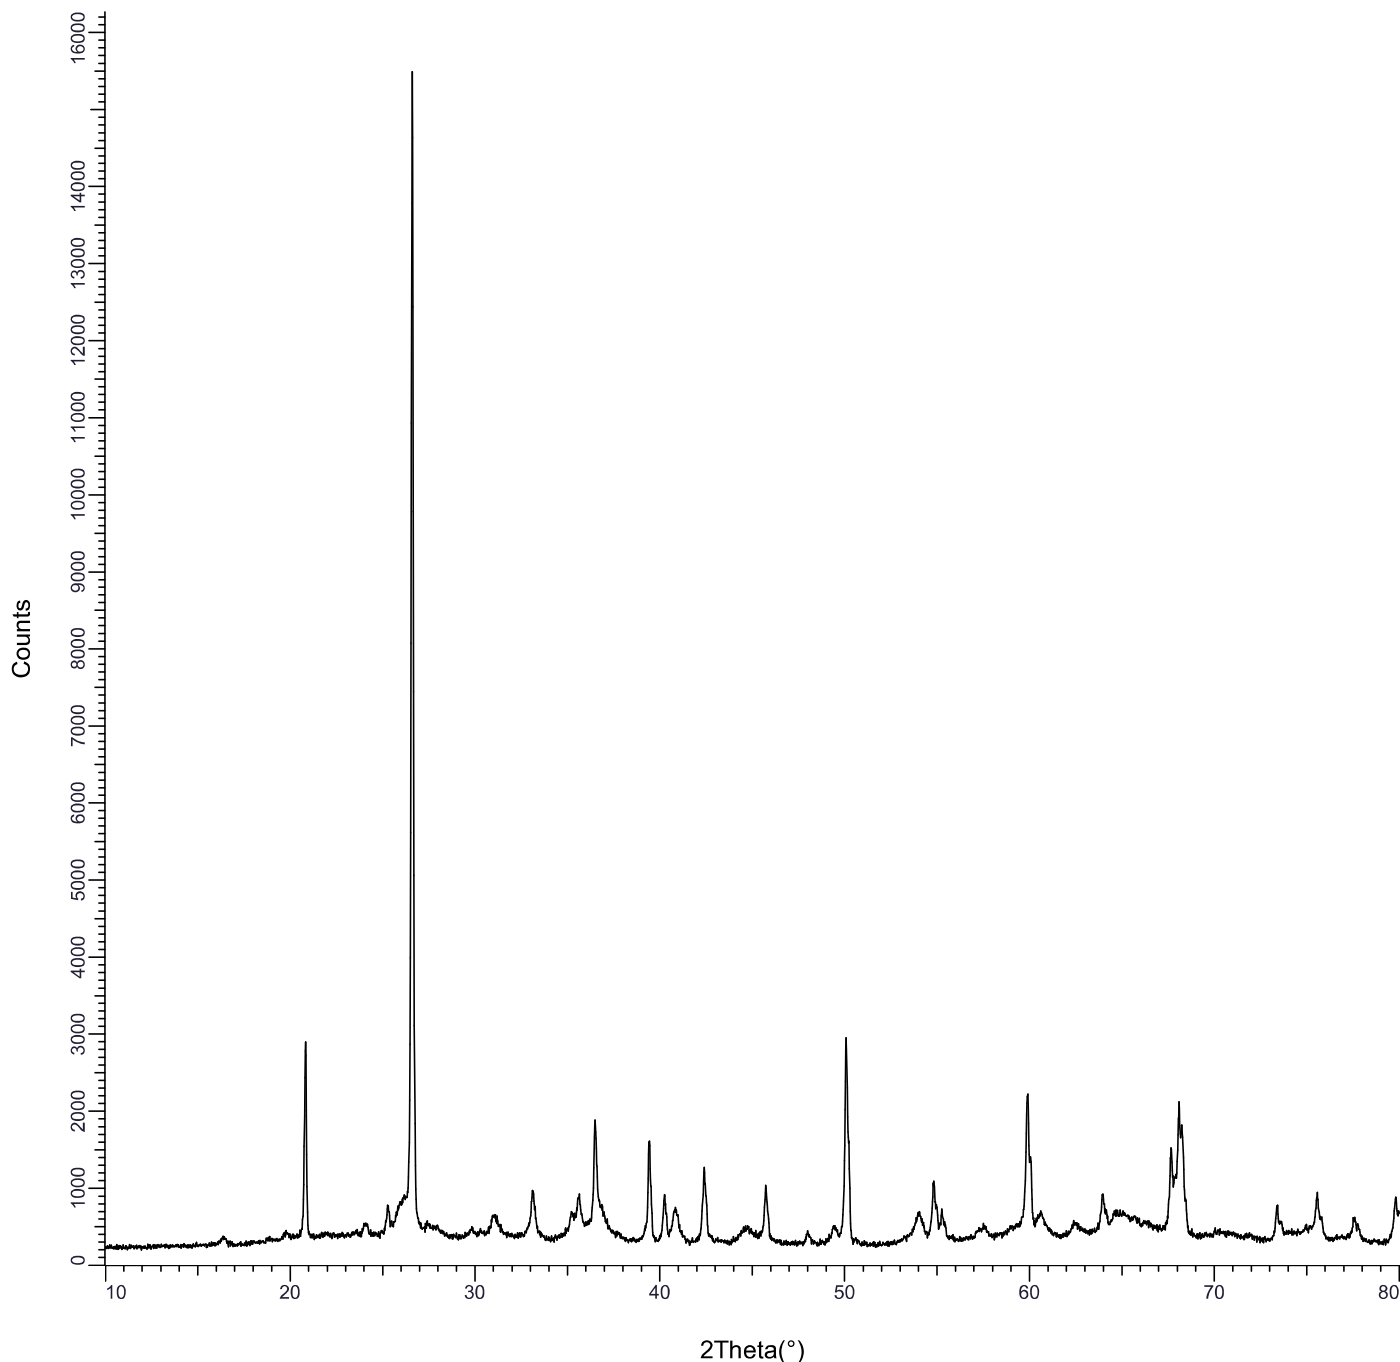

Experiment

User ID	213
Instrument	Gajah Mada University
Time	12/22/2023 4:12:13 PM
Sample ID	2882b CFA - Sodalite - CTAB
Raw File ID	3246
Scan type	Coupled TwoTheta/Theta
Scan mode	PsdFastScan
2Theta	Start: 10 [°] Increment: 0.02045866002 [°] Stop: 80.0096 [°]
Theta	Start: 5 [°] Increment: 0.01022933001 [°] Stop: 40.0048 [°]