



KONICA MINOLTA

New Version

Spectrodensitometer

FD-7 / FD-5

3-in-1 next-generation measurement tool

Color											
Density											
Illumination											

**Streamlines color adjustment in printing,
even on substrates with fluorescent
whitening agents**



Giving Shape to Ideas

A high-accuracy, compact, lightweight, handheld, next-generation spectrodensitometer that measures color, density, and illumination* for applications from R&D to quality control.

*FD-7 only

Color

The world's first measuring instrument that corresponds to Measurement Condition M1 of ISO 13655

- Konica Minolta's original VFS (Virtual Fluorescence Standard) technology enables L*a*b* measurements corresponding to ISO 13655 Measurement Condition M1.
- The FD-7 and FD-5 can take measurements corresponding to all four of the ISO 13655 Measurement Conditions. Measurements corresponding to M1 are enabled by Konica Minolta's original VFS (Virtual Fluorescence Standard) technology, and measurements corresponding to M0 (CIE Illuminant A) and M2 (illumination with UV-cut filter) can also be taken. In addition, by attaching the included polarization filter, measurements corresponding to M3 (M2+ polarization filter) can be taken.

Scan measurements can be performed. (FD-7 only)

- Manual scan measurements can be performed when the instrument is connected to a PC.
- With optional software basicColor catch all, the colorimetric values, density values, and spectral reflectance values of various test charts (MediaWedge ECI2002, IT8.7/3, etc.) can be measured in a single operation.



Spectral output (FD-7 only)

- When the FD-7 is connected to a computer, the spectral reflectance data (380 to 730 nm) of samples under various illuminants and the spectral irradiance data (360 to 730 nm) of the environmental lighting can be measured and output to a computer. This makes the FD-7 ideal for research and development applications.

Illumination



Illumination environment light can be measured. (FD-7 only)

- The illuminance and color temperature in a color viewing cabinet or the actual ambient light under which printed materials will be evaluated can be measured.



Measured environmental light can be set as illumination light source (user illuminant)

- In the past, when measuring printed materials containing fluorescent whitening agents (FWA), large differences between measured values and visual evaluation sometimes occurred. But with the FD-7, colorimetric values can be calculated under the measured environmental light source, providing results which more closely correspond to on-site visual evaluation. This ensures customers receive the colors they want and eliminates time and labor lost resolving customer complaints due to the effects of FWA or metamerism.

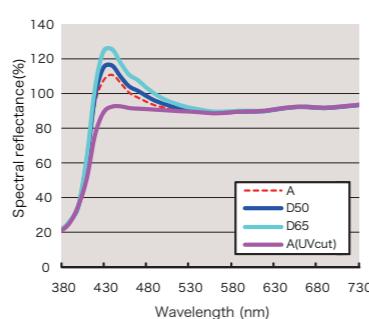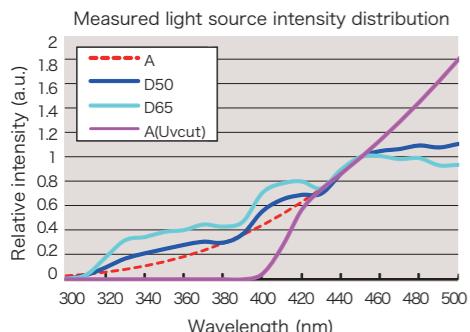

NEW Data Management Software FD-S1w (included as standard accessory)



FD-S1w.exe

Features:

- Transfer of measurement data to Excel® sheet.
- Reading/registering of user illuminant data to/from instrument and storage as PC file
- Color set management functions (for instrument ISO 12647 Check and Target Match functions)*1*2

System Requirements

OS Windows XP, Windows Vista or Windows 7; 32-bit or 64-bit versions
Excel Excel 2003 (Windows XP), Excel 2007 (Windows Vista), or Excel 2010 (32-bit version; Windows 7)

The hardware or the computer system to be used must meet or exceed the recommended system requirements for the compatible OS and Excel version being used.

Compatible Instruments

Spectrodensitometer FD-7, FD-5
Display language English, Japanese, Chinese (Simplified)
(Select one during installation.)

Density

NEW Printing quality control functions including trapping, dot gain, etc.

- A new industry-standard tool for commercial printing and packaging printing to improve productivity and quality at low cost.
 - CMYK density • Dot area • Dot gain • Trapping • Simple density difference
 - PS plate dot area • PS plate dot gain • Spot color density



Improvements in quality control functions to meet more advanced needs at printing locations.

NEW Target Match function *1*2


- Displays the color difference of mixed ink from the target color and the density adjustment needed to bring the mixed color closer to the target color.
- By using the Target Match function, ink color adjustment can be performed without a computer or special software.
- Ideal for spot colors or process colors.
- Displays color difference and density.
- Displays estimated density adjustment needed to bring the mixed color closer to the target color and the predicted color difference after adjustment.

TARGETMATCH	M1 2° D50
<input checked="" type="checkbox"/> Paper	+0.30 D
<input checked="" type="checkbox"/> Target	ΔE*94
<input checked="" type="checkbox"/> Sample	2.54 @ 0.86 D
	>> 0.48 @ 1.16 D
Measure sample	

Measure color difference.
Result: Adjusting the density of spot color with 400 nm peak from 0.86 to 1.16 is predicted to result in a color difference of 0.48.

NEW Functions corresponding to various printing standards

- Pass/fail judgment against ISO, JapanColor, GRACoL®/SWOP®, PSO, or user-defined custom targets can be performed. The FD-7 and FD-5 are ideal for on-site printing quality control.
 - ISO 12647 check *1*2
Color difference, TVI, and mid-tone spread can be evaluated.
 - Gray balance
Gray balance can be evaluated using the G7® evaluation method.

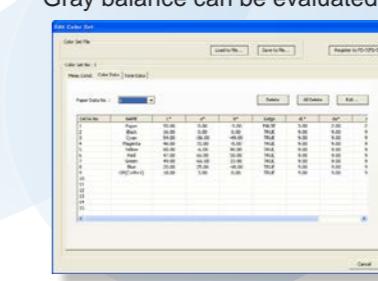


ISO CHECK	M1 2° D50
<input checked="" type="checkbox"/> Yellow40%	ΔL* -0.32
<input checked="" type="checkbox"/> Red	Δa* 0.08
<input checked="" type="checkbox"/> Δb*	-0.22
<input type="checkbox"/> Green	ΔE*ab 0.40
<input type="checkbox"/> Blue	
16/21	CS01 : PT1-AM-BB
Red : Pass	

*1 Target colors (color sets) must be set using the included FD Data Management Software FD-S1w.
*2 Backing conversion function converts the target values to enable evaluation even when backing conditions for samples do not match those of the targets.

Industry's first automatic wavelength compensation function

- Wavelength compensation is performed during white calibration* without requiring additional work.
- Until now, wavelength compensation could only be carried out as one part of manufacturer servicing. This task is now performed whenever white calibration^{*3} is done, helping to maintain the high reliability of measurement values until the next periodic servicing.

^{*3} Except when polarization filter is attached.

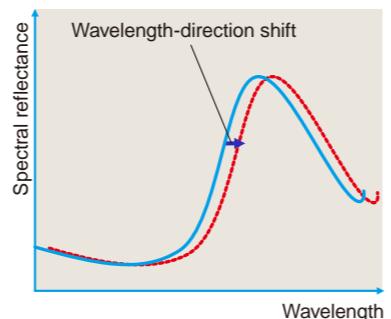

World's lightest^{*4}

- The main body weighs only about 350g, and even with the target mask attached it's only about 430g, lighter than any previous spectrodensitometer.
- This reduces the load on the user's arm during work, improving efficiency when taking measurements over a long time.


^{*4} Display-equipped spectrodensitometer. As of December 1, 2012



Worry-free after-sales service


- Worldwide service centers provide rapid support when needed.
- A comprehensive service network is in place to ensure that your instrument is always in top shape.

SYSTEM DIAGRAM

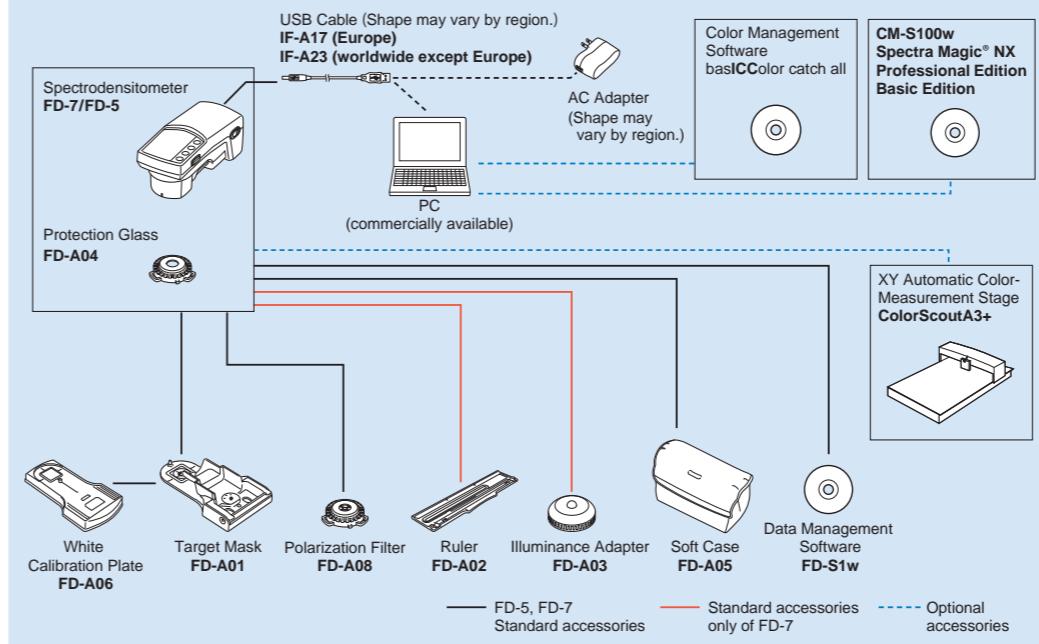

DIMENSIONS (Units: mm)

With removable target mask attached

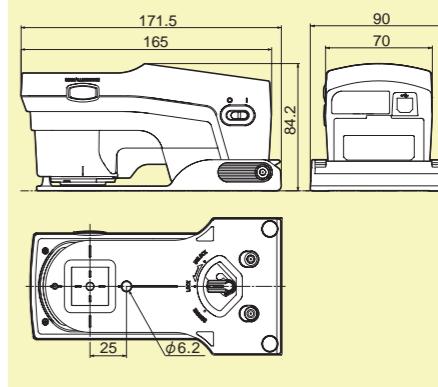

Optional accessories

XY Automatic Color-Measurement Stage ColorScoutA3+^{*1}

The ColorScoutA3+ enables accurate, high-efficiency measurements of color charts with the Spectrodensitometer FD-7 and FD-5. It enables automatic positioning and measurement of the instrument, providing higher repeatability and reducing labor compared to manual measurements.




XY automatic color-measurement stage.

Table available with either white surface or black surface.

Using the ColorScoutA3+ with the FD-7 or FD-5 makes it easier to measure colorimetric data of color charts under ISO 13655 Measurement Condition M1 or a user-defined illumination light source (user illuminant) to create user color profiles that more closely match visual evaluation.

Maximum measurable chart size of 320 x 460 mm improves measurement efficiency by allowing even large color charts to be measured in a single procedure without the need to cut up or tile the charts.

Measurement of user-designed charts is also possible. The included ClrChrt software makes it easy to create a definition file for measuring the user-designed chart.

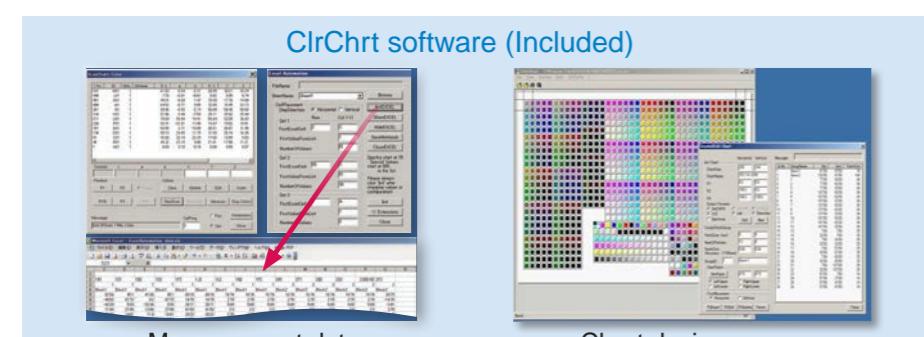

ColorChart minimum computing requirements	
OS; CPU	Windows® XP(32-bit), Windows® Vista(32-bit); 300MHz or faster
Hard disk; Memory	30MB or more available disk space; 64MB or more

Color Management Software basICColor catch all^{*1}

Ideal software for quality control of process color printing targets for offset printing.

For major efficiency increases in daily color control work.

- Enables color reproduction closer to visual evaluation with simple operation.
 - With basICColor catch all, commonly used templates and jobs are already included, so there is no need for measurement preparations such as setting target values, tolerances, etc.
 - When the software is started, just select the required measurement conditions in the Job Management screen. You can then connect immediately to the Spectrodensitometer FD-7 or FD-5, and PDF reports can be created and output automatically.
 - Data are stored in ISO format (ISO 12642-2), so they can be fed back to profile creation software. Using Measurement Condition M1 or a user-defined illumination light source (user illuminant) enables color reproduction closer to visual evaluation.

For ISO 12647-2 printing certification checks and print process quality management.

- Enables measurement of Fogra® and IDEAlliance® standards and certification checking.
- In addition to CIELAB for color, evaluation results for CMYK dot gain and mid-tone spread as required for the above certification checking can also be easily obtained. This can help discover and resolve problems in the printing process at an early stage.

Minimum computing requirements	
OS	Windows® XP SP3 (32-bit); Windows® Vista (32-bit); Windows® 7 (32-bit)
CPU	Intel® Pentium® 4 Processor
Memory	512MB
Hard disk	At least 100MB of available disk space

NEW Color Data Software SpectraMagic® NX^{*1}


Ideal for color-difference control of spot colors relative to target colors.

^{*1} Measurements with polarization filter attached cannot be performed.


Achieves overall ease of use with free selection of evaluation equations and report formatting.

With the new E^{*94} and E₀₀ color difference equations as well as a user index that allows users to freely set their own evaluation equations, SpectraMagic® NX can meet a wide variety of user needs.


Measurement data can be displayed in list form or in objects such as spectral graphs, color-difference graphs, etc. that the user can freely lay out, and those objects can be copied and pasted as is into other software such as Excel® for easy data control. In addition, printing screens can also be designed using the same objects to create user-defined formats for easy-to-read reports.




Printing screen

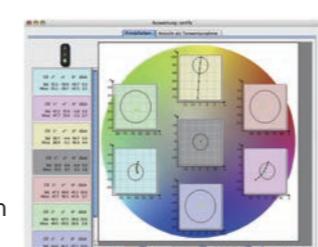

List display

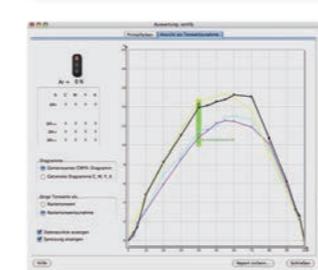

Color-difference graph object

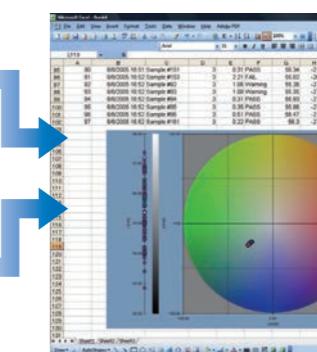

Pasted into Excel®

Minimum Computing Requirements

OS	Windows® XP Professional 32-bit SP3, 64-bit SP2; Windows® Vista Business 32-bit, 64-bit; Windows® 7 Professional 32-bit, 64-bit (English, Japanese, German, French, Spanish, Italian, Traditional Chinese, Simplified Chinese, Portuguese, and Hangul versions)
CPU	The hardware of the computer system to be used must meet or exceed the greater of the recommended system requirements for the compatible OS being used or the following specifications.
Memory	Pentium® III 600 MHz or higher (recommended)
Hard disk	128 MB (256 MB recommended)

Function	* ★ New	FD-7	FD-5
----------	---------	------	------

Density measurement functions			
Density, density difference	●	●	
Dot area	●	●	
Dot gain	●	●	
Trapping	★	★	
PS plate dot area	★	★	
PS plate dot gain	★	★	
Spot color density	★	★	
Gray balance	★	★	
Midtone spread	★	★	
ISO 12647 check	★	★	
Target match	★	★	
Colorimetric measurement functions			
L*a*b*	●	●	
L*C*h	●	●	
Hunter Lab	●	●	
Yxy	●	●	
XYZ	●	●	
ΔE*ab (CIE1976)	●	●	
ΔE*94 (CIE1994)	●	●	
ΔE00 (CIE2000)	●	●	
ΔE (Hunter)	●	●	
CMC (l:c)	●	●	
Illuminance measurement functions			
Illuminance	●		
Correlated color temperature	●		
Paper index			
WI/Tint (ASTME313-96)	●	●	
ISO Brightness (ISO2470-1)	●	●	
D65 Brightness (ISO2470-2)	●	●	
Fluorescence index	●	●	
Spectral reflectance			
Spectral data output	●		
Memory			
Target density	30	30	
Target color	30	30	
Color sets of 15 colors each*3	50	50	
Other functions			
Manual scan*2	●		
Automatic function (density, dot area, color)	●	●	
PASS/FAIL judgment	●	●	
Software			
basICColor catch all	●	●	
FD-S1w	★	★	
SpectraMagic NX	★	★	
ClrChrt (Included with ColorScoutA3+)	●	●	

Main specifications

Illumination/viewing system	45°a: 0°(annular illumination)*1 Conforms to CIE No. 15, ISO 7724/1, DIN5033 Teil 7, ASTM E 1164, and JIS Z 8722 Condition a for reflectance measurements.
Spectral separation device	Concave grating
Wavelength range	Spectral reflectance: 380 to 730 nm; Spectral irradiance (FD-7 only): 360 to 730 nm
Wavelength pitch	10 nm
Half bandwidth	Approx. 10 nm
Measurement area	Ø3.5 mm
Light source	LED
Measurement range	Density: 0.0D to 2.5D; Reflectance: 0 to 150%
Short-term repeatability	Density: σ0.01D Without polarization filter: 0.0D ~ 2.5D, Yellow 0.0D ~ 2.0D With polarization filter: 0.0D ~ 2.5D, Yellow 0.0D ~ 1.8D (When measurements taken 30 times at 10-second intervals after white calibration has been performed) Colorimetric: Within ΔE00 0.05 (Without polarization filter) (When white plate is measured 30 times at 10-second intervals after white calibration has been performed)
Inter-instrument agreement	Within ΔE00 0.3 (Average of 12 BCRA Series II color tiles compared to values measured with a master body under Konica Minolta standard conditions; without polarization filter)
Measurement time	Approx. 1.4 s (single-point reflectance measurement without polarization filter)
Measurement conditions	Corresponding to ISO 13655 Measurement Conditions M0 (CIE Illuminant A), M1 (CIE Illuminant D50), M2 (illumination with UV-cut filter), and M3 (M2 + polarization filter); User-defined illuminant
Illuminants	A, C, D50, D65, ID50, ID65, F2, F6, F7, F8, F9, F10, F11, F12, User-defined illuminant
Observers	2° Standard Observer, 10° Standard Observer
Density	ISO Status T, ISO Status E, ISO Status A, ISO Status I; DIN16536
Display language	English, French, German, Spanish, Japanese, Chinese (Simplified)
Interface	USB 2.0
Output data*2	Displayed values; Spectral reflectance data (FD-7 only) ; Spectral irradiance data (FD-7 only)
Power	Rechargeable internal lithium-ion battery (Number of measurements per charge: Approx. 2,000 when new without polarization filter); AC adapter; USB bus power
Dimensions (W × D × H)	70 × 165 × 83 mm (Body only); 90 × 172 × 84 mm (With target mask attached)
Weight	Approx. 350 g (Body only); Approx. 430 g (With target mask attached)
Operating temperature/humidity range	10 to 35°C, 30 to 85% relative humidity with no condensation
Storage temperature/humidity range	0 to 45°C, 0 to 85% relative humidity with no condensation
Standard accessories	White Calibration Plate, Target Mask, Protection Glass, AC Adapter, USB Cable, Soft Case, Polarization Filter, Data Management Software FD-S1w, Illuminance Adapter (FD-7 only), Ruler (FD-7 only)
Optional accessories	Color Management Software basICColor catch all, XY Automatic Color Measurement Stage Color Scout A3+, Color Management Software SpectraMagic NX

*1 Illumination for wavelengths under 400nm is unidirectional.

*2 Available when using PC software.

*3 Used for ISO 12647 Check / Target match; Must be set using included FD-S1w software.

- Displays shown are for illustration purpose only.
- The specifications and drawings given here are subject to change without prior notice.
- KONICA MINOLTA and the Konica Minolta logo and the symbol mark, and "Giving Shape to Ideas" and SpectraMagic™ are registered trademarks or trademarks of KONICA MINOLTA, INC.
- The basICColor logo is a registered trademark of basICColor GmbH.
- Other company names and product names used herein are trademarks or registered trademarks of their respective companies.



SAFETY PRECAUTIONS

For correct use and for your safety, be sure to read the instruction manual before using the instrument.

- Always connect the instrument to the specified power supply voltage. Improper connection may cause a fire or electric shock.



Certificate No : LRO 0960094/A

Certificate No : JOA-E-80027



Registration Date : March 12, 1997

KONICA MINOLTA, INC.
Konica Minolta Sensing Americas, Inc.
Konica Minolta Sensing Europe B.V.

Osaka, Japan
New Jersey, U.S.A.
European Headquarter /BENELUX
German Office

Phone : 888-473-2656 (in USA), 201-236-4300 (outside USA)
Nieuwegein, Netherlands
München, Germany

Fax : 201-785-2482
Fax : +31 (0) 30 248-1280
Fax : +49 (0) 89 4357 156 0

French Office

Roissy CDG, France

Fax : +49 (0) 1 80 11 10 70

UK Office

Warrington, United Kingdom

Fax : +44 (0) 1925 467300

Italian Office

Cinisello Balsamo, Italy

Fax : +39 02849488.00

Swiss Office

Dietikon, Switzerland

Fax : +41 (0) 43 322-9800

Nordic Office

Västra Frölunda, Sweden

Fax : +46 (0) 31 7099464

Polish Office

Wroclaw, Poland

Fax : +48 (0) 71 33050-01

SE Sales Division

Shanghai, China

Fax : +86 (0) 21-5489 0202

Beijing Office

Beijing, China

Fax : +86 (0) 10-8522 1551

Guangzhou Office

Guangdong, China

Fax : +86 (0) 20-3826 4220

Chongqing Office

Chongqing, China

Fax : +86 (0) 23-6773 4988

Qingdao Office

Shandong, China

Fax : +86 (0) 532-8079 1871

Wuhan Office

Hubei, China

Fax : +86 (0) 27-8544 9942

Konica Minolta Sensing Singapore Pte Ltd.

Konica Minolta, Inc.

Konica Minolta, Inc.

Optics Company, Korea

Optics Company, Sensing Business

Thailand Representative Office

Seoul, Korea

Bangkok, Thailand

Fax : +65 6563-5533

Fax : +82 (0) 2-523-9726

Fax : +66-2361-3730

Addresses and telephone/fax numbers are subject to change without notice. For the latest contact information, please refer to the KONICA MINOLTA Worldwide Offices Web page :

©2010 KONICA MINOLTA, INC.

<http://konicaminolta.com/instruments/network>

9242-4897-10 BDEGPK⑦