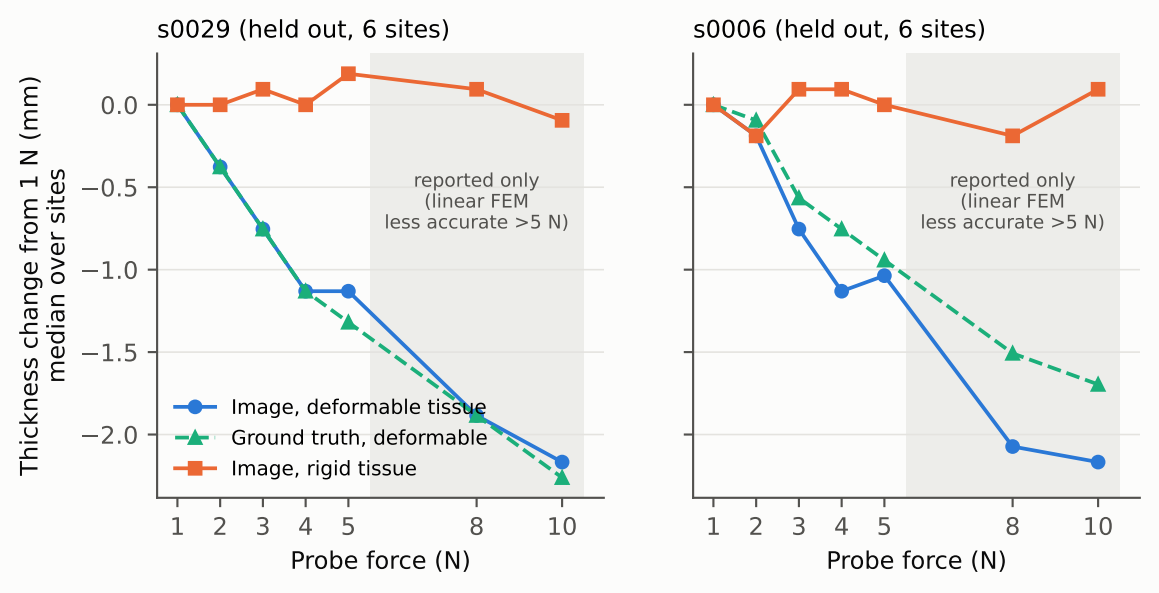
s0029 (held out, 6 sites)
s0006 (held out, 6 sites)
Thickness change from 1 N (mm)
median over sites
0.0
−0.5
−1.0
−1.5
−2.0
reported only
(linear FEM
less accurate >5 N)
Image, deformable tissue
Ground truth, deformable
Image, rigid tissue
1
2
3
4
5
8
10
Probe force (N)