



OOD Probe Ladder -- Two-Regime Test of the Distributional Normalizer


(A) Noise divergence from prior, per probe

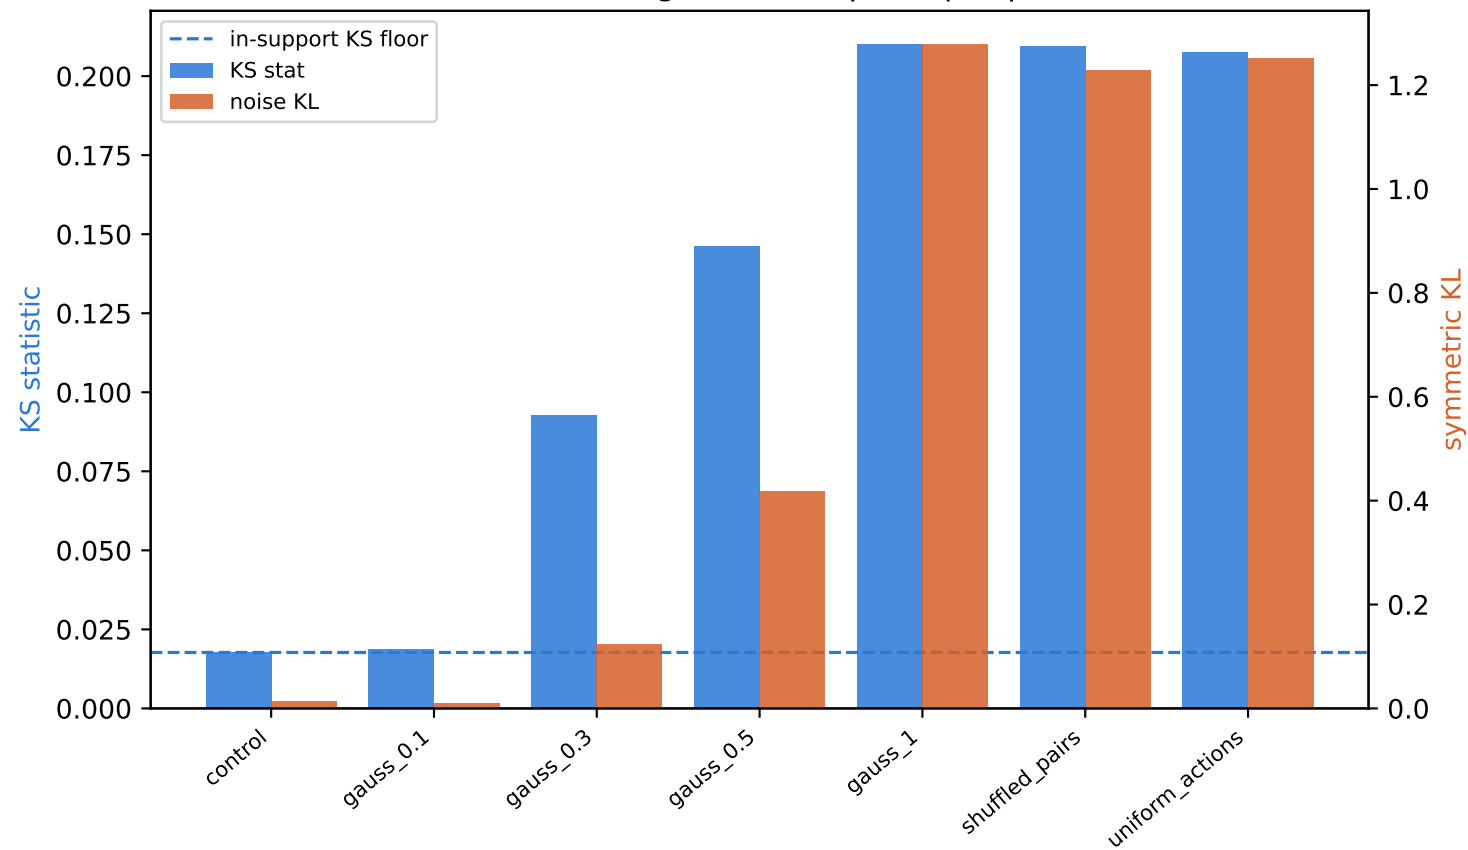

(B) Dose-response across the support boundary

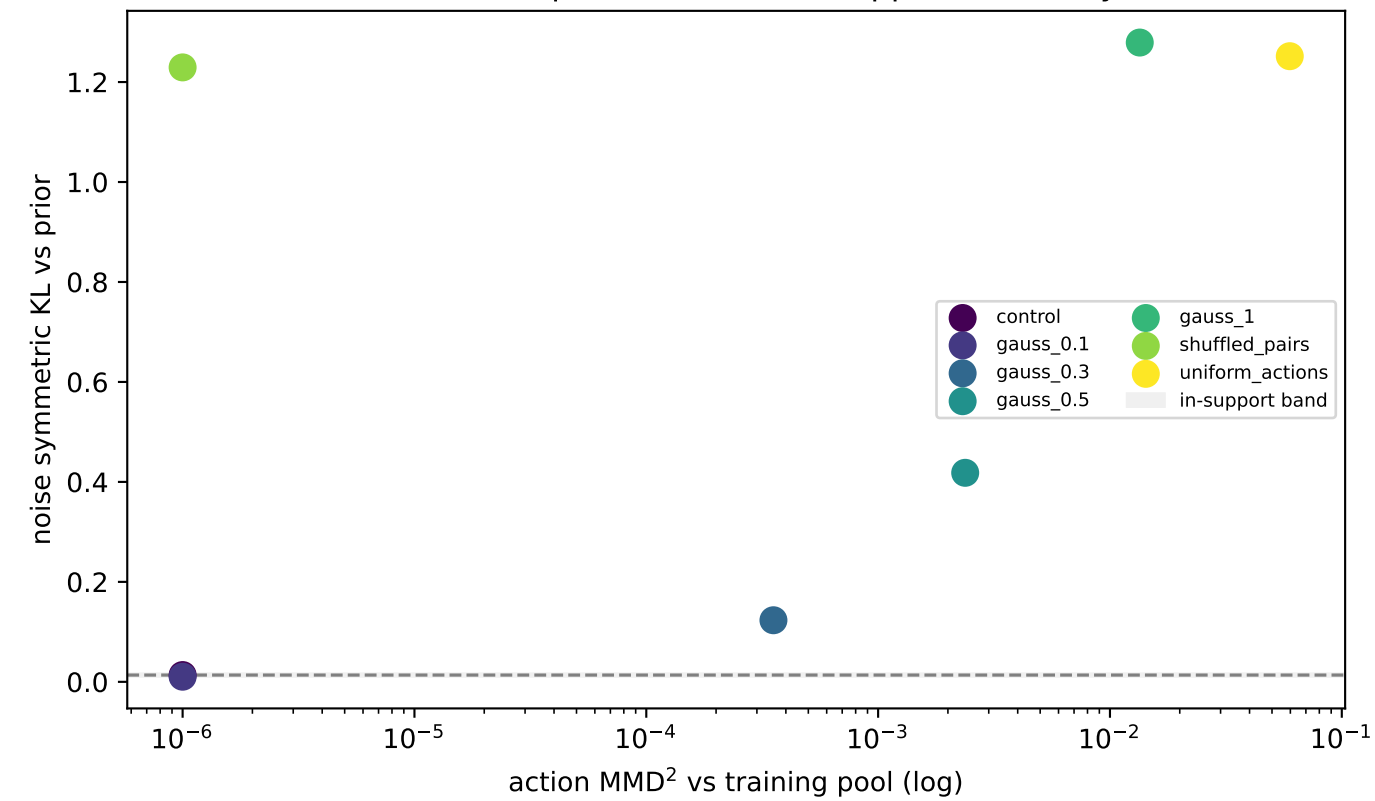

(C) Recovered-noise squared norms vs prior

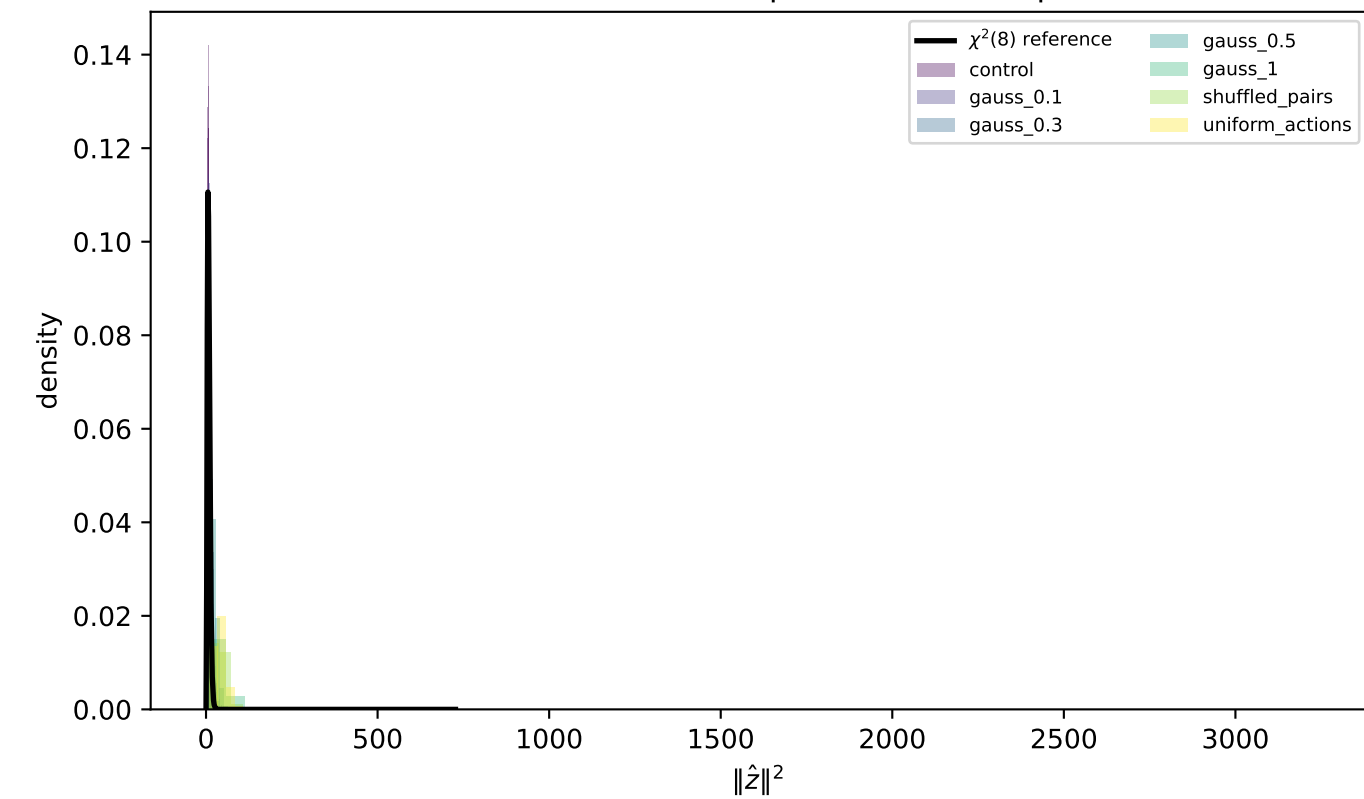

(D) Per-action OOD detectability

