



**VERTEX**  
POWERED BY INNOVATION

# INX -PAN

## Dental Panoramic System



**AERB Approved**



Scanned with OKEN Scanner

Scanned with OKEN Scanner

Scanned with OKEN Scanner

Scanned with OKEN Scanner



## Panoramic Mode


Patient Selection	Adult, Child selection
Selection Parameters	KV Selection
Exposure Time	OPG: 17 Sec
Cassette Size	10" x 12"



## Panoramic View



## TM Joints

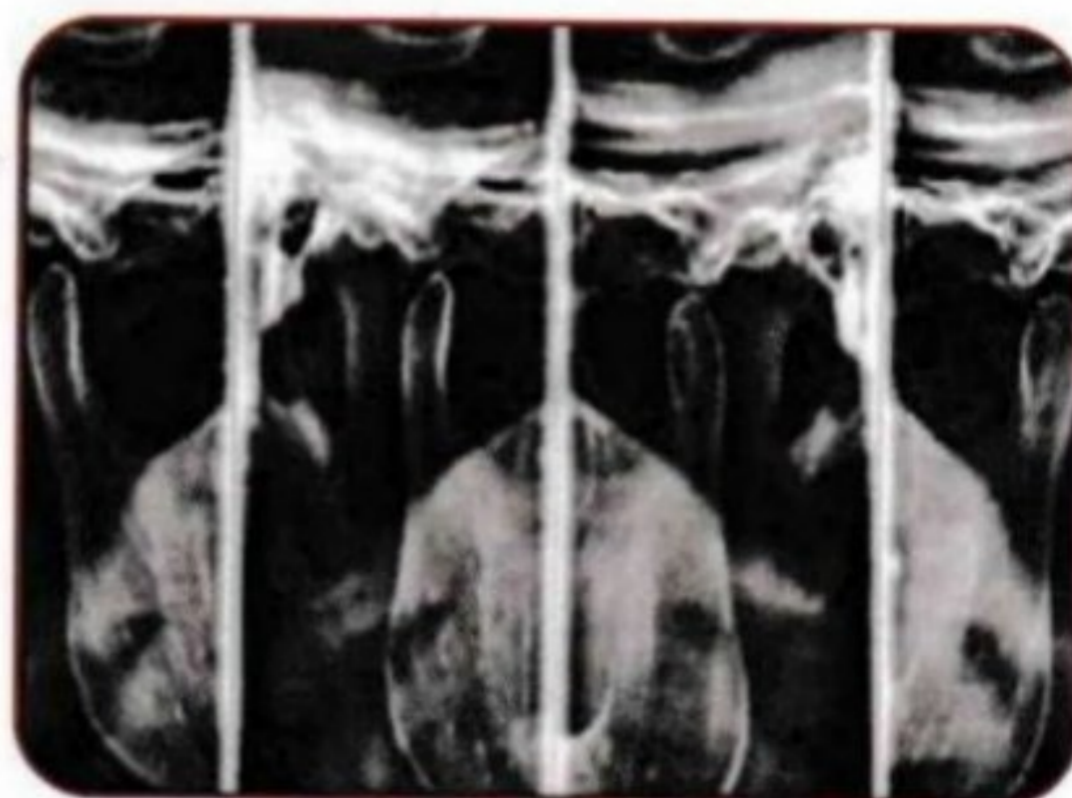



## Cephalogram Mode

Patient Selection	Adult, Child selection
Selection Parameters	KV. time selection
Cassette Size	10" x 12"
Exposure Time	0.5 to 10 Sec.



## Cephalogram



## TM Joints

Patient Selection	Adult, Child selection
Selection Parameters	KV Selection
Exposure Time	4"x4" Sec
Cassette Size	10" x 12"

## Technical Specifications

1.	Generator	Full wave rectified
2.	Control Display	Microcontroller based 5 Line LCD Display
3.	Anode Voltage	50 Kvp to 85 Kvp
4.	Anode Current	8 to 10 mA
5.	Tube Focus	0.5mm x 0.5 mm fine focus
6.	Total Filtration	2.5 mm Al
7.	Max. Power	1.0 KW
8.	Max. Line Current	5.0 A
9.	Power Requirements	230 V AC/50 Hz
10.	Vertical Movement	Motorised

\* Regulatory Requirement : AERB Type Approval

### Innovation Meditech Pvt. Ltd.

H.O. and Works:

B-6, Sector-88, Phase 2, NOIDA-201301. UP. India

Phone: 01203671764

Email: sales@innovationmeditech.com

Web: www.innovationmeditech.com



**BRANCH OFFICE & RESIDENT: JAIPUR • LUCKNOW • PATNA • HYDERABAD  
BHOPAL • HISAR • KOLKATA**