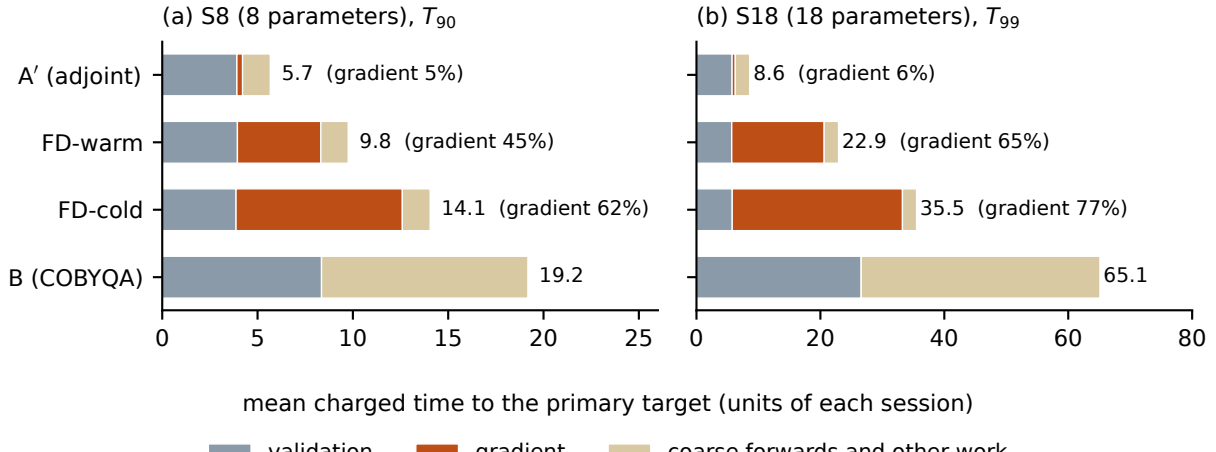
(a) S8 (8 parameters), T_{90}
(b) S18 (18 parameters), T_{99}
A′ (adjoint)
FD-warm
FD-cold
B (COBYQA)
5.7 (gradient 5%)
9.8 (gradient 45%)
14.1 (gradient 62%)
19.2
8.6 (gradient 6%)
22.9 (gradient 65%)
35.5 (gradient 77%)
65.1
0
5
10
15
20
25
0
20
40
60
80
mean charged time to the primary target (units of each session)
validation
gradient
coarse forwards and other work