

**BIOGRAPHICAL SKETCH**

Provide the following information for the Senior/key personnel and other significant contributors.  
Follow this format for each person. **DO NOT EXCEED FIVE PAGES.**

NAME: Olalekan P. Ogunmolu

eRA COMMONS USER NAME (credential, e.g., agency login): lakehanne

POSITION TITLE: Postdoctoral Researcher

EDUCATION/TRAINING (*Begin with baccalaureate or other initial professional education, such as nursing, include postdoctoral training and residency training if applicable. Add/delete rows as necessary.*)

INSTITUTION AND LOCATION	DEGREE (if applicable)	Completion Date MM/ YYYY	FIELD OF STUDY
The University of Sheffield, Sheffield, England	M.Sc (in Eng.)	11/2012	Control Systems
The University of Texas at Dallas, Richardson, TX	Ph.D	08/2019	Electrical Engineering (Robotics and Control Track)
The University of Chicago, Chicago, IL	Visiting Postdoc	09/2019	Radiation and Cellular Oncology
The University of Pennsylvania, Philadelphia, PA	Postdoc	Current	Radiation Oncology

### A. Personal Statement

I am an interdisciplinary researcher who combines the elegance of control theory with the practical impact of robotics. My long-term research goal to harness cutting-edge control systems in modern robot configurations as substitutes for existing rigid mechanisms used in clinics today for patient motion management in stereotactic radiosurgery (SRS), as well as brain and head-and-neck cancer radiation therapy (RT). In my postdoctoral training, I am investigating ways of improving the stereotactic precision of radiation delivery in emerging magnetic resonance imaging (MRI) and linear accelerator (LINAC) systems for radiation therapy (RT). This is so as to improve the efficiency of modern radiation therapy cancer treatment outcomes. My goal with this vision is to leverage the superior image scanning resolution and quality of magnetic resonance imaging (MRI) for feedback in managing the geometric uncertainties associated with modern treatment planning in RT. My robot designs leverage parallel configurations and radiation integrity/compliance for correcting head motion in closed-loop feedback SRS and head and neck cancer treatments.

My sponsor, Dr. Wiersma, is a recognized leader in robot-based head motion compensation in SRS and he has a good record of training researchers. The proposed research will provide me with new conceptual and technical training in bioengineering and applied medical physics. In addition, the proposed training plan outlines a set of career development activities – e.g. grant writing, public speaking, lab management, and mentoring students – designed to enhance my ability to be an independent investigator. My choice of sponsor, research project, and training will give me a solid foundation to reach my goal of safely and precisely repositioning patients in RT and SRS.

### B. Positions and Honors

- Research

**2019 – Present.** Postdoctoral Scholar, Department of Radiation Oncology, University of Pennsylvania.

**2019.** Postdoctoral Researcher, Department of Radiation and Cellular Oncology, University of Chicago.  
**2018.** Robotics Research Intern, Preferred Networks, Otemachi, Chiyoda-ku, Tokyo, Japan.  
**2017 – 2019.** Graduate Research Assistant, Medical Artificial Intelligence and Automation Laboratory, Division of Medical Physics and Engineering, UT Southwestern Medical Center.  
**2017-2018.** Research Assistant, Dr. Tyler Summers, Mechanical Engineering, UT Dallas.  
**2014 – 2019.** Research Assistant, Electrical Engineering Department, University of Texas at Dallas.  
**2016.** Hardware Integration Intern, Amazon Robotics LLC, Summer.

- **Teaching**

**2020 – Present.** Adjunct Instructor, Robot manipulation, planning and control, Brandeis University  
**2014 – 2016.** Teaching Assistant, Introduction to Robotics, University of Texas at Dallas

- **Honors**

**October 2018.** Google AI Travel and Conference Grant  
**August 2018.** IEEE RAS/IROS Travel Award (IROS 2018)  
**August 2017.** Finalist at the 3rd Entrepreneurship Forum and Startup Competition, Sponsored by  
**August 2017.** IEEE Robotics and Automation Society, KUKA AG, and Univ. Hamburg  
**August 2017.** NSF Doctoral Consortium Award (IROS 2017)  
**August 2017.** Mary and Richard Templeton Graduate Fellowship  
**July 2017.** ROSCon Scholarship, (Open Software for Robotics Foundation)  
**Nominated Feb. 2017.** President's Teaching Excellence Award for Teaching Assistants  
**Dec. 2016.** Golden Key International Honour Society  
**August 2016.** IEEE RAS/ISAM Travel Award (CASE 2016)  
**2015 – 2016.** Ericsson Graduate Fellowship  
**2014 – 2015.** Jonsson Scholarship  
**Fall 2014.** Achievement Award, University of Florida (Declined)  
**2011.** PTDF Overseas Scholarship Award, £25,500+ for one year, (~1.7% acceptance).  
**2002.** Federal Government (of Nigeria) Scholarship (~3.6% acceptance)  
**2004.** Ondo State (Nigeria) Scholarship, (~10% acceptance)

- **Professional Memberships And Services**

**2020-Present.** The New York Academy of Sciences, Member.  
**2017-Present.** The IEEE Robotics and Automation Society, Member.  
**2020-Present.** The American Association of Physicists in Medicine, Junior Member, Member.  
**2020-Present.** The American Society for Radiation Oncology, Member.

## C. Contributions to Science

Soft robotics is an emerging sub-specialty in the field of robotics which mitigates the difficulty of operating in unstructured, congested and nonlinear environments unlike their rigid robot counterparts. Inspired from the dynamics of living organisms such as muscular hydrostats (octopus and elephant trunks), and made out of artificial muscles and connective tissues, robots with a soft structure and delicate tissue have redundant degrees of freedom that are helpful in delicate control in cluttered or complex nonlinear dynamical systems. They have the potential to provide versatile adaptability and flexibility for an object's movement, support or manipulation. My research capitalizes on soft robot designs to manipulate body parts during brain as well as head and neck radiation therapy treatments of cancer tumors. To the best of my knowledge, I am the only researcher in the United States who undertakes this accurate patient positioning research challenge of addressing dose efficacy while guaranteeing patient comfort, eliminating dose attenuation and obtaining an AAPM task group approved accuracy requirement -- by using soft tissue materials to achieve these goals. By controlling the amount of fluid in the internal cavities of my soft robots, I have compensated motion deviation using non-parametric models derived from indirect adaptive control. My hardware design absorbs the reactive pressure from the patient's displacement during manipulation, thus guaranteeing patient's comfort. The radio-

transparency of these soft robots to ionizing radiation make situating them close to the tumor source an attractive option for fast motion compensation -- mitigating against the inherent delay between the computation of control signals and actuation in rigid compensation works that have been proposed so far. My continuum, compliant and configurable (C3) inflatable air bladders (IABs) mitigate the highlighted issues that rigid robot compensation mechanisms and the state of the art Cyberknife system introduce. My soft elastomeric actuators provide therapeutic patient motion compensation during RT through inflation, deflation, extension or contraction governed by their material moduli, incompressibility or internal pressurization when given a reference trajectory.

Since soft robots are much cheaper to mass-produce compared to rigid robots, my platform reduces the cost of providing healthcare for cancer patients, and has the potential to spur other research directions in scaling composite models for real-time deployments in control systems: in space robotics, consumer robotics (warehouses) and democratize human-friendly robots in homes and society at large. I have responded to the challenges in my field by proposing a novel and precise position immobilization system using soft actuators that guarantees patient comfort, and dose efficacy and an efficient clinical outcome.

Other than my applied engineering studies in clinical healthcare, I have made contributions to robust reinforcement learning by improving the transfer learning of learned control policies in real-time robot control deployments. I have also used deep learning architectures in the past to drastically improve the time it takes to find *near-optimal* solutions to the beam orientation optimization in intensity modulated radiation therapy. My control theory and robotics educational training along with the experience I have gathered in industry will be helpful in quickly realizing the objectives of my robotic radiosurgery and MRI integration goals in this proposal.

#### **D. Additional Information: Research Support and/or Scholastic Performance**

##### **Scholastic Performance**

YEAR	COURSE TITLE	GRADE
UNIVERSITY OF SHEFFIELD		
2011	Foundations of Control Systems	82 (P)
2012	Advanced Industrial Control	70 (P)
2012	Robotics and Multi-Sensor Systems	75 (P)
2011	Embedded Systems, Reliability and Fault Diagnosis	76 (P)

University of Sheffield graduate courses are graded P (pass) or F (fail). A grade in the range 70-100 signifies work of a Class I standard (First-Class Honours Degree).

YEAR	COURSE TITLE	GRADE
UNIVERSITY OF TEXAS AT DALLAS		
2015	Nonlinear Systems	A
2015	Stability of Switched Systems	A-
2015	Convex Optimization	P

Convex Optimization was taken as a research course. Grades were either pass (P) or fail (F).

- Peer Reviewing Activities**

- 2019.** JBHI, An IEEE Journal of Biomedical and Health Informatics Access.
- 2019.** External Grants Reviewer, AI for Species Discovery, National Geographic Society.
- 2018, 2019.** Automatica, The International Federation of Automatic Control (IFAC).
- 2017, 2018, 2019.** Access, IEEE Access Journal.
- 2017, 2018, 2019.** NCA, Springer's Neural Computing and Applications .
- 2017, 2020.** ICML, International Conference on Machine Learning .
- 2018, 2019, 2020.** CDC, IEEE International Conference on Decision and Control, Flagship Control and Decision-Making Control Conference Proceedings in the World.

**BIOGRAPHICAL SKETCH**

Provide the following information for the Senior/key personnel and other significant contributors.  
Follow this format for each person. **DO NOT EXCEED FIVE PAGES.**

NAME: Rodney D. Wiersma

ERA COMMONS USER NAME (credential, e.g., agency login): RWIERSMA

POSITION TITLE: Associate Professor

EDUCATION/TRAINING (*Begin with baccalaureate or other initial professional education, such as nursing, include postdoctoral training and residency training if applicable. Add/delete rows as necessary.*)

INSTITUTION AND LOCATION	DEGREE (if applicable)	Completion Date MM/YYYY	FIELD OF STUDY
University of Alberta, Canada	B.Sc.	06/1999	Physics
Simon Fraser University, Canada	M.Sc.	06/2002	Physics
Max-Plank-Institute, Germany	Ph.D.	06/2006	Physics
Stanford University, USA	Postdoc	01/2009	Medical Physics

**A. Personal Statement**

My research is primary focused on image guidance radiation therapy (IGRT), treatment planning optimization, quality assurance (QA) systems, and the application of robotics to radiation therapy (RT). I have a successful track record in project leadership, teaching/mentoring, securing external funding, and translating research from the lab to the clinic. I hold several US patents, with two presently licensed to commercial companies, and I am a founder of a QA startup company that employs several full-time people. The goal of my robotics research is to replace current stereotactic radiosurgery methods that have therapeutic drawbacks and are highly invasive to patients with an approach that uses real-time 6 degree of freedom (6DoF) patient head motion tracking and active robotic control systems to continuously correct patient head motion during treatment. In 2012 I was awarded a 4 year Research Scholar Grant (RSG) from the American Cancer Society (ACS) for this research and have since established the feasibility of the approach. In the a current tangential research, we aim to explore the potential of using pencil beam scanning (PBS) proton therapy to deliver FLASH therapy and evaluate it in animal systems. Heavy particle FLASH would overcome many of the inherent difficulties of electron FLASH in terms of penetration depth allowing deep seated tumors to be treated. We have created a well-rounded team, where my expertise in robotics, optimization, and QA will complement the significant proton expertise of my colleagues. To implement PBS in our dedicated small animal research room, I will contribute to the development of a robotic based PBS system as well as a 6-degree-of-freedom treatment table for canine studies. In addition, I will be involved with FLASH treatment parameter optimization and the development of FLASH specific QA procedures.

**B. Positions and Honors****Positions**

- 2009-2011 Instructor, Radiation and Cellular Oncology, University of Chicago  
 2011-2019 Assistant Professor, Radiation and Cellular Oncology, University of Chicago  
 2019- Associate Professor, Radiation Oncology, University of Pennsylvania  
 2019- Director of Research, Physics, Radiation Oncology, University of Pennsylvania

**Honors**

- 1996-1999 Alberta Rutherford Scholarship for undergraduate studies  
 2002 Simon Fraser University graduate research award  
 2002-2006 Deutsche Promotionstipendium (German PhD Scholarship)

2004	Selected to attend 54th Nobel Laureates Meeting in Lindau, Germany
2007	ASTRO travel award
2010	Feature article Medical Physics Web, "Stereotactic Radiosurgery: Losing the Frame".
2014	Feature article Medical Physics Web, "Combined MV+KV planning enables real-time tracking".
2015	The Kurt Rossmann Award for Excellence in graduate medical physics teaching
2017	Medical Physics Journal Editor's Choice, "Use of Proximal Operator Graph Solver for Radiation Therapy Inverse Treatment Planning"

### Other Experience and Professional Memberships

2006-	Member, American Association of Physicists in Medicine (AAPM)
2009-	State of Illinois IEMA Division of Nuclear Safety
2010-	American Board of Radiology (DABR) in Therapeutic Radiologic Physics
2010-	American Cancer Society grant reviewer for Epidemiology and Clinical Research

### C. Contributions to Science

#### Use of robotic systems in radiation therapy

I was the first to develop a method for performing real-time patient head motion cancellation in frameless stereotactic radiosurgery (SRS). Currently, to achieve the 1-2 mm precision for intracranial SRS, a metal head ring is rigidly fixated to the patient's skull using screws under local anesthesia, and then bolted on the treatment couch. The discomfort, inconvenience, and invasive nature associated with the frame preparation have been identified as the main cause of poor patient compliance and poor clinical efficiencies when SRS is medically indicated. Frameless SRS methods based on a thermoplastic mask placed over the face and fixed to the couch has been reported to limit head motion to approximately 2 - 3 mm due to rotation about the fulcrum at the back of the skull. My group is working to develop a frameless and maskless SRS technique that uses real-time 6DOF optical tracking together with a 6DOF robotic head stage for cancellation of patient head motion. This approach has the potential to be less invasive than current frameless SRS techniques while still achieving accuracies better or equal than traditional frame based SRS.

1. Belcher AH, Liu X, Chmura S, Yenice K, Wiersma RD. Towards frameless maskless SRS through real-time 6DoF robotic motion compensation. *Physics in Medicine & Biology*. 2017 Nov 13;62(23):9054
2. Wiersma RD, Wen Z, Sadinski M, Farrey K, Yenice KM. Development of a frameless stereotactic radiosurgery system based on real-time 6D position monitoring and adaptive head motion compensation. *Physics in medicine and biology*. 2009 Dec 17;55(2):389
3. Kang HJ, Grelewicz Z, Wiersma RD. Development of an automated region of interest selection method for 3D surface monitoring of head motion. *Medical physics*. 2012 Jun 1;39(6):3270-82
4. Liu X, Belcher AH, Grelewicz Z, Wiersma RD. Robotic real-time translational and rotational head motion correction during frameless stereotactic radiosurgery. *Med Phys*. 2015 Jun;42(6):2757-63.

#### Image-guided radiation therapy and treatment planning optimization

I was the first to develop the combined MV+KV imaging technique for the purpose of performing real-time 3D tumor tracking during radiation therapy. This method is particularly suited to modern LINACs which come pre-equipped with onboard MV and KV imaging devices arranged orthogonally on the gantry. This orthogonal geometric arrangement offers a natural stereoscopic pair, and thus can be used for 3D tumor position monitoring. The MV-KV tracking method has also been verified to operate successfully on next generation volumetric modulated arc therapy (VMAT). I am also the primary inventor of the combined MV+KV treatment planning approach which allows optimal incorporation of the KV dose into the MV treatment plan.

1. Wiersma RD, Mao W, Xing L. Combined kV and MV imaging for real-time tracking of implanted fiducial markers. *Medical physics*. 2008 Apr 1;35(4):1191-8
2. Liu W, Wiersma RD, Mao W, Luxton G, Xing L. Real-time 3D internal marker tracking during arc radiotherapy by the use of combined MV–KV imaging. *Physics in medicine and biology*. 2008 Nov 28;53(24):7197
3. Wiersma RD, Riaz N, Dieterich S, Suh Y, Xing L. Use of MV and kV imager correlation for maintaining continuous real-time 3D internal marker tracking during beam interruptions. *Physics in medicine and biology*. 2008 Dec 5;54(1):89

4. Grelewicz Z, Wiersma RD. Combined MV+ kV inverse treatment planning for optimal kV dose incorporation in IGRT. Physics in medicine and biology. 2014 Mar 10;59(7):1607

Quality assurance methods for modern radiation therapy

I have been actively involved in improving patient safety in radiation therapy (RT) through the development of several modern quality assurance (QA) methods. Success of RT critically depends on the proper function of many complex devices such as linear accelerators (LINAC), computer tomography (CT), magnetic resonance imaging (MRI), positron emission tomography (PET), and high dose brachytherapy (HDR). Clinically, an adequate confidence that these devices will satisfy the given requirements for quality is achieved by performing QA consisting of a series of planned and systematic actions (ISO 9000:1994). QA reduces uncertainties and errors in dosimetry, equipment performance, treatment delivery, etc., thereby improving dosimetric and geometric accuracy and the precision of dose delivery. Clinically, this improvement is translated into enhanced tumor control as well as reduced complication and likelihood of accidents and errors occurring. Here I have developed QA methods that allow for high temporal resolution tests of radiation beam gating cycles, 6D phantoms for performing LINAC QA, and tests for both EPID and optical patient motion tracking devices.

1. Wiersma RD, Tomarken SL, Grelewicz Z, Belcher AH, Kang H. Spatial and temporal performance of 3D optical surface imaging for real-time head position tracking. *Medical physics*. 2013 Nov 1;40(11)
  2. Wiersma RD, Xing L. Examination of geometric and dosimetric accuracies of gated step-and-shoot intensity modulated radiation therapy. *Medical physics*. 2007 Oct 1;34(10):3962-70
  3. Belcher AH, Liu X, Grelewicz Z, Pearson E, Wiersma RD. Development of a 6DOF robotic motion phantom for radiation therapy. *Medical physics*. 2014 Dec 1;41(12)
  4. Wiersma RD, McCabe BP, Belcher AH, Jensen PJ, Smith B, Aydogan B. High temporal resolution characterization of gating response time. *Medical physics*. 2016 Jun 1;43(6):2802-6

## **Complete List of Published Work in My Bibliography**

<http://www.ncbi.nlm.nih.gov/sites/myncbi/1rAZJDFGA9Ckq/bibliography/49466503/public/?sort=date&direction=descending>

**D. Additional Information: Research Support and/or Scholastic Performance**

### Ongoing research support

NIH-R21 1R21EB028103-01 Wiersma (co-PI) 06/01/2019 - 05/31/2021  
Enhanced megavoltage imaging for radiotherapy by light-field imaging of scintillators: we propose to overcome the EPID contrast obstacle by increasing the photon detection layer to 10-50mm using a transparent scintillator and then capturing its 4D light field using a specially designed optical camera system.

NIH-R01 1R01CA227124-01A1 Wiersma (PI) 12/04/2018 - 11/30/2023  
Development of a portable and compact robotic system for frameless and maskless stereotactic radiosurgery:  
the goal of this project is to design, construct, and implement a robotic SRS system for early clinical trials on brain cancer patients.

## **Completed Research Support**

American Cancer Society RSG-13-313-01-CCE Wiersma (PI) 07/01/2013 - 06/30/2018  
Frameless SRS based on robotic motion cancellation: to develop a next generation frameless maskless SRS approach where small intrinsic patient head motions are continuously cancelled out during frameless SRS treatment.

CTSA-Institute for Translational Medicine      Wiersma (PI)      06/01/2016 - 06/01/2017  
Genetically modified bacteria for transport and synthesis of iron oxide nanoparticles at the tumor site: creation of tumor targeting bacteria containing iron oxide for hyperthermia therapy purposes.

**BIOGRAPHICAL SKETCH**

Provide the following information for the Senior/key personnel and other significant contributors.  
Follow this format for each person. **DO NOT EXCEED FIVE PAGES.**

NAME: Turner, Kevin T.

ERA COMMONS USER NAME (credential, e.g., agency login): KEVINTTURNER

POSITION TITLE: Professor and Chair, Mechanical Engineering and Applied Mechanics, The University of Pennsylvania

EDUCATION/TRAINING (*Begin with baccalaureate or other initial professional education, such as nursing, include postdoctoral training and residency training if applicable. Add/delete rows as necessary.*)

INSTITUTION AND LOCATION	DEGREE (if applicable)	Completion Date MM/YYYY	FIELD OF STUDY
Johns Hopkins University	B.S	05/1999	Mechanical Engineering
Massachusetts Institute of Technology	M.S	05/2001	Mechanical Engineering
Massachusetts Institute of Technology	Ph.D	05/2004	Mechanical Engineering
Massachusetts Institute of Technology	Postdoctoral	08/2005	Materials Science and Engineering

**A. Personal Statement**

My research addresses fundamental and applied problems at the intersection of the fields of surface and interface mechanics and micro- and nanosystems. Surface and interface mechanics, which encompasses fracture, contact, and adhesion mechanics, plays a crucial role in determining the behavior of many micro- and nano-scale systems and manufacturing processes. My research group uses a combination of experimental measurements, analytical modeling, and numerical simulations to improve and realize innovative micro- and nanomanufacturing processes as well as to develop new approaches to measure the mechanical properties of interfaces at small scales. My current work includes projects in nanocomposites, materials with tunable adhesive properties, and flexible electronics.

The proposed project includes development of soft mechanical sensors. I will leverage my expertise in sensors, mechanics of materials, and flexible electronics in my mentoring role on the proposed project.

**B. Positions and Honors****Position and Employment**

1999-2004	Research Assistant, Massachusetts Institute of Technology, Cambridge, MA
2004-2005	Postdoctoral Associate and Lecturer, Department of Materials Science and Engineering, Massachusetts Institute of Technology, Cambridge, MA
2005-2011	Assistant Professor of Mechanical Engineering, University of Wisconsin, Madison, WI
2006-2011	Faculty Affiliate, Materials Science Program, University of Wisconsin, Madison, WI
2007-2011	Faculty Affiliate, Biomedical Engineering, University of Wisconsin, Madison, WI
2011-2011	Associate Professor of Mechanical Engineering, University of Wisconsin, Madison, WI
2011-present	co-Founder, systeMECH, Inc, Madison, WI
2011-2016	Associate Professor of Mechanical Engineering and Applied Mechanics (primary) and Materials Science and Engineering (secondary) University of Pennsylvania, Philadelphia, PA
2012-2017	Director, Quattrone (Wolf) Nanofabrication Facility, University of Pennsylvania
2016-2019	Graduate Group Chair, Mechanical Engineering & Applied Mechanics, University of Pennsylvania
2019-present	Chair, Mechanical Engineering & Applied Mechanics, University of Pennsylvania

## **Memberships**

1998-present Member, American Society of Mechanical Engineering  
2000-present Member, Materials Research Society  
2008-present Member, Adhesion Society

## **Honors**

2008	ASEE Ferdinand P. Beer and E. Russell Johnston, Jr. Outstanding New Mechanics Educator
2009	National Science Foundation CAREER Award
2009	3M Non-tenured Faculty Award
2009	R&D 100 Award for UNCD AFM probes
2011	Young Adhesion Scientist Award, the Adhesion Society
2011	Outstanding Young Manufacturing Engineer Award, the Society of Manufacturing Engineers
2012	NAE Frontiers of Engineering Symposium, invited participant
2014	ASME Sia Nemat-Nasser Early Career Award

## **C. Contribution to Science**

1. Microelectronic and microelectromechanical devices need to have robust and stable performance over long service lives. The performance of these devices hinge critically on the mechanical properties of the materials and interfaces formed during the fabrication process. Thus, characterization of the mechanical properties of devices and materials after fabrication is critical. Turner has developed and implemented numerous small-scale mechanical testing to interrogate mechanical properties in fabricated devices. Because of the size of the devices and features, innovative mechanical testing and modeling techniques are often required. Examples of such work are included in the following publications.
  - a. Grierson DS, Liu J, Carpick RW, and **Turner KT** (2013) Adhesion of nanoscale asperities with power-law profiles, *Journal of Mechanics and Physics of Solids*, 61: 597-610.
  - b. Wald MJ, Considine JM, and **Turner KT** (2013) Determining the Elastic Modulus of Compliant Thin Films Supported on Substrates from Flat Punch Indentation Measurements," *Experimental Mechanics*, 53: 931-41.
  - c. Cavallo F, Grierson DS, **Turner KT**, and Lagally MG (2011) "Soft Si": Effective stiffness of supported crystalline nanomembranes, *ACS Nano*, 5: 5400-7.
  - d. Tadepalli R and **Turner KT** (2008) A chevron specimen for the measurement of mixed-mode interface toughness of wafer bonds, *Engineering Fracture Mechanics*, 75: 1310-19.
2. Wear of materials is a ubiquitous problem that limits the performance of many systems, ranging from bearings to microscale devices to biomechanical joints. Wear is a significant issue that limits the lifetime of atomic force microscope probes in nanometrology and nanofabrication processes. Turner, in collaboration with others, has investigated the wear of atomic force microscope probes at the nanoscale and developed new understanding of the mechanisms of wear. Specifically, the papers below show an atom-by-atom attrition process with a rate that increases with applied stress.
  - a. Vahdat V, Ryan KE, Keating PL, Jiang Y, Adiga SP, Schall JD, **Turner KT**, Harrison JA, and Carpick RW (2014) Atomic-scale wear of amorphous hydrogenated carbon during intermittent contact: a combined study using experiment, simulation, and theory, *ACS Nano*, 8: 7027-40.
  - b. Vahdat V, Grierson DS, **Turner KT**, and Carpick RW (2013) Mechanics of interaction and atomic-scale wear of amplitude modulation atomic force microscopy probes, *ACS Nano*, 7: 3221-35.
  - c. Liu J, Grierson DS, Moldovan N, Notbohm J, Li S, Jaroenapibal P, O'Connor SD, Sumant AV, Neelakantan N, Carlisle JA, **Turner KT**, Carpick RW (2010) Preventing nanoscale wear of atomic force microscopy tips through the use of monolithic ultrananocrystalline diamond probes, *Small*, 6: 1140-49.
  - d. Liu J, Notbohm J, Carpick RW, and **Turner KT** (2010) Method for characterizing nanoscale wear of atomic force microscope tips, *ACS Nano*, 4: 3763-72.

**Complete List of Published Work in MyBibliography:**

## D. Research Support

### Current Research Projects

NSF 1542153 (PI: M. Allen)	09/01/15-08/31/20
NNCI: Mid-Atlantic Nanotechnology Hub (MANTH) for Research, Education, & Innovation	
The goal of this award is to make nanotechnology infrastructure at the University of Pennsylvania broadly available to academic and industrial users in the mid-Atlantic region.	
Role: co-Principal Investigator	
NIH/NIAMS R01 AR071718 (PI: X. Liu)	04/01/17-03/31/22
Effects of reproduction and lactation on postmenopausal bone health	
The major goals of this project are to identify the critical phenotypic bone structure, material properties, and mechano-sensitivity resulting from reproduction and lactation that protect the maternal skeleton from future postmenopausal bone loss.	
Role: Senior personnel	
NSF 1663037 (PI: K. Turner)	04/01/17-03/31/21
Collaborative Research: Exploiting tunable stiffness for dynamic adhesion control at the macro- and micro-scale	
The major goal of this project is to exploit materials with tunable stiffness to realize surfaces with dynamic and switchable adhesion properties.	
Role: Principal Investigator	
U.S. Endowment for Forestry & Communities, Inc (PI: K. Turner)	05/01/17 – 09/30/20
3D Printing of Cellulose Nanofibril Materials	
The major goal of this proposal is to investigate the fabrication of bulk nanocellulose parts via additive manufacturing (i.e. 3D printing) techniques.	
Role: Principal Investigator	
NSF 1662695 (PI: D. Lee)	06/01/17-03/31/21
Nanostructured Composite Coatings to Harden and Toughen Polymer Surfaces	
The major goal of this project is to investigate the processing, structure, property relationships of nanoparticle composite films synthesized through capillary rise infiltration.	
Role: co-Principal Investigator	
USDA/NIFA 2016-08810 (PI: K. Turner)	07/01/17-06/30/20
Engineering Cellulose Nanomaterials with High Toughness	
The major goal of this project is to investigate the toughness and crack growth resistance of materials based cellulose nanomaterials.	
Role: Principal Investigator	
NSF 1720530 (PI: A. Yodh)	09/01/17-08/31/23
Materials Research Science and Engineering Center (MRSEC)	
The major goal of Turner's work in this center is to examine the mechanics and fracture of disordered solids, including molecular glasses and nanoparticle films.	
Role: Senior Personnel	
NSF 1761726 (PI: J. Bassani)	04/01/18-03/31/21
Tailoring interface geometry to realize controlled and directionally-dependent adhesion	
The major goal of this project is to investigate strategies to tailor the interface toughness (fracture resistance) through micro- and nano-patterning.	

Role: co-Principal Investigator

NSF 1830475 (PI: K. Turner)

09/01/18 – 08/31/21

NRI:INT:COLLAB: Soft Active Contact Pads with Tunable Stiffness and Adhesion for Customizable Robotic Grasping

The major goal of this project is to develop robotic gripping strategies based on materials with tunable stiffness.

Role: Principal Investigator

#### **Past Research Projects (<3 years old)**

NSF 1435745 (PI: Turner)

09/01/2014-08/31/2018

Structured Composite Materials with Variable Adhesion Properties

This grant supports the design, fabrication, and characterization of novel micro- and nano-structured surfaces with tunable adhesion.

Role: Principle Investigator

**BIOGRAPHICAL SKETCH**

Provide the following information for the Senior/key personnel and other significant contributors.  
Follow this format for each person. **DO NOT EXCEED FIVE PAGES.**

NAME: George Pappas

eRA COMMONS USER NAME (credential, e.g., agency login):

POSITION TITLE: UPS Foundation Professor of Transportation and Chair, Electrical and Systems Engineering (ESE), Computer and Information Science (CIS), Mechanical Engineering and Applied Mechanics (MEAM), The University of Pennsylvania

EDUCATION/TRAINING (*Begin with baccalaureate or other initial professional education, such as nursing, include postdoctoral training and residency training if applicable. Add/delete rows as necessary.*)

INSTITUTION AND LOCATION	DEGREE <i>(if applicable)</i>	Completion Date MM/YYYY	FIELD OF STUDY
University of California, Berkeley	PhD	1998	Electrical Engineering & Computer Sciences
Rensselaer Polytechnic Institute	MS	1992	Computer & Systems Engineering
Rensselaer Polytechnic Institute	BS	1991	Computer & Systems Engineering

**A. Personal****Statement**

My research broadly exists at the intersection of control theory, robotics, machine learning, and cyber-physical systems. I have a strong track record in leading multidisciplinary teams, multi-institutional and multifunctional teams and I enjoy mentoring and training young researchers and engineers – most of whom who have gone on to win the most prestigious awards at the highest impact publication avenues in control theory and robotics throughout my career. In April of 2017, I won the University of Pennsylvania's *Provost Award for Distinguished PhD Teaching and Mentoring*. I am a Fellow of IEEE, and I have received several awards including the Antonio Ruberti Young Researcher Prize, the George S. Axelby Award, the O. Hugo Schuck Best Paper Award, the National Science Foundation's Presidential Early Career Awards for Scientists and Engineers (PECASE), and the George H. Heilmeier Faculty Excellence Award.

Along with my students, postdocs, institutional and company/organization collaborators, I am executing and addressing foundational engineering problems that have significant impact on modern society. Under the National Science Foundation award CNS-1035715, I was the physiological closed-loop control Co-PI for the medical device cyber physical systems (CPS) project (funded by both NIH and NSF) where we worked on patient modeling, caregiver mental models, and the distributed control and sensing in networked medical device systems for physiological closed-loop treatment of the patient in therapy delivery. This project has enabled the introduction of closed-loop feedback in the clinical practice, helping reduce the caregivers' burden as well as cost of healthcare. Currently, I am a principal investigator (PI) or Co-PI on various projects control and modeling projects amounting in excess of thirty-nine million dollars (\$39,000,000+). These projects range in topics from medical devices modeling for cyber physical systems<sup>4-9</sup> to control of biomolecular<sup>1-4</sup> networks among others. Given my project management experience and control expertise, I believe I am in a good position in helping Olalekan successfully execute the goals he articulated in the K99 Aims II and III of his research strategy.

1. Robust Economic Model Predictive Control of Continuous-time Epidemic Processes. Nicholas Watkins, Cameron Nowzari, and George J. Pappas. *IEEE Transactions on Automatic Control*. In press
2. Minimal reachability is hard to approximate. Ali Jadbabaie, Alex Olshevsky, George J. Pappas, and Vassilis Tzoumas. *IEEE Transactions on Automatic Control*, 64(2):783-789, February 2019.

3. Resilient Active Target Tracking with Multiple Robots. Lifeng Zhou, Vasileios Tzoumas, George J. Pappas, Pratap Tokek. *IEEE Robotics and Automation Letters*. 4(1):129-136, January 2019.
4. Harnessing bacterial power for micro scale manipulation and locomotion. A. Julius, S. Sakar, E. Steagery, U. Cheangy, M. Kim, V. Kumar, and G. J. Pappas. *IEEE International Conference on Robotics and Automation*, Kobe, Japan, May 2009.
5. **Metabolic network analysis using convex optimization.** Agung Julius, Marcin Imielinski, and George J. Pappas. *IEEE Conference on Decision and Control*, Cancun, Mexico, December 2008.
6. **Genetic network identification using convex optimization.** A. Agung Julius, Michael Zavlanos, Stephen P. Boyd, and George J. Pappas. *IET Systems Biology*, 3(3):155-166, May 2009.
7. **Hybrid model predictive control of induction of Escherichia coli.** Agung Julius, Selman Sakar, Alberto Bemporad, and George J. Pappas. *IEEE Conference on Decision and Control*, New Orleans, LA, December 2007.
8. **Identification of stable genetic networks using convex programming.** Michael M. Zavlanos, Agung Julius, Stephen P. Boyd, and George J. Pappas. *American Control Conference*, Seattle, WA, June 2008.
9. **Hybrid modeling and simulation of biomolecular networks.** Rajeev Alur, Calin Belta, Franjo Ivancic, Vijay Kumar, Max Mintz, George J. Pappas, Harvey Rubin, and Jonathan Schug. *Hybrid Systems : Computation and Control, Lecture Notes in Computer Science*, volume 2034, Springer, March 2001

## B. Positions and Honors

### PROFESSIONAL EXPERIENCE:

- **2008 – Present. Joseph Moore Professor**, Department of Electrical and Systems Engineering (ESE), University of Pennsylvania, Philadelphia, PA.
- **2007- 2008. Professor**, Department of Electrical and Systems Engineering, University of Pennsylvania, Philadelphia, PA.
- **2004 – 2007. Associate Professor**, ESE, University of Pennsylvania, Philadelphia, PA.
- **2000 – 2004. Assistant Professor, ESE**, University of Pennsylvania, Philadelphia, PA.

### SELECT PROFESSIONAL SERVICE

- **April 2008. Co-organizer**, NSF Cyber-Physical Systems Summit, St. Louis, MI.
- **May 2007. Participant**, NSF-NSA Biosecurity workshop, Baltimore, MD.
- **October 200 Program Committee**, NSF Workshop on Cyber-Physical Systems, Austin, TX
- **July 2008 Symposium Co-Chair**, Inter. Symposium on Experimental Robotics (ISER), Athens, Greece
- **2006 - Present. Steering Committee Chair**, Hybrid Systems : Computation and Control.
- **2007 - Present. Steering Committee Chair**, Cyber-Physical Systems Week.
- **2006 - Present. International Advisory Board Member**, Embedded Systems Institute, Netherlands.

### SELECT FELLOWSHIPS AND AWARDS:

- **July 2020.** International Federation of Automatic Control (IFAC) Fellow.
- **July 2019.** Finalist, Best Student Paper Award, American Control Conference (as advisor).
- **Dec 2018.** IEEE Control Systems Magazine Outstanding Paper Award, IEEE CSS.
- **Dec 2017.** Finalist, Best Student Paper Award, IEEE CDC, Melbourne, Australia, (as advisor).
- **July 2017.** Finalist, Young Author Prize, IFAC World Congress, Toulouse, (as advisor).
- **May 2017.** Best Conference Paper Award, IEEE ICRA, Singapore.
- **May 2017.** Finalist, Best Robotic Vision Paper Award, IEEE ICRA, Singapore.
- **April 2017.** Provost's Award for Distinguished Ph.D. Teaching and Mentoring,
- **April 2017.** Best Poster Award, IoT Design & Implementation (IoTDI),
- **July 2016.** O. Hugo Schuk Best Paper Award (theory), American Automatic Control Council
- **April 2015.** Finalist, Best Paper Award, ICCPS, Berlin, Germany,
- **March 2015.** George H. Heilmeier Faculty Award for Excellence in Research
- **June 2014.** O. Hugo Schuk Best Paper Award (theory), American Automatic Control Council.

- **April 2014.** Best Paper Award, ICCPS, Berlin, Germany.
- **April 2014.** Finalist (two papers), Best Paper Award, ICCPS, Berlin, Germany.
- **2011.** Finalist, Best Manipulation Paper Award, IEEE ICRA, Shanghai, China
- **2010.** Antonio Ruberti Young Researcher Prize, IEEE Control Systems Society.
- **2009.** George S. Axelby Outstanding Paper Award, IEEE Control Systems Society.
- **2009.** IEEE Fellow, Class of 2009
- **2007.** N.A.E.-A. von Humboldt German-American Frontiers of Engineering Program.
- **2006.** Finalist, Best Student Paper Award, IEEE CDC, San Diego, CA (as advisor).
- **2004 .** NSF Presidential Early Career Award for Scientists and Engineers (PECASE) Award.
- **2002.** National Science Foundation CAREER Award.
- **1999.** Eli Jury Award for Excellence in Systems Research, University of California at Berkeley

### C. Contributions to Science

George J. Pappas has made pioneering contributions to the analysis, design, and control of cyber-physical systems with applications to safe and secure autonomy. Modern cyberphysical systems, such as autonomous cars or aerial robots, are complex interconnections of control systems and software systems, making safety analysis of the combined cyberphysical system very challenging. In [1], he developed an award winning theory of hierarchical model approximation across continuous-time (control models), discrete-event (software models), and hybrid systems (cyberphysical models). This resulted in a paradigm of approximate symbolic abstractions for continuous and hybrid control systems, bridging semantically continuous-time and discrete-event systems. He subsequently leveraged his approximation theory in order to develop the first rigorous theory of robustness for temporal logic safety specifications and analysis for continuous control systems [2]. These foundational and influential achievements enabled the development of numerous safety analysis and synthesis tools by the cyberphysical systems community. A major impact of these ideas can be found in [3], where Pappas was the first to introduce formal methods notions of safety verification in robot mission planning in partially known environments, paving the way for what is now known as safe autonomy. Furthermore, autonomous systems (cars) are increasingly being operated in unknown environments, making safety in the presence of sensing and learning very important and timely topic. The safety of robotic autonomy critically depends on the ability to reason safely in an unknown but learned environment. In his award winning paper ([5]) Pappas introduced the notion of semantic mapping and localization (Semantic SLAM), which leverages advances in object detection in order to build meaningful (to humans) semantic maps of the world. Such semantic maps can be used for safe mission planning for autonomous cars or robots in uncertain semantic environments. In addition to safety, Pappas has also launched a program for secure and private cyberphysical systems with applications to automotive systems and avionics. His paper on resilient state estimation in the presence of sensor attacks [4], resulted in safe estimation of an autonomous car even if half of the car sensors were cyberattacked.

**[1] Approximation metrics for discrete and continuous systems** (George S. Axelby Outstanding Paper Award). A. Girard and G. J. Pappas. IEEE Transactions on Automatic Control, 52(5):782-798, May 2007;

**[2] Robustness of temporal logic specifications for continuous-time signals**, G. Fainekos and G. J. Pappas, Theoretical Computer Science, 410(42):4262-4291, September 2009;

**[3] Temporal-logic-based reactive mission and motion planning.** H. Kress-Gazit, G. Fainekos, and G. J. Pappas. IEEE Transactions on Robotics, 25(6):1370-1381, December 2009;

**[4] Attack-resilient state estimation for noisy dynamical systems.** Miroslav Pajic, Insup Lee, George J. Pappas. IEEE Transactions on Control of Network Systems, Special issue on Cyber- physical systems security, 4(1):82-92, March 2017.

**[5] Probabilistic data association for semantic SLAM** (Best Paper Award) S. Bowman, N. Atanasov, K. Daniilidis, and G. J. Pappas. IEEE Conference on Robotics and Automation, May 2017.

**D. Additional Information: Research Support and/or Scholastic Performance**

**Research Support**

- **9/1/2019-8/30/2024.** Autonomy in Contested Environments, AFOSR/AFRL  
PI : George J. Pappas. co-PI(s) : Dan Koditschek (Penn)  
**Award Amount:** \$2,500,000
- **1/1/2019-6/30/2021.** CIRCLES: Congestion Impact Reduction via CA-in-the-loop Lagrangian Energy Smoothing  
National Science Foundation Cyber-Physical Systems Program  
PI : A. Bayen (Berkeley) co-PI(s) : G. Pappas (Penn), D. Work (Vanderbilt), B. Piccoli (Rutgers)  
**Award Amount:** \$1,400,000
- **9/1/2018-8/31/2021.** CPS: Medium: Rethinking Communication and Control for Low-Latency, High Reliability IoT Devices, National Science Foundation Cyber-Physical Systems Program  
PI : George Pappas (Penn) co-PI(s) : Hamed Hassani, Alejandro Ribeiro  
**Award Amount:** \$1,000,000
- **5/1/2018-4/30/2022.** Integrated Approaches to High Assurance for Learning Based CPS, DARPA Assured Autonomy  
PI : Insup Lee, co-PI(s): George Pappas, R. Alur, O. Sokolsky, J. Weimer, N. Bezzo (Virginia)  
**Award Amount:** \$4,800,000
- 3/1/2017-2/28/2022. ARL CRA Distributed and Collaborative Intelligent Systems and Technology (DCIST)  
Principal Partner : University of Pennsylvania  
General Partners : Georgia Institute of Technology, MIT, U.C. Berkeley, USC, UCSD  
Penn PI : Vijay Kumar, co-PI(s) : George J. Pappas (Area Lead), A. Ribeiro, K. Daniilidis  
**Award Amount:** \$27,000,000.
- **9/1/2017-8/31/2020.** Low-Latency Communication for Wireless Autonomous Systems. Intel Science and Technology Center  
PI : Alejandro Ribeiro (Penn), George Pappas, Rahul Mangharam, Vijay Kumar  
**Award Amount:** \$1,200,000,
- **3/1/2017-3/31/2021.** Science of Resilience in Financial and Technological Networks, Rockefeller Foundation  
PI : George J. Pappas (Penn), Rakesh Vohra, Victor Preciado  
**Award Amount:** \$250,000.
- **1/1/2017-12/31/2020.** ECEDHA Research Community Planning Grant, National Science Foundation  
PI : George J. Pappas (Penn), Bill Sanders (UIUC), Steve Mc Laughlin (Georgia Tech), Sheila Hemami (Northeastern)  
**Award Amount:** \$99,150,
- **1/1/2017-12/31/2020.** Active Semantic Distributed Perception, Office of Naval Research  
PI : Kostas Daniilidis,, co-PI(s) : George. J. Pappas  
**Award Amount:** \$1,140,255.

**RECENT KEYNOTES**

- **July 2020.** Plenary Speaker, 39th Chinese Control Conference, Shenyang, China.
- **July 2020.** Semi-Plenary Speaker, 21st IFAC World Congress, Berlin, Germany.
- **April 2020.** Keynote, CyberPhysical Systems Week, CPS-IoT WEEK, Sydney.

**Participating CPSWEEK conferences: HSCC, ICCPS, IPSN, RTAS**

- **March 2019,** Plenary Speaker, 38th Benelux Meeting on Systems and Control, Belgium.

**BIOGRAPHICAL SKETCH**

Provide the following information for the Senior/key personnel and other significant contributors.  
Follow this format for each person. **DO NOT EXCEED FIVE PAGES.**

NAME: James H. Pikul

eRA COMMONS USER NAME (credential, e.g., agency login): PIKULJ

POSITION TITLE: Assistant Professor, Mechanical Engineering and Applied Mechanics, The University of Pennsylvania

**EDUCATION/TRAINING** (*Begin with baccalaureate or other initial professional education, such as nursing, include postdoctoral training and residency training if applicable. Add/delete rows as necessary.*)

INSTITUTION AND LOCATION	DEGREE (if applicable)	Completion Date MM/YYYY	FIELD OF STUDY
University of Illinois at Urbana-Champaign	PhD	2015	Mechanical Engineering
University of Illinois at Urbana-Champaign	MS	2011	Mechanical Engineering
University of Illinois at Urbana-Champaign	BS	2009	Mechanical Engineering

**A. Personal Statement**

I have the expertise, leadership, training, and motivation necessary to successfully mentor Olalekan Ogunmolu for his K99 fellowship. I am a mechanical engineer with expertise in materials engineering, micro and nanoscale fabrication, soft robotics, and electrochemistry. My group combines these expertise to enable new robotic capabilities. This is demonstrated by my recent publication in *Science*<sup>1</sup>, which presents a new physical approach for controlling the shape transformation of stretchable material surfaces, in an engineered system that provides reversible actuation, fast response, large forces, geometric and sequential control, and ease of fabrication. I also have expertise in electrochemistry, which I have used to improve the mobility of robots<sup>2</sup>, to make the world's most power dense batteries<sup>3</sup>, and realize the first room-temperature healing of metal<sup>4</sup>. I have also led many projects, including several \$1,000,000 plus projects sponsored by NSF and DARPA. I will use this expertise to mentor Olalekan in science, leadership, and management throughout his project.

1. James H. Pikul, Shuo Li, Hedan Bai, Roger T. Hanlon, Itai Cohen, Robert F. Shepherd, "Stretchable surfaces with programmable 3-D texture morphing for synthetic camouflaging skins", *Science*, vol. 358, pp. 210-214, October 18, 2017.
2. Cameron A. Aubin, Snehashis Choudhury, Rhiannon Jerch, Lynden A. Archer, James H. Pikul, Robert F. Shepherd, "Electrolytic Vascular Systems for Energy Dense Robots", *Nature*, 1, June, 2019.
3. James H. Pikul, Huigang Zhang, Jiung Cho, Paul V. Braun, and William P. King, "High power lithium ion micro batteries from interdigitated three-dimensional bicontinuous nanoporous electrodes", *Nature Communications*, vol. 4, pp. 1732, 2013
4. Zakaria Hsain, James H. Pikul, "Low-energy Room-temperature Healing of Cellular Metals", *Advanced Functional Materials*, pp. 1905631, August 2019.

## B. Positions and Honors

### Positions

2017 – Present	Assistant Professor	University of Pennsylvania
2015 – 2017	Postdoctoral associate	Cornell University

### Honors

- 2020 Moore Inventor Fellow through the Gordon and Betty Moore Foundation  
2019 Best Paper Award at The 19th International Conference on Micro and Nanotechnology for Power Generation and Energy Conversion Applications (PowerMEMS), Krakow, 2019  
2019 NSF CAREER award in ECCS - CCSS  
2019 Scialog Fellow through the Research Corporation for Science Advancement - Advanced Energy Storage  
2019 Office of Naval Research Young Investigator Award  
2013 Materials Research Society Gold Award

## C. Contributions to Science

### 1. Control and mobility of soft robotics

Technologies using soft, stretchable materials are increasingly important, yet we are unable to control how they stretch with much more sophistication than inflating balloons. Nature, however, demonstrates remarkable control of stretchable surfaces: for example, cephalopods can project hierarchical structures from their skin in milliseconds for a wide range of textural camouflage, run across the ocean floor, change color, and hydrojet at high speeds through the ocean. Inspired by nature, I have developed theoretical and experimental techniques that enable the design, fabrication, and control of soft robotics. I have pioneered shape control of soft, stretchable materials by prescribing strain in inflated and expanded 2-D surfaces. My combined theoretical and experimental work has led to state-of-the-art capabilities for controlling the shape of soft surfaces that deform into complex shapes. I have also demonstrated the use of flow battery chemistries to increase the energy density of machines, vehicles, and robots by adding energy storage functionality into existing fluidic actuators. This improves the energy density of the robot by more than 4X. I have received an NSF CAREER award for this work.

- A. James H. Pikul, Shuo Li, Hedan Bai, Roger T. Hanlon, Itai Cohen, Robert F. Shepherd, "Stretchable surfaces with programmable 3-D texture morphing for synthetic camouflaging skins", *Science*, vol. 358, pp. 210-214, October 18, 2017.
- B. Steven Ceron, Itai Cohen, Robert F. Shepherd, James H. Pikul, Cindy Harnett, "Fiber Embroidery of Self-Sensing Soft Actuators", *Biomimetics*, vol. 3, September 2018.
- C. Cameron A. Aubin, Snehashis Choudhury, Rhiannon Jerch, Lynden A. Archer, James H. Pikul, Robert F. Shepherd, "Electrolytic Vascular Systems for Energy Dense Robots", *Nature*, 1, June, 2019.
- D. T.J. Wallin, J.H. Pikul, S. Bodkhe, B.N. Peele, B.C. Mac Murray, D. Therriault, B.W. McEnerney, R.P. Dillon, E.P. Giannelis, R.F. Shepherd, "Click chemistry stereolithography for soft robots that self-heal", *Journal of Materials Chemistry B*, vol. 5, pp. 6249-6255, 2017.

### 2. Energy storage with increased energy and power

In my research group, we seek to realize new battery architectures that enhanced battery performance or enable entirely new functionality. Metal-air batteries offer higher energy densities than lithium ion batteries. We have recently expanded the architectural advantage of metal-air batteries by demonstrating the ability to electrochemically extract energy from external metal surfaces using a metal-air scavenger (MAS) composed of a hydrogel electrolyte connected to a cathode current collector. This new approach can power microelectronics and cm scale robotic devices that operate on or near metal surfaces. The effective energy density of the metal-air scavenger was 2.3 times greater than prior metal-air batteries and 12.7 times greater than commercial lithium-ion batteries. This work is being funded through an ONR-YIP. There is also increasing need for higher performance microbatteries due to the increased growth of internet-connected devices (125 billion by 2030) and micro-robotics. I have been a global leader in developing high performance microbatteries for the last 8

years, and my group is continuing to make significant strides in this area. My prior work showed that we could make microbatteries with the power density of supercapacitors, 1,000 times higher than the power density of commercial batteries. Current work in my lab is focused on three funded DARPA SHort-Range Independent Microrobotic Platforms projects. I am the PI on one and co-PI on the other two. The goal of these projects is to realize novel energy storage technologies for microrobots.

- A. Min Wang, Unnati Joshi, James H. Pikul, "Powering electronics by scavenging energy from external metals" *ACS Energy Letters*, 2020
- B. James H. Pikul, Paul V. Braun, William P. King, "Performance modeling and design of ultra-high power microbatteries", *Journal of the Electrochemical Society*, vol. 164.11, pp. E3122-E3131, 2017.
- C. Hailong Ning, James H. Pikul, Runyu Zhang, Xuejiao Li, Sheng Xu, Junjie Wang, John A. Rogers, William Paul King, and Paul V. Braun, " Holographic Patterning of High Performance on-chip 3D Lithium-ion Microbatteries", *Proceeding of the National Academy of Sciences*, vol. 112, no. 21, pp. 6573-6578, 2015.
- D. James H. Pikul, Huigang Zhang, Jiung Cho, Paul V. Braun, and William P. King, "High power lithium ion micro batteries from interdigitated three-dimensional bicontinuous nanoporous electrodes", *Nature Communications*, vol. 4, pp. 1732, 2013

### **3. Multifunctional Materials**

My lab's work on multifunctional materials is inspired by the complex functionalities in natural materials (like self-healing fractures in bone) and the incredible benefit similar functionalities would offer to engineered systems. We use modern engineering and design principles to realize new synthetic materials with mechanical and chemical properties not available in natural or man-made materials. In one project, we have combined new models of nanoscale self-assembly with electrochemical deposition to realize high-strength and light-weight metals. I recently published work showing that these materials (with 200-500 nm pore sizes) could achieve the strength of titanium and the density of water. My group has also demonstrated rapid, effective, low-energy, and room-temperature healing of metallic materials by using electrochemistry and polymer-coated cellular nickel to mimic the transport-mediated healing of bone. This is the first room temperature healing of metals since humans have first used metals 6,000 years ago.

- A. James H. Pikul, Sezer Özerinç, Burigede Liu, Runyu Zhang, Paul V. Braun, Vikram S. Deshpande, William P. King, " High strength metallic wood from nanostructured nickel inverse opal materials", *Scientific Reports*, 9.1, 2019.
- B. James H. Pikul, Paul V. Braun, and William P. King, "Micromechanical devices with controllable stiffness fabricated from regular 3D porous materials", *Journal of Micromechanics and Microengineering*, vol. 24, 105006, 2014
- C. Zakaria Hsain, James H. Pikul, "Low-energy Room-temperature Healing of Cellular Metals", *Advanced Functional Materials*, pp. 1905631, August 2019.

**D. Additional Information: Research Support and/or Scholastic Performance**

**Ongoing Research Support**

DARPA: PI

- “Electrochemical deposition of thick and continuous electrodes for high voltage and energy density lithium metal microbatteries”
  - Co-PI are Paul Braun (University of Illinois at Urbana-Champaign) and John Cook (Xerion Advanced Battery Corp.)
  - 03-01-2019 to 02-28-2022

Office of Naval Research Young Investigator Program: PI

- “Understanding electrochemically induced surface evolution and transport at metal-hydrogel interfaces for metal-air scavenger power sources”
  - 04-15-2019 to 04-14-2022

NSF: PI

- “EFRI C3 SoRo: 3-D surface control for object manipulation with stretchable Materials”
  - Co-PIs are Michael Posa, Mark Yim, Chris Santangelo (U. Mass – Amherst), Ryan Hayward (U. Mass – Amherst)
  - 01-01-2020 to 12-31-2023

NSF: PI

- “MRSEC: Surface Evolution of Dealloyed Mesoporous Metals for Oxygen Metals for Oxygen Reduction Catalysts in Metal-Air Battery and Fuel Cell Electrodes”
  - Co-PI are Eric Detsi (MSE) and Eric Stach (MSE)
  - 09-01-2018 to 08-31-2020

NSF CAREER: PI

- “CAREER: Power and information transmission kinetics in multifunctional electrolytic vascular systems”
  - 02-01-2020 to 01-31-2025

DARPA: co-PI

- “Integrated High Voltage Battery and Magnetic Conversion Micropower Systems for Efficient Power Delivery to Microbiotic Actuators”
  - PI is Mark Allen, Co-PI is Sue Bidstrup-Allen
  - 03-01-2019 to 02-28-2022

**Completed Research Support**

None

**Title:**

research expenses not to exceed \$30K -9,717 12,966

Title:

R00 Year 1-3 4/1/2023-3/31/2026												
Personnel	Role	Effort	Salary Yr 3	Salary Yr 4	Salary Yr 5	%Salary requested	YR3 (plus Ebs)	%Salary requested	YR4 (plus Ebs)	%Salary requested	YR5 (plus Ebs)	Total 3 year period
Lekan Molu	PI	100%	110,000	110,000	113,300	110,000	143,550	110,000	143,550	113,300	147,857	434,957
<b>Total Personnel</b>							<b>143,550</b>		<b>143,550</b>		<b>147,857</b>	<b>434,957</b>
<b>Equipment</b>												0
3D Printing Machine			6,500									0
<b>Travel</b>												
Conference & Travel		5,500	5,500	5,500								0
<b>Supplies</b>												0
												0
												0
<b>Other Expenses</b>												
Publication Expenses		4000	4000	4000								0
<b>Total Direct Costs</b>							<b>143,550</b>		<b>143,550</b>		<b>147,857</b>	<b>434,957</b>
<b>MTDC Base</b>							<b>143,550</b>		<b>143,550</b>		<b>147,857</b>	<b>434,957</b>
F&A Costs		61%					<b>87,566</b>		<b>87,566</b>		<b>90,192</b>	<b>265,323</b>
<b>Total Costs</b>		126000	119500	122800			<b>231,116</b>		<b>231,116</b>		<b>238,049</b>	<b>700,280</b>
							over/under		17,885		17,885	10,951

## Budget Justification

**Olalekan Ogunmolu, PhD, Principal Investigator, 12-month calendar year effort:** Dr. Ogunmolu is a control systems engineer and roboticist by training. He also has medical physics experience in the areas of treatment planning and patient head motion correction in cancer RT. Prior to joining the University of Pennsylvania in Philadelphia as a postdoctoral fellow, he was a visiting postdoctoral scholar at the University of Chicago's Pritzker School of Medicine. Dr. Ogunmolu has many years of experience in hardware design, software architecture, system synthesis, and project management. Dr. Ogunmolu will develop the pneumatic hardware, integrate it with the electronic controllers, as well as write the motion planning software for this project. He will frequently consult with his co-mentors in order to address the aims proposed in K99 aims I-III and the R00 aim. Finally, Dr. Ogunmolu will be responsible for overall supervision of this project and collaboration with other experiments and testing procedures.

### Mentored Phase, 2 years

Apart from salary support, many of the research-related costs of the project during the mentored phase will be subsidized by the research facilities and supplies already available in the labs of the mentors, Drs. Rodney Wiersma, James Pikul, and Kevin Turner.

#### Personnel: Olalekan Ogunmolu, PhD, Principal Investigator

A total of \$113,963 is required for salary support for Dr. Olalekan Ogunmolu during the mentored phase (2 years). Year 1: \$56,139; Year 2: 57,824.

#### Other Expenses

Postdoc health insurance is requested based on the University of Pennsylvania published rates for FY21. A total of \$15,834 is requested for Dr. Ogunmolu's postdoc health insurance for two years: \$7,800 in the first year and \$8,034 in the second year.

#### Equipment

- \$3,000 – Proportional Solenoid Valves (12 at \$250 each from Dakota Instruments) to regulate air flow in and out of the respective air bladders.
- \$1,240 – Venturi pumps (8 at \$155 each) to create reverse air flow out of the actuators as needed.
- \$7,500 – Universal laser cutting machine to precisely cut the fabrics used in reinforcing the actuators as well as other precision cutting tasks for the radiation-transparent and non-magnetic PVC foam encasement.

#### Supplies

\$11,176 for Y1 and Y2, for silicone materials, fabric, pressure transmitters, load cell and displacement sensors, hand-held corona device and other general-purpose lab materials.

#### Travel

\$5,000 per year for travel to scientific conferences for all project members.

#### Publications

\$4,000 per year is requested for open access publication in journals as results may be of potential interest to the general public.

### Independent Phase, 3 Years

#### Personnel: Olalekan Ogunmolu, PhD, Principal Investigator, 12-month calendar year effort

The total estimated salary for Dr. Ogunmolu in the three years of independent phase of the award is \$454,348.8. Fringe benefits have been estimated at 30% which is based on the university average for fringe benefits for current junior faculties at most tier-1 research institutions, but with an understanding that it may change based on the requirement that the institution where the independent position is secured will be responsible for a portion of the salary.

#### Other Expenses

Health insurance is requested based on the University of Pennsylvania published rates for FY21.

#### Equipment

\$6,500 – In the independent years, I will not have access to Dr. Wiersma's FDM 3D printer. Therefore, an FDM 3D Printer is requested to 3D print molds, and robot components.

#### Travel

\$5,500 per year is requested for travel to scientific conferences, adjusted for inflation from the K99 years.

#### Publications

\$4,000 per year is requested for open access publication in journals as results may be of potential interest to the general public.

## **Project Summary/Abstract**

Targeting dose to submillimeter or subdegree accuracy to tumors in a patient's target volume is crucial for successful tumor control. Currently, computed tomography (CT) images are employed in segmenting critical structures from organs-at-risk (OARs) in radiation therapy (RT). CT images however exhibit low delineation contrast for the soft tissues of brain and head-and-neck (H&N) lesions. Magnetic resonance imaging (MRI) techniques can be an effective means for diagnosing tumors owing to its clear-cut internal tissues imaging capabilities. Recently, researchers have started exploring a combination of MRI with linear accelerator RT to assure a better tumor control. The artifacts that arise from inadvertent patient head motion within the tubular structure of the MR are however a downside to realizing a better soft tissues' delineation; this hampers effective tumor control. The excursions of head motion outside a given confidence band is a problem that hinders the effectiveness of other radiation oncology beam targeting techniques such as stereotactic radiosurgery or highly conformal H&N RT.

Today in clinics, the state-of-the-art is to immobilize the patient's head with rigid Brown-Robert-Wells SRS head frames or thermoplastic face masks. Patients find these devices to be inconvenient, and highly invasive nature. Matter-of-factly, it causes poor patient compliance with prescribed radiation dose or poor clinical efficiencies. For patients with extreme cranial anatomy or prior surgical bone flaps, frame placement is impossible. Research aimed at eliminating the frame through thermoplastic face masks have resulted in less accuracy as mask flex can lead to systematic drift of up to 2-3 mm away from the intended target – owing to rotation about the fulcrum at the back of the skull. More so, mask-based immobilization accuracy is highly dependent on mask manufacturing quality, skill of the person applying the mask, shrinkage of the mask during treatment, and physical changes of the patients head due to swelling or weight. In my previous investigations, I have shown the effectiveness of soft robots at head motion correction up to submillimeter accuracy. Even so, Wiersma et al have demonstrated a frameless maskless robotic SRS system that can stabilize head motion to under 0.5mm/0.5deg for 99% of treatment time. In this sentiment, we hypothesize that a soft manipulator, actuated by compressed air, and adaptable to the confined space within the MR machine and under the MR coils can further help eliminate these motion artifacts that lower MR imaging quality and treatment efficacy in SRS scenarios. We will develop a motion-planning algorithm and construct a full-scale soft robot for a real-time patient head motion correction that is adaptable to MR machines and emerging MRI-linear accelerator treatment procedures. When this has been tested on phantoms human volunteers, we will validate its suitability on human trials at the University of Pennsylvania's radiation oncology clinic.

## **Project Narrative**

Accurate dose targeting to malignant cancers in radiation oncology requires clearly delineated and richly contrasted soft tissues within the human body so that the treatment examiner can clearly tell critical structures apart from organs-at-risk. Currently, CT images are used in this segmentation task which lack these delineation capability. This project will leverage the high-contrast that magnetic resonance scans provide with the non-magnetic and radio-transparent compliance that soft robots provide cranial position manipulation so as to assure better clinical outcomes for head and neck (H&N) as well as brain cancer treatments in maskless stereotactic radiosurgery. This will further accelerate the current maskless and frameless brain and H&N cancer research by making it more available to a wider population of patients.

## References

- [1] Raaymakers, B., Jürgenliemk-Schulz, I., Bol, G., Glitzner, M., Kotte, A., Van Asselen, B., De Boer, J., Bluemink, J., Hackett, S., Moerland, M., et al.: First patients treated with a 1.5 t mri-linac: clinical proof of concept of a high-precision, high-field mri guided radiotherapy treatment. *Physics in Medicine & Biology* **62**(23), L41 (2017)
- [2] Belcher, A.: Patient Motion Management with 6-DOF Robotics for Frameless and Maskless Stereotactic Radiosurgery. Ph.D. thesis, The University of Chicago (2017)
- [3] Herrmann, C., Ma, L., Schilling, K.: Model Predictive Control For Tumor Motion Compensation In Robot Assisted Radiotherapy. IFAC Proceedings Volumes **44**(1), 5968–5973 (2011)
- [4] Ostyn, M., Dwyer, T., Miller, M., King, P., Sacks, R., Cruikshank, R., Rosario, M., Martinez, D., Kim, S., Yeo, W.H.: An Electromechanical, Patient Positioning System For Head And Neck Radiotherapy. *Physics in Medicine & Biology* **62**(18), 7520 (2017)
- [5] Raaymakers, B., Lagendijk, J., Overweg, J., Kok, J., Raaijmakers, A., Kerkhof, E., Van der Put, R., Meijssing, I., Crijns, S., Benedosso, F., et al.: Integrating a 1.5 t mri scanner with a 6 mv accelerator: proof of concept. *Physics in Medicine & Biology* **54**(12), N229 (2009)
- [6] Mutic, S., Dempsey, J.F.: The viewray system: magnetic resonance-guided and controlled radiotherapy. In: Seminars in radiation oncology, vol. 24, pp. 196–199. Elsevier (2014)
- [7] Fallone, B.G.: The rotating biplanar linac–magnetic resonance imaging system. In: Seminars in radiation oncology, vol. 24, pp. 200–202. Elsevier (2014)
- [8] Keall, P., Barton, M., Crozier, S., et al.: Linac program, including contributors from ingham institute, illawarra cancer care centre, liverpool hospital. Stanford University, Universities of Newcastle, Queensland, Sydney, Western Sydney, and Wollongong. The Australian magnetic resonance imaging-linac program. *Semin Radiat Oncol* **24**(3), 203–206 (2014)
- [9] Lagendijk, J.J., Raaymakers, B.W., Raaijmakers, A.J., Overweg, J., Brown, K.J., Kerkhof, E.M., van der Put, R.W., Hårdemark, B., van Vulpen, M., van der Heide, U.A.: Mri/linac integration. *Radiotherapy and Oncology* **86**(1), 25–29 (2008)
- [10] Méndez Romero, A., Wunderink, W., Hussain, S.M., De Pooter, J.A., Heijmen, B.J., Nowak, P.C., Nuyttens, J.J., Brandwijk, R.P., Verhoef, C., Ijzermans, J.N., et al.: Stereotactic body radiation therapy for primary and metastatic liver tumors: a single institution phase i-ii study. *Acta oncologica* **45**(7), 831–837 (2006)
- [11] Xing, L., Lin, Z.X., Donaldson, S.S., Le, Q.T., Tate, D., Goffinet, D.R., Wolden, S., Ma, L., Boyer, A.L.: Dosimetric effects of patient displacement and collimator and gantry angle misalignment on intensity modulated radiation therapy. *Radiotherapy and Oncology* **56**(1), 97–108 (2000)
- [12] Chelvarajah, R., Leighton, B., Martin, L., Smith, W., Beldham-Collins, R.: Cranial immobilisationis there a better way? *Radiographer* **51**(1), 29–33 (2004)
- [13] Ogunmolu, Olalekan and Wiersma, Rodney: A Real-Time Patient Head Motion Correction Mechanism for MRI-Linac Systems. J.R. Cameron and J.R. Cunningham Young Investigator Symposium, AAPM/COMP Meeting, The International Journal of Medical Physics Research and Practice. (2020)
- [14] Keall, P.J., Mageras, G.S., Balter, J.M., Emery, R.S., Forster, K.M., Jiang, S.B., Kapatoes, J.M., Low, D.A., Murphy, M.J., Murray, B.R., et al.: The Management of Respiratory Motion in Radiation Oncology Report of AAPM Task Group 76 A. *Medical physics* **33**(10), 3874–3900 (2006)
- [15] Takakura, T., Mizowaki, T., Nakata, M., Yano, S., Fujimoto, T., Miyabe, Y., Nakamura, M., Hiraoka, M.: The geometric accuracy of frameless stereotactic radiosurgery using a 6d robotic couch system. *Physics in Medicine & Biology* **55**(1), 1 (2009)
- [16] Liu, X., Belcher, A.H., Grelewicz, Z., Wiersma, R.D.: Robotic stage for head motion correction in stereotactic radiosurgery. In: 2015 American Control Conference (ACC), pp. 5776–5781. IEEE (2015)
- [17] Liu, X., Wiersma, R.D.: Optimization based trajectory planning for real-time 6DoF robotic patient motion compensation systems. *PloS one* **14**(1), e0210,385 (2019)
- [18] McNeil, D.G.: M.R.I.’s Strong Magnets Cited in Accidents. *The New York Times* pp. A-1 (2005). URL <https://www.nytimes.com/2005/08/19/health/mris-strong-magnets-cited-in-accidents.html>

- [19] Ogunmolu, O.P., Gu, X., Jiang, S., Gans, N.R.: A Real-Time, Soft Robotic Patient Positioning System for Maskless Head and Neck Cancer Radiotherapy: An Initial Investigation. In: Automation Science and Engineering (CASE), 2015 IEEE International Conference on, Gothenburg, Sweden, pp. 1539–1545. IEEE (2015)
- [20] Ogunmolu, O., Kulkarni, A., Tadesse, Y., Gu, X., Jiang, S., Gans, N.: Soft-NeuroAdapt: A 3-DOF Neuro-Adaptive Patient Pose Correction System for Frameless and Maskless Cancer Radiotherapy. In: IEEE/RSJ International Conference on Intelligent Robots and Systems (IROS), Vancouver, BC, CA, pp. 3661–3668. IEEE (2017)
- [21] Ogunmolu, O., Gans, N., Jiang, S., Gu, X.: An Image-Guided Soft Robotic Patient Positioning System for Maskless Head And Neck Cancer Radiotherapy: A Proof of Concept Study. *Medical Physics: The International Journal of Medical Physics Research and Practice*, Presented at the AAPM Meeting, Anaheim, CA **42**, 3266–3266 (2015)
- [22] Ogunmolu, O.P., Gu, X., Jiang, S., Gans, N.R.: Vision-based Control of a Soft Robot for Maskless Head and Neck Cancer Radiotherapy. In: Automation Science and Engineering (CASE), 2016 IEEE International Conference on, Fort Worth, Texas, pp. 180–187. IEEE (2016)
- [23] Ljung, L.: System Identification Theory for the User, second edn. Prentice Hall, Upper Saddle River, NJ, USA. (1999)
- [24] Ogunmolu, O., Liu, X., Gans, N., Wiersma, R.: Mechanism and Constitutive Model of a Continuum Robot for Head and Neck Cancer Radiotherapy. In: IEEE International Conference on Robotics and Automation (ICRA), Paris, France (2020)
- [25] Ishizaka, S., Moromugi, S., Kobayashi, M., Kajihara, H., Koga, K., Sugahara, H., Ishimatsu, T., Kurata, S., Kirkness, J.P., Oi, K., et al.: A remote-controlled airbag device can improve upper airway collapsibility by producing head elevation with jaw closure in normal subjects under propofol anesthesia. *IEEE journal of translational engineering in health and medicine* **2**, 1–9 (2014)
- [26] Baskar, R., Lee, K.A., Yeo, R., Yeoh, K.W.: Cancer and radiation therapy: current advances and future directions. *International journal of medical sciences* **9**(3), 193 (2012)
- [27] Ogunmolu, O.P.: A Multi-DOF Soft Robot Mechanism for Patient Motion Correction and Beam Orientation Selection in Cancer Radiation Therapy. Ph.D. thesis, The University of Texas at Dallas; UT Southwestern Medical Center (2019)
- [28] Ogunmolu, O.: Kinematics and Kinetics of an In-Parallel-Actuated Soft Robot Manipulator (2020). URL <https://scriptedonachip.com/downloads/Papers/jmr20.pdf>
- [29] Hanlon, R.T., Messenger, J.B.: Adaptive coloration in young cuttlefish (*sepia officinalis* l.): the morphology and development of body patterns and their relation to behaviour. *Philosophical Transactions of the Royal Society of London. B, Biological Sciences* **320**(1200), 437–487 (1988)
- [30] Hanlon, R.T., Messenger, J.B.: Cephalopod behaviour. Cambridge University Press (2018)
- [31] Pikul, J., Cohen, I., Shepherd, R.: Stretchable surfaces with programmable texture (2019). US Patent App. 16/161,029
- [32] Walker, L.B., Harris, E., Pontius, U.: Center of gravity of human head and neck. In: ANATOMICAL RECORD, vol. 169, p. 448. WILEY-LISS DIV JOHN WILEY & SONS INC, 605 THIRD AVE, NEW YORK, NY 10158-0012 (1971)
- [33] Walker, L.B., Harris, E.H., Pontius, U.R.: Mass, volume, center of mass, and mass moment of inertia of head and head and neck of human body. Tech. rep., SAE Technical Paper (1973)
- [34] Clauser, C.E., McConville, J.T., Young, J.W.: Weight, volume, and center of mass of segments of the human body. Tech. rep., Antioch Coll Yellow Springs OH (1969)
- [35] Mooney, M.: A theory of large elastic deformation. *Journal of applied physics* **11**(9), 582–592 (1940)
- [36] Rivlin, R.S., Saunders, D.W.: Large Elastic Deformations of Isotropic Materials. VII. Experiments on the Deformation of Rubber. *Philosophical Transactions of the Royal Society A: Mathematical, Physical and Engineering Sciences* **243**(865), 251–288 (1950). DOI 10.1098/rsta.1951.0004
- [37] Xu, P.A., Mishra, A., Bai, H., Aubin, C., Zullo, L., Shepherd, R.: Optical lace for synthetic afferent neural networks. *Science robotics* **4**(34), eaaw6304 (2019)
- [38] Zhao, H., OBrien, K., Li, S., Shepherd, R.F.: Optoelectronically innervated soft prosthetic hand via stretchable optical waveguides. *Science Robotics* **1**(1), eaai7529 (2016)

- [39] Muth, J.T., Vogt, D.M., Truby, R.L., Mengüç, Y., Kolesky, D.B., Wood, R.J., Lewis, J.A.: Embedded 3d printing of strain sensors within highly stretchable elastomers. *Advanced Materials* **26**(36), 6307–6312 (2014)
- [40] Wehner, M., Truby, R.L., Fitzgerald, D.J., Mosadegh, B., Whitesides, G.M., Lewis, J.A., Wood, R.J.: An integrated design and fabrication strategy for entirely soft, autonomous robots. *Nature* **536**(7617), 451–455 (2016)
- [41] Keplinger, C., Li, T., Baumgartner, R., Suo, Z., Bauer, S.: Harnessing snap-through instability in soft dielectrics to achieve giant voltage-triggered deformation. *Soft Matter* **8**(2), 285–288 (2012)
- [42] Anderson, I.A., Gisby, T.A., McKay, T.G., OBrien, B.M., Calius, E.P.: Multi-functional dielectric elastomer artificial muscles for soft and smart machines. *Journal of applied physics* **112**(4), 041,101 (2012)
- [43] Firouzeh, A., Higashisaka, T., Nagato, K., Cho, K., Paik, J.: Stretchable kirigami components for composite meso-scale robots. *IEEE Robotics and Automation Letters* **5**(2), 1883–1890 (2020)
- [44] Sedal, A., Memar, A.H., Liu, T., Menguc, Y., Corson, N.: Design of deployable soft robots through plastic deformation of kirigami structures. *IEEE Robotics and Automation Letters* (2020)
- [45] Truby, R.L., Della Santina, C., Rus, D.: Distributed proprioception of 3d configuration in soft, sensorized robots via deep learning. *IEEE Robotics and Automation Letters* (2020)
- [46] Haubert, K., Drier, T., Beebe, D.: Pdms bonding by means of a portable, low-cost corona system. *Lab on a Chip* **6**(12), 1548–1549 (2006)
- [47] Ogunmolu, O., Folkerts, M., Nguyen, D., Gans, N., Jiang, S.: Deep BOO! Automating Beam Orientation Optimization in Intensity Modulated Radiation Therapy. In: *Algorithmic Foundations of Robotics, XIII Workshop*, Merida, Mexico. Published in Springer’s Proceedings in Advanced Robotics (SPAR) book (2018)
- [48] Ogunmolu, O., Gu, X., Jiang, S., Gans, N.: Nonlinear systems identification using deep dynamic neural networks. arXiv preprint arXiv:1610.01439 (2016)
- [49] Ogunmolu, O., Gans, N., Summers, T.: Minimax Iterative Dynamic Game : Application to Nonlinear Robot Control. *IEEE International Conference on Intelligent Robots and Systems* (2018)
- [50] Sadeghnejad Barkousaraie, Azar and Ogunmolu, Olalekan and Jiang, Steve and Nguyen, Dan: A Fast Deep Learning Approach for Beam Orientation Selection Using Supervised Learning with Column Generation on IMRT Prostate Cancer Patients. *Medical Physics, American Association of Physicists in Medicine* (2019)
- [51] Ogunmolu, O., Sadeghnejad Barkousaraie, A., Dan, N., Gans, N., Jiang, S.: Deep Learning Neural Network for Beam Orientation Optimization. In: *International Conference on the use of Computers in Radiation Therapy XVI* (2019)
- [52] Adler, J.R., Cox, R.S.: Preliminary clinical experience with the cyberknife: Image-guided stereotactic radiosurgery. In: *Radio-surgery 1995*, vol. 1, pp. 316–326. Karger Publishers (1996)
- [53] Ogunmolu, Olalekan, Liu, Xinmin and Wiersma, Rodney: A Motion-Planner for Robot Head Motion Correction in Stereotactic Radiosurgery. *AAPM/COMP Meeting, The International Journal of Medical Physics Research and Practice*. (2020)
- [54] LaValle, S.M.: Planning algorithms. Cambridge university press (2006)
- [55] Ioannou, P., Fidan, B.: Adaptive control tutorial. SIAM (2006)
- [56] Lavretsky, E., Wise, K.: Robust Adaptive Control with Aerospace Applications. Springer (2005)
- [57] Freeman, R.A., Kokotovic, P.V.: Inverse optimality in robust stabilization. *SIAM journal on control and optimization* **34**(4), 1365–1391 (1996)
- [58] Lozano-Perez, T.: Spatial planning: A configuration space approach. In: *Autonomous robot vehicles*, pp. 259–271. Springer (1990)
- [59] Hunt, K.H.: Kinematic Geometry of Mechanisms. Oxford University Press (1977)
- [60] Kingston, Z., Moll, M., Kavraki, L.E.: Exploring implicit spaces for constrained sampling-based planning. *The International Journal of Robotics Research* **38**(10-11), 1151–1178 (2019)
- [61] Kalman, R.E., Bertram, J.E.: Control system analysis and design via the second method of lyapunov: Icontinuous-time systems (1960)

- [62] Hricak, H., Amparo, E.: Body mri: alleviation of claustrophobia by prone positioning. *Radiology* **152**(3), 819–819 (1984)
- [63] Khansari-Zadeh, S.M., Billard, A.: Learning control Lyapunov function to ensure stability of dynamical system-based robot reaching motions. *Robotics and Autonomous Systems* **62**(6), 752–765 (2014)
- [64] Ogunmolu, O., Thompson, R.S., Dattari, R.P.: Learning Control Lyapunov Functions in Python. <https://github.com/lakehanne/lyapunovearner> (2020). Accessed February 10, 2020
- [65] Hunt, K.H.: Structural Kinematics of In- Parallel-Actuated Robot-Arms **105**(December 1983), 705–712 (1983)
- [66] Merlet, J.: Parallel robots. Springer (2015). DOI 10.1007/978-1-4471-4670-4\_99
- [67] Hopkins, J.B.: Design of Flexure-based Motion Stages for Mechatronic Systems via Freedom, Actuation and Constraint Topologies (FACT). Ph.D. thesis, Massachusetts Institute of Technology (2010)
- [68] Hopkins, J.B., Rivera, J., Kim, C., Krishnan, G.: Synthesis and Analysis of Soft Parallel Robots Comprised of Active Constraints. *Journal of Mechanisms and Robotics* (2015)
- [69] Spivak, M.: A Comprehensive Introduction to Differential Geometry. Vol. V. Berkeley: Publish or Perish. Inc. XI (1979)
- [70] Treloar, L.R.G.: The physics of rubber elasticity. Oxford University Press, USA (1975)
- [71] Truesdell, C.: A First Course in Rational Mechanics, vol. 1. Academic Press, Inc. (1997)
- [72] Faure, F., Duriez, C., Delingette, H., Allard, J., Gilles, B., Marchesseau, S., Talbot, H., Courtecuisse, H., Bousquet, G., Peterlik, I., Cotin, S.: SOFA: A Multi-Model Framework for Interactive Physical Simulation. In: Y. Payan (ed.) Soft Tissue Biomechanical Modeling for Computer Assisted Surgery, *Studies in Mechanobiology, Tissue Engineering and Biomaterials*, vol. 11, pp. 283–321. Springer (2012). DOI 10.1007/8415\\_2012\\_125

# **Institutional Environment**

## ***Institutional Intellectual Environment***

The University of Pennsylvania offers an ideal setting to work at the intersection of soft matter, mechanism design, robotics, control systems and radiation oncology. My sponsor, Rodney Wiersma, is the director of the Physics Research Program in the Department of Radiation Oncology at the University of Pennsylvania. We work on hardware and real-world translational clinical problems that intersect at the interface of control systems, robotics and radiation therapy. Our lab's robotics research goal is to replace current stereotactic radiosurgery methods that have therapeutic drawbacks and are highly invasive to patients with a real-time 6 degree of freedom (6DoF) patient head motion tracking and active robot-based control systems to continuously correct patient head motion during treatment. In 2012, Dr. Wiersma was awarded a 4 year Research Scholar Grant (RSG) from the American Cancer Society (ACS) for this research and he has since established the feasibility of the approach. Our lab is in the University of Pennsylvania school of medicine, which consistently ranks as one of the top four medical school in the United States. The world-class radiation therapy facilities in the medical school, as well as world-class faculties, students, postdocs and staff that I can learn from make Penn Medicine the ideal place to carry out. What is even more unique about the University of Pennsylvania is its world-class engineering program: throughout its history, Penn Engineering has led cutting-edge research in autonomous robots, computer vision, mechanobiology, and the physics of cancer. Its excellent faculties in the areas of expertise needed to successfully complete this research present an opportunity to learn from the best minds in the field and create a truly world-class product that has a transformational clinical potential that would stand the test of time.

## ***Institutional commitment to training***

The University of Pennsylvania was the first institution in the country to recognize the need for formal postdoctoral training and created the Biomedical Postdoctoral Program (BPP). The school of medicine has the largest cohorts of postdocs anywhere in the United States (1200 postdocs). BPP supports training programs in laboratory management, scientific and grant writing, scientific presentation skills and responsible conduct of research. In addition, BPP partners with the Penn Career Services office to offer one-on-one career counseling and resume critiques as well as seminars in networking, negotiation skills, navigating the academic job search process and the "Faculty Conversations" seminar series which explores aspects of the early academic career stage. The school of engineering has rapid prototyping labs (RPL), additive manufacturing labs and world class mechanical manufacturing machines such as lathes that are available to all university researchers who are working on an innovative technology. In addition, the University of Pennsylvania is one of the few institutions of higher learning in the United States with an entity that links the intellectual and entrepreneurial initiatives necessary for advancing knowledge and generating economic development (called Pennovation Works). I will leverage all these rich resources available to me while I am executing the mentored phase of this research to assure a timely and effective execution of my aims.

## ***Access to material resources for training***

My sponsor's lab is located in the John Morgan Building. In addition to a designated desk and bench space for my work, the lab houses an FDM 3D printer, auxiliary electronics and soft matter fabrication supplies. My mentor will provide me with the medical physics training needed to fulfill the radiation oncological clinical trials proposed in this project. Working closely with my co-mentors in the school of Engineering, I will have access to the tension testing, laser-cutting and lathe machines I would need in the hardware fabrication. Many additional instrumentation and training resources are available from core facilities located on campus; while none of these are required for my proposed project, they may be necessary for alternative approaches and offer opportunities for further training in follow-up studies to my proposal.

# Candidate Information and Goals for Career Development

## ***Candidate's Background***

I am an interdisciplinary researcher who combines the scientific elegance of machine learning and control theory with the practical impact of modern robotics to create technological solutions that improve healthcare delivery for cancer patients.

### ***Predoctoral Research***

My first major scientific project was my undergraduate thesis when I worked on the single fractional parentage coefficients in the sd-shell nuclei under the mentorship of famed Nigerian nuclear physicist, Ademola Amusa. This project exposed me to the art of peer review, piquing existing knowledge in a subject from what other people have done by gleaning scholastic literature, understanding the breadth and depth of the subject matter, finding inconsistencies between existing claims and observed results; reimagining a whole new way to solve an old problem, or finding a new problem and solving it with new tools thereunto. This project stretched my intellect as well as broadened my view about research – that it is essentially a project that usually spans many fields and requires being skilled at more than one area in order to be able to successfully execute. As calculating the single-particle and many-particle angular momentum of wavefunctions for s- and d-configurations in the sd-shell proved tedious, I had to automate my calculations by writing codes in C++ and Matlab. After three months of consultations with my advisor, him directing me to books and research papers, and my continual intellectual probing, I ended up solving for all the coefficients of fractional parentage using the Clebsch-Gordon coefficients for the  $d^2$ ,  $d^3$  and  $d^4$  configurations. I learned the importance of consistency, hardwork and constant questioning of facts. The seeds of research excellence were just beginning to germinate.

I would go on to study for a masters degree in Control systems at the University of Sheffield where I specialized in robotics under the mentorship of Tony Dodd. I fiddled with mobile robots, designed vision-based algorithms for quadcopter flights, and participated in unmanned aerial vehicle navigation student competitions in Europe. In 2013, our university team came up third in Eindhoven when we participated in the UAV racing project. Among other things, I was also part of the Engineers without Borders where we built low-cost wind-turbine for the Heeley farm in Sheffield, England as well as designed a robotic prosthetic arm for a child suffering from epilepsy – these two projects made our society earn the society of the year award from our University. In the second year of my PhD (I do not count 2016 to be a PhD year since I was out in industry).

### ***Doctoral Research***

Armed by these hardware and software design skills as well as having a firm grasp of the research process, I decided to enroll at the University of Texas at Dallas where I would collaborate with radiation oncology researchers and medical physicists at the University of Texas Southwestern Medical Center in building soft robots for the real-time patient head motion correction in radiation therapy (RT) treatment procedures. I found the opportunity to develop a technology that would have a positive impact on real-world patients to be enticing and this project resulted in three first-authored publications at major avenues for disseminating robotics and automation research. In the course of time, my UT Southwestern advisor (Steve Jiang) was impressed by my artificial intelligence (AI) automation and software skills that he requested for me to come join his lab permanently for the rest of the duration of my PhD. There I continued to work on other radiation oncology problems such as building a robust database of clinical dose based on past doctor's prescriptions for anonymized patients to be used by our research team for RT treatment planning studies; developing an automated framework for solving the non-convex beam orientation optimization problem in RT; as well as assisting other postdocs and graduate students in the lab. Based on my dose calculation development work, up to ten top medical physics and robotics<sup>1</sup> journal publications have resulted from this research group. Of those, I am a first-author and a co-author on those research papers. In addition, many scientific dissemination were produced at top conferences such as the American Association of Physicists in Medicine's annual meetings or IEEE robotics and automation top conferences such as the International Conference on Robotics and Automation (ICRA) or the Intelligent Robots and Systems (IROS). In the last year of my doctoral studies, my various research outputs culminated in various invited talks at top Universities and top robotics research organizations in the United States such as Stanford's Department of Energy Resources, the University of Chicago's department of radiation and cellular oncology or Open Robotics in Mountain View (the largest open-source for robotics foundation in the world). After graduating in 2019, I decided to join Dr. Wiersma's laboratory at the University of Chicago in order to continue honing my discipline expertise at the interface of robotics, control systems, medical physics/radiation oncology and largely biomedical science.

### ***Postdoctoral Research***

I am currently a postdoctoral researcher at the University of Pennsylvania's School of Medicine and I was previously a visiting postdoctoral scholar at the University of Chicago's School of Medicine. In my postdoctoral research duties, I work on problems spanning conceptualization of new hardware and software tools for improving the *treatment planning* process in *cancer radiation therapy*. My work has made meaningful impact in disciplines within and outside medicine, with citations from government and highered learning research institutions across the globe. Example institutions that have used my work include the National Aeronautics and Space Agency's Jet Propulsion Laboratory (NASA JPL), the 6th R&D institute of South Korea's Agency for Defense Development, Uber AI Labs, and the Chinese Academy of Sciences among others.

<sup>1</sup>My work was presented at the 13<sup>th</sup> algorithms for robotics workshop in 2018 and subsequently published in the Springer's Proceedings in Advanced Robotics book in 2019.

Since Starting my postdoc in the Wiersma group, both at UChicago and UPenn, I have straddled working on perfecting the motion-planning algorithm on the 6-6 Stewart-Gough platform, phasing out the buggy codebase for motion-compensation to a modular and simplified python code, as well as started building a full-fledged 6-DoF real-time soft robot motion compensator in RT treatment procedures as well as the emerging magnetic resonance imaging (MRI)-linear accelerator(LINAC) RT technologies. Since joining Dr. Wiersma's lab last Fall, my work has resulted in two first-authored publications at the 2020 joint annual meeting of the AAPM and COMP – one of these works, based on the soft robot mechanism for MRI-LINAC being proposed herein was selected for a presentation at the prestigious J.R. Cameron-J.R. Cunningham symposium. Another paper was accepted and recently presented at 2020's ICRA.

My next research goal is to develop a comprehensive motion planning framework for both of our lab's robot platforms for head motion correction. Leveraging preliminary work from the Kavraki lab on exploring implicit spaces in constrained sampling-based motion planning, I want to leverage a robust control Lyapunov function scheme in ensuring the stability and manifold-constraints' satisfaction of feasible collision-free paths during head motion correction in RT or emerging MRI-LINAC RT techniques. Afterwards, I will incorporate this motion planner on the physical build of my soft robot mechanism as well as Dr. Wiersma's Stewart-Gough robot.

### ***Career Goals and Objectives***

This year alone, it is projected that 1,762,450 new cases of cancer will be diagnosed, and 606,880 people will die from the disease. This constitutes a national expenditure of \$147.3 billion or 4.2% of overall healthcare spending per 2017 budget. Along with the excellent researchers that I collaborate with at Penn Medicine and Penn Engineering, I am working on the next stages of deploying these robots on real-world cancer patients to help doctors, medical physicists, dosimetrists and lab clinicians better manage cancer treatments. I am also interested in making the application of my control and robotics technologies pervasive in consumer robotics and the internet of things (IoT) industry as my research career progresses.

### ***Training Objectives***

In order to accomplish my long-term career and research goals I require 2 more years of mentored research for the following reasons. While a doctoral student, I worked between three projects, namely (i) the development of the soft robot mechanism with my primary doctoral thesis advisor; (ii) guaranteeing the robustness of deep reinforcement learning policies with my UT Dallas co-advisor, Dr. Tyler Summers; and (iii) improving the solve time of the non-convex classical beam orientation optimization problem in intensity modulated radiation therapy (IMRT) – with my UT Southwestern advisor, Dr. Steve Jiang. These projects, while exciting to work on in their own rights, left me stretched too thin that my contributions to science was not as impactful as I would like it to be. I produced top-scholastic papers at major high-impact conference venues but had little time to turn my work into world-class journals. To properly put things in perspective, I have only spent two years on this soft robot project, which has not been long enough to establish research independence as well as make me competitive on the job market. I need to learn from discipline experts such as Dr. Pikul and Dr. Turner (both are on my co-mentoring team) so I can demonstrate further novel contributions to soft robot sensing, modeling and control. I will also be learning a great deal from Dr. Pappas, who specializes in control theory and machine learning, in synthesizing the potential of these two fields in my robot designs and scientific inquiries. I want to spend two more years at Penn because these assembled team of excellent mentors would be invaluable and critical for further honing my intellectual curiosity and in me establishing an independent career.

### ***Mentored Phase Objectives***

**Firstly**, I want to scale my erstwhile developed soft robots and algorithms up to full six degree of freedom-capable motion for complete head-motion compensation that is reliable and repeatable in clinical experiments using real human subjects. In the mentored phase of this award, I will work on the motion planning algorithm that is safety-aware and is suitable for executing optimal collision-free paths between head motion transition modes such that manipulating the patient's head does not expose normal brain tissues to high radiation doses *i.e.* the patient's head motion in the robot's complete workspace must be *collision-free* and must satisfy manipulation mode constraints. Realizing smooth head transitions in space requires going from one state space mode to another so that the planner must find a sequence of single-mode motions and valid transitions between modes that realize this multi-modal motion manipulation. For geometric manipulation problems under manifold constraints such as the one proposed here, the general approach in robotics is to use trajectory optimization or sampling-based planning schemes. I will use an hierarchical multi-planning system that takes cues from a discrete "lead" for biasing search into robustly stable and optimal mode transitions. Stability will be assured by generating exponentially stable paths in the underlying dynamic system. Leveraging online search protocols, we will bias search for robustly optimal and feasible paths to a sequence of modes that yield a smooth representation of head motion. This would fulfill my aim II in the K99 years. **Secondly**, to fulfill my K99 aim 1, I will develop a distributively-innervated, non-magnetic, and radiation-transparent soft actuator. This aim will scale my previous soft actuator designs to a fully parallel soft robot capable of providing head manipulation along 6 DoFs and will be compatible with pre-existing LINACs. The actuators will be fiber-reinforced to constrain deformation along specific Eulerian directions in order to simplify control. Made entirely out of radio-transparent and non-metallic parts, this Gen 2.0 design will be adaptable under MR coils and the large tubular MR magnets and hence suitable for patient head motion compensation in emerging MRI-LINAC treatment procedures. **Lastly**, I will synthesize the actuators and motion planning in one motion-correction mechanism, adaptable under MR coils and in RT treatment protocols (as outlined in my K99 Aim III). In my independent years, I will recruit human volunteers and test the motion-planning algorithm and soft robot mechanism in real-time, first on phantoms and then on healthy human volunteers, in an MR machine as well as RT treatment machines to ascertain its effectiveness at real-time head motion compensation. When the veracity of this

mechanism is proven, I will then conduct a clinical trial on 20 whole brain patients where validation of this system will be determined by a statistical endpoint. Success will be that a 6D intracranial target is  $\leq 0.5\text{mm}$  and  $\leq 0.5^\circ$  for greater than 95% of the treatment time. Upon successful completion and novel use in maskless MRI-LINAC systems, this project will demonstrate that soft robotic SRS is ready for widespread clinical deployment.

#### Independent Phase Objectives

This pathway to independence research would advance my long-term career objectives which is ***to transition into an independent investigator role***, i.e. a tenured principal investigator role at an R1 research institution, where I can continue to solve problems in emerging medical robotics fields such as hybrid control and cyber physical systems research that has a clear-cut clinical effect on real-world patients. This proposed research will be the foundation of my future research funding. As soon as I accept a tenure-track position, I plan to apply for the NSF CAREER award, NIH New Innovator Award and Pew Biomedical Scholars Award. This will prepare me for my first R01 grant submission to the national cancer institute.

As I am currently a non-tenured faculty at Brandeis University graduate school of professional education where I teach and mentor masters students in robot autonomy, robot kinematics and dynamics, I have found this role to be fulfilling and stimulating in my career path as it enables me in rediscovering established concepts and imparting my knowledge to the next generation of bio-roboticists. My goal is that after the mentored phase of the K99 award, I would find myself in a suitable research-intensive location where I can continue to direct and lead important biomedical scientific research discoveries as well as continue to train the next generation of applied roboticists who will make important contributions to our research enterprise over the coming decades.

#### ***Training Activities Plan During Award Period***

I have outlined a training plan to accomplish my career goals and gain the necessary skills to be an effective and independent research investigator, teacher, and mentor as an assistant professor at a research-intensive university. Additional coursework, meeting participation, and consultation with my mentorship committee will enhance my training experience. A mentored job search is also a part of my training plan, which will be critical to my future success in securing a faculty position. All of this are itemized in the chart below.

# Project Training Activities

ACTIVITY	Modality	Specific Activities	ACTUAL START	ACTUAL DURATION	PERIODS				
					Y1	Y2	Y3	Y4	Y5
<b>Motion-planning synthesis for soft robot</b>	Seminars	Penn GRASP Lab Seminar Series	2020	2Y	X	X			
Extend knowledge of manifold constraints in implicit places to motion planning in soft robotics		Penn IME Seminars and Events			X	X			
Prove stability analysis of motion planner for soft robot-head system using the inverse stability from robust planning paradigm	Coursework	Motion Planning	2021	0.5 Y		X			
Apply these results to K99 Aim I of Research Strategy	Training	Mentor: Weekly Meeting	2020	2Y	X	X			
		Co-Mentors: Monthly/Quaterly	2020	2Y	X	X			
<b>Continuum-Mechanical Model and Actuators Construction</b>	Seminars	Penn Laboratory for Research on the Structure of Matter (LRSM) Seminars and Lectures	2020	2Y	X	X			
Receive training in continuum mechanics and soft matter fabrication technologies		Penn XRT Invited Speaker Seminar Series			X	X			
Conduct research specified in Aims II and III of K99 research strategy	Coursework	MEAM 514: Design for Manufacturability	2020	0.5 Y	X		X		
		MEAM 630: Advanced Continuum Mechanics			0.5 Y				
Apply these results to K99 Aim II and III of Research Strategy	Training	Mentor: Weekly Meeting	2020	2Y		X			
		Co-Mentors: Monthly/Quaterly	2020	2Y	X	X			
<b>Career Development</b>	Seminars	Penn Laboratory for Research on the Structure of Matter (LRSM) Seminars and Lectures	2020	2Y	x	x			

ACTIVITY	Modality	Specific Activities	ACTUAL START	ACTUAL DURATION	PERIODS				
					Y1	Y2	Y3	Y4	Y5
Effective communication skills	Coursework	Penn XRT Invited Speaker Seminar Series	2020	2Y	X	X			
		Courses in teaching/speaking	2020	0.5 Y	X	X	X		
		Courses in leadership/people management		0.5 Y	X	X	X	X	
		Manuscripts and grants-writing	2020	2Y	X	X	X	X	
		Serve as associate editor for robotics/control/medical physics journals and top conferences	2020	2Y	X	X	X	X	

## Specific Aims

Integrating magnetic resonance imaging (MRI) functionality with radiation therapy (RT) linear accelerator (LINAC) can better render the visualization of the soft tissues of lesions and surrounding healthy organs-at-risks (OARs) during cancer RT treatment planning and procedures. This is because MR scans, in contrast to the prevalent computed tomography (CT) scans used in clinics today, provide a richly contrasted image of internal body tissues. More importantly, MRI-LINAC integration can be done in an unrivaled, online, and real-time fashion to aid a more precise radiation dose delivery in RT [1]. However, the quality of MR scans are limited by head motion artifacts. Given the consistency of head motion requirement for proper beam targeting in stereotactic radiosurgery (SRS) and highly conformal head-and-neck (H&N) RT, rigid head frames or thermoplastic face masks are currently clinically used as static head immobilizers. However, frames are uncomfortable and highly invasive – causing poor patient compliance and clinical inefficacy; and masks reduce dose targeting accuracy – since mask flex can lead to drifts of up to 6 mm from an intended target. Robot mechanisms for real-time head motion correction that have been investigated are made out of linear actuators and rigid metallic components which are incompatible with MR [2–4]. During my PhD, I used soft manipulators for head motion correction in RT treatment planning in lower task space dimensions. Here, we propose a novel non-magnetic and radiation-transparent soft robot for automating the online, real-time patient head motion correction in emerging MRI-linear accelerator (LINAC) RT treatment procedures. Our team, comprised of material mechanics, medical physics, control systems and soft matter experts, will address these issues via the following specific aims:

### K99 Aim I: To Develop a Distributively-Innervated, Non-magnetic, and Radiation-Transparent Soft Actuator.

My preliminary soft manipulator designs have been used to control H&N motion in RT for up to 3 DoFs. This aim will scale my previous designs to a fully parallel soft robot capable of providing head manipulation along 6 DoFs and will be integrable with pre-existing LINACs. The actuators will be fiber-reinforced to constrain deformation along specific Eulerian directions in order to simplify control. Made entirely out of radio-transparent and non-metallic parts, this Gen 2.0 design will be adaptable under MR coils and the large tubular MR magnets and hence suitable for patient head motion compensation in emerging MRI-LINAC treatment procedures. A hierarchical sensing and control scheme is proposed: the soft actuators will deform in a manner similar to the fast activation ( $\leq 2\text{secs}$ ) of, for example, the papillae of the octopus, and will have rich surface innervation (e.g. similar to the cuttlefish skin) to aid rich system state perception; this will enable accurate feedback control of the pressurization within the actuator's air chambers. *We expect that this bleeding-edge application will demonstrate for the first time that soft actuators can excel at precise deformation schemes that are safe and compliant for real-world medical applications.*

### K99 Aim II: To Develop a Multi-Modal and Robustly Stable Optimal Motion-Planner.

Our preliminary results show the need for a head manipulation motion planner that is safety-aware for executing optimal collision-free paths between transition modes such that manipulating the patient's head does not expose normal brain tissues to high radiation doses. This aim will find a robustly stable and optimal head motion trajectory for moving the head from a start location  $\xi_i \in SE(3)$  to a goal location  $\xi_f \in SE(3)$  safely. As the desired head motion is continuous with discrete underlying structures, the manipulation problem is multi-modal with a continuous admixture of modes. The current convention in robotics is to use layered planning whereby search is hastened by solving a planning problem at various abstraction levels. However, such planners often miss stability-guarantees in their optimal path formulations hence resulting in paths that are not stably robust for assuring safety in the execution of planned paths. *We will address the current gap in geometric manipulation problems under manifold constraints that leave out stability analysis by leveraging an asymptotically stable robust control Lyapunov function optimally stable motion-planning feedback controller in order to safely generate optimally-robust single modes that guide transitions that precisely move the head in the presence of medical constraints in the head-robot workspace.*

### K99 Aim III: Mechanism Assembly, Phantom, and Healthy Volunteer Experiments.

A soft robot mechanism will be constructed, able to fit under the MR coils and able to (re)position the patient as needed during treatment. In addition, a 3D surface imaging sensor will measure patient's head position and feed it to the motion planner's head position feedback controller. Patient safety systems based on automated treatment beam shut off will be incorporated into the finished design. The motion-planner in K99 Aim II will be used in the real-time head motion correction in mock MRI-LINAC RT phantom and healthy human volunteer experiments. An end-to-end testing with 3D-printed head phantoms containing dosimetric gel will be used to evaluate 3D radiation dose accuracy for both single and multiple target SRS plans. A 20 volunteer study with a mock radiation beam will be conducted in a clinical environment to verify linear and angular head position control and patient safety systems.

### R00 Aim: Patient Oncological Clinical Trials.

A clinical trial on 20 whole brain patients will be performed where validation of this system will be determined by a statistical endpoint. Success will be that a 6D intracranial target is  $\leq 0.5\text{mm}$  and  $\leq 0.5^\circ$  for greater than 95% of the treatment time. Upon successful completion and novel use in maskless MRI-LINAC systems, this project will demonstrate that soft robotic SRS is ready for widespread clinical deployment. With its transformational clinical potential, our soft robot head motion compensation in MRI-LINAC RT will enable the availability of novel radiation dose delivery to a larger population of patients, improve therapeutic outcomes, reduce patient invasiveness, improve clinical efficiencies by reducing current setup times from hours to minutes, and will be compatible with thousands of pre-existing LINACs.

**Future Plans: I plan to expand this project into my own independent research laboratory where I will study to design and control soft robots for broad biomedical engineering applications in human-robot interfaces.**

# Research Strategy

## Significance

Integrating magnetic resonance imaging (MRI) functionality with radiation therapy (RT) linear accelerator (LINAC) can better render the visualization of the soft tissues of lesions and surrounding healthy organs-at-risks (OARs) during cancer RT treatment planning and procedures. This is because MR scans, in contrast to the prevalent computed tomography (CT) scans used in clinics today, provide a richly contrasted image of internal body tissues. More importantly, MRI-LINAC integration can be done in an unrivaled, online, and real-time fashion to aid a more precise radiation dose delivery in RT [1]. There are now MRI-LINAC systems such as the ones developed by Raaymakers et al [1, 5], further commercialized by Elekta AB (Sweden) [1]; it uses a 1.5 T diagnostic image quality MRI system from Phillips Ingenia in conjunction with a linear accelerator. The MRIdian system is another one of such technologies, essentially an MRI-based image-guided RT [6] that was developed by Viewray (USA). There is the Aurora RT system from MagnetTx (Canada) [7], or the non-commissioned Australian MRI-Linac project [8]. While MRI-LINAC integration has been widely researched [1, 5, 9, 10], the effect of random and involuntary patient motion causes motion artifacts which lowers the quality of MR imaging scans for use in brain and head and neck (H&N) RT. These artifacts in image collection lower the accuracy of online and real-time precise radiation dose delivery, which in turn affects clinical efficacy.

Therefore, it is paramount to keep the patient accurately positioned on the treatment table, especially in applications aimed at more precise irradiation using the newly emerging MRI-LINAC machines. The importance of accurate patient positioning is further underscored by accumulating evidence that patient displacement and collimator and gantry angle misalignment during RT showed high sensitivity to small perturbations: a 3-mm error in anterior-posterior direction caused 38% decrease in minimum target dose or 41% increase in the maximum spinal cord dose [11]. Thus, to automatically align patient motion during RT, state-of-the-art clinical approaches use either a frame or a mask to stabilize patient motion on the treatment couch.

## Known roles of frames in positioning compensation

In frame-based approaches, a metal ring is attached to the patient's skull using screws, and then bolted to the treatment table, Fig. 1a. Treatment discomfort and severe pain often results from long hours of minimally invasive surgery where the skull is fixed with pins for head immobilization during stereo-tactic radiosurgery (SRS). The invasiveness and discomfort associated with the frame are a principal cause of poor patient compliance and poor clinical efficacy. For some patients, frame placement is not possible due to extreme cranial anatomy or prior surgical bone flaps. In cases where multiple radiation therapy (RT) deliveries are needed, patients cannot be subjected to daily attachment and removal of the frame.

## Known roles of masks in positioning compensation

These limitations of frames have spurred clinics to start using thermoplastic face masks. Here, a porous mask is deformed to fit the geometry of the patient's head and neck region and then fastened to the treatment table. As the mask is flexible, during the course of treatment, it loses its firmness around the patient so that inaccuracy of dose targeting is inevitable. The flexibility of mask has been identified to cause a drift of up to 2-6mm. This is unacceptable given the AAPM TG-42 positioning accuracy guidelines that specify < 2 mm accuracy [14]. Changes in the mask's physical texture from repeated application and shrinking, Fig. 1b, can also lower treatment accuracy. These inconsistencies are not suitable for deep tumors located nearby critical structures such as the brain stem or for newer treatment modalities such as single isocenter multiple-target SRS, which are highly sensitive to rotational head motions. Even so, conventional LINACs used at most cancer centers are insufficient for the high geometric accuracy and precision required of SRS for isocenter localization [15].

## Known roles of rigid robots in positioning compensation

To overcome these issues, explorative robotic positioning research studies have demonstrated the feasibility of maintaining stable patient cranial motion consistent with treatment plans. For example, the Wiersma Lab's Stewart-Gough (SG) platform [2, 16, 17], illustrated

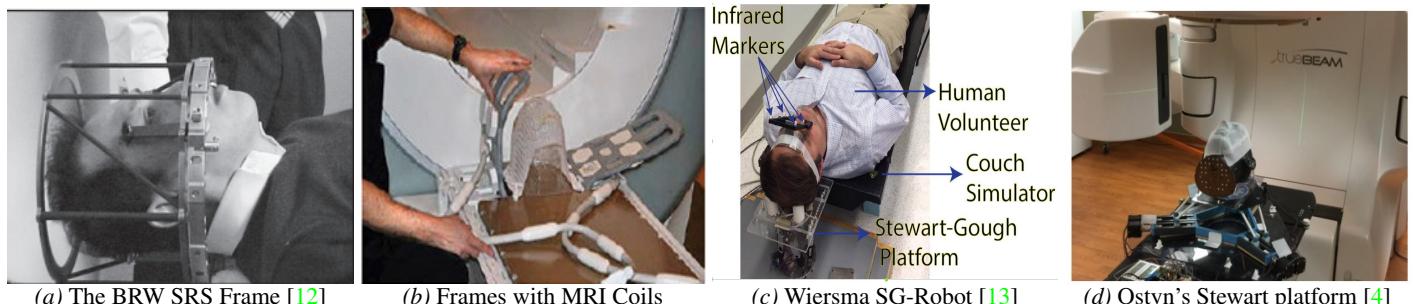


Figure 1: Existing frame and mask (a-b), and frameless and maskless robotic systems (c-d).

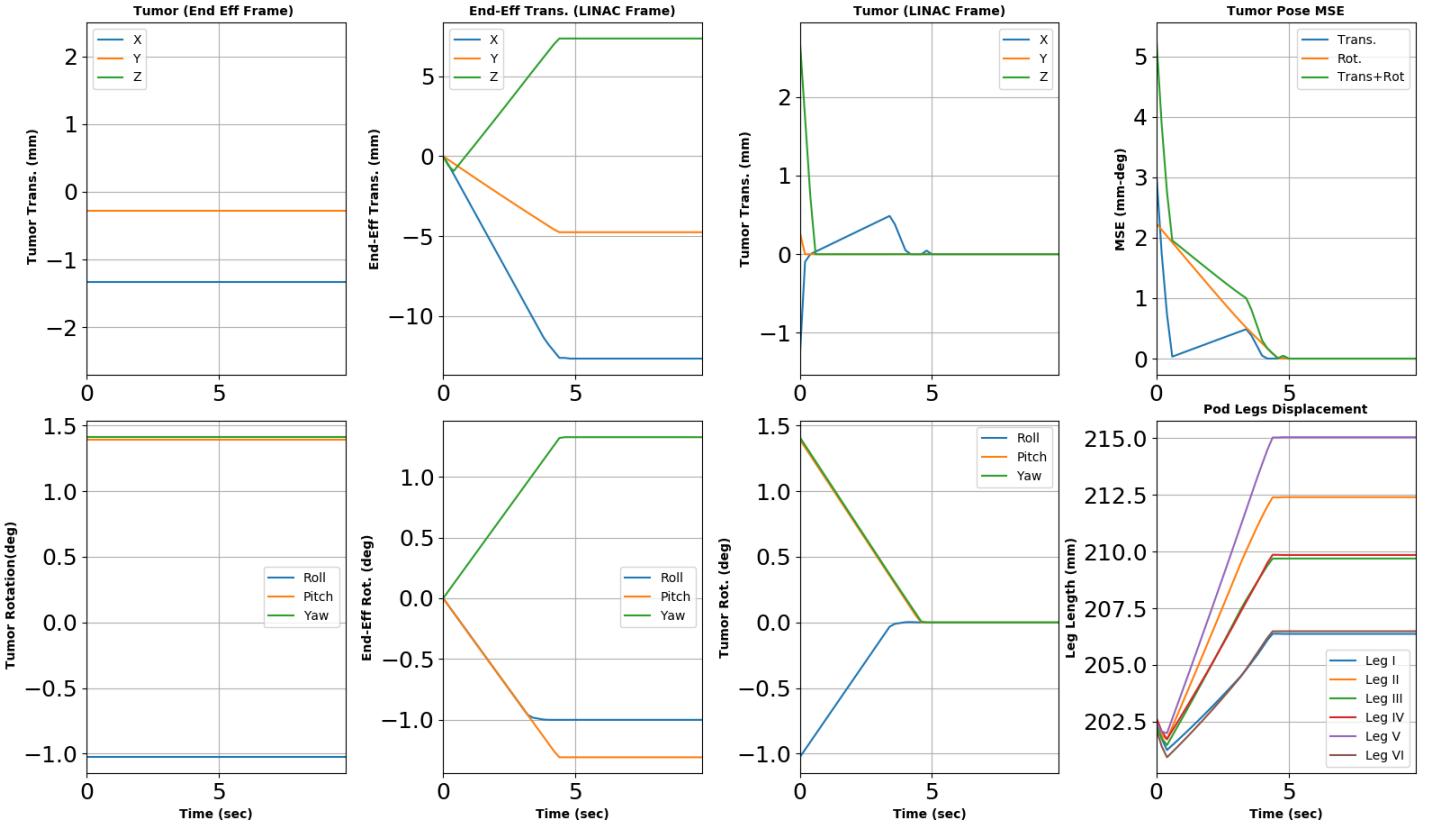


Figure 2: Isocenter Head Stabilization Results Using the Wiersma Rigid Stewart-Gough Platform. Reprinted with permission from [17].

in Fig. 1(c), achieves  $\leq 0.5\text{mm}$  and  $\leq 0.5^\circ$  positioning accuracy 90% of the time. It is constructed as a 6-6 SG platform out of linear actuators, electric motors and rigid metallic components. While effective at head position compensation in SRS treatment procedures, it is not adaptable for new MRI-integration with LINAC RTs that offer better real-time soft tissues delineation for a precise radiation dose delivery. The Ostyn et al research group sought to alleviate this rigid build structure by 3D printing the mechanical components of the Stewart-Gough platform [4]. It is worth noting, however, that this platform uses stepper motors as well (see Fig. 1(d)) to actuate the legs of the robot. This by nature leads to radiation attenuation. With the potential to aid better clinical accuracy in SRS-based systems when commissioned, these systems are not suitable for the emerging MRI-LINAC machines. This is because they utilize rigid metallic components, electric motors and linear actuators which are not suitable for the large tubular magnets of the MR machine: they interfere with the magnetic fields of the MR machine and have been known to lead to patient fatality or significantly damage the MR machine when clinicians have been careless about bringing metallic materials into the treatment room [18].

#### Known roles of soft robots in RT

Published work from the Wiersma lab shows that a rigid parallel robot can provide the online, real-time patient motion compensation in mock SRS and RT treatments (see Fig. 2). Here, using an L-BFGS-based trajectory optimization formulation for patient head motion compensation, the algorithm was able to maintain a  $\leq 0.5\text{mm}$  and  $\leq 0.5^\circ$  clinical tolerance objective for 100% of the treatment time [17]. But observe that not all constraints are adhered to: for example, observe the overshoot along Z for the tumor in the LINAC frame and the wriggly trajectories along the rotational axis of the tumor before it reaches steady state. *It is my hypothesis that a motion-planner that continually refines found paths, in the presence of manifold constraints, in the robot-head workspace can alleviate this.* Furthermore, while this robot does work well for SRS treatment procedures, it does not translate to integrating MRI functionality with LINACs owing to its structural mechanical characteristics.

My preliminary work on soft manipulators for patient head motion compensation in RT shows that novel soft robot manipulators can compensate head motion within the submillimeter and subdegree accuracy of the AAPM-TG42 stipulation for up to 3 DoFs [19–22]. In a cascaded PID-PI controller loop, I initially showed head motion correction for head setpoint- and trajectory-following to be accurate to within  $\leq 1.5\text{mm}$  for a task of lowering or raising the head along 1 DoF on a treatment table [19]. These results are duplicated in Fig. 3. Furthermore, Fig. 4 illustrates the testbed used in generating the 3-DoF control results of Fig. 5. Here, the setup consists of a phantom with a neck simulator that models the ball joint in the human torso. A vision-based 3D sensor acquires the face's point cloud in real-time, which is then processed for features-extraction and the 6D coordinates of the head (here using the tip of the nose) are sent to a microcontroller (National Instruments®myRIO); the myRIO then regulates the flow of compressed air into a set of proportional

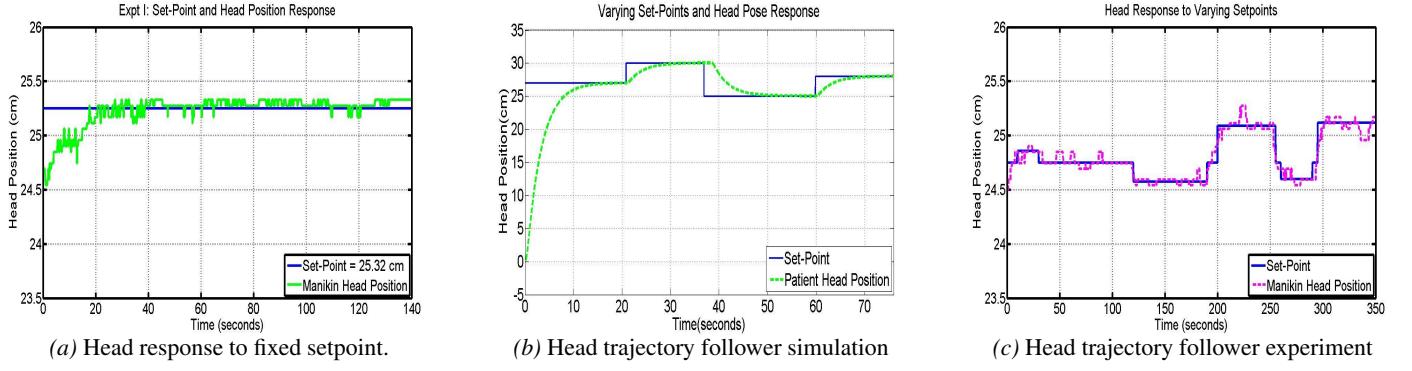


Figure 3: 1-DoF Online, Real-Time Head Motion Correction. Reprinted from [19].

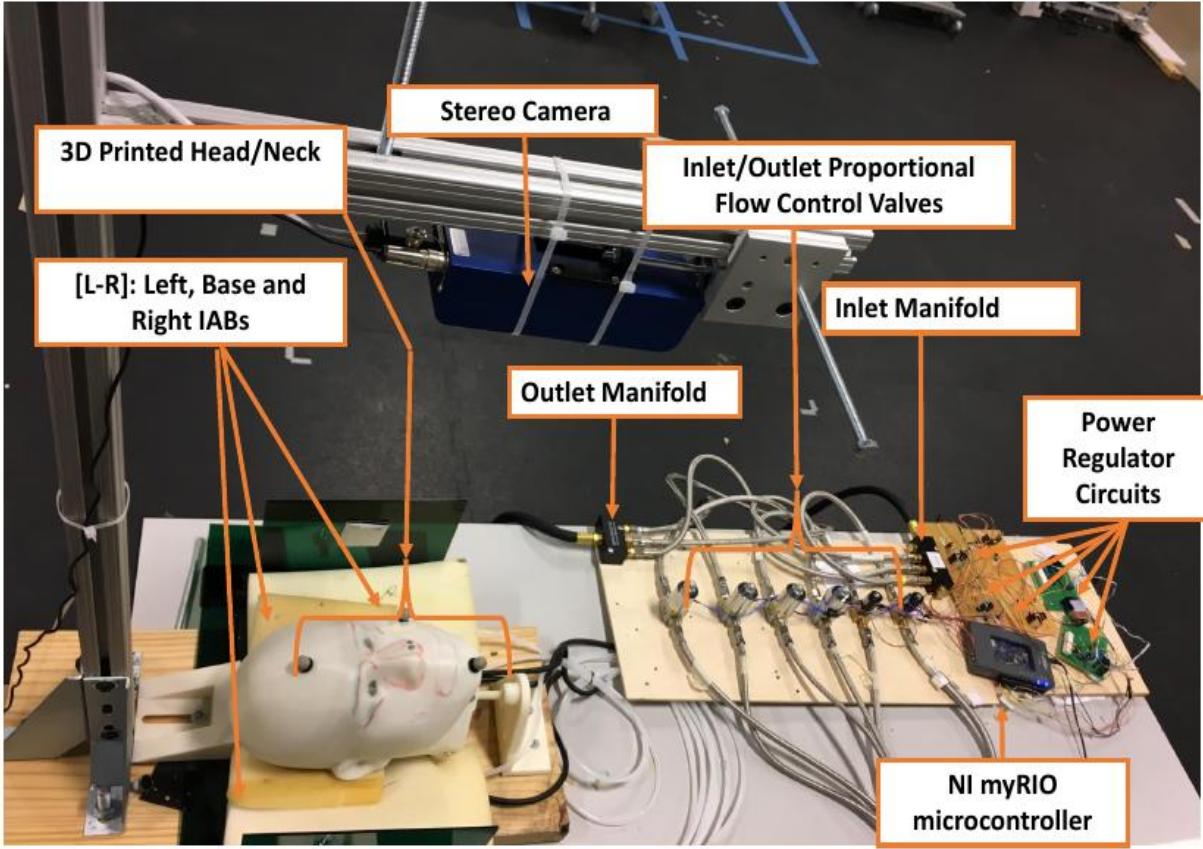


Figure 4: Three DoF Testbed. Reprinted from [20].

solenoid valves. The amount of air within the set of inflatable air bladders (IABs), in turn raise, lower, or tilt the head on the mock treatment table. The dynamics of the head interaction with the IABs and air pressure supply were carried with a lumped prediction error model [23]. This model was then used in a controller that leveraged indirect model reference adaptive control with optimal state regulation in order to ensure the head follows set trajectory through steady-state [20]. Some of these results are reprinted in Fig. 3 and Fig. 5 respectively.

Now, in a new class of soft actuator designs, and contrary to stochastic system identification techniques I used in my previous models [19, 20, 22], we can now specifically regulate volume fractions within the IABs as well as accurately control their spatial deformations based on specific nonlinear elastic deformation relationships [24]. Being continuum, compliant and configurable (C3) for manipulation tasks, we recently demonstrated in control experiments that they are as well capable of providing patient head motion compensation [13]. Contrary to remote-controlled airbags that have been used in upper mandible and head manipulation [25], our actuators deform based on their material moduli, compressed air pressurization and incompressibility constraints when given a reference trajectory. To our knowl-

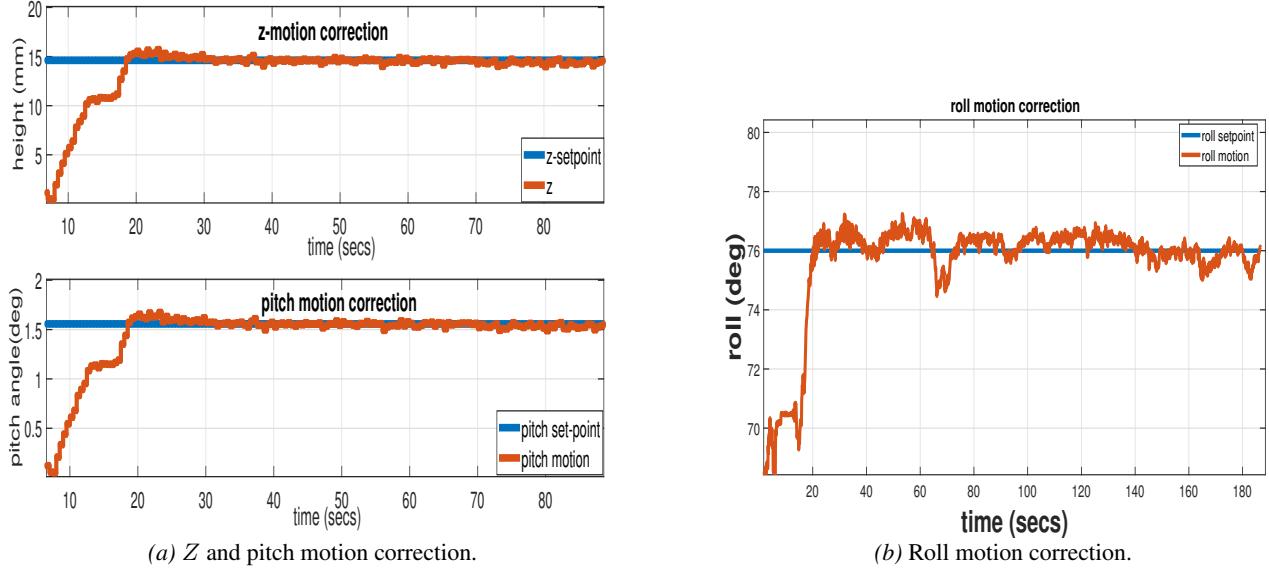


Figure 5: 3-DoF Online, Real-Time Head Motion Correction. Reprinted from [20].

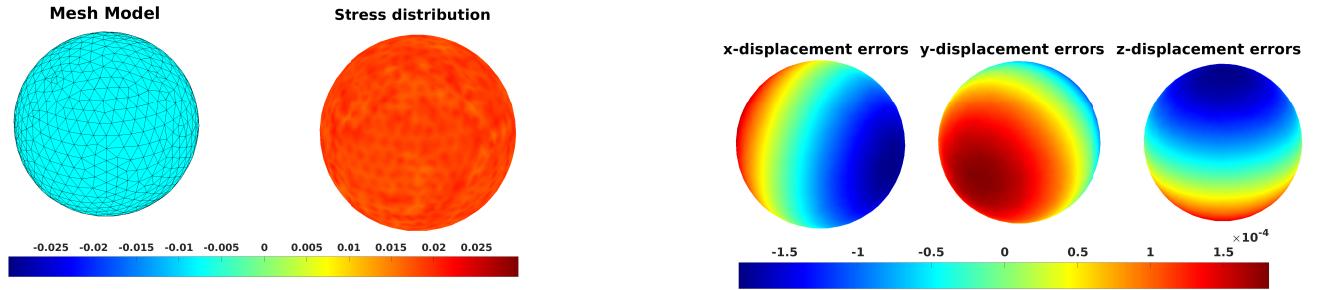


Figure 6: Volumetric Deformation of a Soft Actuator (Expansion). Reprinted from [24].

edge, ours are the first to explore C3 materials as actuation systems for cranial manipulation in robotic radiotherapy. Deforming based on prescribed internal pressurization, their surface displacement errors are accurate to the order of  $< 1.5 \times 10^{-4} \text{ mm}$  [24]. These results are reiterated in Fig. 6 where a spherically-textured soft actuator was prescribed to deform from an initial internal radius,  $R_i = 2.7 \text{ mm}$  from the reference configuration to  $r_i = 3.3 \text{ mm}$  in the current configuration. Based on my derived constitutive relation between the applied pressure and the radius of the actuator, a pressure of 0.76 psi was found to be suitable to realize this deformation. The charts of Fig. 6 illustrates the response of the actuator based on a prescribed pressure, where  $C_1$  and  $C_2$  are appropriate material moduli. With the standard local volume preservation principle, we notice a displacement error of  $1.5 \times 10^{-4}$  along the rectangular Cartesian coordinates and a zero volumetric change i.e.  $\Delta V \approx 0$ . This shows that with *highly accurate pressure sensors*, and equipped with properly calibrated proportional solenoid valves, we can regulate the air within a soft actuator's chamber so that specific and highly precise deformation behaviors are realizable for consumer soft actuators.

### Hypothesis

My **leading hypothesis** is to use MRI/LINAC-compatible soft robot system that can provide 6-DoF head motion correction in precision RT procedures to serve as a viable alternative to current mask-based as well as frameless and maskless robot-based cranial manipulation systems. In this sentiment, I hypothesize that **time-resolved MRI-LINAC techniques, which provide superior soft tissue scans, in conjunction with non-magnetic and radiation transparent soft robots can provide superior brain or H&N radiation dose targets**

**for precise MRI-LINAC RT treatment procedures.** Existing frame-based immobilization devices, Fig. 1a&b, and frameless and maskless rigid robotic motion correction mechanisms, Fig. 1c&d, are not suitable for this because of their electro-mechanical parts that introduce serious safety concerns. Furthermore, I hypothesize that an asymptotically stable in the large and optimal motion-planner can find collision-free paths that satisfy head motion constraints can resolve the abnormalities inherent in current controllers used in head motion correction systems [2, 3, 16, 20]. I will test this leading hypothesis to see if 6-DOF target motion of a patient is  $\leq 0.5$  mm and  $\leq 0.5^\circ$  for greater than 95% of the treatment time using MRI imaging for soft robot-based motion compensation.

Along with other experiments where I verified that vision-based control of soft robots can geometrically correct patient motion precisely fast-enough in real-time up to three DOFs [19–22], and existing hybrid MRI-compatible RT systems [5, 9, 10], we will test these hypotheses that soft robots can provide position accuracy that is consistent for use in standalone MRIs, MRI-LINAC RT systems or SRS-alone treatment procedures in order to (i) negate the deleterious effects of *interfractional* setup variation on patients; (ii) correct the complex *intrafractional geometric uncertainties* such as posture changes, and body deformation with minimal invasiveness; (iii) eliminate radiation attenuation associated with the metallic components of frames and rigid robotic patient motion compensation systems; and (iv) correct the flex associated with thermoplastic face masks; while *not interfering with the MR machine's magnetic field*.

## Innovation.

Our study is innovative in the following respects:

- my work was the first to demonstrate the feasibility of vision-based 3 DOF control of soft manipulators for cranial motion management in RT [19–22]; we are extending this to 6-DOF control with my novel advanced mechanism;
- this mechanism is made entirely of no metal (hence not susceptible to magnetic fields) and is radiation-transparent so that it is compatible with both MRI-LINACs;
- this mechanism can be adapted to confined spaces under MRI coils (see Fig. 1b) given its compactness, and light weight.
- it possesses little invasiveness to the patient, and
- exhibits a quick-connect, quick-disconnect modularity on a couch – important for patients with varying cranial anatomy – thus easing the logistical setup workload of current immobilization and maskless robotic systems.

To our knowledge, **no currently-available technology exists today that can perform real-time head position stabilization without dose attenuation in an online, real-time fashion whilst guaranteeing patient safety similar to our proposed MRI-LINAC non-magnetic and radio-transparent soft robot RT positioning system.** As photon-based cancer treatment accounts for > 50% of all cancer treatments [26], these exploratory experiments are relevant to public health and have transformational clinical potential because they may provide (i) proof-of-concept evidence that soft robots are compatible with standalone MRI imaging modalities; (ii) evidence of precise and automatic motion management with non-magnetic and radiation-transparent soft robots in emerging hybrid MRI-accelerator RT; (iii) an emergence of a better brain and H&N cancer management technology that can be adapted to confined spaces under MRI coils (see Fig. 1b). Upon successful completion, this soft robot will be used for active head motion stabilization within an MR machine. It will be adaptable for standalone MRIs, emerging MRI-LINAC technologies, and brain as well as H&N RTs. It will provide accurate RT beam targeting as well as preventing patient motion MRI imaging artifacts. This technology will improve therapeutic outcomes, and eliminate patient invasiveness.

## Approach.

### K<sub>99</sub> Aim I: To Develop a Distributively-Innervated, Non-magnetic, and Radiation-Transparent Soft Actuator.

**Rationale:** For though the design of Fig. is relevant to head motion control on an RT treatment table, it is not a complete motion correction system owing to its underactuated mechanism: it is only able to correct motion for up to three DoFs. Motion of the head occurs along six DoFs and they are not independent. Therefore, to realize a full patient motion compensation, more actuators are needed in the mechanism. To this end, and iterating further on my previous designs [20–22], I now propose a new class of continuum, compliant and configurable (C3) light, and agile soft actuators [24, 27, 28] which are the composition of a non-magnetic and radiation-transparent soft robot for use in MRI-LINACs to further aid dose delivery precision. The component soft actuators are planar and circular in their reference configuration. Upon compressed air actuation, they deform along the radial direction (see computer model in Fig. 7) based on the physical constraints baked into the elastomer-fabric matrix. This actuation design is inspired by the behavior of the skin papillae of certain Cephalopods (octopus, cuttlefish, bivalves and mollusks) which can transform their physical texture from 2D to 3D in less than 2 seconds [29, 30]. The actuators exhibit a radially symmetric deformation and are constrained along their circumferential axis under pneumatic actuation based on their novel design. There exists no electrical wirings or embedded electronics to assure that the actuators reach a desired configuration.

**Hypothesis:** Based on previous success of air actuated elastomeric chambers for manipulating patient head motion correction in real-time, I hypothesize that a fully-compliant and parallel soft robot can effectively correct patient head motion (given a robustly stable and

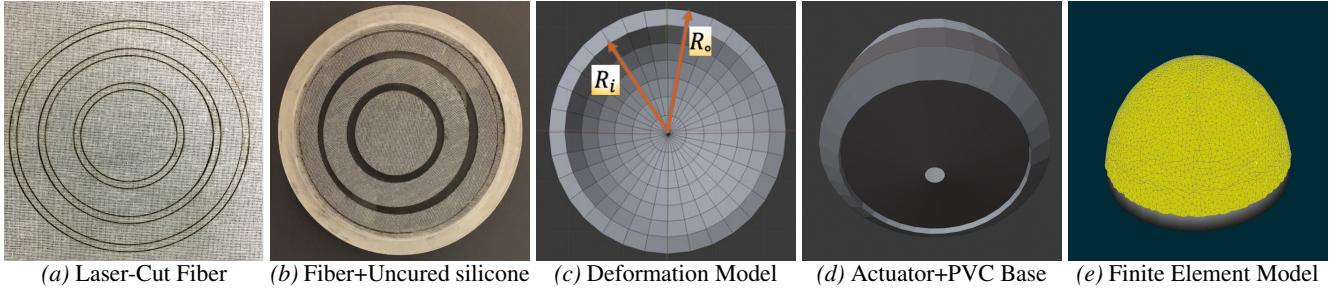


Figure 7: Soft actuator fabrication procedure.

optimal controller) such that the motion artifacts that are prone in MR imaging can be eliminated. This will assure an improved RT treatment outcomes in modern MRI-LINAC RTs.

#### Procedure.

**A. Soft Actuator Design:** The soft actuator fabrication methodology is illustrated in Fig. 7. A thin-layered fabric is laser cut into circular patterns (Fig. 7a), the cut meshes are removed and laid onto uncured silicone (Fig. 7b) which has been poured into mold. We further add a silicone topcoat layer to the fabric before we allow it to cure. Upon low pneumatic pressurization, the cured rubber deforms, obeying a Circumferentially-COnstrained And Radially Stretched fiber-Elastomer (CCOARSE) property [31] (Fig. 7c). This unique deformation pattern is similar to the way a balloon would stretch along its axial direction if a rope were tied around its circumference. The soft robot, after cure, is laid onto an impact-resistant, low-temperature rigid PVC insulation foam sheet, encased in a carbon fiber material. This aids radiation transparency (Fig. 7d). The finite elastic deformation mesh model of the soft robot for simulation purposes is shown in (Fig. 7e). This proposed fabrication method allows us to rapidly iterate different designs using compressed low air pressure (1-15 psi) that is (i) cheaply available, (ii) environmentally-friendly, (iii) avoids electrical wirings, (iv) is lightweight, and (v) inviscid which will make the soft robot adaptable for MRI-LINAC systems – creating a clean and safe human-robot workspace. As the air inflow into the air chambers of the elastomers need to be carefully regulated, we will build current source electronic regulator circuits that proportionally vary the amount of airflow through connecting hoses that lead into the proportional solenoid valves used in earlier experiments [20].

**B. Pneumatic System Design:** We now describe the integration of the soft actuator design proposed above with the rest of the pneumatic actuation system. This system is illustrated in Fig. 8. A self-contained compressed air canister supplies air at a fixed pressure (e.g. 15 psi) through a firm polyurethane air tubing into a 4-20mA output-M12 pressure transducer plug connection. The choice of pressure transmitter is important owing to the accuracy requirement for air volume within the chamber of the soft actuator. In our experience, the G2 series of pressure transducers from Ashcroft® are an excellent choice for such application as this: it offers a  $\pm 1.00\%$  total error band accuracy; being highly configurable, it offers a pressure range that meets our actuation needs and it can be easily integrated into our overall mechanism. The outlet of this pressure transmitter conveys the airflow into a proportional solenoid valve. We use proportioning valves to control the amount of airflow into the actuator’s air chamber because of the air flow precision requirement needed to correctly manipulate the head. The outlet of this solenoid valve then leads to the inlet air connector of the soft actuator. The electronic regulating circuit shown in Fig. 8 is a standard current source circuit that varies the air flow rate within the proportional valve by adjusting the current flowing through its shunt resistor. In addition, a venturi pump removes air at a proportional pressure compared to the inlet supply pressure. This pressure differential helps maintain head along a setpoint or follow a varying trajectory.

**C. Preliminary Actuation Experiments:** We have initial experiments that reproduces deformation behavior similar to the spike observed in the skin papillae of the Octopus. This is described in what follows. We cast silicone from Smooth-On Inc’s dragon skin (475 psi tensile strength and 10A shore hardness), whose material properties exhibit enough softness for patient comfort and enough firmness that withstands extremely nonlinear deformation from the wrench produced by the typical human head (55-65 kg [32–34]. The ingrained fabric membrane within the elastomer imposes the CCOARSE property, constraining the circumferential expansion of the rubber and exerting a radially symmetric stretch as shown in the bottom row of Fig. 9. This considerably simplifies the dynamics model that governs the deformation [28]. Two different designs are shown in the top and bottom rows of Fig. 9. The rubber material is screwed onto a bottom PVC foam sheet using a laser-cut acrylic planar ring. We use **nylon** Phillips screws. The behavior at different levels of pressurization are indicated in each column of the figure. The top row shows the cured silicone without fabric while the bottom row shows the silicone with the entrenched fiber matrix within the elastomer. As can be seen, the material in the top row exhibits a circumferential bulge as well as radial bulge while the ones in the bottom row only extend along the axial direction. As can be seen in the bottom row, we can generate a full *Gaussian deformation* and return to the reference planar configuration in 2 seconds (see more images and videos in [scriptedonachip.com/soro](http://scriptedonachip.com/soro)) similar to the spikes produced by the skin papillae of the Octopus. These quick Gaussian spikes will be useful for rapid head motion correction in MRI-LINACs. The soft compliance and tensile strength of this silicone material make it well-suited for treatment procedures where non-magnetic and radiation-transparent components can boost stereotactic precision as well as improve tumor control in MRI-LINACs.

**D. Flexible Piezoresistive Distributed Sensor Integration:** In a recent formulation [24], we mapped the relationship between the

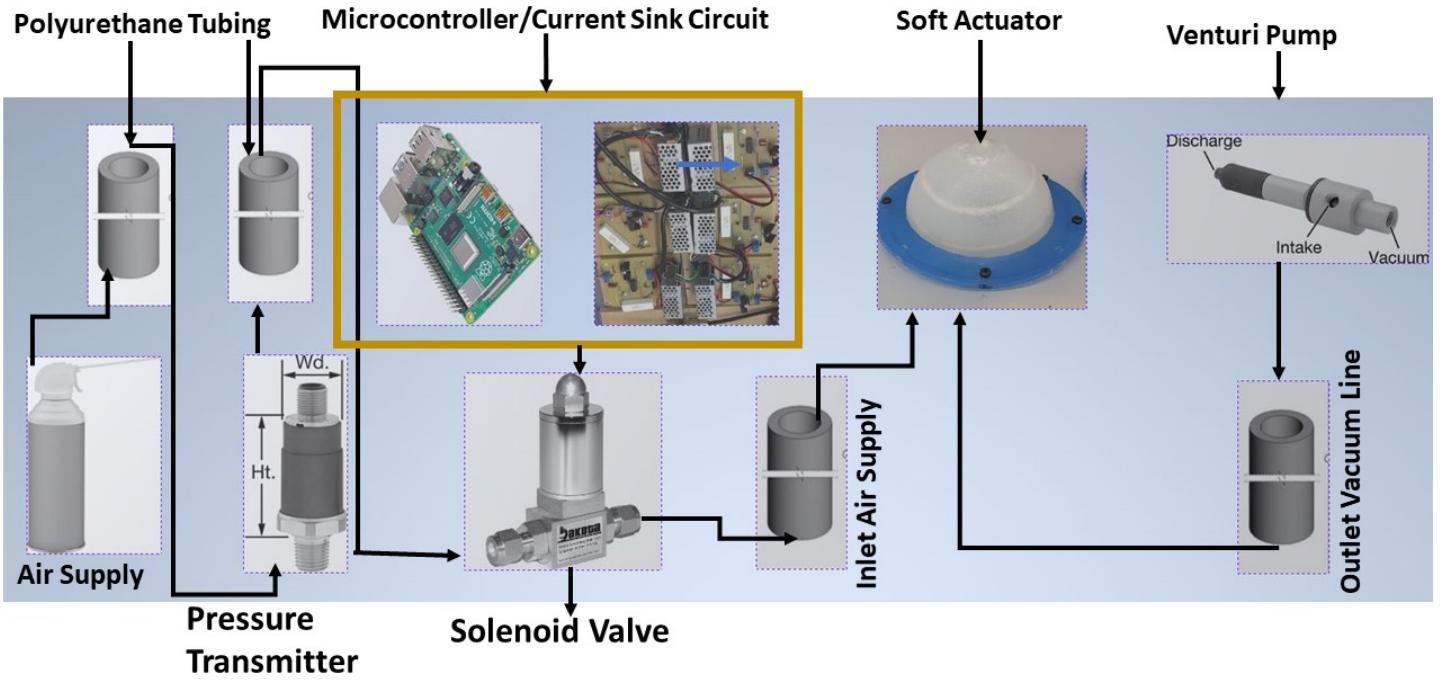


Figure 8: Pneumatic System showing proportional solenoid valve, electronic pressure regulators and raspberry pi microcontroller.

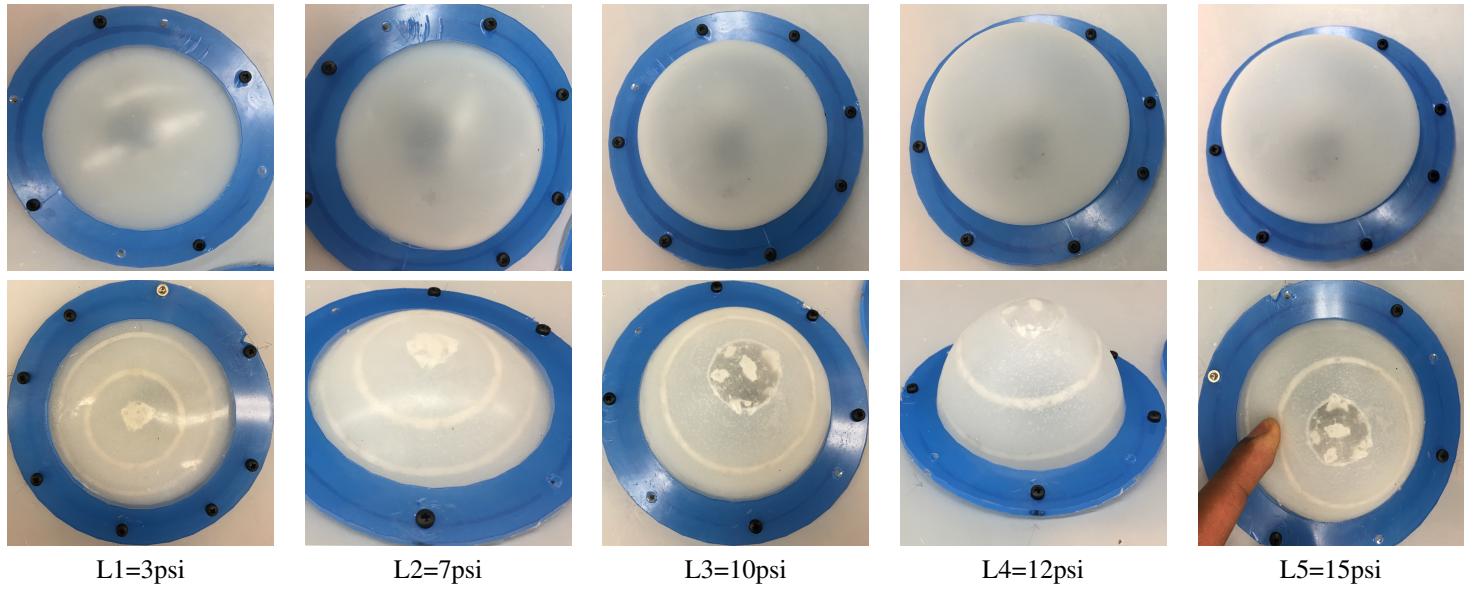


Figure 9: Deformation Levels of elastomer (top) and Elastomeric-Fiber Matrix (bottom) under Low Air Pressurization (3-15psi).

applied pressure to the deformed radius of a soft actuator using the standard Mooney-Rivlin formulation [35, 36]. Suppose that  $C_1$  and  $C_2$  are appropriate material moduli for the soft actuator, then the applied pressure in the internal walls of the actuator is given by the relation

$$P(r) = \int_{r_i}^{r_o} \left[ 2C_1 \left( \frac{r}{R^2} - \frac{R^4}{r^5} \right) + 2C_2 \left( \frac{r^3}{R^4} - \frac{R^2}{r^3} \right) \right] dr \quad (1)$$

where  $r_i$  and  $r_o$  are respectively the internal and external radius of the actuator walls in the current configuration, and they have

corresponding forms  $R_i$  and  $R_o$  in the reference configuration. Taking cues from the precise control schemes of rigid robot manipulators made possible by presence of joint encoders and harmonic drives that enable precise control of the joint angles between robot links, a means of sensing the “measure of deformation” based on the amount of pressure in the actuator’s air chamber is necessary for a successful control.

There have been various measures proposed in literature over the past few years about sensing volumetric deformation of a soft actuator. For example, embedded optically-laced fiber sensors based on the principle of frustrated total internal reflection, and distributed throughout a 3D printed elastomer, were used to generate a cointegrated body, sensing, and communication network for a soft robot’s state sensing [37]. They have also found applications in innervated soft finger prosthetic hand designs [38], where a very lossy optical waveguide was used in an open-loop control setting to detect shape and texture. While in softness grasp dexterity, they appear promising, they are not yet suitable for human-level texture-based sensitivity (nanometers) despite their complex design. Stretchable sensors with rheological properties have been erstwhile embedded within an elastomer using 3D printing techniques [39]; and though they have been shown to be mechanically receptive, and scalable up to e.g.  $\sim 400\%$  strain, their electrical resistance gives at strains  $> 400\%$  owing to the percolation of the networked components [39]. Pneumatic actuator networks patterned within an elastomeric robot body via a multi-material, embedded 3D printing technique have been tried [40]. Dielectric elastomers (DE) making use of the static charge properties of passive electronic components have been shown capable of measuring strain by up to 1692% under the Maxwell pressure law [41]. This DE actuators generally rely on electrostatic voltage discharge to sense deformation [42].

Owing to our precise manipulation requirement, a richly innervated means of sensing actuator deformation at high strains (owing to large reactive head forces) is necessary for effective closed-loop feedback control of head motion. Borrowing cues from the observational and short/long-term learning skills arising from the afferent neural networks on the exteroceptive skins of Cephalopods [30, Ch. 2], we will integrate volumetric tactile mechano-receptors on the soft actuators’ skins. As we aim to avoid rigid electro-mechanical sources that can hamper radiation delivery within the design, we will shun DEAs. Optical waveguides would be attractive but they are expensive to integrate for volumetric sensing. Instead, I propose tactile stretchable kirigami sensors made out of polyimides (Kapton sheets) and fiberglass membranes. Meso-scale stretchable Kirigami layer-by-layer manufacture of soft robots have recently been shown to be relevant for fast and precise deployment of robots [43, 44] with high sensing accuracy . Even so, the 3D perception of the environment of these piezoresistive innervated soft robot skins can be perceived using deep learning [45]. In this sentiment, I will laser-cut electrical grade Kapton sheets, weave them in twisting formations with fiberglass materials to mimic the bending of beams that enable accurate sensing [43]. The sensors will then be neatly covalently bonded (without adhesives) to the soft actuators surface by plasma treatment [46]. The proprioception of the soft actuators will be captured by an LSTM deep-learning network such as I used in my previous works [47–49]: this will predict the configuration of each soft actuator during both prescribed and random actuation sequences, even with feedback from non-monotonic, hysteretic, soft piezoresistive sensors. This fabrication approach is attractive because (i) it allows the separation of the fabrication of the soft actuator design from the piezo-resistive sensors; (ii) we can separately characterize the deformation sensing properties of the piezoresistive fiberglass-polyimide sensors for QA purposes before respective integration onto the component actuators; and (iii) it offers a modular and cheap fabrication design methodology that eases troubleshooting during the construction phase.

**E. Expected results:** Based on the series of experiments proposed in this section, I expect to see individual soft actuators obeying the prescribed pressure law given in (1) so that the deformation radius of the actuators exactly follows an applied pressure similar to the presented simulation results of Fig. 6, further elaborated in [24]. In addition, as I am skilled and well-versed in inference using deep-learning methods (see representative publications [47, 48, 50, 51]), I expect that the stretchable Kirigami sensor layers embedded within the elastomeric actuator membranes will produce rich innervated data that can be processed with deep learning based methods [45] for onward control processing.

## K<sub>99</sub> Aim II: To Develop a Multi-Modal and Robustly Stable Optimal Motion-Planner.

**Rationale:** Current SRS-based immobilization and head motion compensation techniques are pre-programmed and heavily calibrated within their environment in order to find the optimal and safest path required in moving a patient’s cranial structure from one location to another in the robot workspace [3, 13, 16, 52, 53]. Techniques used range from PID control schemes [2, 19], reduced-order observer feedback control design [22], optimal and robustly stable indirect model reference adaptive control design [20], to local trajectory optimization schemes [17]. While these schemes work manually for specific automation task, they require extensive calibration and adjustment of parameters so as to get them to work in each new environment and for every new head motion control task. For these robots to execute tasks autonomously, a motion planning system capable of generating feasible motion from high-level requirements is needed. In addition, this motion planning system must respect the constraints on a task in order achieve success, such as turning the translating the head about its cranial-caudal axis, or rotating the head about its neck fulcrum. *I will reformulate these control tasks into a manifold-constrained geometric motion planning problem, concerned with finding a feasible optimal and collision-free path for a patient’s head motion.*

In order to optimally move the patient’s head in an optimally safe and collision-free path that avoids the exposure of normal tissues to high radiation dose, and is not task-dependent, it is important to develop a motion-planner that (i) executes head motion in the robot’s workspace by first finding a collision-free path; (ii) improves the plan into a better plan if the original plan is not efficient or does not satisfy C-space constraints; this may involve multiple iterations; (iii) considers how to move the head along a path that is stable and robust for execution in spite of modeling errors and uncertainties, while maintaining various speeds that satisfy various momentum

considerations; and lastly (iv) the found plan must be included in a hierarchical planning framework so that the original plan reaches termination, in order to allow larger plans in the hierarchy to roll out as needed. This planning approach is consistent with motion planning algorithms used in robotics [54].

**Hypotheses:** The requirements produced by this problem and in many other safety-critical problem domains (e.g., household caretaking, IMRT, assistive robots in epileptic patients, and disaster recovery) motivate the study of safety-aware motion planners with constraints. Therefore, **I hypothesize that a layered planning algorithm will find a hierarchical multi-planning sequences of motion that biases search into optimal mode transitions.** This layered composition of plans will first compute collision-free paths  $\mathcal{C}_{free}$  for moving the head between the start and goal poses. A higher hierarchical planning layer will then leverage encoded manipulation constraints within the robot-head interface to ensure that sensitive H&N structures are not damaged by radiation while the lower collision-free path in the hierarchy is to be executed. This layer of the planning algorithm might need to be repeatedly carried out in a fast computational loop to ensure all  $\mathcal{C}$ -space constraints are satisfied. Then a higher level plan takes the actions from the two previous lower level plans and generates a robustly stable controller in the sense of Lyapunov such that it can move the head along the  $\mathcal{C}_{free}$  paths even in the presence of parametric errors, or uncertainty in model dynamics [20, 55, 56]. **I further hypothesize that the overall hierarchical plan be sequentially structured so that head motion transitions between planning modes (i.e. from an initial location  $\xi_i \in SE(3)$  to a goal region  $\mathcal{Q}_{goal}$ ) are executed by leveraging online search protocols, which bias search for optimal and feasible paths to a sequence of modes that yield a smooth representation of head motion.** By these hypotheses, *I will address the current gap in geometric manipulation problems under manifold constraints that leave out stability analysis in the feedback control mode of the motion planner. I will achieve this by leveraging a Lyapunov-based stable estimator of the underlying dynamic system in safely generating optimally-robust single modes that guide transitions that precisely move the head.*

**Procedure:** I will formulate a stable geometrical representation of the underlying dynamical system and bias search toward optimally stable and robust short-task plans by providing an optimality-based method for choosing a control law once an robust control Lyapunov function (RCLF) [57] is known. I will develop an optimally stable and probabilistically-complete multi-modal planner that has broad applications to general multi-modal planning tasks in safety-critical problems in medical robotics.

**A. Preliminaries:** Let the set of all possible configurations of the head-robot system be  $\mathcal{Q}$  in the C-space  $\mathcal{C}$  [58]. Suppose that after a number synthesis of the proposed mechanism [59], the dimension of the robot is  $n$ . A particular configuration of the robot is defined by  $\xi \in \mathcal{Q}$ . We assume that the  $\mathcal{C}$  is a closed and bounded metric space, and that  $\mathcal{Q}$  is a measurable space  $(\mathcal{Q}, \mathcal{B}_{\mathcal{Q}})$  for a  $\mathcal{B}_{\mathcal{Q}}$  Borel  $\sigma$ -algebra on  $\mathcal{C}$ , generated from the metric [60]. The set of obstacles to be avoided are a closed set  $\mathcal{Q}_{obs}$ , which defines the free configuration space  $\mathcal{Q}_{free}$ , such that  $\mathcal{Q}_{free} = cl(\mathcal{Q} \setminus \mathcal{Q}_{obs})^2$ . Our goal is to find a path from  $\xi_i$  to some region of interest  $\mathcal{Q}_{goal} \subset \mathcal{Q}$ , i.e. a continuous injective map  $\sigma : [0, 1] \rightarrow \mathcal{Q}_{free}$  such that  $\sigma(0) = \xi_i$ , and  $\sigma(1) \in cl(\mathcal{Q}_{goal})$ . In addition, a smooth positive definite and radially unbounded function  $V(\xi)$  is a control Lyapunov function (CLF) for the head-robot control affine system  $\dot{\xi} = f(\xi) + g(\xi, u)$  if

$$\frac{\partial V}{\partial \xi}(\xi)f(\xi) + \frac{\partial V}{\partial \xi}(\xi)g(\xi)q(\xi) \leq -P(\xi) \quad \forall \xi \neq 0 \quad (2)$$

where  $P(\xi)$  is some positive definite function,  $u \in \mathbb{R}^6$  is a control input, and  $f(0, 0) = 0$ .

**B. An asymptotically stable in the large and optimal motion-planner:** Our goal is to find an optimal collision-free path,  $c$ , with respect to a CLF  $V(\xi) : \mathbb{R}^n \rightarrow \mathbb{R}^d$  such that

- $V(\xi)$  is positive for all  $\xi \in \mathbb{R}^d \setminus \mathcal{Q}_{goal}$ ; and  $V(\xi)$  exhibits a unique global minimum in the target region  $\mathcal{Q}_{goal}$ , where  $V(\mathcal{Q}_{goal}) = 0$ ;
- as the head moves along any of the trajectories, we must have  $V(\xi^{t,n}) > V(\xi^{t+1,n})$ , and  $V(\xi^{T^n,n}) = 0$ ; i.e.  $V(\xi)$  decreases as time increases and  $V(\cdot)$  vanishes when the actuators reach steady state after deformation;
- in addition, we require  $V(\cdot)$  to satisfy the CLF requirement in (2)
- robust head motion during motion execution shall be guaranteed by devising *robust stabilizability via continuous state feedback* [57], provided that there exists an RCLF on the control-affine system.

We want to choose a control input  $u = q(\xi)$  for some function  $q(\xi)$  with  $q(0) = 0$  so that equilibrium  $\xi_e = 0$  of the closed-loop system

$$\dot{\xi} = f(\xi, q(\xi)) \quad (3)$$

is asymptotically stable in the large [61]. The first condition ensures the cost function is a valid Lyapunov function while the second option maintains the stability property in the sense of Lyapunov (i.e.  $\dot{V}$  being negative semi-definite for all  $\xi \in \mathbb{R}^d \setminus \mathcal{Q}_{goal}$ ). To avoid wasting control energy and missing optimality during motion execution, as is common with the cancellation or domination of nonlinear terms in feedback linearization, the third option will leverage the *inverse optimal stabilization* in a differential game setting based on the pointwise min-norm control law of [57]. This is attractive because rather than solve a Hamilton-Jacobi-Isaacs (HJI) equation for a

---

<sup>2</sup>cl( $X$ ) is the closure of a set,  $X$ .

control law that yields the path  $c$ , the pointwise min-norm control law yields a robustly stabilizable and optimal synthesis of the head motion correction problem.

**C. Manifold Constraints:** It is not enough for us to find a valid path  $c$  that is free of collisions. We also want the head motion to follow constraints that are functions of the robot's geometry, avoids radiation hitting critical structures, follows a path that does not increase proneness to claustrophobia [62], and lower the problem's dimensionality. Similar to [60], we define these *manifold constraints* to capture loop closure constraints, end-effector constraints etc. A forward kinematic map from the configuration of the  $i^{th}$  IAB,  $\chi_{iab_i}$ , maps from respective IAB configurations to head position and orientation *i.e.*  $K_{iab_i} : \chi_{iab_i} \rightarrow SE(3)$ . The head velocity with respect to a fixed base frame in terms of IAB velocities can be written in terms of the forward kinematics Jacobian:

$$\begin{pmatrix} v_{iab_i} \\ \omega_{iab_i} \end{pmatrix} = \frac{\partial K_{iab_i}}{\partial \mathbf{r}_i} \frac{d\mathbf{r}}{dt} K_{iab_i}^{-1} = \mathbf{J}_i(\mathbf{r}_i) \dot{\mathbf{r}}_i \quad (4)$$

where  $\mathbf{r}_i$  is the spatial position of IAB  $i$  in generalized coordinates, and  $(v_{iab_i}^T, \omega_{iab_i}^T) \in \mathbb{R}^6$  represents the linear and angular velocity of the  $i^{th}$  IAB about its screw basis. In essence,  $\mathbf{r}_i \in \mathbb{R}^3$  with its rows are mapped to scalars by an appropriate choice of norm<sup>3</sup>. The contact between the head and the IABs is mapped by the Jacobian

$$\mathbf{J}_{c_i}(\xi_h, \xi_{iab_i}) = \begin{bmatrix} \mathbf{I} & \hat{\mathbf{w}}(r_{c_i}) \\ \mathbf{0} & \mathbf{I} \end{bmatrix} J_{r_i}, \quad (5)$$

where  $\mathbf{J}_{c_i} : \dot{\xi}_{r_i} \rightarrow [v_{c_i}^T, w_{c_i}^T]^T$ ,  $r_{c_i} \in \mathbb{R}^3$  is a vector between the head reference point (e.g. the center of mass) and the contact with the  $i^{th}$  IAB,  $\xi_h$  is the position and relative orientation of the head,  $\xi_{iab_i}$  is the position and relative orientation of the  $i^{th}$  soft robot in world coordinates,  $\hat{\mathbf{w}}(r_{c_i})$  is an anti-symmetric matrix for the vector  $r_{c_i}$ , and  $\xi_r = (\xi_{r_1}, \xi_{r_2}, \dots, \xi_{r_k})$ ,  $(1 \leq k \leq n)$  are the positions and orientations for each of the IABs. For  $C^2$ -smooth  $k$ -constraint functions  $G_1, \dots, G_k$  ( $1 \leq k \leq n$ ), a constraint is fulfilled when  $g_i(\xi) = 0$  and we write out the composite constraint function  $G : \mathbb{R}^n \rightarrow \mathbb{R}^k$  with respect to the contact Jacobians as

$$G_i^T(\xi_h, \xi_{iab_i}) \xi_h = B_i^T(\xi_h, \xi_{iab_i}) \mathbf{J}_{c_i}(\xi_h, \mathbf{r}_i) \dot{\xi}_{iab_i} \quad (6)$$

for an IAB's selection matrix  $B_i^T(\xi_h, \xi_{iab_i}) \in \mathbb{R}^{m_i}$ , where  $m_i$  is the range of all the forces and moments for the chosen contact primitive (or union of contact primitives). Therefore, for  $k$  actuators in the soft robot, we have the following manipulation constraint

$$\begin{bmatrix} G_1^T \\ \vdots \\ G_k^T \end{bmatrix} \begin{pmatrix} v_h \\ w_h \end{pmatrix} = \text{diag} \begin{pmatrix} B_1^T \mathbf{J}_{c_1} \\ \vdots \\ B_k^T \mathbf{J}_{c_k} \end{pmatrix} \begin{pmatrix} \dot{\mathbf{r}}_{iab_1} \\ \vdots \\ \dot{\mathbf{r}}_{iab_k} \end{pmatrix}. \quad (7)$$

The details of this derivation are presented in my unpublished work [28]. We call  $\mathcal{M}_{free}$  the free constraint manifold of the overall manifold,  $\mathcal{M}$ , which is defined as  $\mathcal{M}_{free} = \mathcal{M} \cap \mathcal{Q}_{free}$ .

**Problem 1** (Constrained RCLF Motion Planning). *Find an RCLF collision-free path  $\sigma^* : [0, 1] \rightarrow \mathcal{M}_{free}$  given a path planning problem  $(\mathcal{Q}_{free}, \xi_i, \mathcal{Q}_{goal})$ , manipulation constraint,  $G$ , and cost function  $V$  such that  $V(\sigma^*) = \min_{\sigma \in \Sigma_{\mathcal{M}_{free}}} V(\sigma)$  if one exists.*

**Expected results:** Previously, the stabilizing command for items 1 and 2 in subsection B above was computed by solving a constrained optimization problem to choose the collision-free stabilizing command among the possible solutions. My implementation takes a greedy approach using the L-BFGS optimization algorithm with box constraints, in contrast to the quadratic nonlinear constrained optimization used by [63], to find the minimal value of the control law  $u$  at each time step such that  $u$  it is stable. Results of this implementation on toy robot nonlinear control from example demonstrations in 2D task space, implemented in python (see [64]), are reprinted in Fig. 10. When the problem identified in Prob. 1 is solved, I should expect my results to provide better trajectory tracking than the non-RCLF implementation I implemented in [64] owing to the account for all possible manifold constraints in the problem formulation.

### K<sub>99</sub> Aim III: Mechanism Assembly. Phantom and Healthy Volunteer Experiments.

#### Rationale.

**Case for a parallel soft manipulator:** Open-loop kinematic chains have a low transportable load and poor accuracy since the weight of the segments that follow each link and the load of the structure contributes to the large flexure of torques; their links magnify errors from shoulder out to the end-effector, consequently hampering their use for sophisticated control strategies that may minimize or eliminate load-dependent error. Thus, most serially-joined manipulators are stiffened during the manufacturing process – thus, inherently exhibiting a high load-to-weight ratio and a complicated actuation system. Moreover, their passive bending stiffness overwhelms the degree of deformation. Parallel configurations, in spite of their higher number of actuated joints, distribute the weight of the load around the links of the robot, improve manipulation accuracy, have a desirable lightness property (albeit at the expense of a reduced workspace), and minimize the flexure torques that are otherwise common with open-loop kinematic chains. Given the non-cumulative nature of actuator errors in parallel configurations, greater precision is possible with minimal control-complication [65].

<sup>3</sup>I used the  $l_2$ -norm in my implementation.

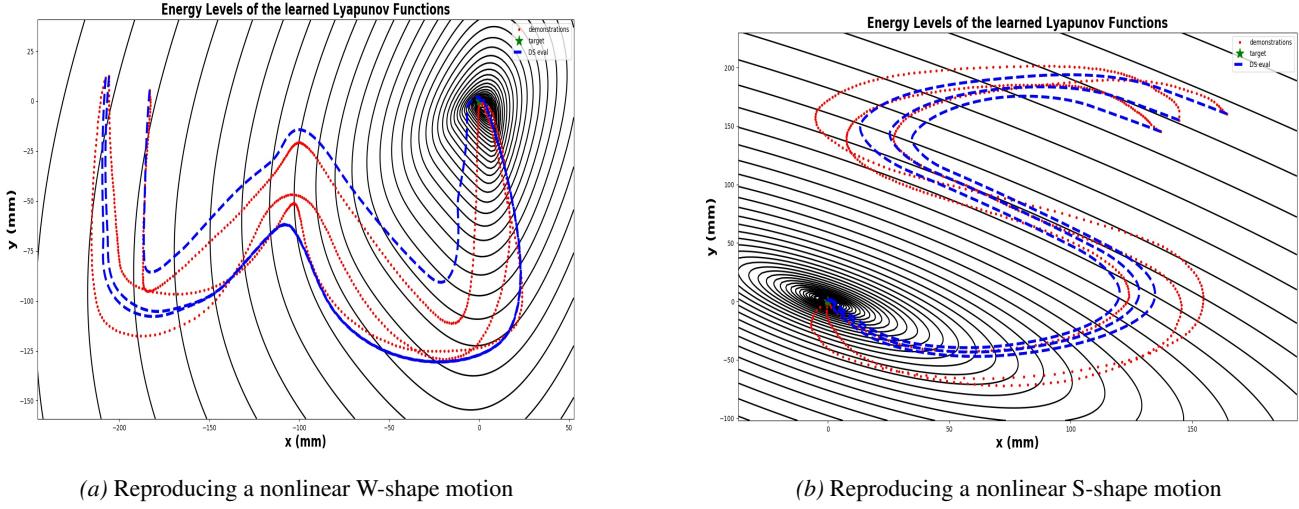


Figure 10: A CLF motion executor (red curves) that shows convergence to local attractors (green asterisks) and follows 3 different set trajectories (blue curves) for 2D nonlinear motion-trajectory problems on the WAM robot.

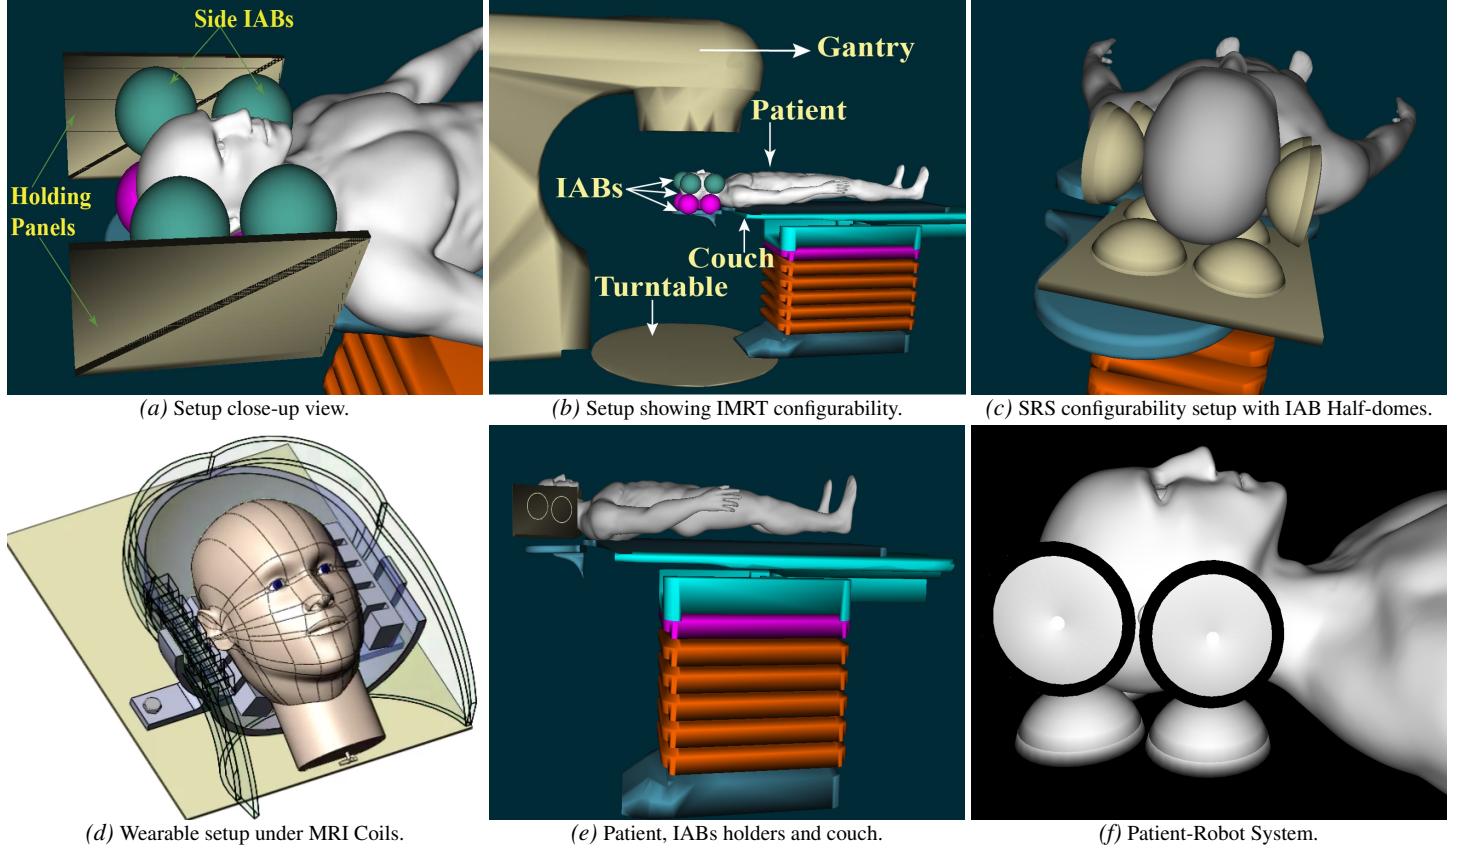


Figure 11: Proposed MRI-compatible LINAC patient motion compensation system.

### Hypothesis.

Owing to the success of parallel robot mechanisms at precise manipulation tasks [2, 20, 66–68], **I hypothesize that a parallel soft-manipulator mechanism will yield the desired submillimeter and subdegree accuracy necessary for online, real-time head motion control in MRI-LINAC RT.**

### Procedure.

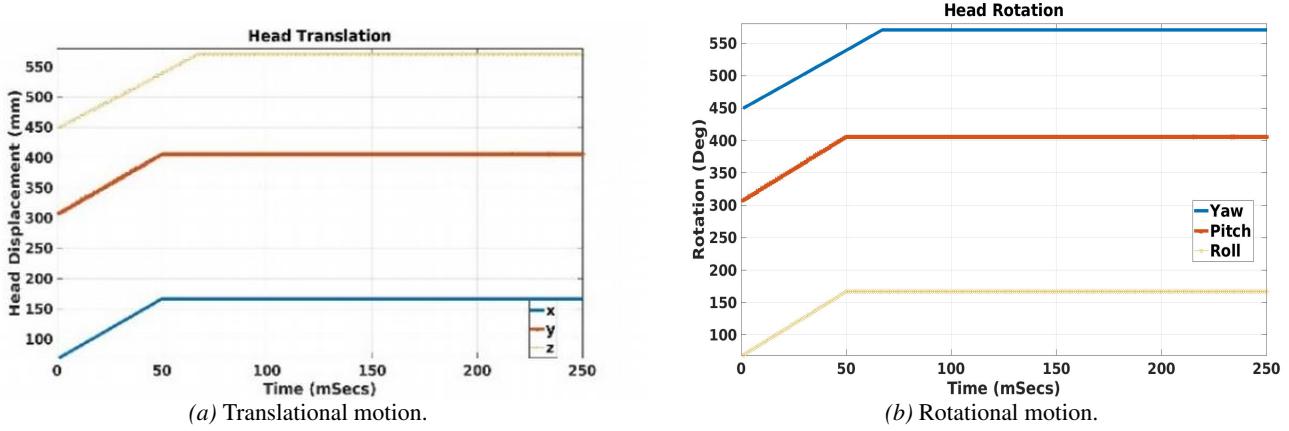


Figure 12: Open-loop setpoint-following for patient’s head motion in  $\mathbb{SE}(3)$ . Reprinted from [13].

**A. Head Motion Correction in  $\mathbb{SE}(3)$ :** I will systematically synthesize and analyze parallel soft robot manipulators for head and neck motion correction in MRI-LINAC systems. I will then leverage the kinematics and kinetics of soft manipulators which I proposed in [28] to construct the hierarchical motion planner in Aim II. Synthesizing multi-DOF parallel soft robots is challenging given the interdependency of the parameters that characterize the deformation, the individual robot constraints’ relative three dimensional orientation, permitted motion orientations, the three dimensional relation between constraints and allowed motions, and the possibility of multiple assembly modes that may result in the same end-effector pose [66]. The configuration that shall be investigated shall consist of soft actuators so arranged that their independent or coupled actuation can produce the needed head motion correction along the left-right (LR), the anterior-posterior (AP) , and/or the ssuperior-inferior (SI) axes. I will analyze the manipulation map, kinematics and kinetics of the respective closed-loop chains, and analyze the contact equations between the IAB system and head.

Fig. 11b shows an example standalone motion correction prototype for an IMRT system while Fig. 11c shows the proposed mechanism for MRI-LINAC systems (without MRI coils). Owing to the modular design, the coils of an MRI can be easily integrated onto this mechanism. In a parallel kinematic manner, the soft domes are positioned around the patient’s cranial region while the patient lies supine on a typical MRI/RT treatment couch (Fig. 11b). The soft domes will be held in place around the head by impact-resistant low-temperature rigid PVC foam insulation sheet that is encased in carbon fiber. Velcro stickers (not shown) will be affixed to the planar soft dome holders to accommodate different patient cranial geometry – thus providing a modularization that ensures re-usability for different patients. The side actuators will correct head motion along the LR axis of the head anatomy *i.e.* (yaw and roll motions), while the bottom ones will correct head motion along the AP direction. The SI motion will be adjusted by the two lower actuators on the bottom of the neck. These will conform deformation in a non-Gaussian fashion through an appropriate configuration of fiber-reinforcing (see [videos](#)). The domes underneath the forehead would control pure  $z$  translation and pitch rotatory motions.

In preliminary work [28], I have synthesized differential kinematics [69], continuum mechanics [70,71] and multi-bodied kinematics. Equation (7) yields the cranial manipulation constraint between the soft actuators and the head so that we can find the respective translational and rotational head velocity components,  $v_h, \omega_h$  respectively in world frames. We can easily find the pseudo inverse of the manipulation map,  $G$  in (7), so as to determine head velocity on the treatment couch. The derivation of this equation is detailed in [27].

**B. Expected Results:** I would expect that my results will follow the open-loop head motion control simulation results in the SOFA [72] framework as presented in my recently accepted publication [13] using the proposed setup of Fig. 11f: raising or rotating the head in  $\mathbb{SE}(3)$  resulted in steady-state reference trajectory tracking along all 6-DoFs of head motion as shown in Fig. 12.

#### R<sub>00</sub> Aim: Patient oncological clinical trials.

To verify accuracy of delivered dose, a complete end-to-end evaluation of the robotic MRI-compatible RT system will be conducted using anthropomorphic phantom studies. From the preliminary data (Fig. 3, 5, 12), whereupon excellent agreement was found between head motion and given target trajectory using the adaptive controller proposed in [20]. Once we ascertain the efficacy of this, we will move to healthy human volunteer trials.

**Statistical Plan:** Phantom-based and healthy human volunteer trials will be conducted after we finish the design and build of the proposed system. A complete end-to-end testing with 3D printed head phantoms containing dosimetric gel will be used to evaluate 3D radiation dose accuracy for both single and multiple target MRI-compatible RT plans. A 20 volunteer study with a mock radiation beam will be conducted in a clinical environment to verify 6DOF head control and patient safety systems. A clinical study on 20 whole brain patients will be performed where validation of method will be determined by a statistical endpoint defining success as to whether or not the 6D intracranial target is  $\leq 0.5\text{mm}$  and  $\leq 0.5^\circ$  for greater than 95% of the treatment time.

# **Training in the Responsible Conduct of Research**

To instruct postdoctoral researchers in responsible conduct of research, the University of Pennsylvania Biomedical Postdoc Program mandates postdoctoral training in responsible conduct of research. This training consists of both online and in-person components.

## ***Format***

The Responsible Conduct of Research (RCR) training consists of both online and in-person components. First year postdocs must complete two introductory online courses designed by the Collaborative Institutional Training Initiative (CITI) at the University of Miami ([citiprogram.org](http://citiprogram.org)). Online courses are intended as a framework for further discussion and development through monthly 90-minute in-person courses in specific topics in responsible conduct of research led by faculty members and staff of the university.

## ***Subject Matter***

Introductory online courses cover: Research misconduct, data management, mentoring, conflicts of interest, publication practices, ethical issues in research, and the use of human and animal subjects. Monthly in-person seminar topics planned for 2020 include collaboration with industry, ethical issues in genome research, ethical issues in peer review, data collection and management, handling conflicts of interest, responsible laboratory procedures, University of Pennsylvania policies concerning research integrity and misconduct reporting, ethical issues in human and animal research, the mentor/mentee relationship, and more.

## ***Faculty Participation***


The RCR seminars are directed by the Biomedical Postdoctoral Program and is led by faculty and staff including professors in the medical and graduate schools, members of the Institutional Animal Care and Use Committee (IACUC), the Institutional Review Board (IRB), as well as staff such as members of the legal department and senior administrators engaged in research compliance efforts. My mentor, Dr. Rodney Wiersma, conducts an annual laboratory-specific RCR session for all lab members. One-on-one training and discussion will also be provided by Dr. Wiersma through supervision of research activities, sharing experience and insight and reviewing scientific issues and ethical challenges associated with my project and related work in the lab.

## ***Duration of Instruction***

The University of Pennsylvania's RCR seminars are 90 minutes long, consisting of ~60 minutes of lecture and ~30 minutes of faculty/staff led discussion or small group case-study exercises.

## ***Frequency of Instruction***

Postdocs must attend at least 8 sessions (12 hours) of these in-person trainings during their tenure at the university.

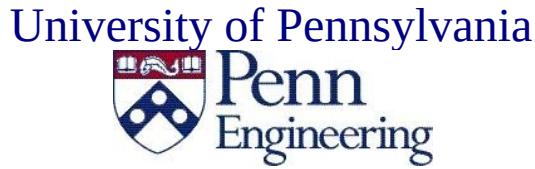

School of Engineering and Applied Science  
Department of Mechanical Engineering  
and Applied Mechanics  
272 Towne Building  
220 South 33<sup>rd</sup> Street  
Philadelphia, PA 19104-6315

Dr. James Pikul  
*Assistant Professor*

Tel: 215.573.2786  
Fax: 215.573.6334  
[pikul@seas.upenn.edu](mailto:pikul@seas.upenn.edu)

May 21, 2020

Dear Selection Committee Members,

I am writing this letter to enthusiastically support Dr. Ogunmolu and his K99/R00 Pathway to Independence Award Application. Dr. Ogunmolu is a wonderful individual who combines excellence as a scholar, a passion to solve health challenges by applying engineering solutions, a bright and cheerful character, and leadership potential. I believe these qualities perfectly align Dr. Ogunmolu with the K99/R00 Pathway to Independence Award, as he will produce excellent fundamental research, realize important benefits for patients, and transition into a strong independent leader.

I have known Dr. Ogunmolu, who goes by ‘Lekan’, since the Fall of 2019 when he contacted me about collaborating on his project to stabilize patient heads during radiation therapy using soft robots. Since that time, I have had several conversations with Lekan and have been able to assess his competency as a researcher and vision for his proposed work, and I have been impressed. Lekan has shown a deep understanding of his field and also quickly learns new information, which makes him a great asset in cross-disciplinary research. Lekan has published work in the top robotics conferences, which shows his ability to plan and realize high quality research. I should mention that publication in these conferences, such as the IEEE International Conference on Robotics and Automation, is equivalent to publishing in a top field journal in the robotics community. This prioritization for conference publications is different than many fields, so I want to make it clear that Lekan has a strong publication record compared to other researchers at his level in the robotics community. Lekan’s invited talks to Open Robotics, Stanford University, and University of Chicago show that he is being recognized for his contributions and is an emerging leader. Lekan has also mentored six students, including two master’s theses. Overall, Lekan has a strong track record of research and mentoring success and a very promising trajectory that make him an excellent candidate for the K99/R00 Pathway to Independence Award.

I am the right mentor for Lekan because I can provide him with the technical advice required for his proposed research to succeed and I have recently started my own lab at the UPenn, so I have a breadth of recent and relevant experiences to share with Lekan. I am looking forward to discussing and supervising Lekan’s experimental designs and professional development. As an example of my professional success as an Assistant Professor, I am mentoring seven graduate

students, two post-doctoral scholars, three master's students (2 graduated), and twelve undergraduates. Fostering a creative research group with diverse experiences is important for me, which is why I have mentored seven female students and four underrepresented minority students. While growing my lab, my group and I have published 9 journal articles (One in *Nature*, several in 10+ IF journals), 5 refereed conference proceedings (one best paper award), and 3 patents applications. To fund this growth, I have led several successful grant proposals including three DARPA projects (one as PI, two as co-PI), an NSF Emerging Frontiers in Research and Innovation on soft robotics (PI), an NSF CAREER award (PI), and an ONR Young Investigator Program award (PI), which sum to total awards over \$6,000,000. I have, additionally, contributed to my research community and University. I am leading the Formula-SAE Penn Electric Racing Team which placed 3<sup>rd</sup> in the nation last summer. I will apply my experience and accumulated knowledge as an Assistant Professor to mentor Lekan. In addition to mentoring Lekan to achieve his own version of success, I will introduce him to other faculty in my network whose work overlaps with Lekan's interest, including the four co-PIs on my NSF EFRI grant that seeks to understand fundamental problems related to the soft devices that Lekan will use.

In summary, I strongly support Lekan's application for the K99/R00 Pathway to Independence Award. He has the technical talent, experiences, and leadership to be a successful PI. This award will allow Lekan to realize his goals of applying engineering solutions and soft robotics to critical health problems, which will ultimately benefit many patients throughout his career.

Sincerely,



James H. Pikul