

4P Assay Tool


Assay Analysis Report

Source file: assay_dataset_3.csv
Generated: 2026-06-07 16:43

Model Parameters

Parameter	Value
A (Low)	2.6895
B (Slope)	1.2642
C (EC50)	43.084
D (High)	0.026
R2	0.9642
SSE	2.7113
Residual SD	0.2241
Estimated LLOQ	10.0
Estimated ULOQ	1000.0

Calibration Curve

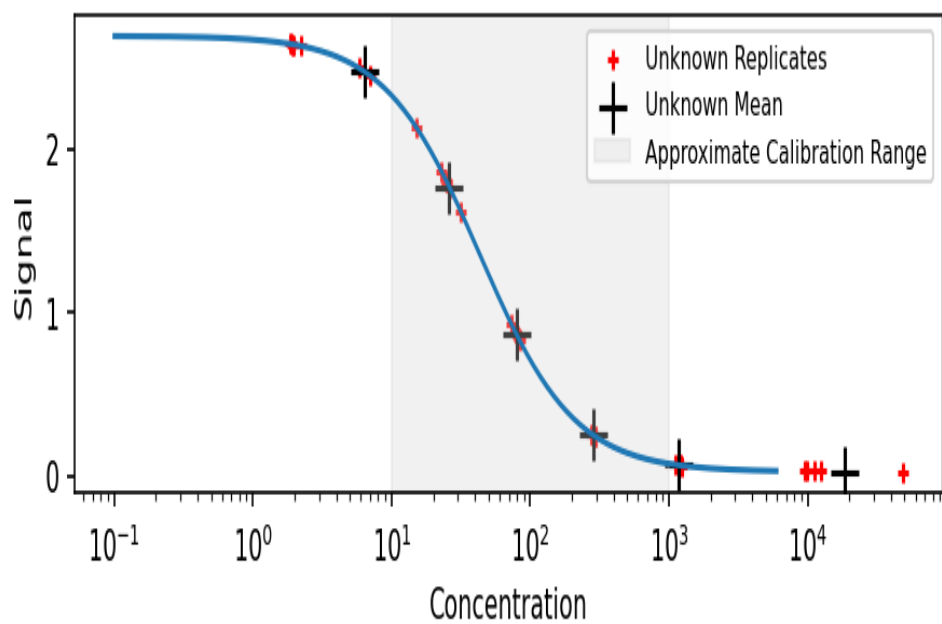

Unknown Samples

Sample ID	N Reps	Mean	CV%	Min	Max	Outliers	Status
S1	5	nan	nan	nan	nan	---	ND
S2	5	nan	nan	nan	nan	---	ND
S3	5	6.4	85.0	1.9	15.2	---	Below LOQ
S4	5	26.1	12.7	22.8	31.7	---	In Range
S5	5	79.7	5.2	73.3	83.8	---	In Range
S6	5	286.0	3.1	275.6	295.3	---	In Range
S7	5	1183.0	4.2	1104.8	1234.6	---	Above LOQ
S8	5	18362.5	92.8	9588.6	48778.4	---	Above LOQ

Calibrators

Calibrator ID	Level	N Reps	Signal Mean	CV%	Concentration Average	% Recovery	Outliers
CAL_0000	0.0	5	3.0571	12.97	---	---	---
CAL_00001	0.1	5	3.0225	13.96	nan	nan	---
CAL_00003	0.3	5	2.4094	16.89	7.92	2639.8	---
CAL_0001	1.0	5	2.5492	7.77	4.38	438.2	---

Calibrator ID	Level	N Reps	Signal Mean	CV%	Concentration Average	% Recovery	Outliers
CAL_0003	3.0	5	2.658	6.91	1.3	43.2	---
CAL_0010	10.0	5	2.3305	2.21	9.9	99.0	---
CAL_0030	30.0	5	1.6561	2.98	30.04	100.1	---
CAL_0100	100.0	5	0.7017	2.17	101.16	101.2	---
CAL_0300	300.0	5	0.2464	1.69	288.88	96.3	---
CAL_1000	1000.0	5	0.0767	2.17	974.08	97.4	---
CAL_3000	3000.0	5	0.0357	1.39	3658.64	122.0	---
CAL_6000	6000.0	5	0.0284	12.96	11012.66	183.5	[0.035]

Appendix — Raw Data

Unknown Sample Raw Replicates

Sample ID	Replicate	Signal	Outlier
S1	1	2.7282	
S1	2	2.7692	
S1	3	2.6406	
S1	4	2.628	
S1	5	2.9087	
S2	1	2.9105	
S2	2	2.7159	
S2	3	2.8625	
S2	4	2.775	
S2	5	2.6378	
S3	1	2.4923	
S3	2	2.6363	
S3	3	2.4437	
S3	4	2.6396	
S3	5	2.1274	
S4	1	1.8656	
S4	2	1.7997	
S4	3	1.7651	
S4	4	1.8001	
S4	5	1.6138	
S5	1	0.8536	
S5	2	0.8785	
S5	3	0.9269	
S5	4	0.8407	
S5	5	0.8282	
S6	1	0.2412	
S6	2	0.2588	
S6	3	0.2515	
S6	4	0.2409	

Sample ID	Replicate	Signal	Outlier
S6	5	0.2538	
S7	1	0.0665	
S7	2	0.0694	
S7	3	0.0638	
S7	4	0.0651	
S7	5	0.0649	
S8	1	0.0264	
S8	2	0.0289	
S8	3	0.0288	
S8	4	0.0284	
S8	5	0.0281	

Calibrator Raw Replicates

Calibrator ID	Level	Replicate	Signal	Outlier
CAL_0000	0.0	1	3.0782	
CAL_0000	0.0	2	2.7226	
CAL_0000	0.0	3	3.1627	
CAL_0000	0.0	4	3.6529	
CAL_0000	0.0	5	2.6689	
CAL_00001	0.1	1	2.6776	
CAL_00001	0.1	2	3.6093	
CAL_00001	0.1	3	3.1922	
CAL_00001	0.1	4	2.5567	
CAL_00001	0.1	5	3.0767	
CAL_00003	0.3	1	2.5871	
CAL_00003	0.3	2	2.5861	
CAL_00003	0.3	3	2.8992	
CAL_00003	0.3	4	1.9456	
CAL_00003	0.3	5	2.029	
CAL_0001	1.0	1	2.596	
CAL_0001	1.0	2	2.4589	
CAL_0001	1.0	3	2.8628	

Calibrator ID	Level	Replicate	Signal	Outlier
CAL_0001	1.0	4	2.4908	
CAL_0001	1.0	5	2.3373	
CAL_0003	3.0	1	2.9365	
CAL_0003	3.0	2	2.6418	
CAL_0003	3.0	3	2.6929	
CAL_0003	3.0	4	2.4328	
CAL_0003	3.0	5	2.5862	
CAL_0010	10.0	1	2.3667	
CAL_0010	10.0	2	2.2585	
CAL_0010	10.0	3	2.3894	
CAL_0010	10.0	4	2.3057	
CAL_0010	10.0	5	2.3322	
CAL_0030	30.0	1	1.622	
CAL_0030	30.0	2	1.7263	
CAL_0030	30.0	3	1.647	
CAL_0030	30.0	4	1.6026	
CAL_0030	30.0	5	1.6825	
CAL_0100	100.0	1	0.6955	
CAL_0100	100.0	2	0.7178	
CAL_0100	100.0	3	0.684	
CAL_0100	100.0	4	0.6938	
CAL_0100	100.0	5	0.7176	
CAL_0300	300.0	1	0.2512	
CAL_0300	300.0	2	0.2483	
CAL_0300	300.0	3	0.2469	
CAL_0300	300.0	4	0.2459	
CAL_0300	300.0	5	0.2399	
CAL_1000	1000.0	1	0.0761	
CAL_1000	1000.0	2	0.0765	
CAL_1000	1000.0	3	0.0789	
CAL_1000	1000.0	4	0.0777	
CAL_1000	1000.0	5	0.0745	
CAL_3000	3000.0	1	0.0358	
CAL_3000	3000.0	2	0.0353	

Calibrator ID	Level	Replicate	Signal	Outlier
CAL_3000	3000.0	3	0.0351	
CAL_3000	3000.0	4	0.036	
CAL_3000	3000.0	5	0.0363	
CAL_6000	6000.0	1	0.0273	
CAL_6000	6000.0	2	0.0263	
CAL_6000	6000.0	3	0.0266	
CAL_6000	6000.0	4	0.027	
CAL_6000	6000.0	5	0.035	YES