E403 Medical Imaging Using Ionizing Radiation

E4.3.1 · E4.3.2 X-ray attenuation and half-value thickness

A monoenergetic narrow beam in uniform material decreases exponentially in intensity. Half-value thickness halves intensity; each additional such thickness halves what remains. A larger attenuation coefficient means smaller half-value thickness. Coefficient and thickness units must cancel. The model does not predict a sudden complete stop at finite thickness.

$$I = I_0 e^{-\mu x}$$

$$x_{1/2} = \frac{\ln 2}{\mu}$$

Uniform medium and monoenergetic narrow beam: I_0: incident intensity; I: transmitted intensity; μ: linear attenuation coefficient; x: thickness. μx must be dimensionless (e.g. cm^{-1} with cm).

$x_{1/2}$: half-value thickness; μ: linear attenuation coefficient. Match units, e.g. cm and cm^{-1}; natural logarithm.

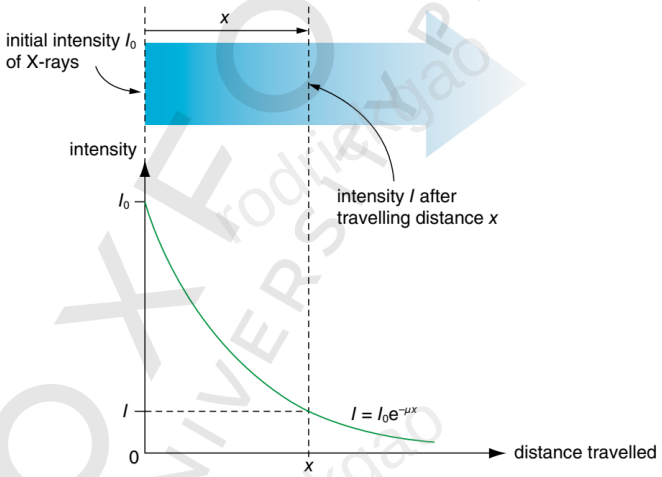


Fig 3.1e *Change in intensity over distance travelled.*

Intensity decreases exponentially with thickness. Equal additional thicknesses reduce the intensity by equal fractions, not equal absolute amounts.

Textbook sources: E403 · PDF 6

E4.3.3 · E4.3.4 Factors affecting X-ray attenuation

Attenuation depends on composition, density and photon energy. With similar composition and energy, greater density generally means stronger attenuation. In common diagnostic-energy ranges away from absorption edges, higher-energy photons usually penetrate more readily. These are conditional trends, not universal rules across all materials and energies.

$$\rho \uparrow \Longrightarrow \mu \uparrow$$

$$E_\gamma \uparrow \implies \mu \downarrow \implies \text{penetration} \uparrow$$

For otherwise comparable material and photon energy, greater density generally increases linear attenuation. Composition and photon energy also matter.

General trend over diagnostic X-ray ranges away from absorption edges, for the same material. Not a universal monotonic law across every photon energy.

Textbook sources: E403 · PDF 7

E4.3.5 Attenuation through several layers

Each layer's transmitted intensity becomes the next layer's incident intensity. Multiply transmission fractions, or add each coefficient-times-thickness term in the exponent. Do not add attenuation percentages directly. Measure each thickness along the actual beam path.

$$I = I_0 e^{-\mu_1 x_1} e^{-\mu_2 x_2} \ldots$$

$$I = I_0 e^{-\sum_i \mu_i x_i}$$

Sequential layers: μ_i: layer attenuation coefficient; x_i: thickness along beam. Each $\mu_i\ x_i$ is dimensionless; exponential narrow-beam model.

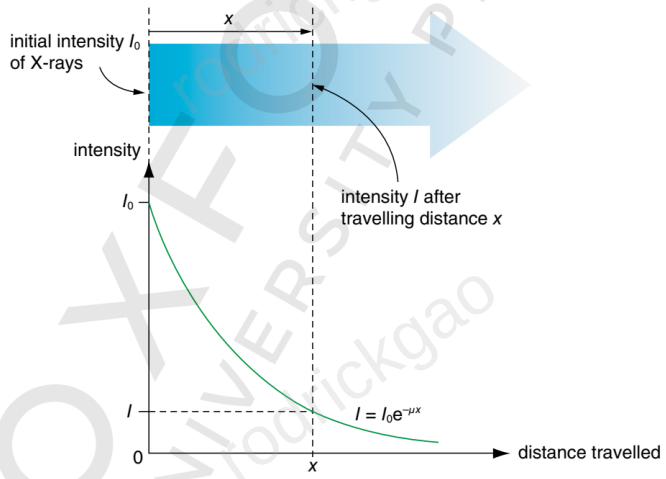


Fig 3.1e *Change in intensity over distance travelled.*

Intensity decreases exponentially with thickness. Equal additional thicknesses reduce the intensity by equal fractions, not equal absolute amounts.

Textbook sources: E403 · PDF 6, 10

E4.3.6 Brightness and darkness in X-ray images

Tissues attenuate X-rays differently, creating contrast in detected transmission. In the conventional textbook display, strongly attenuating structures such as bone appear light and less attenuating regions dark. Digital displays can be inverted, so check the scale. Appearance depends on total path attenuation, not one tissue's density alone.

Textbook sources: E403 · PDF 13


E4.3.7 Contrast agents

An organ is difficult to distinguish when its attenuation resembles surrounding tissue. An appropriate contrast agent changes attenuation in the chosen region, increasing transmitted-intensity differences and contrast. This improves tissue differentiation, not pixel count or the instrument's intrinsic spatial resolution.

Textbook sources: E403 · PDF 16

E4.3.8 CT reconstruction from multiple angles

Computed tomography measures attenuation projections through a section from many directions and reconstructs the distribution of attenuation coefficients computationally. Multiple views separate tissues that overlap in an ordinary projection. A CT section is not a direct photograph from one direction or a result obtainable from one ray alone.

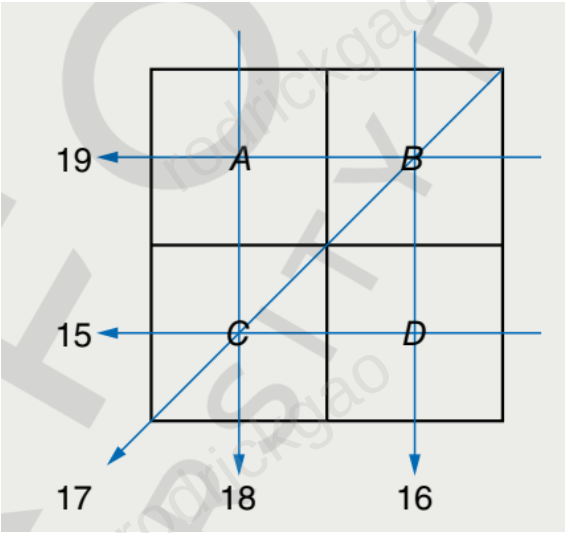

Each beam records attenuation summed along its path. Measurements at several angles constrain the individual regions A–D used to reconstruct the slice.

Textbook sources: E403 · PDF 25

E4.3.9 Pixel area and matrix size

An image matrix states horizontal and vertical pixel counts. For square pixels of area a, side length is $\sqrt{a}$. Express image width W, height H and pixel size in matching units; the matrix is $\frac{W}{\sqrt{a}} \times \frac{H}{\sqrt{a}}$. Multiply the counts for total pixels. A 1024 × 1024 matrix contains 1,048,576 pixels; 1024 is not a physical side length.

Textbook sources: E403 · PDF 26

E4.3.10 Radionuclide imaging

A radioactive tracer distributes within the body according to physiological processes. Detectors measure emitted gamma rays to reconstruct its distribution and reveal function. Unlike external X-ray transmission imaging, the radiation source is inside the body rather than outside with transmitted rays measured beyond it.

Textbook sources: E403 · PDF 35

E4.3.11 Physical half-life

Physical half-life is the time for a nuclide's undecayed population to halve through nuclear decay alone. It is a property of the nuclide and excludes biological removal. Tracer activity in the body can decrease faster because decay and biological clearance operate together.

Textbook sources: E403 · PDF 38

E4.3.12 Biological half-life

Biological half-life is the time for metabolism, excretion or other biological processes to remove half a substance from the body or target region, independently of nuclear decay. It depends on the substance and physiology. Combining it with physical half-life requires approximately independent exponential decreases.

Textbook sources: E403 · PDF 38

E4.3.13 Effective half-life

Tracer quantity decreases through physical decay and biological clearance. For independent exponential processes, removal rates add, giving the reciprocal-sum relation for effective half-life. It is shorter than either finite component half-life, not their mean or sum. Convert both component times to the same units first.

$$\frac{1}{t_e} = \frac{1}{t_p} + \frac{1}{t_b}$$

$$t_e = \frac{t_p t_b}{t_p + t_b}$$

Effective half-life t_e; physical half-life t_p; biological half-life t_b. Independent exponential processes; all three times in identical units. t_e is less than either finite component half-life.

Textbook sources: E403 · PDF 38

E4.3.14 Hot and cold spots in radionuclide images

Hot spots show relatively high tracer uptake and cold spots relatively low uptake. Interpretation depends on the tracer and normal distribution. Textbook greyscale makes hot spots darker and cold spots lighter, but other scales differ. The names do not indicate temperature, nor does every hot spot imply the same diagnosis.

Textbook sources: E403 · PDF 41

E4.3.15 Equivalent dose and radiation weighting

Absorbed dose D is energy absorbed per kilogram, measured in Gy. Equal absorbed doses of different radiation types can have different biological effects. Equivalent dose sums doses multiplied by radiation weighting factors: $H = \sum wD$, in Sv. The textbook uses w = 20 for alpha and w = 1 for beta and gamma. Effective dose additionally accounts for tissue weighting and is not the same quantity.

Textbook sources: E403 · PDF 47