


Clock-preserving microbial residual fusion

Calibration and correction strength selected by inner validation; accuracy assessed in outer participant folds.

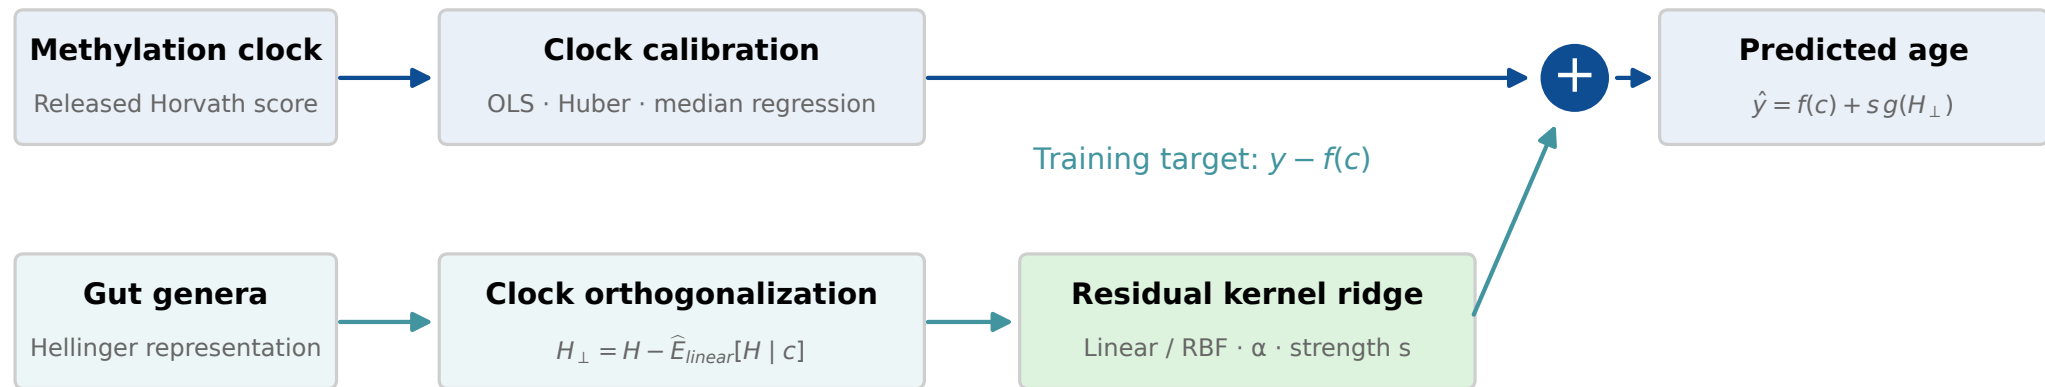

Clock-only fallback: $s = 0$ · All fitted transformations remain inside training folds.