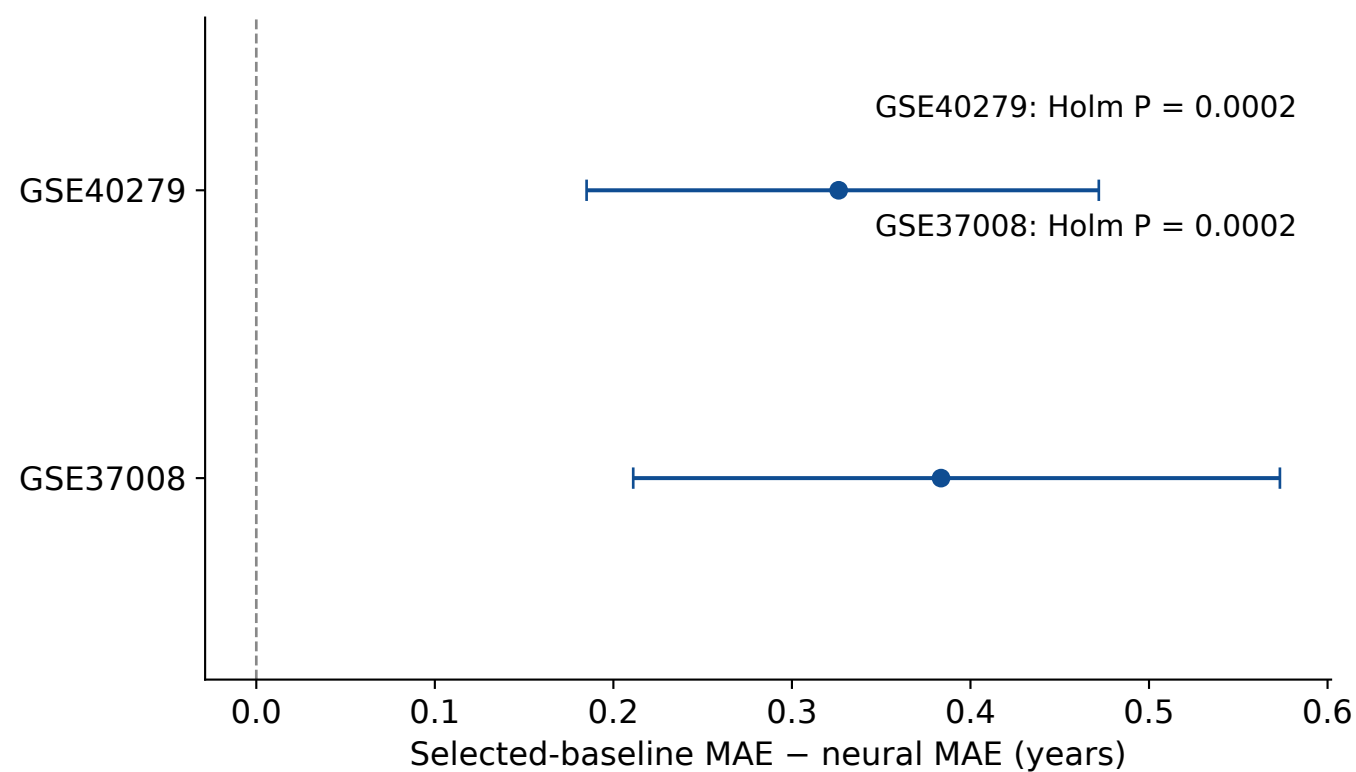
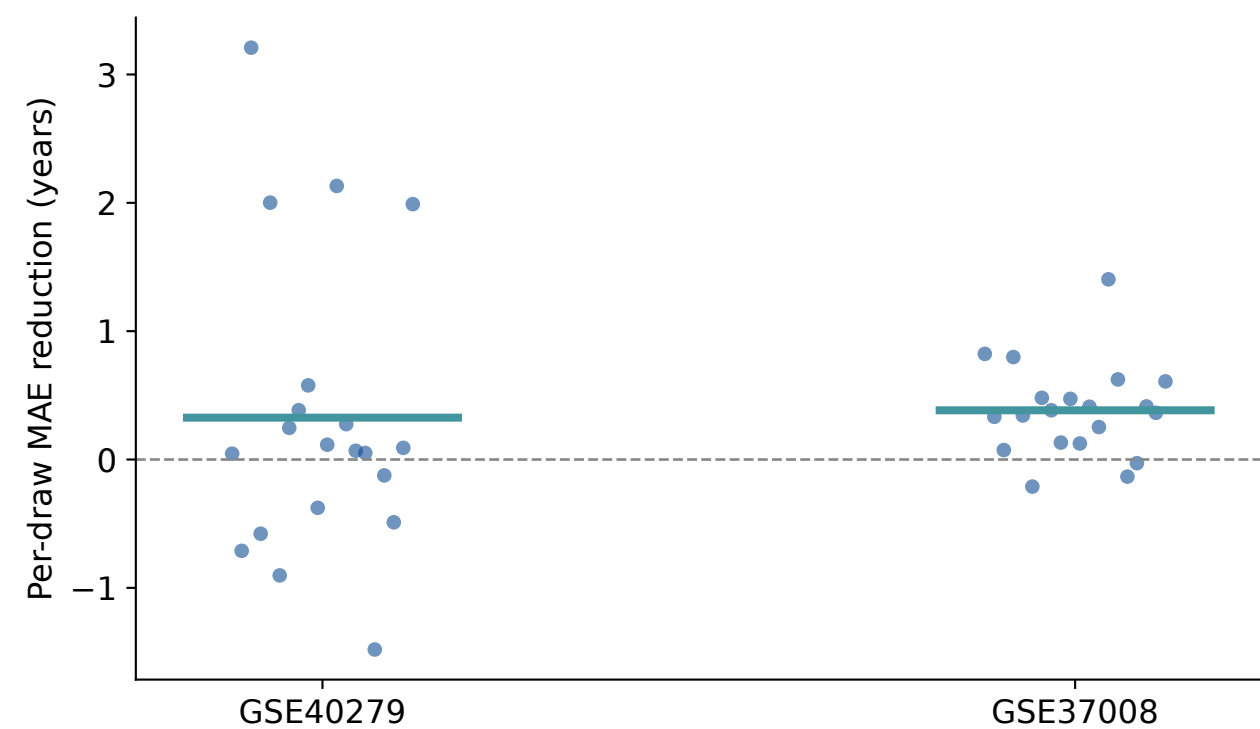
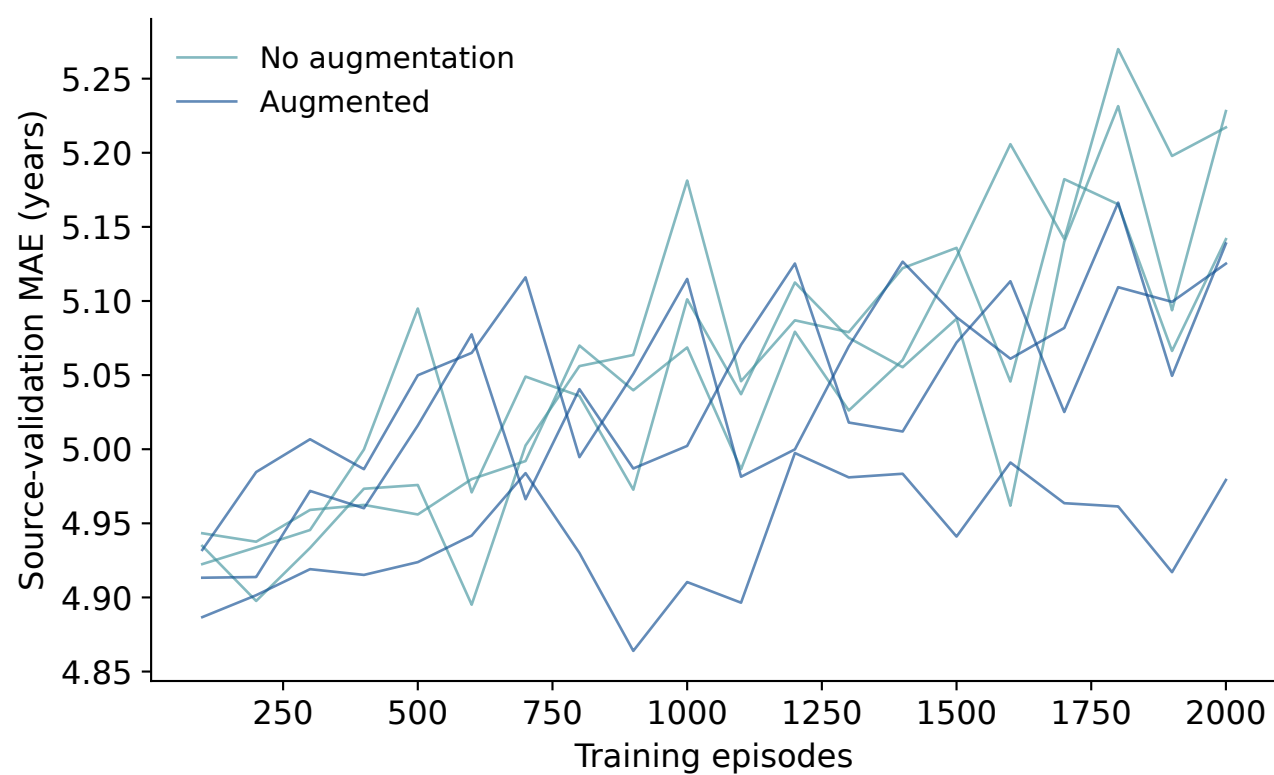
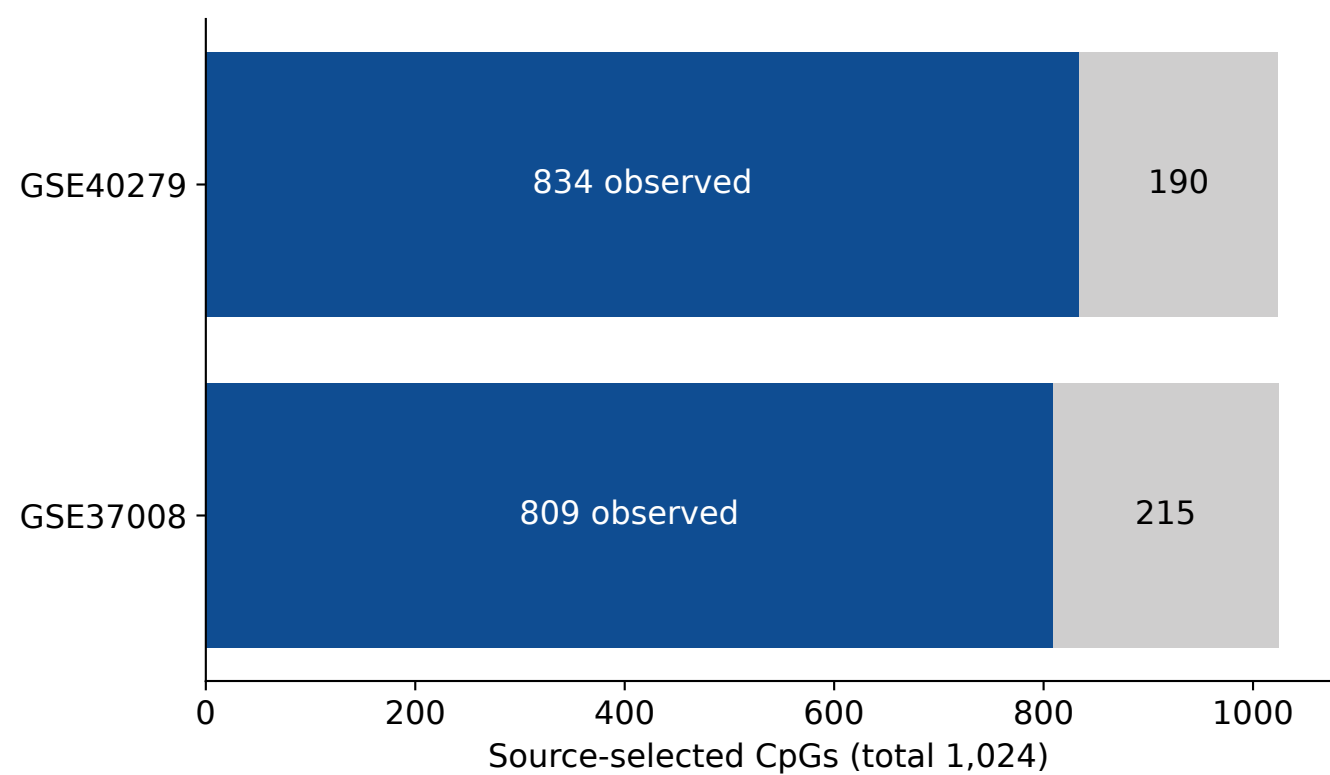
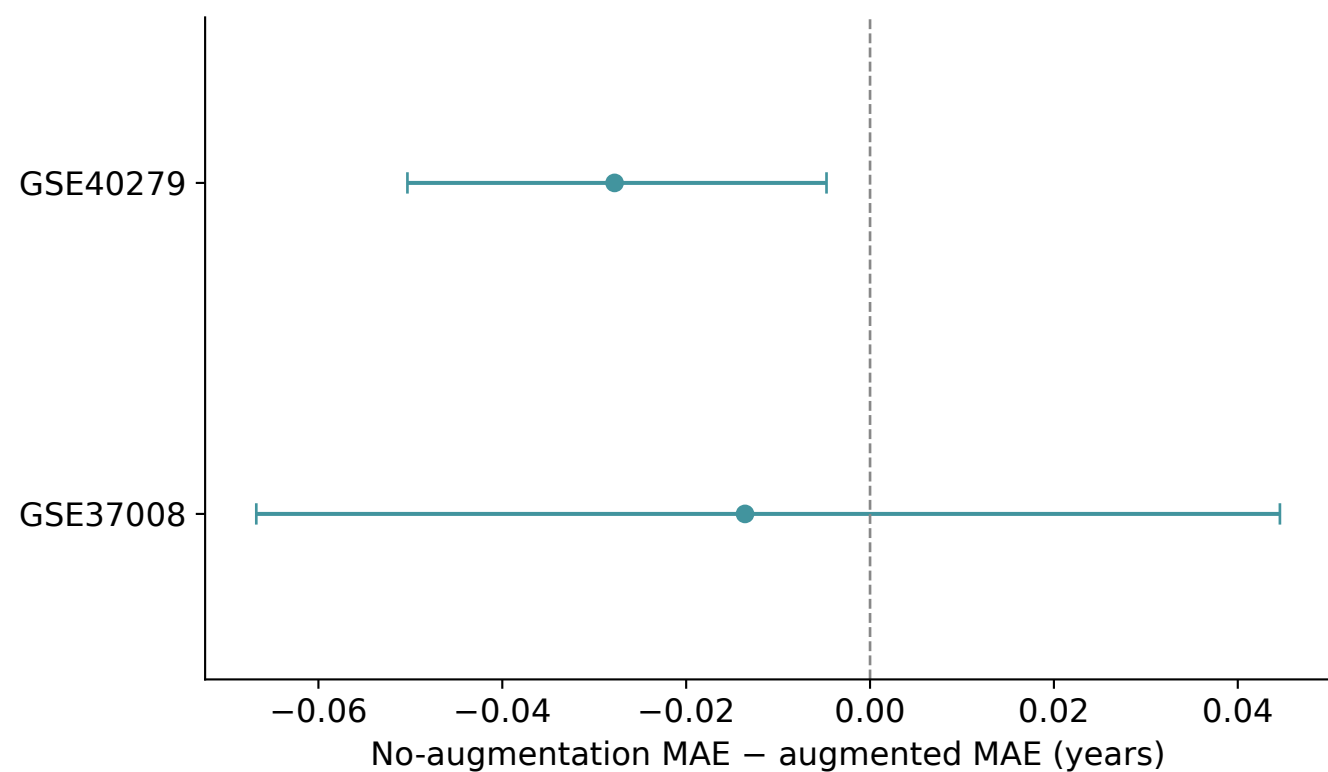


**a Prespecified 16-shot contrasts****b Support-set sensitivity****c Source-only checkpoint selection****d Probe availability in external assays****e Augmentation ablation****f Source-refitting diagnostic (post hoc)**