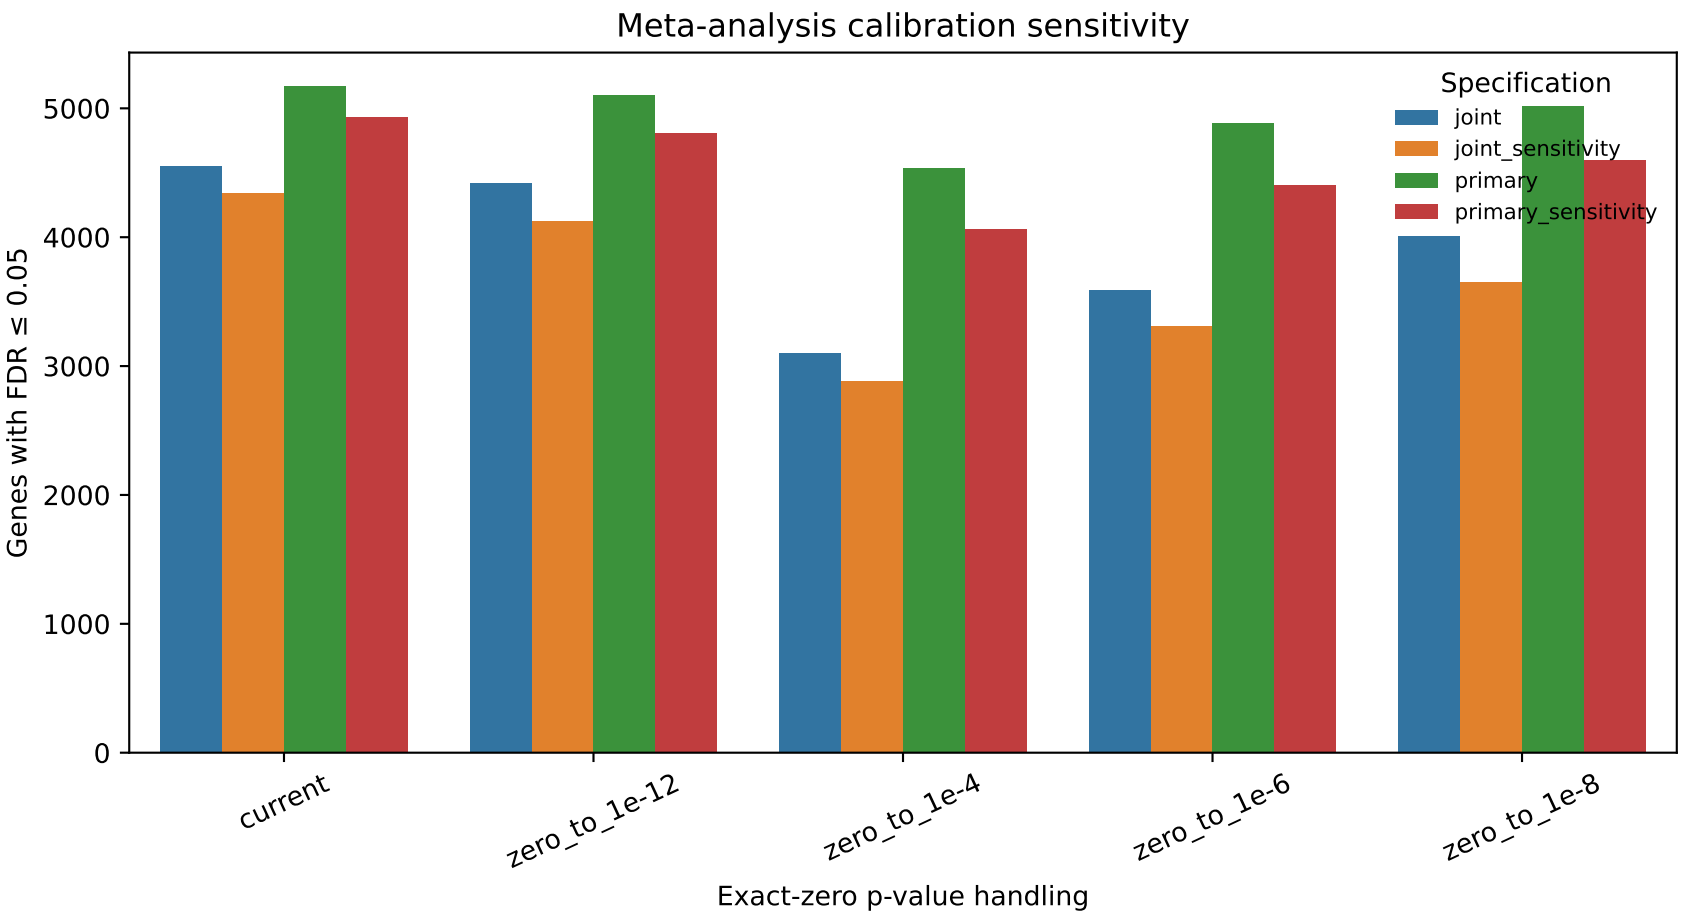
Meta-analysis calibration sensitivity
Specification
joint
joint_sensitivity
primary
primary_sensitivity
Genes with FDR ≤ 0.05
0
1000
2000
3000
4000
5000
current
zero_to_1e-12
zero_to_1e-4
zero_to_1e-6
zero_to_1e-8
Exact-zero p-value handling