VALUE AESTHETIC
MEDICAL SUPPLIER

B E A U T Y S T A R T S W I T H S K I N Q U A L I T Y




LABORATOIRE
REVITACARE
FRANCE

MADE IN FRANCE

Beauty starts with skin quality.

Prevention is the secret to preserve skin youth.
The French secret to keep it, is named CYTOCARE.

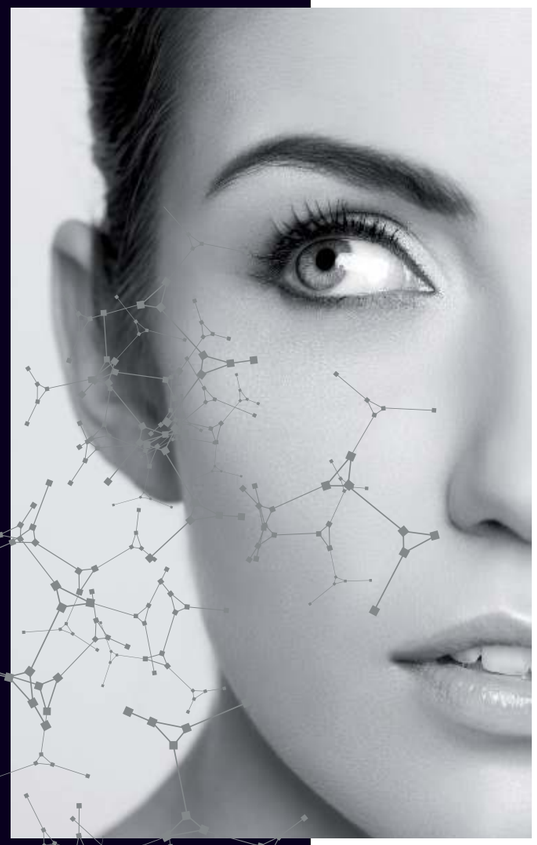

As the years go by, stress, hormonal imbalances and external aggressions such as sun, cold and pollution play a negative role on the quality of the skin.

Fine lines and wrinkles appears, skin becomes thinner, duller and loses its elasticity due to the loss of hyaluronic acid naturally present in the skin.

REVITACARE designs a range of medical devices based on Hyaluronic Acid to:

- Maintain and improve skin quality
- Fill fine lines
- Light up the skin

3 different concentrations of hyaluronic acid (HA) depending on patient skin type.

CYTOCARE 502

(2mg HA / 5mL vial)



maintains skin quality
(filling fine lines, maintaining
hydration and radiance)
of mild skin type

CYTOCARE 516

(16mg HA / 5mL vial)



improves skin quality
(filling fine lines, maintaining
hydration and radiance)
of moderate skin type

CYTOCARE 532

(32mg HA / 5mL vial)



improves skin quality
(filling fine lines, restoration
of radiance) of advanced
skin type

By the end of 3 injection sessions, the patient will observe a slight improvement in the fine lines according to the age and the initial state of the injected area for a duration of 7 days.

VALUE AESTHETIC
MEDICAL SUPPLIER

LABORATOIRE REVITACARE FRANCE



EXCLUSIVE FORMULA

HYALURONIC ACID

(2mg - 16mg - 32mg)

+

REJUVENATING COMPLEX*

=

- Maintains or improves skin quality,
- Preserves skin elasticity**
- Fills fine lines,
- Preserves and restores radiance of the skin,
- Hydrates the skin.**


* Ammonium Molybdate, Ammonium Metavanadate, Calcium Chloride, Iron Sulfate, Potassium Chloride, Copper Sulfate, Magnesium Chloride, Manganese Sulfate, Sodium Acetate, Sodium Hydrogen Carbonate, Sodium Chloride, Sodium Hydrogen Phosphate, Sodium Metasilicate, Sodium Selenite, Tin Chloride, Zinc Sulfate, Alanine, Arginine, Asparagine, Aspartic Acid, Cysteine, Glutamine, Glutamic Acid, Glycine, Histidine, Isoleucine, Leucine, Lysine, Methionine, Phenylalanine, Proline, Serine, Threonine, Tryptophan, Tyrosine, Valine, Adenine, Biotin, Calcium Pantothenate, Coline Chloride, Folic Acid, Inositol, Nicotinamide, Pyridoxine, Riboflavin, Thiamine, Cyanocobalamin, Deoxythymidine, Glucose, Putrescine, Sodium Pyruvate, Lipoic Acid. ** CYTOCARE 502 and CYTOCARE 516

LABORATOIRE REVITACARE FRANCE


VALUE AESTHETIC
MEDICAL SUPPLIER



REVITACARE DATA SOURCE

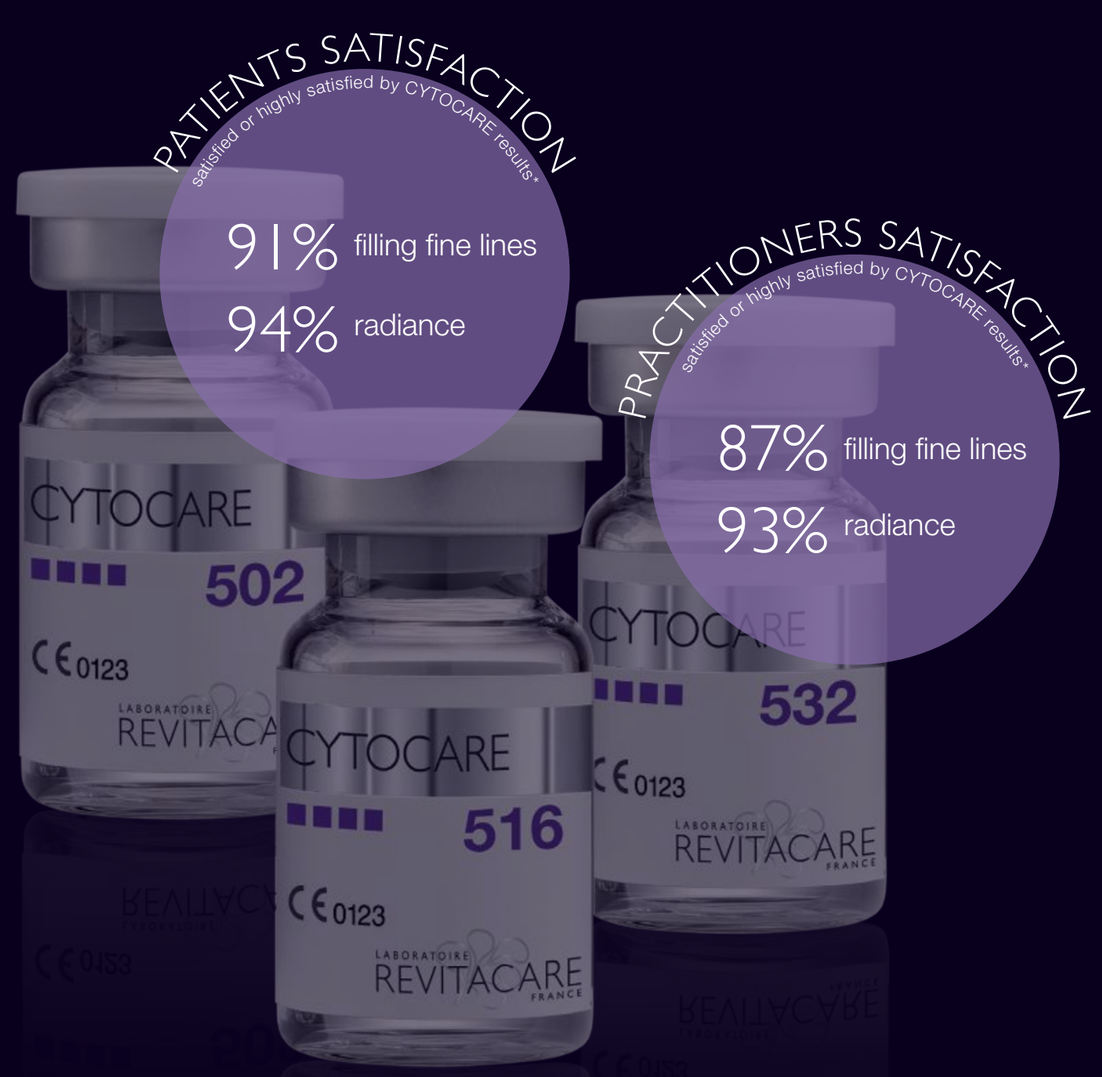

* Multicentric clinical register on 110 patients - Satisfaction upon protocol completion (3 sessions at intervals of 3 weeks)

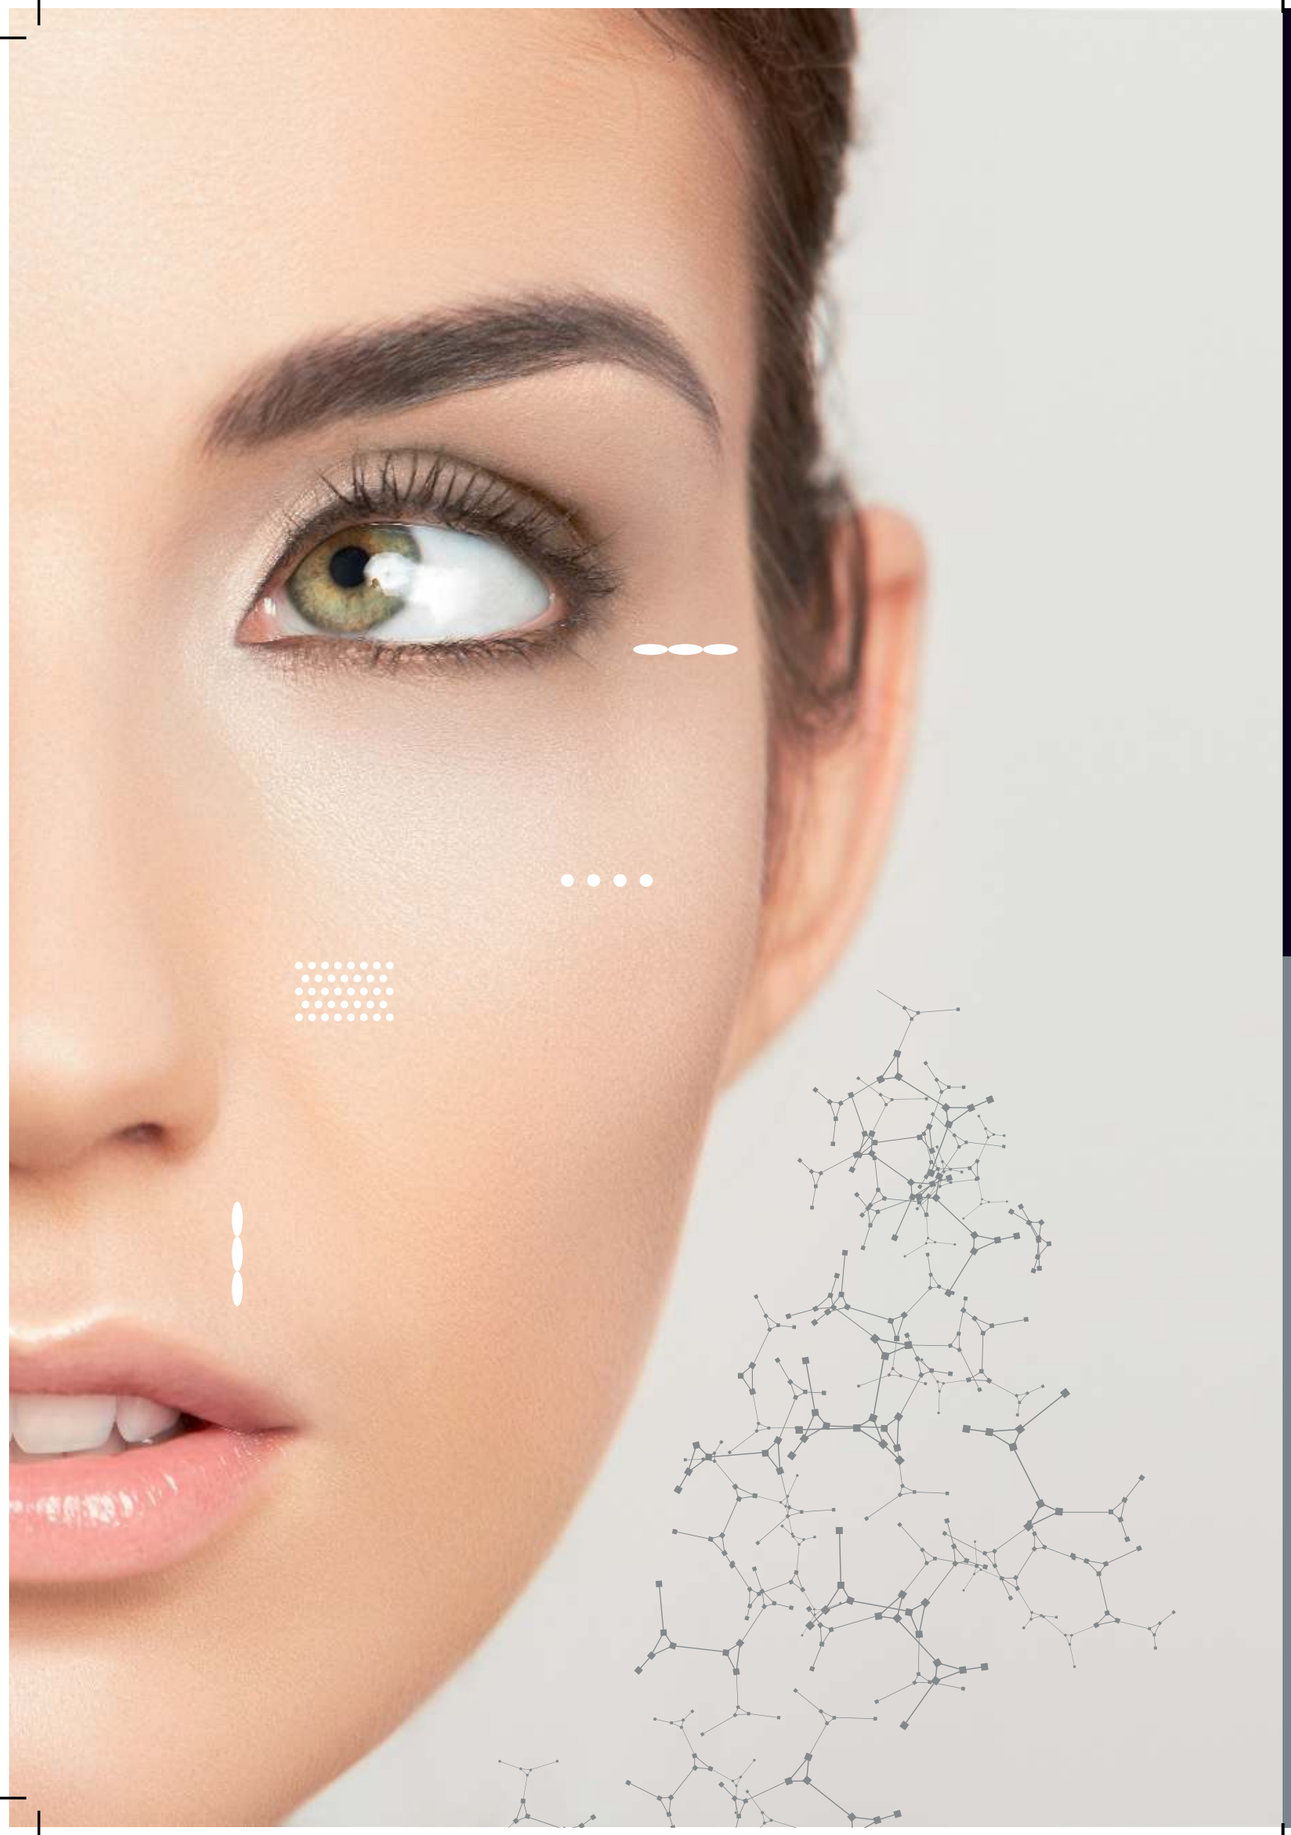

PROTOCOL

- Injection into the medium or superficial dermis of periorbital and perioral lines (vertical lip lines).
- Manual injections with 30G needles.
- Techniques: nappage technique, point by point, retrotracing.
- The protocol is 3 sessions of injections of the content of one vial a maximum of every 3 weeks. Touch-up treatments are needed to maintain the result.
- Read carefully the Instructions For Use before using CYTOCARE 502 -516 -532.

CHARACTERISTICS

- Case: 5 vials x 5 mL - 10 vials x 5 mL
- Sterilization: aseptic filtration
- Pyrogen free
- Ready to use
- Close to neutral pH
- Iso-osmolar solution

CYTOCARE 502-516-532 are sterile single use medical devices class III (CE 0123) manufactured by REVITACARE , indicated to reduce differently ageing effects visible on the face linked to age, life style, or environment. Devices of the CYTOCARE range are intended to be injected into the superficial and medium dermis of periorbital and perioral lines (vertical lip lines). CYTOCARE 502 maintains the skin quality for a short duration (filling fine lines, maintaining hydration and radiance) of mild skin type . CYTOCARE 516 improves skin quality (filling fine lines, maintaining hydration and radiance) of moderate skin type. CYTOCARE 532 improves skin quality (filling fine lines, restoration of radiance) of advanced skin type. By the end of 3 injection sessions, the patient will observe a slight improvement in the fine lines according to the age and the initial state of the injected area for a duration of 7 days. For medical use. Read carefully CYTOCARE 502 - 516 - 532 Instructions For Use before using the product. CYTOCARE 502-516-532 must be injected in an aseptic manner, by duly medical doctor with a good knowledge of the anatomy and physiology of the area to be treated, with sterile and single use equipment not supplied by REVITACARE. Before use CYTOCARE 502-516-532, check the expiry date on the vial labelling, the integrity of the primary packaging and the appearance of the solution. Store between 2°C and 30°C, away from the light in its original secondary packaging. Do not use if package is damaged. Once the vial of CYTOCARE 502-516-532 has been opened, use it immediately. Discard the syringe, needles and the remaining product after use, in accordance with the guidelines in force for their disposal. Single use solution: do not re-sterilise and do not re-use. The medical doctor must inform the patient that there are potential adverse effects linked to the injection of this device, which occur immediately or are delayed.Since CYTOCARE is administered by microinjections, the patient may observe side effects related to the injection techniques. Adverse events observed with CYTOCARE 502-516-532: - pain and bleeding during the injection - tingling, redness, inflammation, hematoma, erythema and itching after the injection - bruising, oedema, nodule, ecchymosis and swelling at the injection site - Infection resulting from incorrect asepsis - Low efficacy. The patient must inform the medical doctor as soon as possible if any adverse events persist for longer than one week. The medical doctor must remedy it by an appropriate treatment. The distributor and / or manufacturer must be alerted to any other adverse event related to the injection of CYTOCARE 502-516-532. Other adverse events observed in the literature with products containing hyaluronic acids (cross-linked or not) or administered by similar methods: - erythema, ecchymosis, swelling, hematoma, bruising, itching, pain, papules, infections, lichenoid eruption, allergy, anaphylaxis, nausea and vomiting, - granuloma, chronic inflammation, bacterial infections with abscess, fibrosis, tissue necrosis, scaring, atrophy, lipodystrophy, post-inflammatory hyperpigmentation, migration of the injected material, - vascular occlusion that may result in impairment of vision. This medical device is a regulated health product which, under this regulation, bears the CE marking. This medical device is not reimbursed by health insurance organisation.

INJECTION TECHNIQUES

Manual injections with 30G needles.

Recommended technique to prevent skin aging effects:

NAPPAGE

Practice very superficial micro-injections spaced of about 1 cm. This technique allows to treat a large skin area following indication.

Recommended techniques to fill cutaneous depressions, smooth epidermis:

POINT BY POINT

Inject linear series of small quantities along the area treated, sufficiently close together to avoid empty space then gently massage the area.


RETROTRACING

Insert the entire length of the needle along the wrinkle to regulary inject the product while removing the needle.

B E A U T Y S T A R T S W I T H S K I N Q U A L I T Y

REVITACARE is a French laboratory, founded in 2003, specialized in research, design, manufacturing of medical devices based on hyaluronic acid, dedicated to aesthetic medicine and cosmetology to prevent, correct the skin aging effects, and treat hair problems.

Our medical devices comply with the essential requirements of the Council Directive 93/42/EEC concerning medical devices and its amendments.

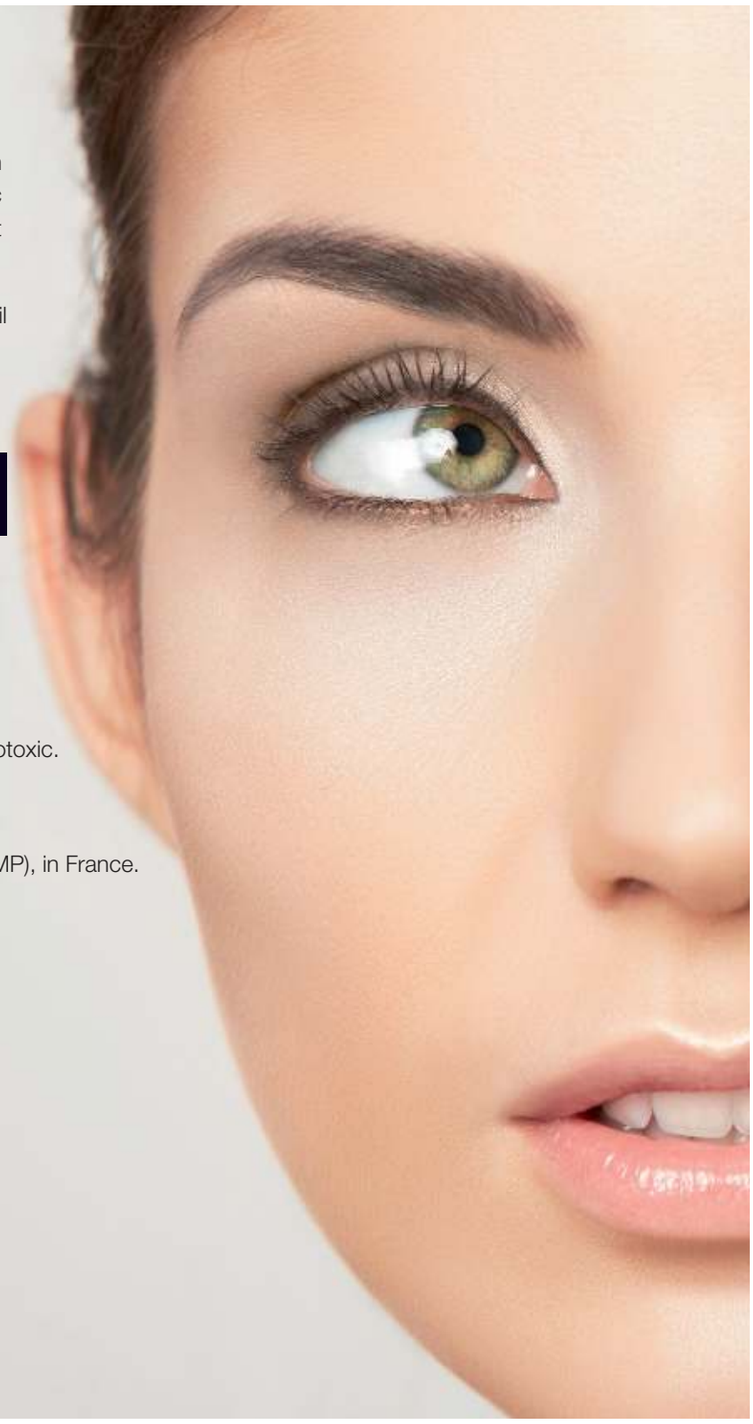

QUALITY • SECURITY • EFFICIENCY

- REVITACARE: EN ISO 13485 certified.
- Class III Medical Devices: CE marking.
- HA quality: biotechnological origin.
- Biocompatible in compliance with ISO 10993 international standards: non cytotoxic - non irritant - non sensitizing - non mutagenic - non genotoxic.
- Microbiological safety.
- Efficiency proved by preclinical and clinical data.
- Manufacturing process according to Good Manufacturing Practices (GMP), in France.

DISTRIBUTOR

VALUE AESTHETIC
MEDICAL SUPPLIER

LABORATOIRE REVITACARE FRANCE

21, avenue de l'Eguillette - Parc d'Activités du Vert Galant
95310 Saint Ouen l'Aumône - FRANCE
Tel: +33 (0) 1 30 37 31 45 - **Email:** contact@revitacare.fr
www.revitacare.net

REF: AIMP091/V04-20-01 – last revision 01/2020