
HAIRCARE
Hair
& Scalp Quality
Sophisticated
Medicine*.
Effortless
Beauty.
*Aesthetic Medicine
VALUE
AESTHETIC
MEDICAL SUPPLIER
REVITACARE
LABORATOIRE · FRANCE

HAIRCARE FORMULA

VALUE
AESTHETIC
MEDICAL SUPPLIER

HAIRCARE

HAIRCARE is a class III device based on non cross-linked Sodium Hyaluronate combined with RHB.



NON CROSS-LINKED SODIUM HYALURONATE

+

RHB: VEHICLE SOLUTION OF NUTRIENTS

- **Amino Acids**

  Arginine, Glutamine, Ornithine, Glycine, Cysteine

- **Vitamins**

  Nicotinamide, Calcium Pantothenate, Folic Acid, Pyridoxine, Biotin, Cyanocobalamin

- **Minerals**

  Zinc Gluconate

Complete list of RHB components: Zinc Gluconate, Arginine, Glutamine, Ornithine, Glycine, Cysteine, Nicotinamide, Calcium Pantothenate, Folic Acid, Pyridoxine, Biotin, Cyanocobalamin, Hepes. None of the components are of animal and/or human origin.



HAIRCARE

VALUE
AESTHETIC
MEDICAL SUPPLIER


HAIRCARE

PACKAGING	10 VIALS OF 5mL
SODIUM HYALURONATE	0.38 mg/mL
RHB	25.66 mg/mL


Intended to improve quality of the hair & the scalp
by restoring hydration and reducing hair loss by anchoring hair follicle




_ Injection depth
Superficial dermis, close to the hair roots



_ Injection techniques
Nappage - Point by point



_ Recommended needle
30G - The use of 5mL syringe and a 18G needle for sampling is recommended.



MODE OF ACTION

HAIRCARE enables to fill the extracellular matrix of the dermal cells, close to hair roots which are invaginated in the scalp dermis, and thus to anchor the hair follicle in the dermal papilla. The duration of tissue residence of HAIRCARE is estimated at 72 to 96 hours.




INJECTION **TECHNIQUES**

HAIRCARE

VALUE AESTHETIC
MEDICAL SUPPLIER


RECOMMENDED INJECTION TECHNIQUES

INJECTION INTO THE SUPERFICIAL DERMIS
with 30G needles, near the hair roots by a medical doctor with experience in the anatomy and physiology of the site of injection.

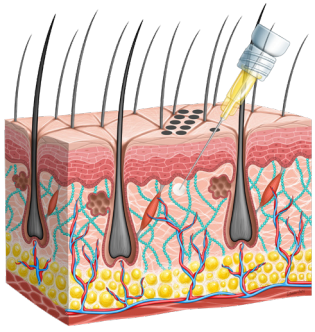

NAPPAGE

Practice very superficial micro-injections.

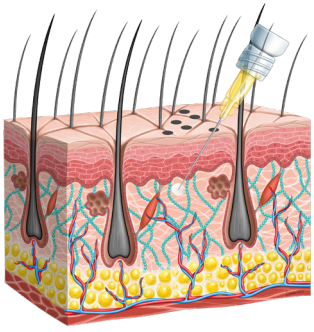

POINT BY POINT

Inject linear series of small quantities, sufficiently close together to avoid empty space then gently massage.




INJECTION **PROTOCOL**

HAIRCARE

VALUE AESTHETIC
MEDICAL SUPPLIER



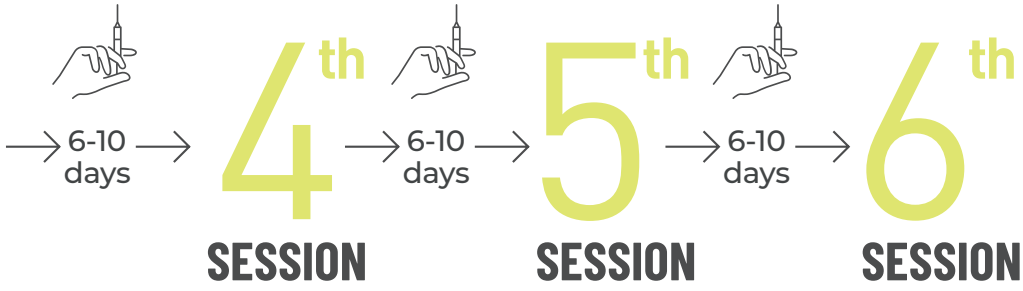

6 SESSIONS	The protocol is 6 sessions of injections of the content of one vial maximum, every 6 - 10 days.
9M	According to the evaluation of the medical doctor, an additional 6-sessions protocol can be performed after observing a minimum of 9-months interval after the last injection session.
	Read carefully the instructions for use before using the product.



HAIRCARE

READ CAREFULLY THE INSTRUCTIONS FOR USE BEFORE USING THE PRODUCT.

HAIRCARE is a sterile single use Class III device (CE 0123) with non medical purpose (mesotherapy) manufactured by REVITACARE, **indicated for** improving quality of the hair and the scalp by restoring hydration and reducing hair loss by anchoring hair follicle. No clinical benefit. HAIRCARE **must be injected** aseptically by a medical doctor with experience in anatomy and physiology of the site to be treated in medical centers, and medical offices, with sterile and single use equipment not supplied by REVITACARE. **Before using** HAIRCARE: Do not use if package is damaged. Check the expiry date on the vial labelling. Check that the solution is transparent. Use at room temperature. Be careful, as the outside of the vials is not sterile. Single use vials, do not reuse or resterilise. Once the vial of HAIRCARE is opened, use it immediately. Discard the vial and the remaining product after use. Refer to the guidelines in force for their disposal. Avoid knocks. **Store** in its original secondary packaging. Store between 2°C and 30°C. Do not freeze. Keep away from frost and heat. Avoid exposure to light. The medical doctor must inform the patient that there are potential undesirable side effects linked to the injection of this device, which may occur immediately or may be delayed. Since HAIRCARE is administered by microinjections, the patient may observe undesirable side effects related to the injection techniques. **Undesirable side effects** observed with HAIRCARE: pain or discomfort during injection, bleeding during the injection, headache, tingling, redness, allergy, swelling, erythema, itching after the injection, lymphadenopathy, infection, haematomas, bruising/ecchymosis, inflammation and oedema. The patient must inform the medical doctor as soon as possible if any **undesirable side effect** persists for longer than one week. The medical doctor must remedy this by an appropriate treatment. The distributor and/or manufacturer must be alerted to any undesirable side effect related to the injection of HAIRCARE. While not observed with HAIRCARE, other undesirable side effects have been observed in the literature with other products containing hyaluronic acids (cross-linked or not) or administered by similar methods: anaphylaxis, necrosis, granuloma, achromia, scalp tightness, pigmentation changes, panniculitis, vascular occlusion, hair loss. While not observed with HAIRCARE, other undesirable side effects have to be considered in common specifications: device visibility through the skin, superficial wound, scarring, hypertrophy, nerve injury, seroma, compartment pressure problems and compartment syndrome. Patient should consult a medical doctor. This device is a regulated **health product** which, under this regulation, bears the CE marking. This device is **not reimbursed** by health insurance organization. HAIRCARE is a Class III device in accordance with Regulation (EU) 2017/745 having obtained CE marking in 2013. HAIRCARE is compliant with the Commission Implementing Regulation (EU) 2022/2346, harmonized standards EN 556-2, EN 556-1, EN ISO 10993-11, EN ISO 10993-16, EN ISO 10993-3, EN ISO 10993-5, EN ISO 13408-2, EN ISO 14155, EN ISO 10993-10, EN ISO 10993-12, EN ISO 10993-17, EN ISO 10993-18, EN ISO 10993-23, EN ISO 10993-9, EN ISO 11137-1+ A2, EN ISO 11137- 2, EN ISO 13485 +A11+AC, EN ISO 14971+ A11, EN ISO 15223-1, and pharmacopoeial monographs EP 2.2.3, EP 2.2.35, EP 2.6.1, EP 2.6.14.

VALUE AESTHETIC
MEDICAL SUPPLIER



Sophisticated Medicine*. Effortless Beauty.
*Aesthetic Medicine

REVITACARE SAS
21, avenue de l'Eguillette
Parc d'Activités du Vert Galant
95310 Saint Ouen l'Aumône - FRANCE
Tel: +33 (0) 1 30 37 31 45
Email: contact@revitacare.fr
revitacare.net

REVITACARE
LABORATOIRE · FRANCE

CO-00531-D
Last modification:
23-03-2026

Document provided and/or issued for strictly personal use in the context of professional medical practice. Do not disclose or altere its content.