

Review of Recent Advancements in RMIS Using dVRK (ROBOTICS M - TECHNICAL ESSAY)

Author:	Ross J. Gardiner
Course code:	ENG5326
Matric nr:	2190583g
Online:	shorturl.at/bnpJY

Abstract

Minimally invasive surgery (MIS) has been shown to reduce patient trauma and accelerate recovery compared with open surgery. Robotically-assisted MIS (RMIS) adds dexterity, surgeon comfort and facilitates higher degrees of precision. The clear market leading device for robotic surgery is the da Vinci system from Intuitive Surgical and additional input from the research community has enabled development of the widely used da Vinci Research Kit (dVRK). In this report, recent advancements for RMIS are explored. This includes novel tooling mechanisms which integrate with the dVRK and a review on automation strategies for subordinate surgical tasks. This work showcases research enabled by the dVRK and contributes some ideas for future developments using the platform.

I. Introduction

In this section, relevant topics are introduced and background context given. The requirement for RMIS is described and dVRK is shown as a key contributor in the literature. Further information is given on report structure.

A. RMIS

Traditional (open) surgery requires large incisions in the body to enable good visibility and ease of access for intricate manoeuvres. Such large incisions can cause internal damage and scar tissue; this creates complications in recovery with many patients never making a return full to health [1].

MIS, also known as keyhole surgery, reduces the amount of harmful incision required. The body is penetrated via small cut openings or natural orifices and tools are manipulated from outside the body with aid from an endoscope. Compared with open surgery, MIS drastically reduces patient trauma, accelerating recovery and the introduction of MIS surgeries have led to lower hospitalisation costs and higher levels of patient comfort [2, 3]. One limitation of MIS is the complex and uncomfortable interface required to manoeuvre instruments. Additionally, the use of remote cameras and viewing displays worsens hand-eye coordination [3, 4]. This is not ergonomic; dexterity and precision are reduced, especially for surgeons performing numerous or lengthy operations.

RMIS make improvements by providing the user with a tailored surgical console. Enhancements include specially designed controls; software for manipulation of surgical end-effectors, including motion scaling and

tremor control; immersive visual displays for improving hand-eye co-ordination and even inclusion of haptic feedback [3]. Instruments are drive-by-wire which even facilitates remote tele-operated surgery and allows for assessment of a surgeon's operating ability [5]. RMIS enables high levels of dexterity and unparalleled surgical precision while providing comfortable and ergonomic controls.

B. Da Vinci and dVRK

RMIS has seen wide adoption throughout the healthcare domain; many systems have been brought to market for a wide range of surgical robotic tasks. Examples include MicroHand from Sang et al. which has recently completed first human trials [6] and the RAVEN-ii robotic surgical system, which presents a platform for researchers with emphasis on modifiable software. However, the RAVEN-ii does not currently operate within appropriate safety margins for human operations [7]. Two more RMIS research platforms are MiroSurge and M7 Surgical Robot [8, Table 1].

Most abundantly used is the da Vinci system, first established in 1999 [5, 9]. This has seen commercial success with over 5 thousand machines in operation worldwide; to date over 7 million surgical procedures have been performed with da Vinci [9]. Da Vinci is ubiquitous in industry - a desirable target platform for researchers.

As da Vinci requires modification to suit researcher needs, Kazanzides et al. introduced the da Vinci Research Kit (dVRK) [10]. The dVRK is open sourced software and hardware allowing a standardised platform for RMIS research on da Vinci machines. In their publication, Kazanzides et al. discuss in detail the mechanical, algorithmic, electronic and sensing aspects of their work and provide access to the dVRK via GitHub channels¹ [10]. The dVRK provides a comprehensive research platform for the most popular RMIS machine in industrial use.

Da Vinci systems and the dVRK have enabled extensive contributions to robotic surgery literature. D'Ettorre et al. report more than 25 thousand articles published using the dVRK platform [9] since 2010. The dVRK is judged the most relevant and mature surgical research platform and this report focuses on publications which make use of it.

C. Report Structure

Introductory material has explained the use-case for MIS and its robotisation, showcased the da Vinci system and highlighted the significance of the dVRK to robotic surgery literature. For the remainder of this report, a search through the literature has been performed, aided by an existing review [9]. Areas of interest established are novel tooling additions compatible with the dVRK and automation of subordinate tasks for RMIS. Literary works in each field are summarised and analysis performed.

¹<https://github.com/jhu-dvrk> - Accessed March 4th 2022

Finally, a conclusion reports overall findings and outlines future research avenues.

II. Tooling Additions

Intuitive Surgical provides a range of da Vinci compatible instruments; a catalogue of tools is available online [11]. The dVRK platform expands this, enabling development of new tooling attachments which may be integrated with da Vinci. In this section, two novel tools in the literature are introduced and analysed.

A. Literature

The da Vinci system lacks a device for bone laceration as is required for some procedures, namely craniotomy [12]. Gordon et al. present an ultrasonic bone cutting tool integrated into the dVRK system [13]. Ultrasound is selected as the cutting method as it lacerates bone much easier than other tissues in the body - particularly advantageous for physically constrictive MIS where an abrasive method may erroneously cut tissues during insertion/manipulation. Design of the system is aided with a finite element analysis model shown to compute a very close resonant frequency for laceration to that recorded in testing. Through use of the dVRK, the system is integrated with the da Vinci software and coupled mechanically. Denavit–Hartenberg parameters for control of the cutting end-effector are also given [13, Table 3].

Work from Diodato et al. showcase a novel manipulator design for improving dexterity using soft robotics [14]. Through use of the dVRK, a da Vinci device is equipped with the pneumatic soft manipulator. An endoscopic camera is attached to its endpoint and control is facilitated via a foot-pedal at the surgeon console. A usability test of the system is carried out, asking non-experts to align the endoscope view with a selection of targets. In this test, controls devised are shown to be easily learnable by humans.

B. Analysis

Significant software and hardware engineering effort has been expended in design of these new apparatus. However, in both cases it is judged that much more realistic evaluations are required to learn about system performance. Work by Gordon et al. includes laceration evaluation on a synthetic bone imitation material². While this serves well as a proof-of-concept, it is known that bone hardness varies throughout the body and between patients [15]; system performance should next be evaluated on a range of real human or animal bone examples.

The work from Diodato et al. includes an evaluation showing the system controls to be easily learnable. However, the testing methodology used is not representative of an MIS scenario. To realistically evaluate system controls, a next step could be to perform a similar procedure using cadavers in place of rudimentary boxes.

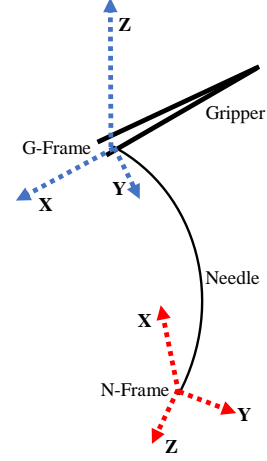


Fig. 1. Gripper (G) and Needle (N) Frames of Reference (adapted from [16, Figure 2(a)]). The G-Frame orients its origin at the tip of the gripper with Z-axis perpendicular to the gripper jaws; X-axis points parallel to the gripper, outwards. The N-Frame orients its origin at the needle tip, in this application needles are curved into a circular shape. The X-axis points towards the centre of needle curvature; Z-axis points tangent to the needle curvature, outwards.

III. Automation

In the recent decade, huge strides in computer vision and AI have enabled machines to automate complex tasks. This section deals with some advances in automation specific to RMIS.

A. Literature - I

Liu and Çavuşoğlu present an extensive study on automated systems for robotic suturing; a novel design account is given for an algorithm to compute optimal needle grasp kinematics [16]. To describe the kinematics, frames of reference are established. Figure 1 shows an adapted illustration.

Four degrees of freedom are given for needle grasp; ω_1 is rotation around the G-Frame Z-axis, ω_2 is rotation around the G-Frame Y-axis, ω_3 is rotation around an axis in the needle plane perpendicular with the X-axis in the N-Frame. Finally, ϑ_0 is the insertion translation for the gripping point selected along the negative X-axis in the G-Frame. Following notation from the paper, φ_0 is the distance in insertion translation while φ_1 , φ_2 , φ_3 are respective rotation angles for ω_1 , ω_2 and ω_3 .

Forward-kinematics are then derived, giving a translation matrix from the G-Frame to the N-Frame, denoted g_{GN} and described by Equations 1 2 and 3 (s_n denotes $\sin(\varphi_n)$; c_n denotes $\cos(\varphi_n)$ and r_n is the radius of needle curvature).

$$g_{GN}(\varphi) = \begin{bmatrix} R(\varphi) & P(\varphi) \\ 0 & 1 \end{bmatrix} \quad (1)$$

$$R(\varphi) = \begin{bmatrix} s_1 s_3 - c_1 c_3 s_2 & -c_1 c_2 & -c_3 s_1 - c_1 s_2 s_3 \\ -c_1 s_3 - c_3 s_1 s_2 & -c_2 s_1 & c_1 c_3 - s_1 s_2 s_3 \\ -c_2 c_3 & s_2 & -c_2 s_3 \end{bmatrix} \quad (2)$$

$$P(\varphi) = \begin{bmatrix} r_n c_1 s_2 (c_3 - 1) - r_n s_1 s_3 - \varphi_0 \\ r_n c_1 s_3 + r_n s_1 s_2 (c_3 - 1) \\ r_n c_2 (c_3 - 1) \end{bmatrix} \quad (3)$$

²Sawbones® Open Cell Foam Block

Needle grasp variants may be explored by changing parameters ϕ_0 , ϕ_1 , ϕ_2 and ϕ_3 . As some configurations are invalid due to reach-ability, joint limits and/or link collision constraints, a feasibility algorithm is developed to assert invalid end-effector positions. Finally, a needle grasp selection algorithm is constructed [16, Algorithm 1]. This operates by taking a set input of potential needle grasps and for each grasp the feasibility over given needle suturing trajectory positions is computed. For needle grasps and trajectory positions deemed feasible, some performance metrics are computed for later comparison.

In experimentation, 3410 pre-set needle grasp positions are evaluated for two suturing trajectories (described as “needle insertion” and “needle extraction”). Findings show that 7.1% of grasps are feasible for needle insertion with 30.1% feasible for extraction. Finally, an optimal grasping pose is shown which scores best on performance metrics for both trajectories.

B. Analysis - I

This work details a process to compare or otherwise discount needle grasp poses for the suturing task. However, for full automation of suturing the question remains as to how these initial pose candidates are generated - no explanation is given for this. The authors mention that execution time for the 3410 poses used on a reasonably high end desktop machine is in the order of minutes. In a real world scenario the algorithm inputs would not be known before a surgery has begun - they would have to be computed ad-hoc. It is judged that minutes of processing time is too lengthy to expend during a surgical procedure. Thus, in its current form this is not usable in theatre. The authors suggest that this may be remedied by implementing the algorithm in faster code. As a proposed alternative, the algorithm described could be used to label numerous grip poses with the evaluation metrics offline (outwith surgery). These labelled data could then be used for supervised deep learning to train a machine capable of inferring an optimal grasp for any given scenario. This model may be more computationally efficient and adjusted for general use by tweaking the training data generated.

C. Literature - II

Surgical procedures can regularly cause bleeding from severed tissue capillaries or internal veins/arteries. Deposited blood must be removed during surgery as to clear the view of the site, this is called hemostasis. Richter et al. propose a solution to automate hemostasis for RMIS [17]. They detail an image processing technique to segment areas of blood identified in camera frames from the operating site. The processing method makes use of multiple temporal frames to identify moving blood pixels, a convolutional neural network is trained to achieve this. With blood location identified, a second algorithm computes the trajectory required for a suction device. These processes are tested on simulated blood flow scenes [17, Figure 4]. In a usability test, the dVRK is used to upload software to a da Vinci machine equipped with camera and a suction tool. An artificial cavity is used with fake blood injected at different points. The system built is shown to consistently remove over 93% of

blood in less than a minute from reaction time through to trajectory completion. Authors note this as the first completely automated hemostasis, complete with dVRK integration.

D. Analysis - II

The publication shows successful development of blood suction automation and a realistic test with a da Vinci machine. However, the computer vision method used necessitates use of multiple frames for detecting moving blood only. This could cause limitations, in particular very slow or stationary blood pools may not be detectable with this method. Further, no test is given where the camera is shaken or otherwise moved as would likely occur in a real surgical procedure, this could cause erroneous segmentation. Per-image segmentation techniques have become highly accurate in recent years. For example Mask R-CNN, developed by Facebook, is shown to score high accuracy on the MS COCO challenge³ [18]. In future research, a per-image segmentation method may yield resilience to camera tremors and/or highly correlated temporal frames.

IV. Conclusions

This essay has investigated software and hardware innovations in RMIS looking specifically at those compatible with the dVRK. For the tooling innovations discussed, it is judged that further evaluation work will better illustrate performance of both devices. For the automation methods, a suggestion is given that the gripper pose selection algorithm could be used as a data labelling mechanism for training a more general AI solution. A suggested variation of the computer vision pipeline for automated hemostasis is also given. Finally, this report complements functionality of the dVRK throughout, enabling all research discussed.

References

- [1] Camran Nezhat, Mailinh Vu, Nataliya Vang, Kavya S. Chavali, and Azadeh Nezhat. “The Journey from Video Laparoscopy to Robotic and Digital Surgery”. In: *Robotic Surgery*. Ed. by Farid Gharagozloo, Vipul R. Patel, Pier Cristoforo Giulianotti, Robert Poston, Rainer Gruessner, and Mark Meyer. Cham: Springer International Publishing, 2021, pp. 3–10. ISBN: 978-3-030-53594-0. DOI: 10.1007/978-3-030-53594-0_1. URL: https://doi.org/10.1007/978-3-030-53594-0_1 (cit. on p. 1).
- [2] Ruben Veldkamp, Esther Kuhry, Wim C J Hop, J Jeekel, G Kazemier, H Jaap Bonjer, Eva Haglind, Lars Pählman, Miguel A Cuesta, Simon Msika, Mario Morino, Antonio M Lacy, and COLon cancer Laparoscopic or Open Resection Study Group (COLOR). “Laparoscopic surgery versus open surgery for colon cancer: short-term outcomes of a randomised trial”. en. In: *Lancet Oncol.* 6.7 (July 2005), pp. 477–484 (cit. on p. 1).

³MS COCO: Microsoft’s Common Objects in Context, online: <https://cocodataset.org/> - Accessed 15th March 2022

- [3] V. Vitiello, K.-W. Kwok, and G.-Z. Yang. “1 - Introduction to robot-assisted minimally invasive surgery (MIS)”. In: *Medical Robotics*. Ed. by Paula Gomes. Woodhead Publishing Series in Biomaterials. Woodhead Publishing, 2012, 1–P1. ISBN: 978-0-85709-130-7. DOI: <https://doi.org/10.1533/9780857097392.1>. URL: <https://www.sciencedirect.com/science/article/pii/B9780857091307500016> (cit. on p. 1).
- [4] Amir Hossein Hadi Hosseinabadi and Septimiu E. Salcudean. “Force Sensing in Robot-assisted Keyhole Endoscopy: A Systematic Survey”. In: *CoRR* abs/2103.11123 (2021). arXiv: 2103.11123. URL: <https://arxiv.org/abs/2103.11123> (cit. on p. 1).
- [5] Ke Liang, Yuan Xing, Jianmin Li, Shuxin Wang, Aimin Li, and Jinhua Li. “Motion control skill assessment based on kinematic analysis of robotic end-effector movements”. In: *The international journal of medical robotics + computer assisted surgery : MRCAS* 14 (June 2017). DOI: 10.1002/rcs.1845 (cit. on p. 1).
- [6] Hongqiang Sang, Shuxin Wang, Jianmin Li, Chao He, Lin'an Zhang, and Xiaofei Wang. “Control design and implementation of a novel master-slave surgery robot system, MicroHand A”. In: *The International Journal of Medical Robotics and Computer Assisted Surgery* 7.3 (2011), pp. 334–347. DOI: <https://doi.org/10.1002/rcs.403>. URL: <https://onlinelibrary.wiley.com/doi/abs/10.1002/rcs.403> (cit. on p. 1).
- [7] Blake Hannaford, Jacob Rosen, Diana W. Friedman, Hawkeye King, Phillip Roan, Lei Cheng, Daniel Glozman, Ji Ma, Sina Nia Kosari, and Lee White. “Raven-II: An Open Platform for Surgical Robotics Research”. In: *IEEE Transactions on Biomedical Engineering* 60.4 (2013), pp. 954–959. DOI: 10.1109/TBME.2012.2228858 (cit. on p. 1).
- [8] Suren Kumar, Pankaj Singhal, and Venkat N. Krovi. “Computer-Vision-Based Decision Support in Surgical Robotics”. In: *IEEE Design Test* 32.5 (2015), pp. 89–97. DOI: 10.1109/MDAT.2015.2465135 (cit. on p. 1).
- [9] Claudia D’Ettorre, Andrea Mariani, Agostino Stilli, Ferdinando Rodriguez y Baena, Pietro Valdastrì, Anton Deguet, Peter Kazanzides, Russell H. Taylor, Gregory S. Fischer, Simon P. DiMaio, Arianna Menciassi, and Danail Stoyanov. “Accelerating Surgical Robotics Research: A Review of 10 Years With the da Vinci Research Kit”. In: *IEEE Robotics & Automation Magazine* 28.4 (Dec. 2021), pp. 56–78. ISSN: 1558-223X. DOI: 10.1109/mra.2021.3101646. URL: <http://dx.doi.org/10.1109/MRA.2021.3101646> (cit. on p. 1).
- [10] Peter Kazanzides, Zihan Chen, Anton Deguet, Gregory S. Fischer, Russell H. Taylor, and Simon P. DiMaio. “An Open-Source Research Kit for the da Vinci Surgical System”. In: *IEEE Intl. Conf. on Robotics and Auto. (ICRA)*. Hong Kong, China, June 1, 2014, pp. 6434–6439 (cit. on p. 1).
- [11] Intuitive Surgical. *Da Vinci Xi: Instrument & Accessory Catalog*. URL: <https://www.intuitive.com/en-us/-/Media/ISI/Intuitive/pdf/davinci-x-xi-instrument-accessory-us-catalog-1052082.pdf> (cit. on p. 2).
- [12] Ricardo J Fernández-de Thomas and Orlando De Jesus. “Craniotomy”. en. In: *StatPearls*. Treasure Island (FL): StatPearls Publishing, Jan. 2022 (cit. on p. 2).
- [13] Alex Gordon, Thomas Looi, James Drake, and Christopher R. Forrest. “An Ultrasonic Bone Cutting Tool for the da Vinci Research Kit”. In: *2018 IEEE International Conference on Robotics and Automation (ICRA)*. 2018, pp. 6645–6650. DOI: 10.1109/ICRA.2018.8460797 (cit. on p. 2).
- [14] Alessandro Diodato, Margherita Brancadoro, Giacomo De Rossi, Haider Abidi, Diego Dall’Alba, Riccardo Muradore, Gastone Ciuti, Paolo Fiorini, Arianna Menciassi, and Matteo Cianchetti. “Soft Robotic Manipulator for Improving Dexterity in Minimally Invasive Surgery”. In: *Surgical Innovation* 25.1 (2018). PMID: 29303068, pp. 69–76. DOI: 10.1177/1553350617745953. URL: <https://doi.org/10.1177/1553350617745953> (cit. on p. 2).
- [15] Wei-wei Wu, Yan-bin Zhu, Wei Chen, Sheng Li, Bing Yin, Jian-zhao Wang, Xiao-juan Zhang, Guo-bin Liu, Zu-sheng Hu, and Ying-ze Zhang. “Bone Hardness of Different Anatomical Regions of Human Radius and its Impact on the Pullout Strength of Screws”. In: *Orthopaedic Surgery* 11 (Mar. 2019). DOI: 10.1111/os.12436 (cit. on p. 2).
- [16] Taoming Liu and M. Cenk Çavuşoğlu. “Optimal needle grasp selection for automatic execution of suturing tasks in robotic minimally invasive surgery”. In: *2015 IEEE International Conference on Robotics and Automation (ICRA)*. 2015, pp. 2894–2900. DOI: 10.1109/ICRA.2015.7139594 (cit. on p. 2, 3).
- [17] Florian Richter, Shihao Shen, Fei Liu, Jingbin Huang, Emily K. Funk, Ryan K. Orosco, and Michael C. Yip. “Autonomous Robotic Suction to Clear the Surgical Field for Hemostasis using Image-based Blood Flow Detection”. In: *CoRR* abs/2010.08441 (2020). arXiv: 2010.08441. URL: <https://arxiv.org/abs/2010.08441> (cit. on p. 3).

- [18] Kaiming He, Georgia Gkioxari, Piotr Dollár, and Ross Girshick. “Mask R-CNN”. In: *2017 IEEE International Conference on Computer Vision (ICCV)*. 2017, pp. 2980–2988. DOI: 10 . 1109 / ICCV . 2017 . 322 (cit. on p. 3).