

## TEST REPORT

(Electronic version)



No:200071822

VERIFICATION WEBSITE: [www.gttc.net.cn](http://www.gttc.net.cn)

VERIFICATION CODE: ENHC-7840-34

ISSUE DATE:2020-04-11

二维码下载报告



APPLICANT: HUNAN NATURE PHARMACEUTICAL CO., LTD  
ADDRESS: NO. 588, HUTANG WEST ROAD, LENG SHUI TAN DISTRICT, YONGZHOU CITY, HUNAN PROVINCE

## SAMPLE INFORMATION:

DISPOSABLE MEDICAL MASK

QUANTITY: FIFTEEN PIECES

MANUFACTURE'S NAME: HUNAN NATURE PHARMACEUTICAL CO., LTD

DATE RECEIVED/DATE TEST STARTED: 2020-04-10

## CONCLUSION:

AIRFLOW RESISTANCE

M


NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT  
"---" -NO COMMENT

## REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200053507.  
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).  
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.  
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

WanLi Hu ENGINEER




PAGE 1 OF 3

# TEST REPORT

(Electronic version)

No:200071822

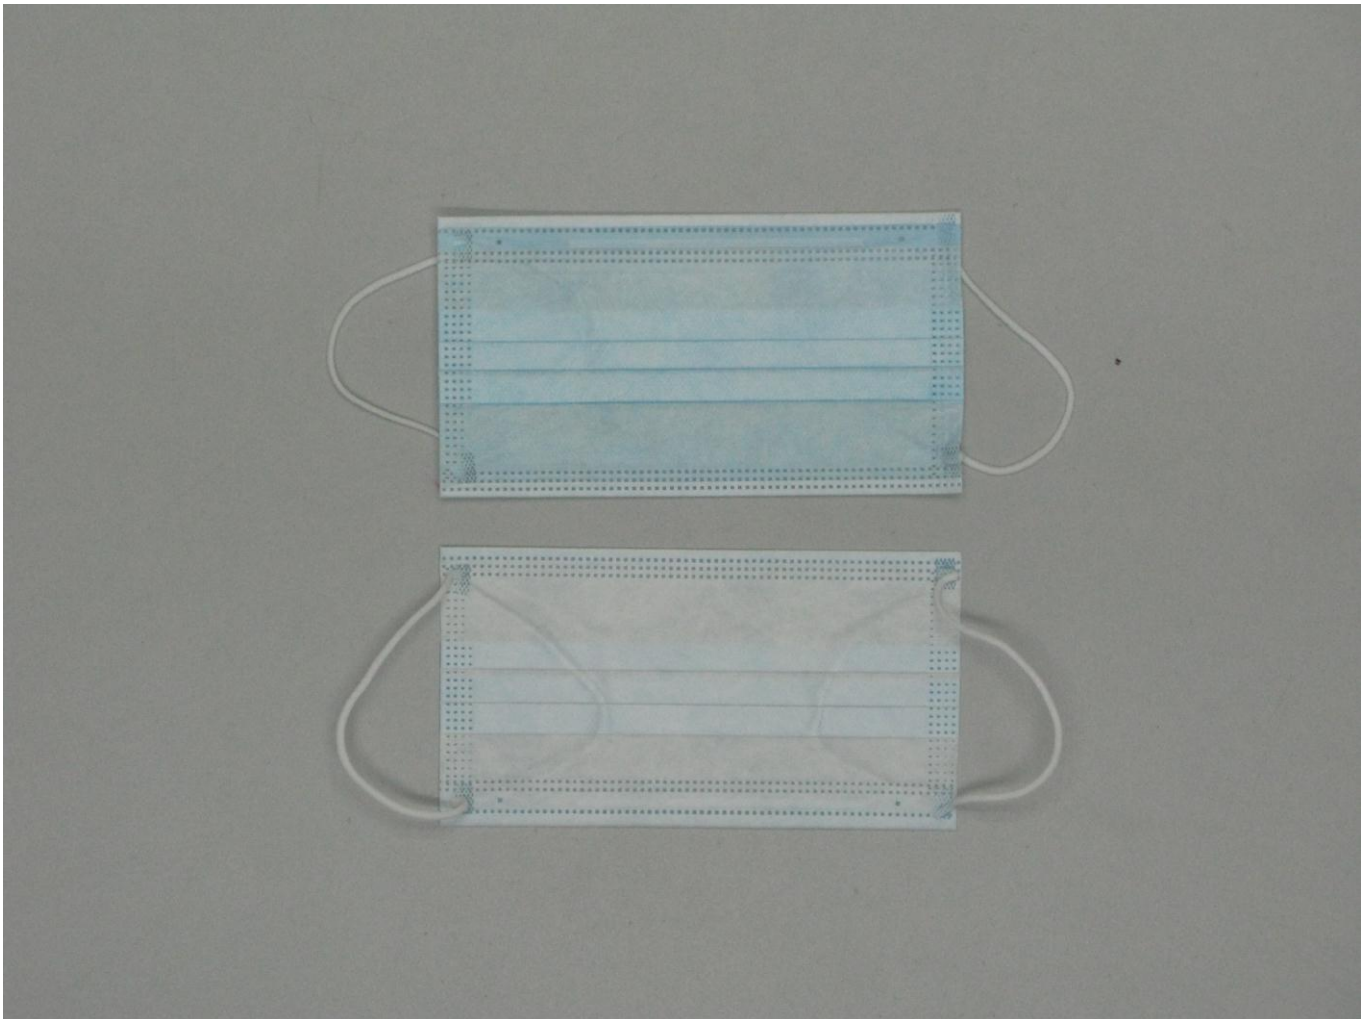

## TEST REPORT

(Electronic version)

No:200071822

AIRFLOW RESISTANCE (Pa/cm<sup>2</sup> )  
(YY/T 0969-2013 5.6)

1# 32.7  
2# 37.1  
3# 34.9

REQUIREMENT  
≤49  
(YY/T 0969-2013)



——End of Report——

PAGE 3 OF 3