



®

[Medical Device Registration Certificate Number] 辽械注准20202140069
[Number of Product Technical Requirements] 辽械注准20202140069
[Production License Number] 辽食药监械生产许20200023号
[Implementation Standards] GB19083-2010

始于1634年

STERILE

STERILE EQ



N95

Medical Protective Mask


CE FDA



Filtration efficiency of non-oily particles is more than 95%.

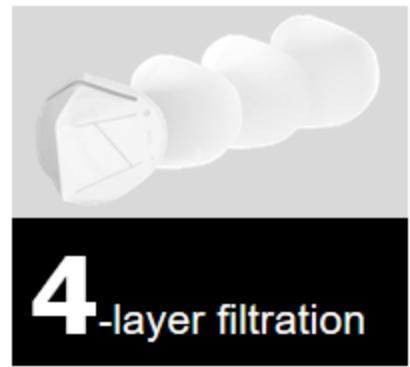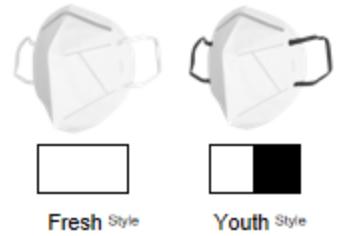

Liaoning Shengjingtang Biotechnology Co., Ltd.

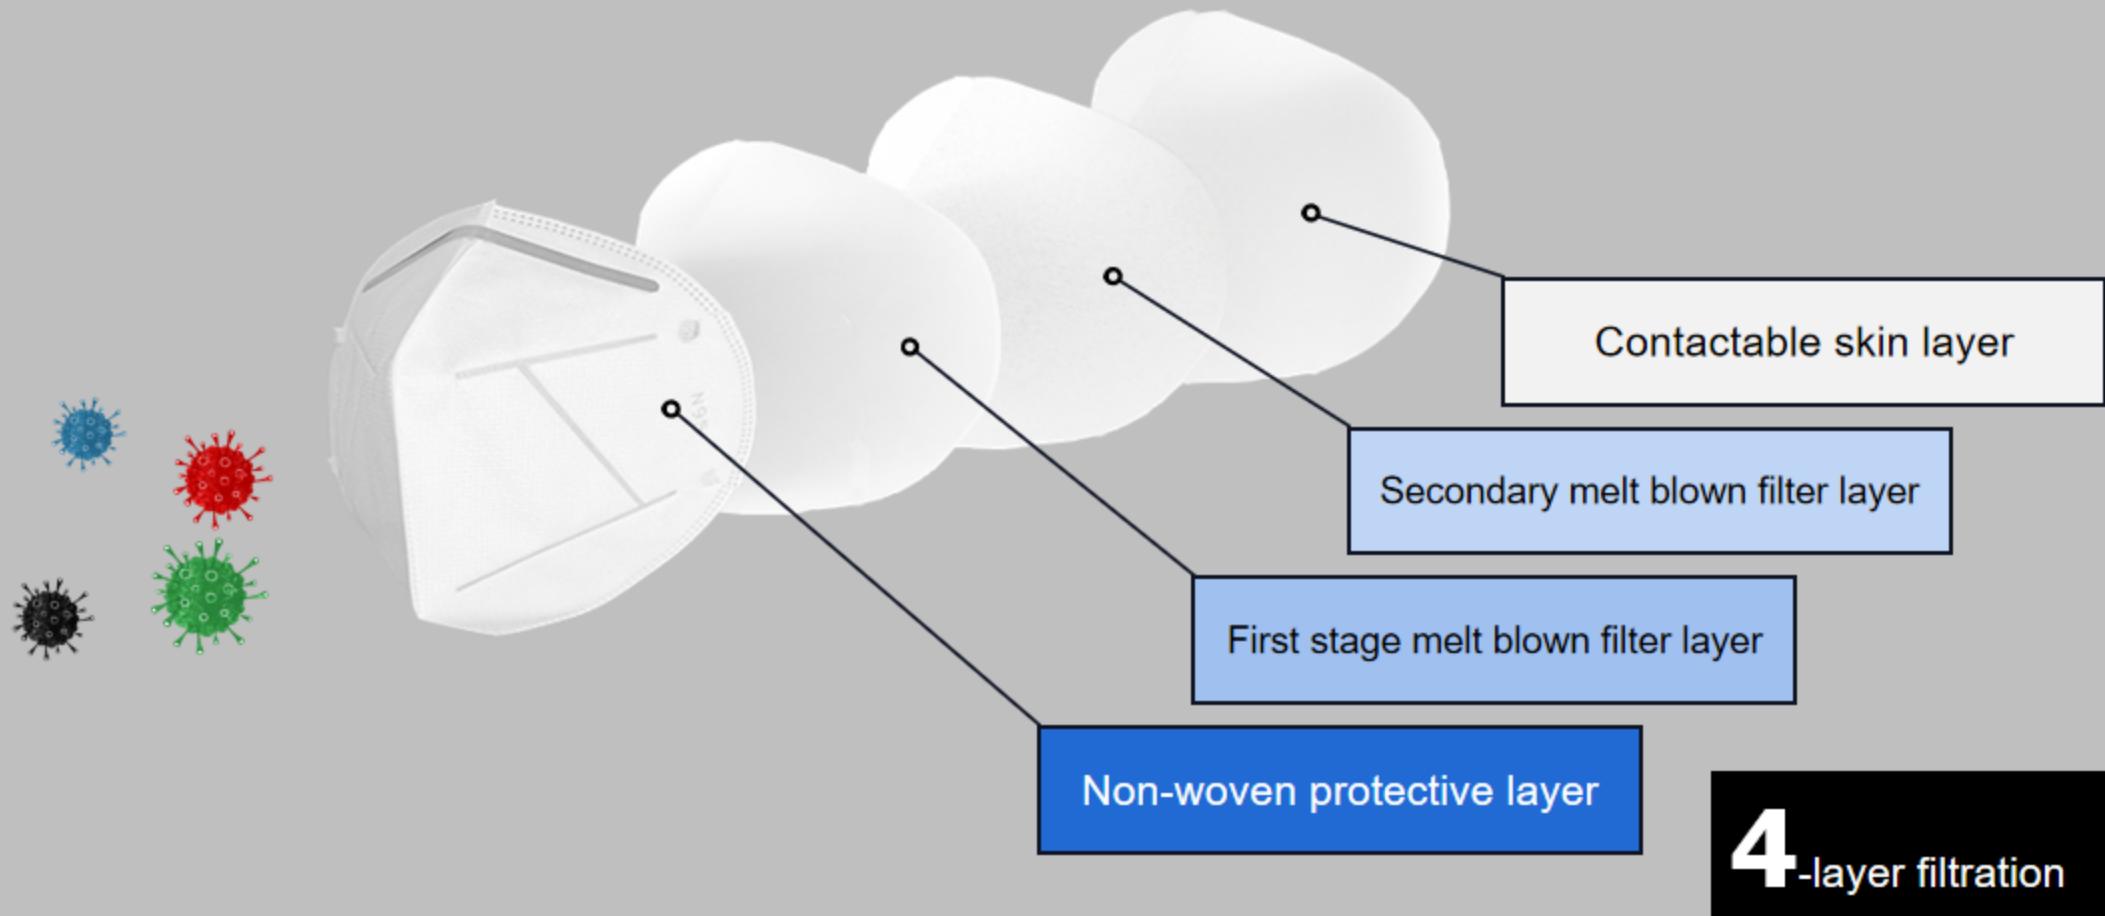




Fresh Style



Youth Style

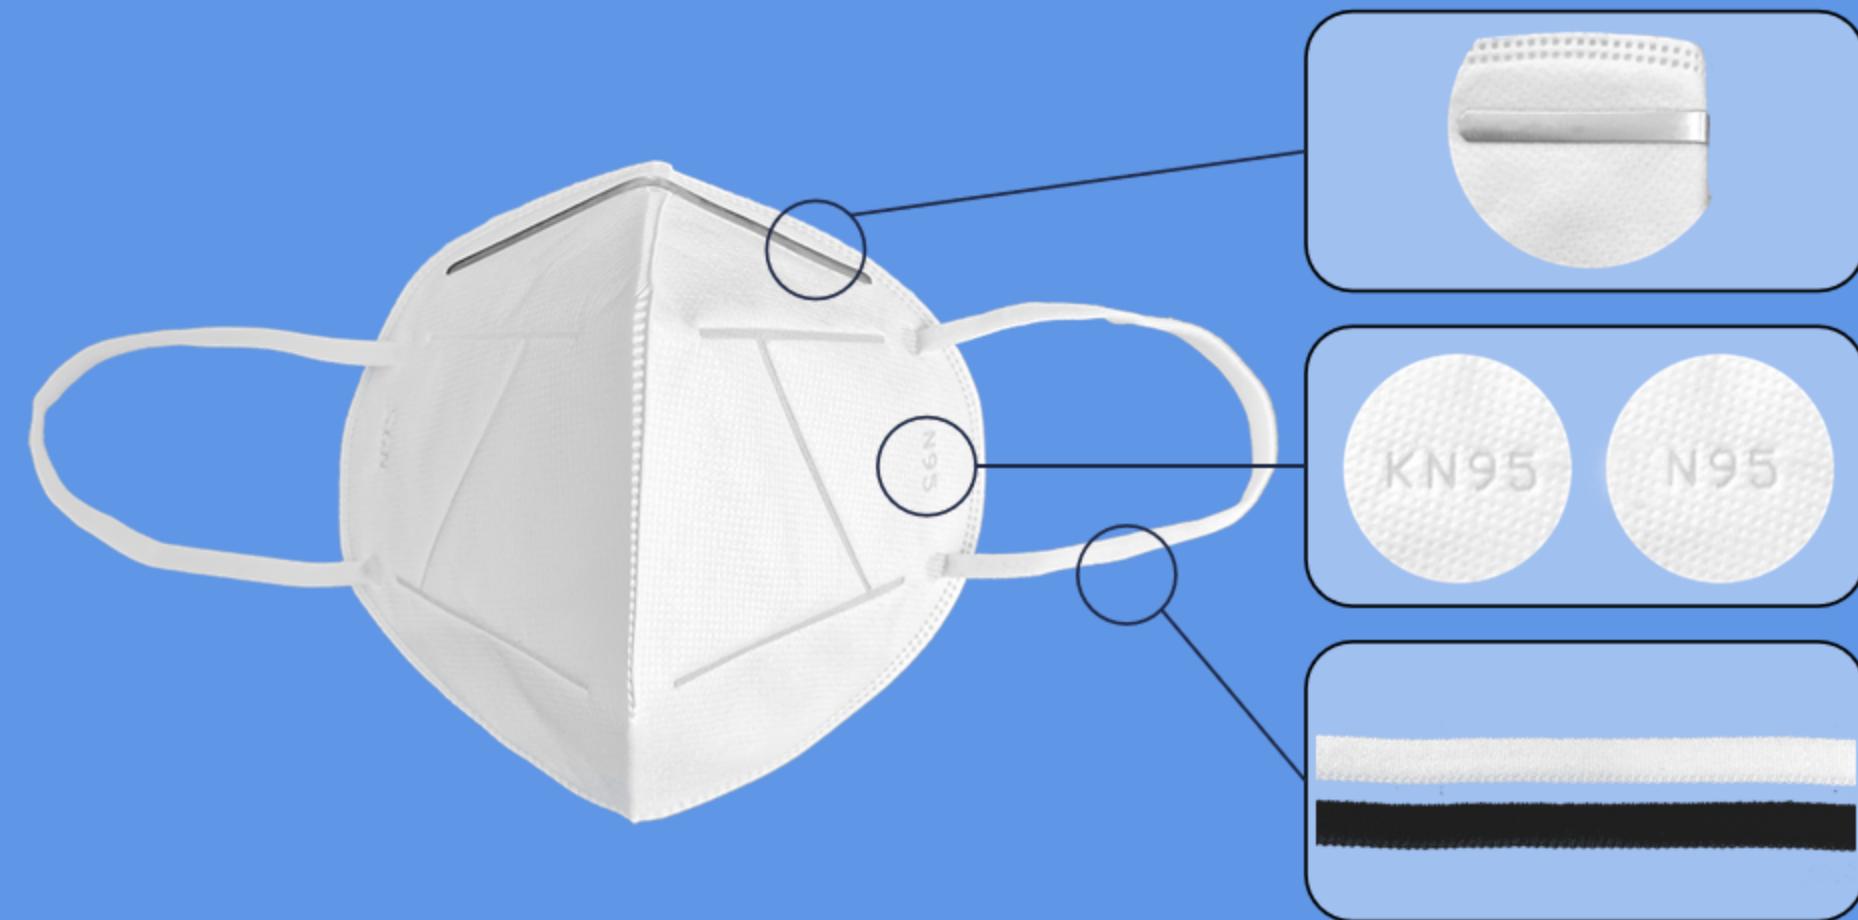

Aluminum nasal bridge clamp

Concave Cover Text

Decorative text has nothing to do with
product performance

Fine braided earband rope



始于1634年



EQ sterilization equipment



Class 100000 Cleanroom



Mask Production Workshop

Brief introduction of Liaoning shengjingtang Biotechnology Co., Ltd

Liaoning Shengjingtang Biotechnology Co., Ltd. was established on July 1, 2016, with a registered capital of 10 million yuan. Is Liaoning Yuhang Investment Group Co., Ltd. "Shengjingtang" trade name of Biotechnology Co., Ltd. It is a professional enterprise integrating R & D, production, sales and service of biological products technology. At the same time, it is a diversified company that manufactures and sells medical devices, health foods, health supplies and cosmetics. The company is engaged in the large health industry. The core team has at least 5 years of experience in this industry. At the same time, the company has obtained a number of patent registration certificates, trademarks, copyrights and other intellectual property registration certificates.



关勋泽董事长（中）陪同辽宁省副省长崔枫林（左）、辽宁省工信厅厅长何庆（右）参观厂区



关勋泽董事长（右）陪同辽宁省副省长崔枫林（左二）、辽宁省工信厅厅长何庆（左一）、沈北新区书记闻然（左三）



沈阳市政府副市长苗治民（上图左一）由盛京堂董事长关勋泽陪同考察口罩厂区



共青团辽宁省委副书记张德智（右）在盛京堂集团董事长关勋泽（左）陪同下调研盛京堂口罩生产厂区



盛京堂集团董事长关勋泽（中）与飞龙药业集团副总裁王景刚（左）陪同沈北新区政府区长刘树敏（右）考察口罩生产车间



沈阳市沈北新区书记闻然（中）、沈阳市工业和信息化局局长韩博（右）莅临辽宁盛京堂生物科技有限公司厂区调研指导工作。辽宁盛京堂生物科技有限公司总经理李可（左）陪同。

Government leaders visited the company during the construction period to guide and assist the work.



Medical Device Production License



Business license

中华人民共和国医疗器械注册证

注册证编号: 辽械注准 20202140070

注册人名称	辽宁盛京堂生物科技有限公司
注册人住所	沈阳市沈北新区乐业街 118-3 号
生产地址	沈阳市沈北新区乐业街 118-3 号
代理人名称	不适用
代理人住所	不适用
产品名称	医用防护口罩
型号、规格	折叠型 (22cm (长) × 16.5cm (宽) ± 10mm)。
结构及组成	由口罩体、鼻夹和口罩带组成，口罩体两面由无纺布制成，中间层由熔喷布制成，口罩带为棉氨材质空心扁带的弹性材料。
适用范围	适用于医疗工作环境下，过滤空气中的颗粒物、阻隔飞沫、血液、体液、分泌物等用。
附件	产品技术要求
其他内容	禁忌症：对非织造布过敏者慎用。
备注	<p>1. 该产品为应急注册审批产品，注册证有效期为一年。 2. 在延续注册时应按照法规要求完善注册申报资料。</p>

审批部门：辽宁省药品监督管理局

批件日期：2020年3月17日
有效期至：2021年3月16日



中华人民共和国医疗器械注册证

注册证编号: 辽械注准 20202140069

注册人名称	辽宁盛京堂生物科技有限公司
注册人住所	沈阳市沈北新区乐业街 118-3 号
生产地址	沈阳市沈北新区乐业街 118-3 号
代理人名称	不适用
代理人住所	不适用
产品名称	医用防护口罩
型号、规格	折叠型 22cm (长) X16.5cm (宽) ± 10mm; 19cm (长) X16cm (宽) ± 10mm; 17.5cm (长) X13.8cm (宽) ± 10mm。
结构及组成	由口罩体、鼻夹和口罩带组成，口罩体两面由无纺布制成，中间层由熔喷布制成，口罩带为棉氨材质空心扁带的弹性材料。采用环氧乙烷灭菌，无菌提供。
适用范围	适用于医疗工作环境下，过滤空气中的颗粒物、阻隔飞沫、血液、体液、分泌物等用。
附件	产品技术要求
其他内容	禁忌症：对非织造布过敏者慎用。
备注	<p>1. 该产品为应急注册审批产品，注册证有效期为一年。 2. 在延续注册时应按照法规要求完善注册申报资料。</p>

审批部门：辽宁省药品监督管理局

批件日期：2020年3月17日
有效期至：2021年3月16日



Sterile

Medical instrument registration certificate



Shenzhen Tian Hai Test Technology Co.,Ltd.

CE Certificate of Conformity

Certification number: TH20CC-176S

Report number: TH20CR-176S

Shenzhen Tian Hai Test Technology Co.,Ltd. hereby declares that testing has been completed and reports have been generated for:

Applicant: Liaoning shengjingtang biotechnology Co.,Ltd.

Address: 118-3 leye street, shenbei new district, shenyang city, liaoning province, China

Manufacturer: Liaoning shengjingtang biotechnology Co.,Ltd.

Address: 118-3 leye street, shenbei new district, shenyang city, liaoning province, China

Product: Medical Protective Mask



Model: Folding type

And, in accordance with the following applicable directives:

(EU) 2016/425 Personal Protective Equipment(PPE)

This product has been assessed against the following applicable standards;

Standard: EN 149:2001+A1:2009

Therefore, Shenzhen Tian Hai Test Technology Co.,Ltd. hereby acknowledges that the applicant may issue a DECLARATION OF CONFORMITY and apply the CE marking in accordance with European Union Rules.

Attestation by:



Thomas Wong



Date of Issue: March 16, 2020

4F,A3 BLDG,The Silicon Valley Power intelligent terminal industrial park,Guan Ian street,Longhua district,Shenzhen

Tel:+86-755-86615100 Fax:+86-755-86615105 http://www.tianhaitest.com



Fiscal Year 2020 CERTIFICATION OF FDA REGISTRATION

Cert. No.: 2020FDA02SPICACN066

This certifies that:

Establishment: LIAONING SHENGJINGTANG BIOTECHNOLOGY CO., LTD

**Registered Address: 118-3 Leye Street, Shenbei New District Shenyang City,
Liaoning, 110141, CHINA**

Registration Number: Not Yet Assigned

has completed the FDA Establishment Registration (as manufacturer) and Device Listing with the US Food & Drug Administration, such registration having been verified as currently effective on the date hereof by SPICA MEDTECH CORP.

Owner/Operator Number: 10063297 (Device Listing#: See annex)

U.S. Agent for FDA: SPICA MEDTECH CORP

Communications: 2288 EMERSON ST Denver,CO,80205,USA

Phone: 720 6176666 Ext .Email: spica_us@yahoo.com

SPICA MEDTECH CORP will confirm that such registration remains effective upon request and presentation of this certificate until the end of the calendar year stated above, unless said registration is terminated after issuance of this certificate.

SPICA MEDTECH CORP makes no other representations or warranties, nor does this certificate make any representations or warranties to any person or entity other than the named certificate holder, for whose sole benefit it is issued. This certificate does not denote endorsement or approval of the certificate-holder's device or establishment by the U.S. Food and Drug Administration.

Pursuant to 21 CFR 807.39, "Registration of a device establishment or assignment of a registration number does not in any way denote approval of the establishment or its products.

**SPICA MEDTECH CORP (in USA)
SHANGHAI SPICA MANAGEMENT CONSULTING CO.LTD (in China)
SPICA MEDTECH CERTIFICATION COMPANY LIMITED (in UK)**

spica_us@yahoo.com • www.spicamedtech.com



Scan code to verify certificate

*For and on behalf of
SPICA MEDTECH CORP*



**Spica Consulting
Regulation Service**

Authorized Signature(s)

SPICA CHINA ADD: No.216 Building,No.500 Jinbai Road, Shanghai 200120, P.R.China



检 验 报 告
准 (医械) 字 (2020) 第 323 号

辽检(医械)字(2020)第323号

受检单位 江苏盛京堂生物科技有限公司
样品名称 医用防护口罩
型号规格 医用型
检验类别 应急检验

辽宁省医疗器械检验检测院

100

告之日起十五日內

由委任
由客户

1

三

辽宁省医疗器械检验检测院
检验报告

（总第）字第（2009）第323号

项目名称	医用防护口罩	型号规格	折叠型
辽宁盛京堂生物科技有限公司	面 疙	滤嘴型	
沈阳市沈河区东金街 183 号	过滤类型	熔喷布型	
辽宁盛京堂生物科技有限公司	生产日期	2020/02/01	
辽宁盛京堂生物科技有限公司	储存日期	—	
辽宁盛京堂生物科技有限公司	生产批号	2020 年 03 月 01 日	
—	储存批号	—	
试验结果	过滤类型	—	
2020-03-01 ~ 2020-03-05	过滤数量	100 个	
聚丙烯熔喷布分项	品项批号	20200219	
该项目符合辽宁盛京堂生物科技有限公司《医用防护口罩》(2020) 医疗器械产品技术要求			

该项目符合辽宁盛京堂生物科技有限公司《医用防护
(2020) 医疗器械产品技术要求

姓名: 到院长 日期: 2020.3.5
性别: 女

Inspection Report



Product Name	Production license	Implementation Standards	Single package size	Specification of each package	Outer box size
Medical Protective Mask (Sterile)	[Medical Device Registration Certificate Number]辽械注准20202140069 [Number of Product Technical Requirements]辽械注准20202140069 [Production License Number]辽食药监械生产许20200023号	GB19083-2010	140mmX160mm 150mmX170mm	500pcs	465mmX433mmX363mm
Medical Protective Mask	[Medical Device Registration Certificate Number]辽械注准20202140070 [Number of Product Technical Requirements]辽械注准20202140070 [Production License Number]辽食药监械生产许20200023号	GB19083-2010	140mmX160mm 150mmX170mm	500pcs	465mmX433mmX363mm