


Surface Tension Calibration Water X-Bar Chart, Aug-Dec, 2011

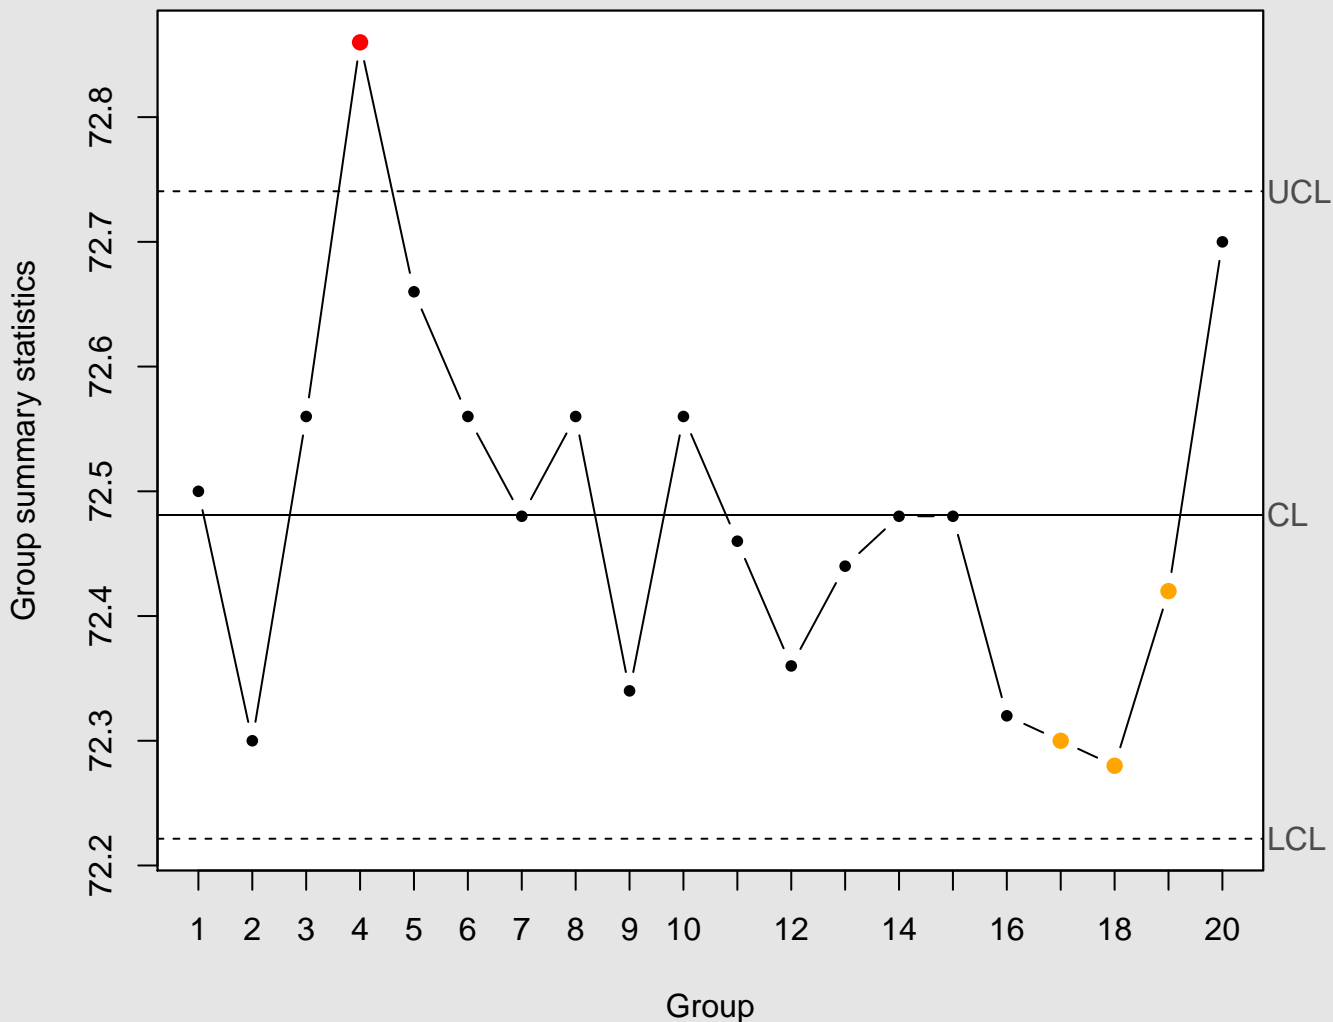

Number of groups = 20

Center = 72.481

StdDev = 0.1934652

LCL = 72.22144

UCL = 72.74056

Number beyond limits = 1

Number violating runs = 3