

Name: [REDACTED] OD OS

ID: [REDACTED] Exam Date: 8/5/2026 8/5/2026 CZMI


DOB: 5/25/1951 Exam Time: 11:27 AM 11:33 AM

Gender: Female Serial Number: 4000-123458 4000-123458





Technician: Operation, Cirrus Signal Strength: 6/10 5/10





ONH and RNFL OU Analysis: Optic Disc Cube 200x200 OD ● OS ●

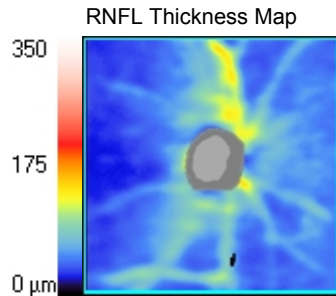


	OD	OS
Average RNFL Thickness	60 μm	52 μm
RNFL Symmetry	67%	
Rim Area	0.98 mm²	0.86 mm²
Disc Area	1.73 mm²	1.63 mm²
Average C/D Ratio	0.65	0.69
Vertical C/D Ratio	0.70	0.75
Cup Volume	0.226 mm³	0.278 mm³

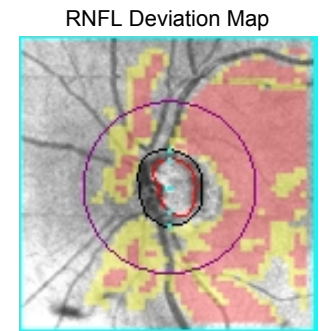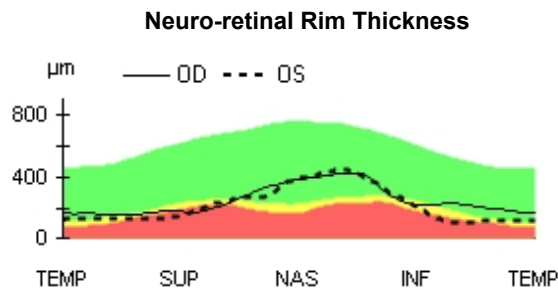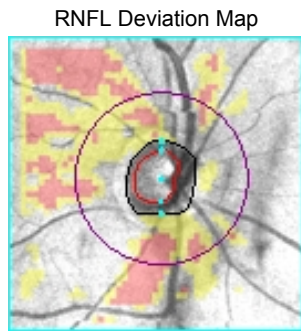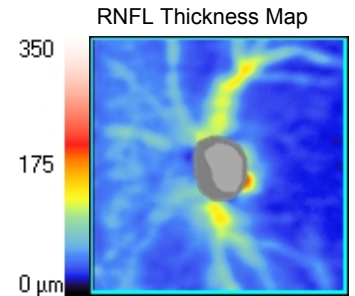


Disc Center(0.06,0.15)mm
Extracted Horizontal Tomogram

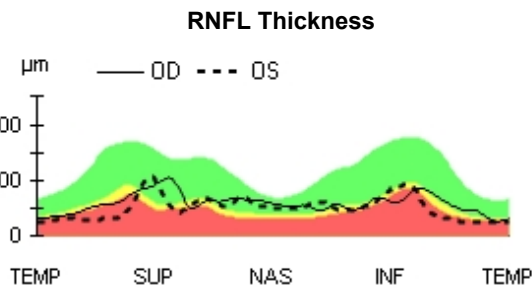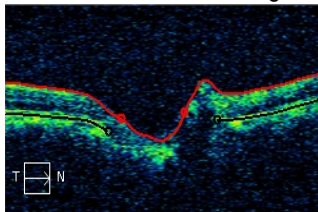


Disc Center(0.00,-0.03)mm
Extracted Horizontal Tomogram

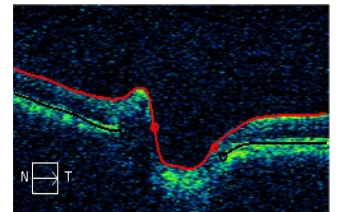


Extracted Vertical Tomogram

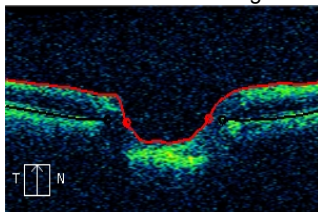



Extracted Vertical Tomogram

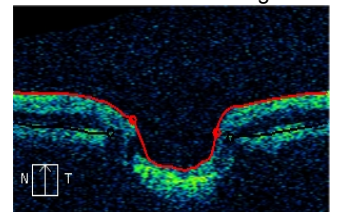

RNFL Circular Tomogram

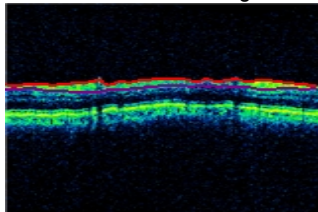

RNFL Circular Tomogram

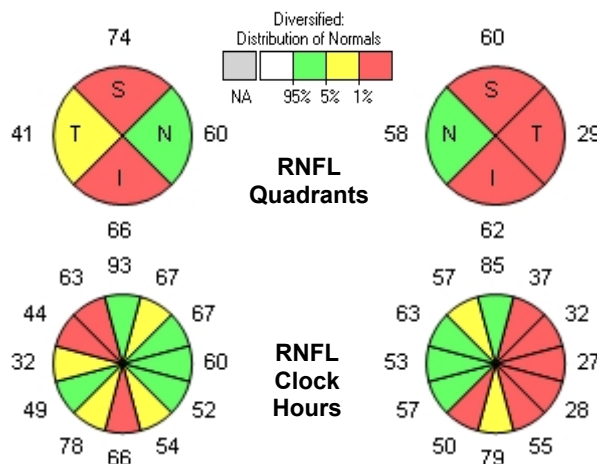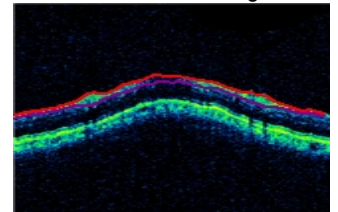

Comments

Doctor's Signature

SW Ver: 7.0.3.19
Copyright 2015
Carl Zeiss Meditec, Inc
All Rights Reserved