



Thermal Strain Imaging — Ultrasound Thermometry (Theorem 11.12.2)

(a) RF echo shift from heating

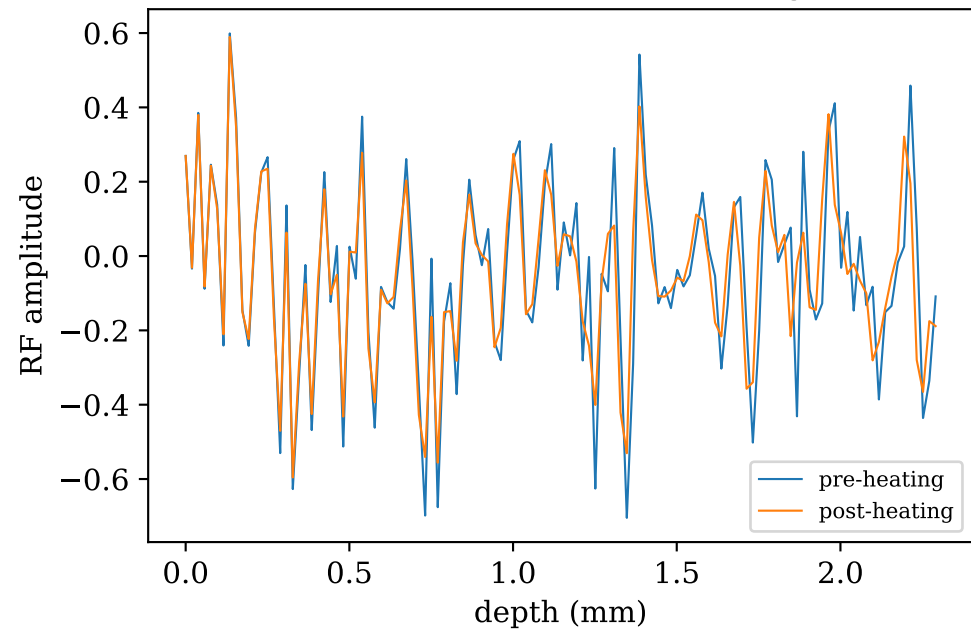

(b) Negative strain (water-based)

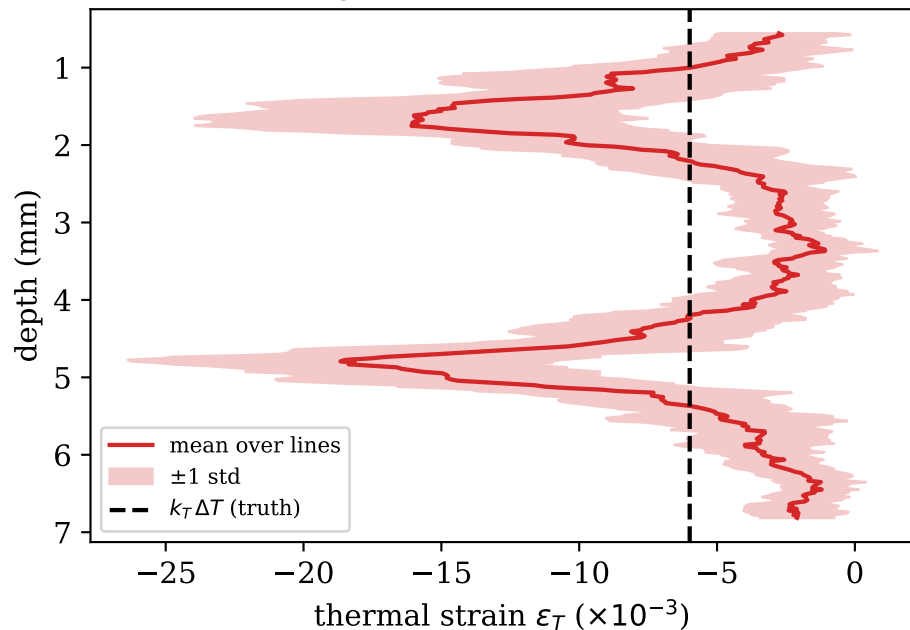

(c) Reconstructed ΔT ($k_T = -9.99e - 04/^{\circ}\text{C}$)

