



kidney — image-then-treat sequence on the same skin-coupled hemispherical phased-array applicator

Planning CT slice + target / organ contour

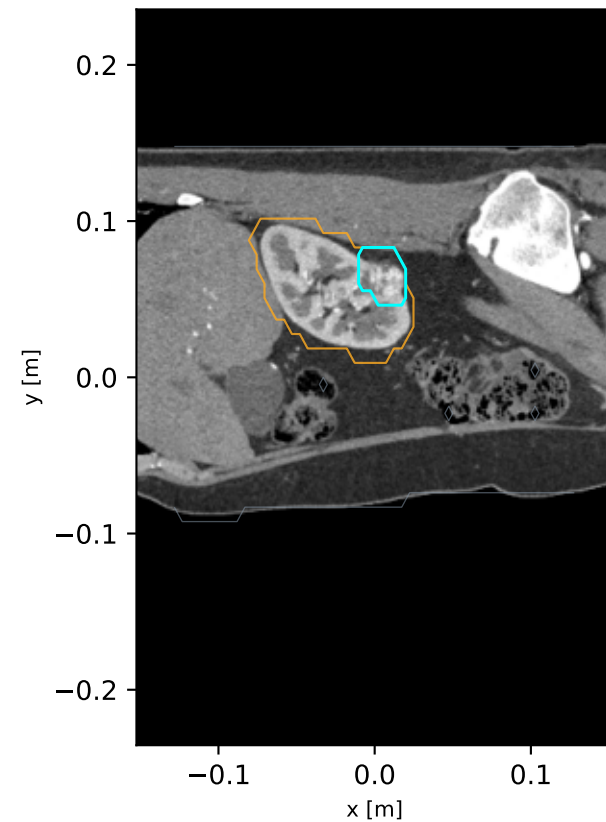

Reconstructed image (linearised Born, single-pass H^1 -Tikhonov)
in-body peak = 0.304 (a.u.), multi-frequency imaging transmit, same aperture

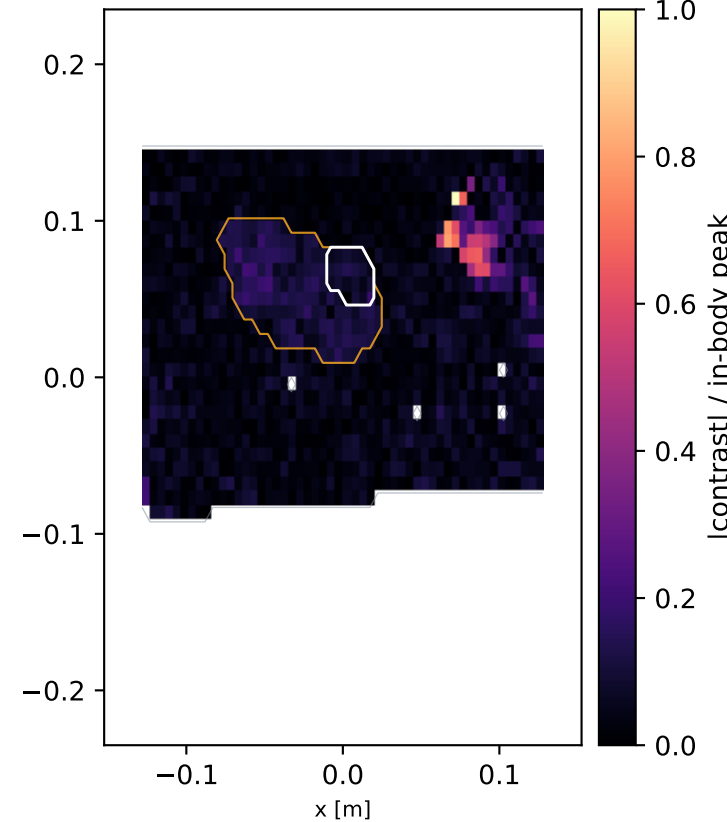

Focused-US in-body peak pressure = 10.7 MPa
(< 26 MPa intrinsic threshold — no cavitation isolate drawn;
raw-grid peak incl. PML edge = 10.7 MPa) $1e7$

