

Portable Ultrasound System for Blood Velocity Estimation
Project Report

Master Thesis
April, 2023

Author:
Jeppe Hinrichs

Advisor(s):
Hyunjoo Lee, Xenofon Fafoutis, Tiberiu Gabriel Zsurzsan

Copyright:	Reproduction of this publication in whole, or in part, must include the customary bibliographic citation, including author attribution, report title, etc.
Cover photo:	RawPixel, 2022
Published by (1):	DTU, Department of Electrical Engineering, Ørstedes Plads, Building 348, 2800 Kgs. Lyngby, Denmark www.elektro.dtu.dk
Published by (2):	KAIST, School of Electrical Engineering, E3-2, Daehak-ro 291, 34141 Daejeon, Republic of Korea www.ee.kaist.ac.kr
Timespan:	Saturday 1 st October, 2022 ~ Wednesday 12 th April, 2023
Credits:	30 ECTS / 9 credits
Degree:	Master of Science
Field:	Electrical Engineering

Approval

This thesis has been prepared over six months at the Brain/Biomedical Microsystems Laboratory, School of Electrical Engineering, at the Korean Advanced Institute of Science and Technology, KAIST, and the Department of Electrical Engineering, Technical University of Denmark, DTU. This thesis is in partial fulfillment for the double degree Master of Science in Electrical Engineering (M.S.E.E.).

Jeppe Hinrichs - s163555

.....
Signature

.....
Date

Contents

Copyright

Approval

Contents I

List of Figures III

List of Tables IV

List of Source Codes V

Abbreviations VI

Glossary VII

Nomenclature VIII

Reading comprehension XI

1 Theory 1

1.1	Ultrasound	1
1.1.1	Scattering	2
1.1.2	Attenuation	3
1.1.3	Transducer	4
1.1.4	Doppler effect	4
1.2	Flow Physics	6
1.2.1	Blood flow	8
1.3	Transducer	8
1.3.1	Impedance matching	10
1.4	Devices	11
1.4.1	Continuous-wave Flowmeter	12
1.4.2	Pulsed-wave Flowmeter	14
1.5	Blood Velocity Estimation	17
1.5.1	Spectral estimation	17

2 Synthesis 19

2.1	Control System	19
2.1.1	Development Environment	20
2.1.2	Zephyr	21
2.1.3	Firmware	24
2.2	Pulse-Width-Modulation Generator	25
2.3	Power Stage	25
2.4	Transmit/Receive Switch	26
2.5	Preamplifier	27
2.6	Demodulation	28
2.7	Sample/Hold	28

2.8	Pulse-Repetition and Wall Filter	29
2.9	Amplifier	29
2.10	Mixer	29
2.11	Adder	29
Bibliography		31

List of Figures

1.1	Particle displacement for a propagating ultrasound wave	1
1.2	Single element ultrasound transducer construction	4
1.3	Transducer types for acquiring B-mode images	5
1.4	Doppler effect diagram	5
1.5	Circulatory system of the human body	7
1.6	Basic CMUT structure	10
1.7	Optical images of various cMUT elements with different membrane shapes .	11
1.8	Diagram of ultrasound wave transmitted and reaching blood vessel with incident angle θ	11
1.9	Block diagram of continuous-wave flowmeter	12
1.10	Doppler signals in time and frequency domain showing demodulation effects	13
1.11	Block diagram of pulsed-wave flowmeter	14
1.12	Sampling for a gate pulsed wave system with a single range	15
1.13	Simulated RF sampling of blood vessel with segmented receiver line with a sample interval denoted by a dotted line (left) and the resulting amplitude of the sample (right)	16
1.14	Stationary tissue sampled signal and stationary tissue sample spectrum . .	17
1.15	Arterial sonogram with time-frequency and Doppler shift	18
2.1	Simplified overview of the system	19
2.2	VSCode editor with CMake Tools active	20
2.3	Devicetree input files and output files	21
2.4	Configuration phase of a Zephyr application	22
2.5	Flowchart of build stage I, pre-build	23
2.6	Flowchart of build stage II, generation and compilation	23
2.7	Flowchart of build stage III, intermediate binary	24
2.8	Flowchart of build stage IV, second intermediate binary	24
2.9	Flowchart of build stage V, final binary	24
2.10	Flowchart of build stage VI, post-processing	25
2.11	Circuit diagram of power stage	26
2.12	Circuit diagram of switch (per channel)	27
2.13	3D Render of PCB in Altium Designer	28

List of Tables

1.1	Approximate density, sound speed, and acoustic impedance of human tissue types	2
1.2	Approximate attenuation values for human tissue	3
1.3	Typical dimensions and flow in human circulatory system	9
1.4	Measured frequency shifts with a Doppler 3 MHz transducer at various velocities at a 45° incident angle	14

List of Source Codes

Abbreviations

Notation	Description
<i>ADC</i>	analogue-to-digital converter
<i>AM</i>	amplitude modulation
<i>BLE</i>	bluetooth low energy
<i>BP</i>	band-pass
<i>CMUT</i>	capacitive micromachined ultrasound transducer
<i>CPU</i>	central processing unit
<i>CW</i>	continuous-wave
<i>DSP</i>	digital signal processor
<i>DTS</i>	device tree source
<i>DTSI</i>	device tree source include
<i>ELF</i>	executable and linkable format
<i>I/O</i>	input/output
<i>IC</i>	integrated circuit
<i>IoT</i>	Internet of Things
<i>MCU</i>	microcontroller unit
<i>PSD</i>	power spectral density
<i>PW</i>	pulsed-wave
<i>PZT</i>	lead circonate titanate
<i>RAM</i>	random access memory
<i>RTOS</i>	real-time operating system
<i>SHA</i>	sample-and-hold amplifier
<i>SoC</i>	system-on-a-chip
<i>US</i>	ultrasound

Glossary

Notation	Description
adiabatic	Any process that happens without heat gain or loss is considered adiabatic
Doppler effect	A change in frequency of a wave in relation to an observer who is moving relative to the wave source
dynamic range	The ratio between the largest and smallest values that a certain quantity can assume, in signal theory usually measured in decibels
flashing	Refers to the process of programming the non-volatile memory of a microcontroller
HIGH	Logic high voltage level
Internet of Things	A term used to describe physical things equipped with sensors, computing power, software, and other technologies that communicate data with other systems and devices across communication networks such as the Internet
LOW	Logic low voltage level
open-source	Refers to software whose original source code is publicly available and may be changed and distributed
piezoelectric	Material that deforms under electric excitation, or reversibly, electric charge that accumulates in response to mechanical stress
quantized	The process of mapping input values from a continuous set to a discrete smaller set with a finite number of elements
transcutaneous	Applied across the depth of the skin without invasive penetration
transducer	A device that converts electrical energy to kinetic energy, or kinetic energy to electrical energy

Nomenclature

Name	Unit	Description
Input filter		
V_{ref}	V	Reference voltage
C_{hp}	F	High pass filter capacitor
R_{hp}	Ω	High pass filter resistor
f_{hp}	Hz	High pass cut-off frequency
C_{lp}	F	Low pass filter capacitor
R_{lp}	Ω	Low pass filter resistor
f_{lp}	Hz	Low pass cut-off frequency
A_v	1	Amplification factor
Modulator		
R_1	Ω	AIM voltage divider resistor
R_2	Ω	AIM voltage divider resistor
R_{in}	Ω	AIM input resistor
R_{fb}	Ω	AIM feedback resistor
C_1	F	AIM capacitor
V_{in}	V	Input signal voltage
V_{span}	V	Voltage range of input signal
V_{pwm}	V	PWM signal
V_H	V	V_{pwm} high level voltage
V_L	V	V_{pwm} low level voltage
V_{out}	V	V_{pwm} voltage range ($V_H - V_L$)
V_{hys}	V	Hysteresis voltage
V_{hw}	V	Hysteresis width
V_{th_H}	V	Hysteresis threshold upper voltage
V_{th_L}	V	Hysteresis threshold lower voltage
V_c	V	PWM carrier voltage
V_{c_H}	V	PWM carrier upper voltage
V_{c_L}	V	PWM carrier lower voltage
f_{sw}	Hz	PWM signal frequency
D	1	PWM signal duty cycle
t_H	s	PWM carrier charge time

Continued on next page

Name	Unit	Description
t_L	s	PWM carrier discharge time
τ	1	PWM carrier charge constant
R_{th}	Ω	PWM carrier thevenin resistance
f_{idle}	Hz	PWM signal idle switching frequency
k_2	1	R_{fb} , R_{in} voltage divider
Gate driver		
D_{dt}	1	Dead-time circuit diode
R_{dt}	Ω	Dead-time circuit resistor
C_{dt}	F	Dead-time circuit capacitor
V_C	V	Dead-time circuit supply voltage
V_s	V	IC supply voltage
t_c	s	Charging circuit time
Power stage		
V_{DD}	V	Power supply voltage
Q_1, Q_2, Q_3, Q_4	1	Power stage switches
V_g	V	Gate driver signal
V_o	V	Output voltage
I_o	A	Output current
R_{BTL}	Ω	Speaker equivalent load resistance
Output filter		
R_f	Ω	Output filter single-ended load
C_{BTL}	F	Output filter differential capacitance
C_f	F	Output filter single-ended capacitance
L_f	H	Output filter inductance
ΔI_L	A	Output filter ripple current
Q	1	Output filter quality factor
f_c	Hz	Output filter cut-off frequency
ω_n	rads^{-1}	Output filter natural frequency
ζ	1	Output filter damping ratio

Continued on next page

Name	Unit	Description
Shunt regulator		
R_{sh}	Ω	Shunt current limiting resistor
I_K	A	Shunt cathode current
$I_{K_{\max}}$	A	Shunt maximum cathode current
$I_{K_{\min}}$	A	Shunt minimum cathode current
I_{su}	A	Shunt supply current
R_{A1}	Ω	Shunt adjust resistor 1
R_{A2}	Ω	Shunt adjust resistor 2
C_L	F	Shunt load capacitance
$V_{\text{ref}_{\text{IC}}}$	V	Shunt internal reference voltage

Reading comprehension

This section of the report will explain to the reader how to reference this document and explain the fundamental structure of the project as well as the report. It is assumed that the reader has a basic knowledge of physics, electrical engineering, computing, and circuit analysis.

Otherwise, please refer to Abbreviations, Glossary, and Nomenclature pages for explanations to terms found within the report.

Sources

Calculus expressions present in the report will typically have a reference explaining their origin. All references are prominently displayed with square brackets and a number, directing to the bibliography section of the report.

1 Theory

This chapter explains the overall theory that forms the fundamental principles of this project. Initially, the characteristics of ultrasound will be explained from an acoustics standpoint. Then, a brief overview of the systemic circulation is explained in vivo. Lastly, the various types of flow-meters are outlined with their strengths and weaknesses.

1.1 Ultrasound

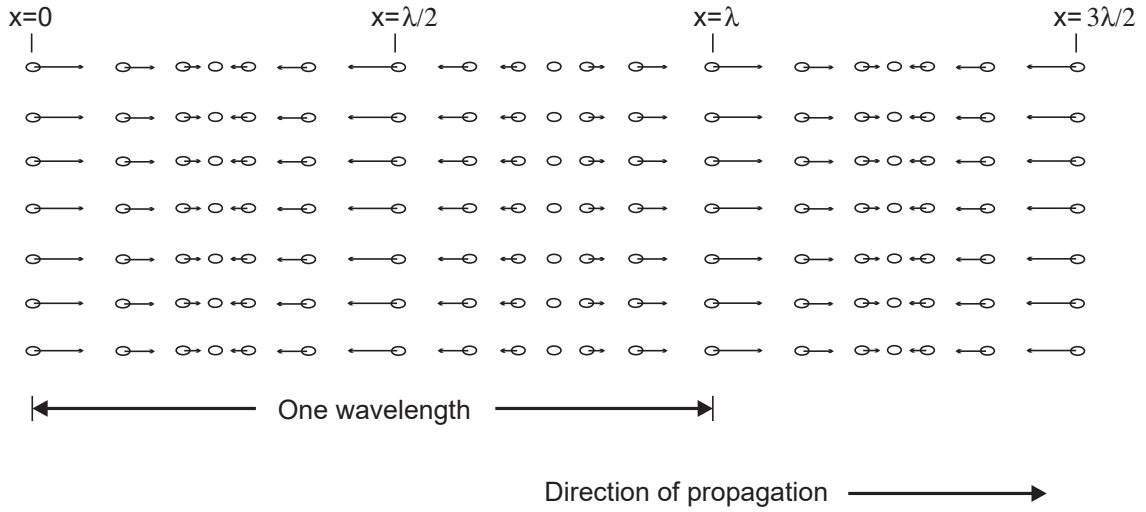


Figure 1.1: Particle displacement for a propagating ultrasound wave [9]

ultrasound (*US*) is a technology that transmit sound wave with frequencies above the audible range (20 to 20 000 Hz) to mechanically vibrate matter. The particles in the medium would be at rest and distributed uniformly before any disturbance. The wave propagates as a disturbance and the particles oscillate around their mean position due to the presence of the ultrasonic wave. Typically the *US* frequency band used in clinical settings are from 1 to 15 MHz [11]. Figure 1.1 visualizes the propagation of a plane wave in matter. The oscillation occurs parallel to the wave's direction, making it longitudinal, and the disturbance will propagate with the variable c , which is determined by the medium and is given by eq. (1.1).

$$c = \sqrt{\frac{1}{\rho_0 \kappa_S}} \quad (1.1)$$

Where ρ_0 is the mean density (kgm^{-3}) and κ_S is the adiabatic compressibility (m^2N^{-1}). Since in the majority of cases, the propagation of ultrasound is linear, it is assumed in this work. The acoustic pressure of the harmonic plane wave is expressed by eq. (1.2).

$$p(t, z) = p_0 e^{j(\omega t - kz)} \quad (1.2)$$

And propagates along the z -axis. ω is the angular frequency, k is the wave number and is expressed by $k = \omega/c = 2\pi/\lambda$, and p_0 is the acoustic pressure amplitude. A spherical wave is expressed by eq. (1.3)

$$p(t, r) = p_0 e^{j(\omega t - kr)} \quad (1.3)$$

Where r is radial distance, and is defined in a polar coordinate system. For each time instance, the acoustic pressure $p(t, r)$ is constant over a fixed radial position. In this scenario, the pressure amplitude is given by $p_0(r) = k_p/r$, where k_p is a constant since the energy of the outgoing wave must be constant. Particle speed u is dependent on the pressure caused by a wave expressed by eq. (1.4)

$$u = \frac{p}{Z} \quad (1.4)$$

Where Z is the characteristic acoustic impedance, defined as the ratio of acoustic pressure to particle speed at a given position in the medium and is expressed by eq. (1.5).

$$Z = \rho_0 c \quad (1.5)$$

Characteristic acoustic impedance Z is one of the most significant variables in the characterization of propagating plane waves. Reference values for density, speed of sound, and characteristic acoustic impedance can be seen in table 1.1.

Table 1.1: Approximate density, sound speed, and acoustic impedance of human tissue types [9]

Medium	Density (ρ_0) kg/m ³	Speed of sound (c) m/s	Acoustic impedance (Z) kg/(m ² s)
Air	1.2	333	0.4×10^3
Blood	1.06×10^3	1566	1.66×10^6
Bone	$1.38\text{--}1.81 \times 10^3$	2070–5350	$3.75\text{--}7.38 \times 10^6$
Brain	1.03×10^3	1505–1612	$1.55\text{--}1.66 \times 10^6$
Fat	0.92×10^3	1446	1.33×10^6
Kidney	1.04×10^3	1567	1.62×10^6
Lung	0.4×10^3	650	0.26×10^6
Liver	1.06×10^3	1566	1.66×10^6
Muscle	1.07×10^3	1542–1626	$1.65\text{--}1.74 \times 10^6$
Spleen	1.06×10^3	1566	1.66×10^6
DI	1×10^3	1480	1.48×10^6

In the following sections, various acoustic wave phenomena will be briefly described.

1.1.1 Scattering

A wave propagating through a medium continues in the same direction until it encounters a new medium. When this occurs, a portion of the wave is transmitted into the new medium with a change in direction. Because the scattered wave is the result of several contributors, it is necessary to define it statistically. The amplitude distribution is Gaussian [9] and can thus be fully described by its mean and variance. The mean value is zero because the dispersed signal is caused by variances in the acoustic characteristics in the tissue. The correlation between multiple data is what allows ultrasound to determine blood velocities. Because minor movements have a significant correlation, it is feasible to discover alterations in location by comparing sequential measurements of moving structures, such as blood cells. In medical ultrasound, only one transducer is used to transmit and receive, and only the backscattered signal is analysed. The power of the scattered signal is defined by the

scattering cross-section, which in small cases means a uniform intensity I_i , and is expressed by eq. (1.6).

$$P_s = I_i \sigma_{sc} \quad (1.6)$$

Where σ_{sc} is the scattering cross-section in square meters. The backscattering cross section is material dependant and determines the intensity of the scattering. If the dispersed energy is evenly emitted in all directions, the scattered intensity is given by eq. (1.7).

$$I_s = \frac{P_s}{4\pi R^2} = \frac{\sigma_{sc}}{4\pi R^2} \cdot I_i \quad (1.7)$$

Where R is distance to the scattering region [9]. This results in a spherical wave. A transducer with radius r gives the power P_r , presuming the attenuation and focus is neglected, and is expressed by eq. (1.8).

$$P_r = I_s \pi r^2 = \sigma_{sc} \frac{r^2}{4R^2} \cdot I_i \quad (1.8)$$

The backscattering coefficient, which characterizes scattering from a volume of scatterers, is another measure of scattering strength. It is defined as the average received power per steradian volume of scatterers when flooded with plane waves of unit amplitude and the unit is 1/cmsr. Backscattering coefficients in the blood are significantly lower than the backscattering coefficients from various tissue types. This poses a challenge when estimating blood flow close to tissue vessel walls [3], [9].

1.1.2 Attenuation

The ultrasonic wave will be reduced as it propagates through the tissue due to absorption and scattering. The attenuation in tissue is frequency dependent, with greater attenuation with increasing frequency. Because of absorption and dispersion, the ultrasonic wave will be attenuated as it travels through the tissue. The relationship between attenuation, distance travelled, and frequency is often linear. Attenuation in the tissue occurs as a result of both dispersion, which spreads energy in all directions, and absorption, which turns it into thermal energy. A table of approximate attenuation values can be seen in table 1.2.

Table 1.2: Approximate attenuation values for human tissue [9]

Tissue	Attenuation dB/(MHz · cm)
Liver	0.6–0.9
Kidney	0.8–1
Spleen	0.5–1
Fat	1–2
Blood	0.17–0.24
Plasma	0.01
Bone	16–23

The pressure of a wave propagating in z -direction decreases exponentially expressed by eq. (1.9)

$$p(z) = p(z = 0)e^{-\alpha z} \quad (1.9)$$

Where $p(z = 0)$ is the pressure in the point of origin and α is the attenuation coefficient. The attenuation coefficient unit is Npcm^{-1} and, alternatively, dBcm^{-1} with the relationship described in eq. (1.10).

$$\alpha = \frac{1}{z} \ln \frac{p(z = 0)}{p(z)} \quad (1.10a)$$

$$\alpha(\text{dBcm}^{-1}) = 20(\log_{10} e)\alpha(\text{Npcm}^{-1}) = 8.68\alpha(\text{Npcm}^{-1}) \quad (1.10b)$$

The significance of absorption and scattering in ultrasonic attenuation in biological tissues is a point of contention. Scattering adds just a few per cent to attenuation in most soft tissues. As a result, it is fair to conclude that absorption is the primary mechanism of ultrasonic attenuation in biological tissues [12].

1.1.3 Transducer

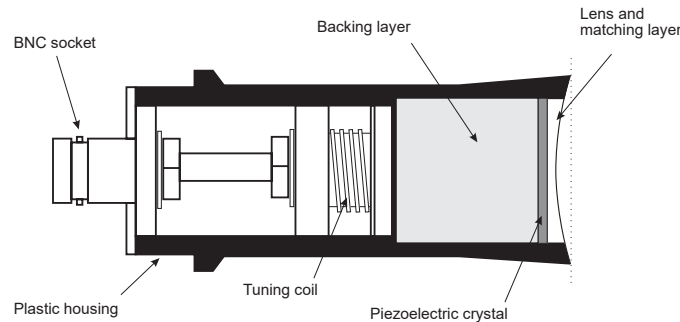


Figure 1.2: Single element ultrasound transducer construction [9]

A layperson knows transducers as speakers and microphones in the context of PA systems. In the case of medical *US* it is the device that generates the acoustic pressure field, which is emitted into the tissue. The transducer has a piezoelectric crystal inside the housing. When excited, this crystal emits ultrasound waves toward flowing blood. The red blood cells will reflect a fraction of the emitted waves. These reflected waves are of a different frequency than the transmitted wave. If the red blood cells move away from the transducer, the frequency will be lower. If the red blood cells are moving towards the transducer, the frequency will be higher. This is caused by the Doppler effect. The reflected ultrasonic waves return to the crystal and are converted back into electrical signals. The single-element transducer shown in fig. 1.2 has a minimal imaging window and has to be mechanically manipulated to obtain a wide window, which is unfeasible for responsive high-frequency imaging. Thus, usually, a transducer array is used. Various types of *US* transducer exist with different strengths and weaknesses, shown in fig. 1.3.

1.1.4 Doppler effect

The Doppler effect is a phenomenon in which an observer perceives a shift in the frequency of sound emitted from a source when either the source or the observer is moving, or both are moving. The reason for the perceived change in frequency is visualised in fig. 1.4. In diagram (a), the source S_p is stationary and produces a spherical distribution pattern of the wave with the perceived frequency of the observer is given by $f = c/\lambda$, where c is the velocity of the wave in the medium and λ is the wavelength. In diagram (b), the sound source is moving towards the right with a velocity v . The locomotion of the source changes the distribution pattern and causes a longer wavelength on the left, indicating a lower

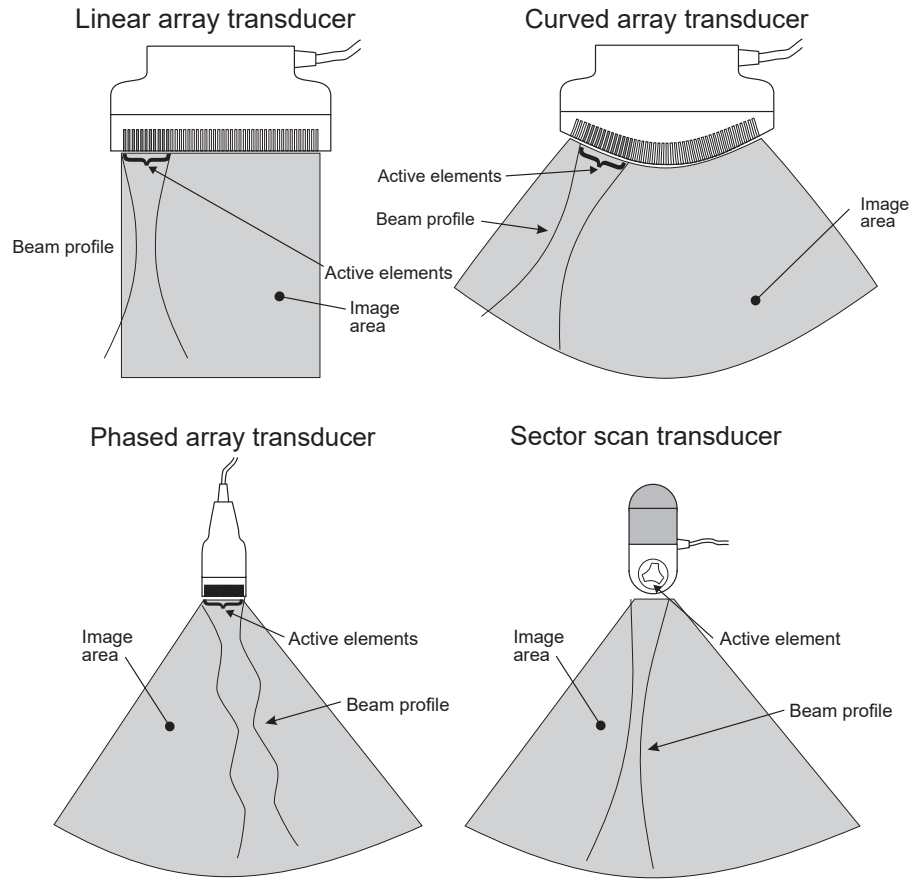


Figure 1.3: Transducer types for acquiring B-mode images [9]

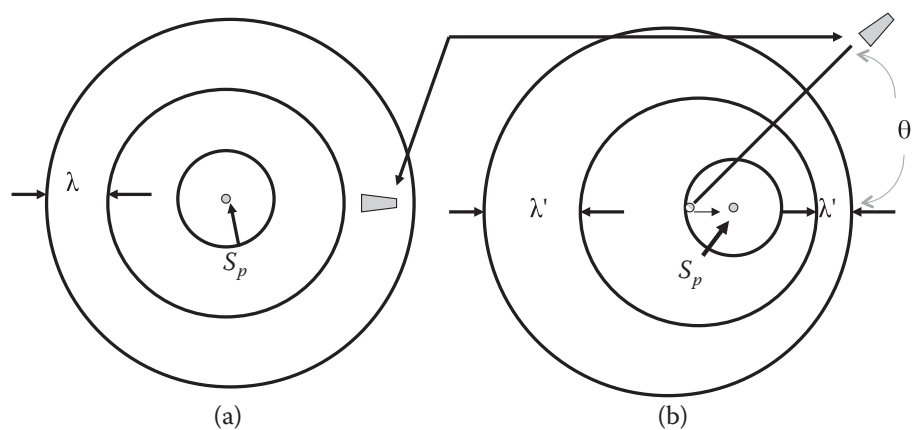


Figure 1.4: Doppler effect diagram. A stationary observer perceives a change in the frequency of a wave generated by a moving source toward the observer as a result of a wavelength shift from λ to λ' . In (a), the source is still. In (b), the source is moving at a velocity v . [12]

perceived frequency, and a shorter wavelength on the right, indicating a higher perceived frequency, both denoted as λ' in the diagram. In the case of the observer on the right side, the perceived frequency becomes eq. (1.11).

$$f' = \frac{c}{\lambda} = \frac{c}{\lambda - vT} = \frac{c}{(c - v)T} = \frac{c}{c - v} \cdot f_0 \quad (1.11)$$

And viceversa, on the left side, the perceived frequency becomes eq. (1.12).

$$f' = \frac{c}{c + v} \cdot f_0 \quad (1.12)$$

This perceived difference between the frequency that is transmitted from the source f_0 , and the perceived frequency f' is also called the Doppler frequency, f_d . When these connections are combined, the Doppler frequency for a source moving with velocity v and an observer travelling with velocity v' is given by eq. (1.13).

$$f_d = f' - f = \left(\frac{c + v'}{c - v} - 1 \right) \quad (1.13)$$

If both source and observer are moving with the same velocity, v , assuming $c \gg v$, the v cancels out and the expression is reduced to eq. (1.14).

$$f_d = \frac{2vf}{c} \quad (1.14)$$

If the velocity of the moving source is traveling with an incident angle θ , the v in eq. (1.14) is replaced with $v(\cos \theta)$. This results in the expression found in eq. (1.15) and forms the basis for applied Doppler effect measurements.

$$f_d = \frac{2v(\cos \theta)f}{c} \quad (1.15)$$

The Doppler effect is used in ultrasonic Doppler devices used to image blood flow transcutaneously. An ultrasonic transducer in these devices sends ultrasonic waves into a blood artery, and the scattered radiation from moving red cells is measured by either the same transducer or a second transducer. The Doppler frequency, which is determined by the velocity of red blood cells, is extracted using modern electronic demodulation techniques which will be explored later.

1.2 Flow Physics

The flow physics of the human circulatory system are sophisticated, and numerous nonstationary flow patterns emerge. The human circulatory system takes care of transporting oxygen and nutrients to organs, as well as disposing of waste products produced by metabolism. It is possible because the blood within the circulatory system contains several smaller subcomponents, such as plasma and formed cellular elements that perform these vital functions. Initially, blood is discharged from the left ventricle of the heart through the aorta and travels to all areas of the body through multiple branches of the arterial tree. When blood flows through the arteries, it enters smaller channels known as arterioles. These arterioles lead to a network of tiny capillaries through which nutrients and waste

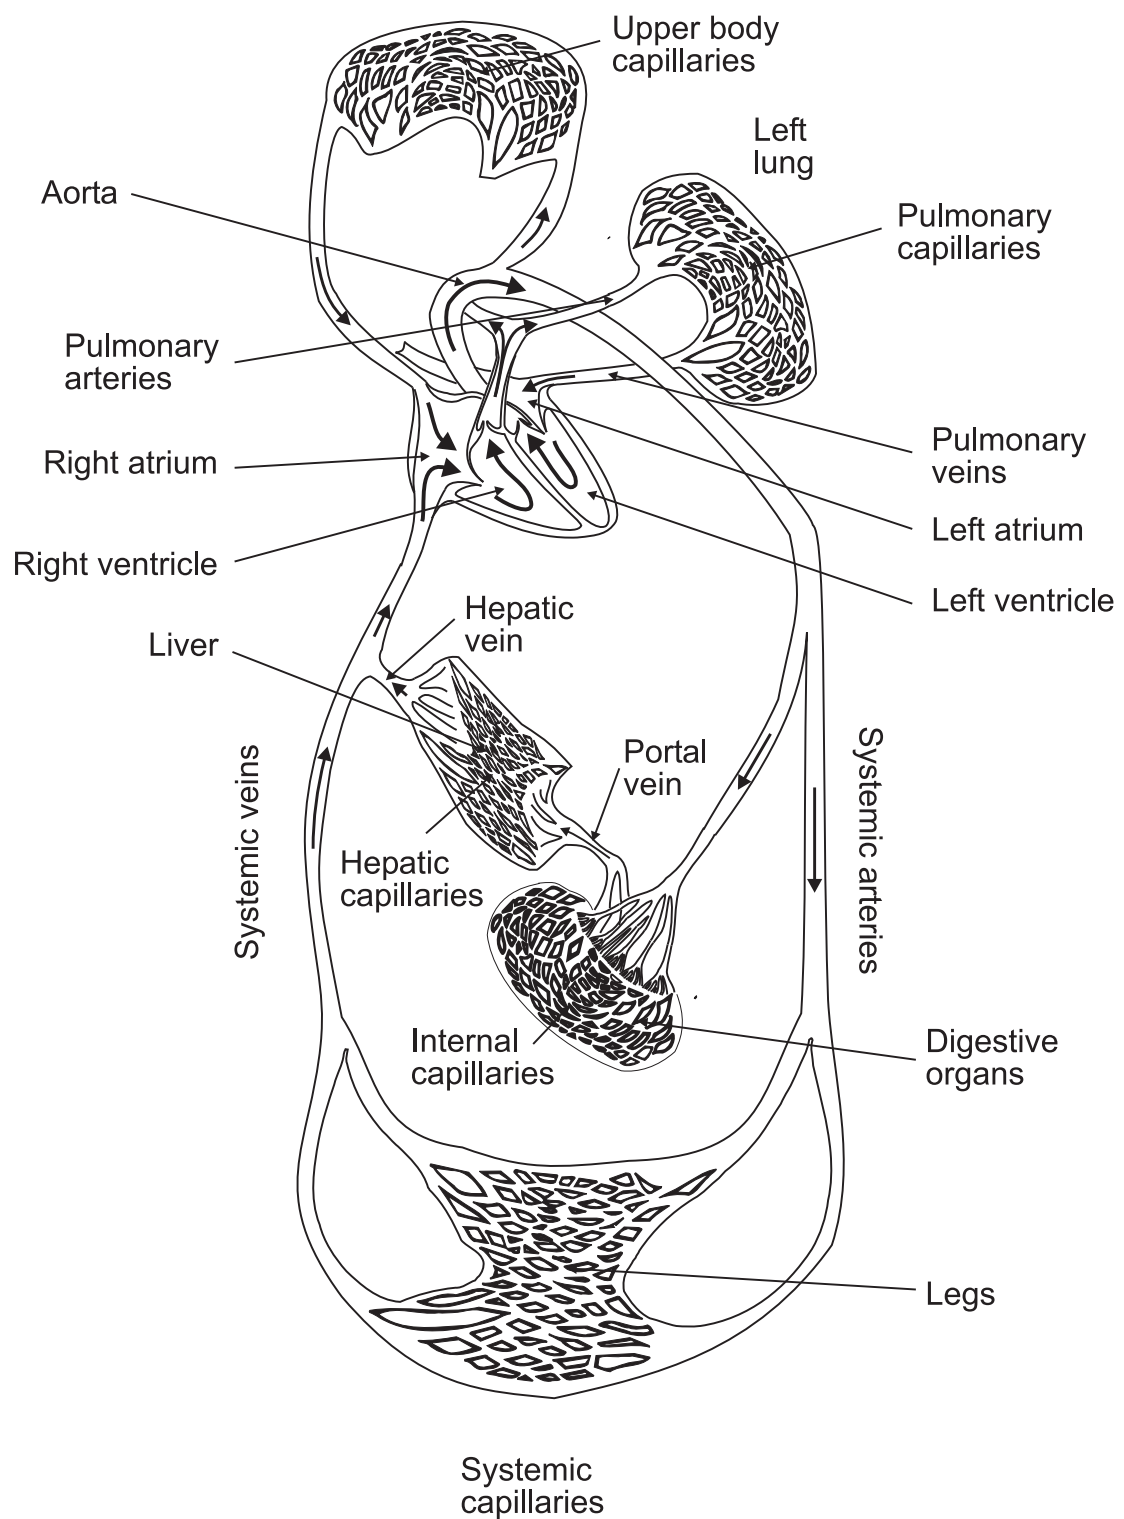


Figure 1.5: Circulatory system of the human body [9]

materials are exchanged between the blood and the organs. The capillaries connect to form a network of venules, which supply the veins and deliver blood back to the heart. This system, in its entirety, is called systemic circulation. A diagram of the circulatory system as described above can be seen in fig. 1.5. In summary, when examining the elements that comprise the circulatory system, it consists of several components:

- Heart, the primary organ of the circulatory system that maintains blood pressure and controls blood velocity.
- Blood, and its sub-components
 - Plasma, which forms the primary volume and contains nutrients and formed cellular elements.
 - Red and white blood cells, which carry oxygen and fight off infections, respectively.
 - Platelets, which are also known as thrombocytes, have the function of clotting during blood vessel injury.
- Blood vessels
 - Arteries (and arterioles), transport oxygenised blood to organs and tissues at high pressure and velocity.
 - Capillaries are thin but wide-ranging blood vessels that perform the exchange of matter between the circulatory system and tissue.
 - Veins (and venules) carry blood back to the heart at low pressure and velocity.

1.2.1 Blood flow

Blood flow is the amount of blood that goes through a blood vessel in a particular period of time, and has a complicated flow pattern due to its pulsing flow. Advanced analysis of haemodynamics is not within the scope of this report, so the explanation will be brief. The primary forces that determine the blood flow F are the pressure difference across a blood vessel and vascular resistance. It is determined by Ohm's law as in eq. (1.16).

$$F = \frac{\Delta P}{R} \quad (1.16)$$

Where ΔP is the pressure difference across the blood vessel and R is the vascular resistance. The pressure difference ΔP is calculated with eq. (1.17).

$$\Delta P = P_1 - P_2 \quad (1.17)$$

Where P_1 and P_2 are the blood pressures measured at each end of the blood vessel. Pressure has a significant importance on blood flow because an increase in arterial pressure not only increases the force that pushes blood through the capillaries but also expands the vessels, lowering vascular resistance. Selected dimensions and flow characteristics can be seen in table 1.3.

1.3 Transducer

Various transducer types are used during the testing of this project. Initially, commercially available transducers were used in order to validate the experimental process of the pulse-echo and Doppler measurements. Commercially available transducers in this context means

Table 1.3: Typical dimensions and flow in human circulatory system [9]

Vessel	Internal diameter (cm)	Wall thickness (cm)	Length (cm)	Young's modulus ($\text{N/m}^2 \cdot 10^9$)	Peak velocity (cms^{-1})	Mean velocity (cms^{-1})	Reynolds number (peak)	Pulse propagation velocity (cms^{-1})
Ascending aorta	1–2.4	0.05–0.08	5	3–6	20–290	10–40	4500	400–600
Descending aorta	0.8–1.8	0.05–0.08	20	3–6	25–250	10–40	3400	400–600
Abdominal aorta	0.5–1.2	0.04–0.06	15	9–11	50–60	8–20	1250	600–700
Femoral artery	0.2–0.8	0.02–0.06	10	9–12	100–120	10–15	1000	800–1030
Carotid artery	0.2–0.8	0.02–0.04	10–20	7–11				600–1100
Arteriole	0.001–0.008	0.002	0.1–0.2		0.5–1		0.09	
Capillary	0.0004–0.0008	0.0001	0.02–0.1		0.02–0.17		0.001	
Inferior vena cava	0.6–1.5	0.01–0.02	20–40	0.4–1	15–40		700	100–700

lead circonate titanate (*PZT*) piezoelectric transducers. PZT is a piezoelectric material that deforms when an electrical voltage is applied, and generates an electrical signal when it is mechanically deformed. PZT transducers are widely used for medical imaging due to their high piezoelectric efficiency, high bandwidth and durability.

At a later stage during the project, CMUTs are used. CMUT, is a newer technology that uses capacitance to convert between electrical and mechanical energy. The transducer consists of a flexible membrane that moves in response to an applied voltage, producing ultrasound signals. CMUTs have advantages in terms of their small size, high frequency, and ability to operate in a broad range of conditions, making them ideal for use in portable and high-resolution imaging devices. They can be produced in large quantities using micro-machining processes that ensure tight parameter specifications, which is difficult to achieve with piezoelectric transducers. Fabricating CMUTs is also simpler than piezoelectric transducers, and batch processing allows for the creation of transducer arrays with various geometries and operating frequencies on a single wafer. The use of standard IC processes also makes it convenient to integrate CMUT arrays with supporting electronics. Additionally, CMUTs can operate over a wider temperature range than piezoelectric devices. Over the last decade, results have demonstrated that CMUTs optimized with regard to design parameters such as device size, membrane radius, thickness, shape, gap height, and operating mode can compare favourably to piezoelectric transducers in terms of bandwidth (170 %), frequency range (100 kHz to 70 000 kHz), dynamic range (130 dBV⁻¹), maximum output pressure (35 kPaV⁻¹), and receive sensitivity (50 dBPa⁻¹Hz⁻¹). There are two types of CMUTs used:

Rigid CMUTs:

- Advantages:
 - Higher mechanical stability, leading to less noise and improved image quality
 - Can handle higher pressures, making them suitable for deeper imaging applications
 - Can have a larger surface area, providing higher sensitivity
- Disadvantages:
 - Less flexible, limiting their use in applications with complex geometries or limited access
 - Higher stiffness, leading to increased power consumption and difficulty in producing high-frequency signals

Flexible CMUTs:

- Advantages:
 - More flexible, allowing them to conform to complex geometries or be used in applications with limited access
 - Can be made thinner and lighter, making them suitable for portable or handheld imaging devices
 - Can be integrated into wearable devices or implanted into the body, enabling new imaging modalities
- Disadvantages:
 - Lower mechanical stability, leading to increased noise and reduced image quality
 - Lower maximum operating pressure, limiting their use in deep imaging applications
 - Smaller surface area, resulting in reduced sensitivity

In summary, the choice between rigid and flexible CMUTs depends on the specific requirements of the application and the trade-off between flexibility, sensitivity, and image quality. For this project, a wearable transducer is desired and therefore the flexible CMUT is preferred.

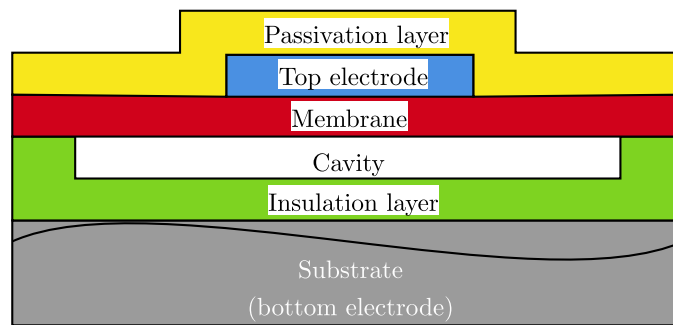
Structure

Figure 1.6: Basic CMUT structure

The key components of the structure are the cavity, membrane, and electrode. CMUT transducers are fabricated using standard integrated circuit (*IC*) fabrication processes, resulting in a capacitor cell that consists of a metallized membrane (top electrode) suspended above a heavily doped silicon substrate (bottom electrode), as depicted in fig. 1.6. An insulating layer is included to prevent the two electrodes from making contact and shorting. A single transducer element consists of multiple small capacitor cells connected in parallel. By arranging transducer elements in various geometries, any array shape can be achieved, as demonstrated in fig. 1.7. In (a), circular membranes with a diameter of $24\text{ }\mu\text{m}$ have approximately 50 % active area coverage. In (b), circular membranes with a diameter of $80\text{ }\mu\text{m}$ have 72 % active area coverage. (c) displays hexagonal membranes with a diameter of $80\text{ }\mu\text{m}$ that have 86 % active area coverage. Finally, (d) demonstrates tented membranes in which the etch holes are located on the post, providing over 90 % active area coverage.

1.3.1 Impedance matching

Impedance matching refers to the adjustment of the output impedance of the transducer to match the input impedance of the receiving system, such as the ultrasound machine or amplifier. This ensures maximum transfer of energy from the transducer to the receiving

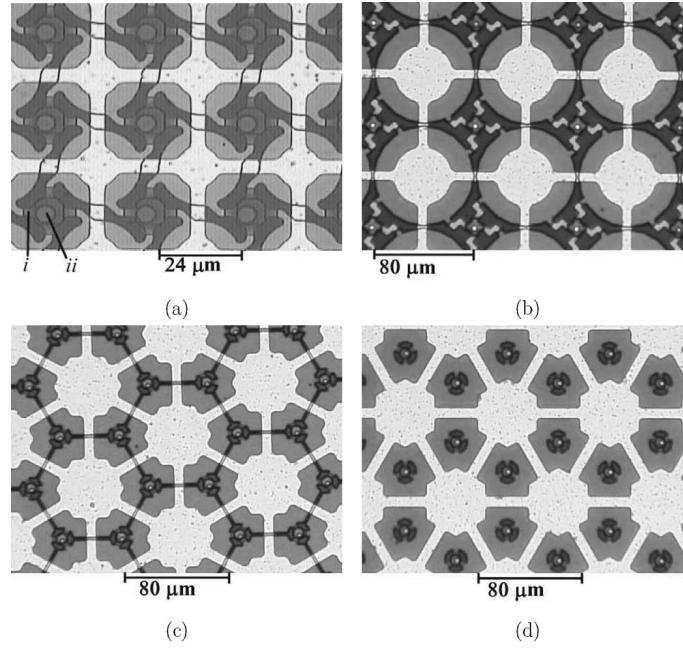


Figure 1.7: Optical images of various cMUT elements with different membrane shapes and sizes are shown to illustrate their relationship to active area coverage [5]

system, leading to improved signal strength and reduced noise in the final image. In ultrasound imaging, the transducer is used to both transmit and receive ultrasound signals. The impedance of the transducer must be carefully matched to the environment it is operating in, to ensure efficient transfer of energy both ways. If the impedance of the transducer and the receiving system do not match, a portion of the transmitted energy will be reflected back to the transducer, leading to reduced signal strength and increased noise in the final image. This can also result in increased power consumption and reduced battery life in portable or handheld imaging devices.

1.4 Devices

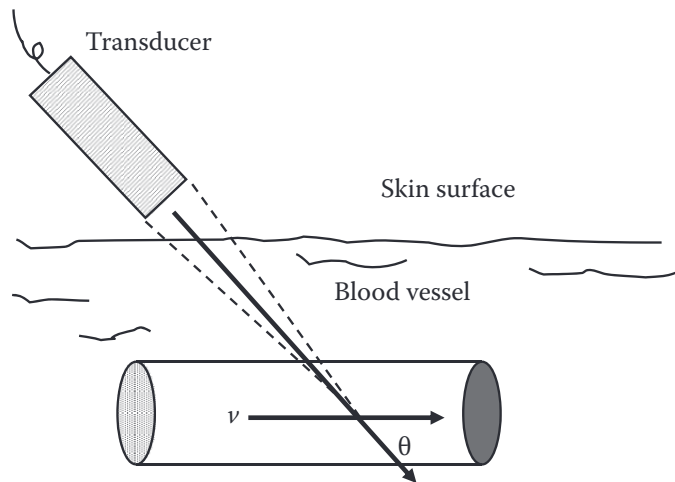


Figure 1.8: Diagram of *US* wave transmitted and reaching blood vessel with incident angle θ [12]

A device that measures the flowing of blood is called a flowmeter. Flowmeters may be used both inside and outside of vessels. One of the flowmeters that may be used outside the vessel to monitor flow is *US*. Figure 1.8 depicts an ultrasonic wave of frequency f insonifying a blood artery, resulting in an angle of θ relative to velocity v . For simplicity, it is assumed that blood flows in a vessel at a constant velocity v . The echoes returned are shifted in frequency as described in eq. (1.15) earlier in the chapter. The echoes scattered by blood after being insonified by an ultrasonic wave convey information about the velocity of blood flow. Blood flow measurements are often used in clinical settings to determine the status of blood vessels and organ functioning. The two commonly used fundamental techniques for ultrasound Doppler flow measurements are continuous-wave (*CW*) and pulsed-wave (*PW*). Both will be explained.

1.4.1 Continuous-wave Flowmeter

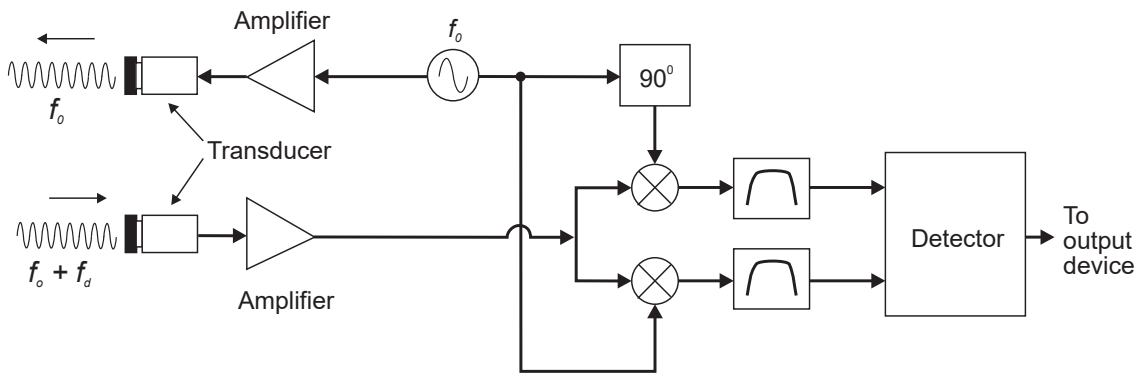


Figure 1.9: Block diagram of *CW* flowmeter [9]

The earliest non-invasive cardiovascular diagnostic technologies relied heavily on *CW* Doppler flowmeters. One of the earliest concepts for a device to estimate and study blood flow was proposed by [1] during the 1950s in Japan. To continuously transmit waves and receive signals from moving reflectors, the *CW* flowmeter uses two transducers. *CW* flowmeters use less sophisticated electronics than *PW* flowmeters. A drawback to the *CW* flowmeter is the lacking depth discrimination due to the continuous characteristic of this device type. A block diagram of a typical *CW* flowmeter can be seen in fig. 1.9. The basic principles of the device are previously explained in section 1.1.4, and the measurement of the device is described in eq. (1.11). The device continuously emits an ultrasonic wave in the first transducer expressed as a function of time by eq. (1.18) [9].

$$e(t) = \cos(2\pi f_0 t) \quad (1.18)$$

While receiving the backscattered signal on the second transducer expressed by eq. (1.19) [9].

$$r_s(t) = a \cos(2\pi f_0 \alpha(t - t_0)) \quad (1.19)$$

$$\alpha \approx 1 - \frac{2v_z}{c} \quad (1.20)$$

$$\alpha t_0 \approx \frac{2d_0}{c} \quad (1.21)$$

Where v_z indicates the velocity in the z direction. Applying the Fourier transform, the expression yields eq. (1.22).

$$r_s(t) \cdot e^{j2\pi f_0 t} \Longleftrightarrow R_s(f - f_0) \quad (1.22)$$

Where $R_s(f - f_0)$ is the Fourier transform of $r_s(t)$. The received signal is then multiplied with a quadrature signal of frequency f_0 to find the Doppler frequency in eq. (1.23).

$$m(t) = a [\cos(2\pi f_0 t) + j \sin(2\pi f_0 t)] \cos(2\pi f_0 \alpha(t - t_0)) \quad (1.23)$$

$$= \frac{a}{2} \left\{ \cos(2\pi f_0 [(1 - \alpha)t - \alpha t_0]) + \cos(2\pi f_0 [(1 + \alpha)t - \alpha t_0]) \right. \\ \left. + j \sin(2\pi f_0 [(1 - \alpha)t - \alpha t_0]) + j \sin(2\pi f_0 [(1 + \alpha)t - \alpha t_0]) \right\} \quad (1.24)$$

As is general for quadrature demodulation, the resulting signal contains the frequency components of the sum and difference of the emitted and received signals' frequencies shown in fig. 1.10, where the signals are shown in time and frequency domains.

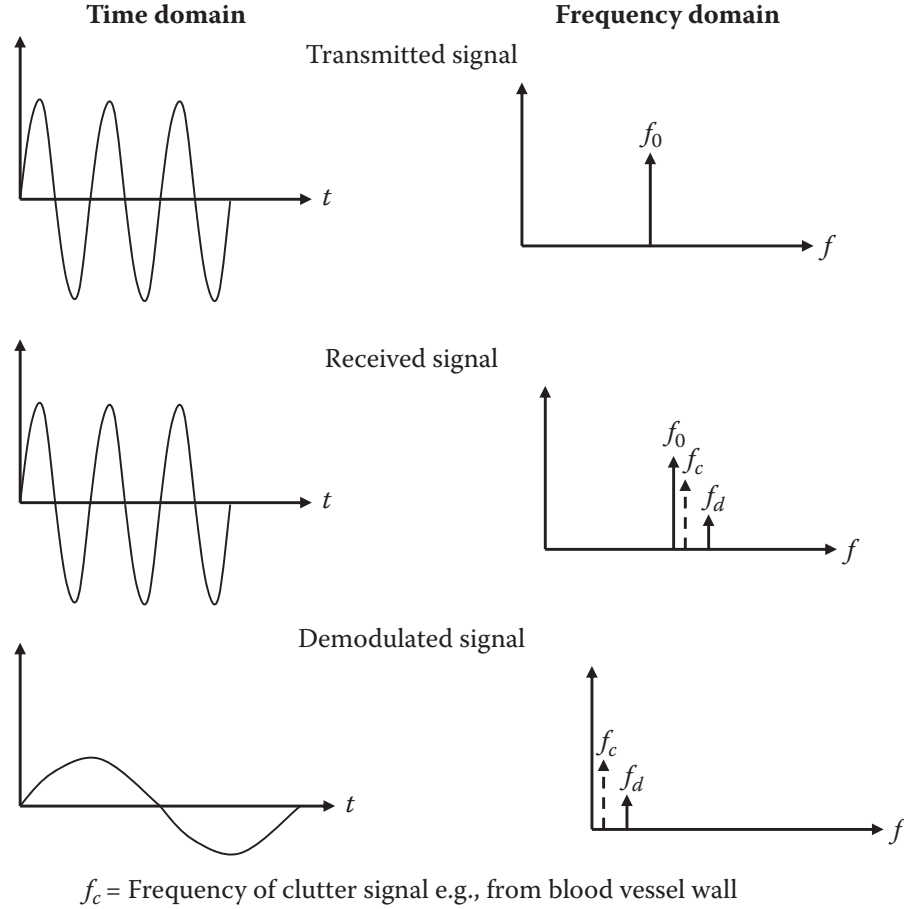


Figure 1.10: Doppler signals in time and frequency domain showing demodulation effects [12]

Generally, a band-pass (*BP*) filter is used on the demodulated signal to remove the high-frequency summed signal at twice the frequency of f_0 . The filtered signal after the *BP* filter is expressed by eq. (1.25) and contains the Doppler shift of the emitted signal.

$$m_f(t) \approx \frac{a}{2} e^{(j2\pi f_0 \frac{2v_z}{c} t)} e^{(-j2\pi f_0 \alpha t_0)} \quad (1.25)$$

Where the second exponential term is the delay proportional to the time between transmission and receiving of the signal. The selected cutoff frequency is chosen to be much lower than the carrier frequency to remove the carrier wave. One issue with ultrasonic Doppler

blood flow monitoring is that the blood vessels that generate large reflected echoes are also moving with a low velocity. These big, slow-moving echoes are referred to as clutter signals in Doppler nomenclature. The band pass filter's low-end cutoff frequency must be designed to minimize interference from these clutter signals. The design of this band pass filter in the low-frequency region, which serves the function of high pass, also known as a clutter rejection filter, has proven troublesome since the magnitude of clutter signals is many orders greater than that of blood and may obfuscate those from slow-moving blood.

Table 1.4: Measured frequency shifts with a Doppler 3 MHz transducer at various velocities at a 45° incident angle [9]

Velocity (v) m/s	Doppler frequency (f_d) Hz
0.01	28
0.1	276
0.5	1377
1	2755
2	5510
5	13 770

Seen in table 1.4 is an example of measured Doppler frequencies using a 3 MHz transducer using the method shown in fig. 1.8. Note that the measured frequencies are all within the audible range.

1.4.2 Pulsed-wave Flowmeter

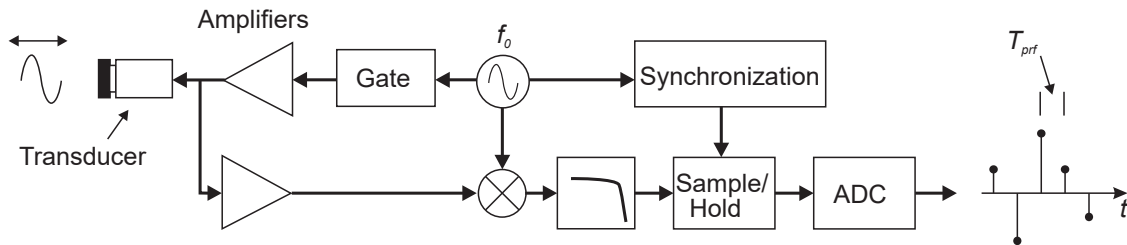


Figure 1.11: Block diagram of *PW* flowmeter [9]

The concept of a pulsed-wave flowmeter was proposed in [2] and other related articles. This type of flowmeter is periodically changing from a transmitter to a receiver. In the transmit mode, the transducer emits a series of pulses. When in the receiving mode, the transducer is listening for the backscattered signal. A simplified block diagram can be seen in fig. 1.11. The movement of particles within the blood causes a displacement in the backscattered signal. These systems are commonly referred to as “Doppler systems” even though it is somewhat misleading. The effects of attenuation are also causing a shift in frequency of a higher magnitude than the velocity of particles in the blood. This is because the conventional Doppler effect is not the straightforward methodology that is applied to the analysis of the back-scattered signal. It is, in fact, an artefact. It is the shift in the location of the scatters that is observed, not the shift in the transmitted frequency. Figure 1.12 shows the received signal after demodulation and filtering; the depth in tissue is fixed here, and the signals displayed on the left side of the figure are the result of a pulse sequence. Each line represents a single pulse, and each pulse is emitted at a pulse

repetition frequency, f_{prf} . Instead, on the right, the dotted line shows the sampled signal formed by taking into account the amplitude of each pulse after a specified time period. To depict the signals on the graph, a single pulse is emitted for each line, and the signals are displaced in amplitude. The sampled signal is displayed on the right.

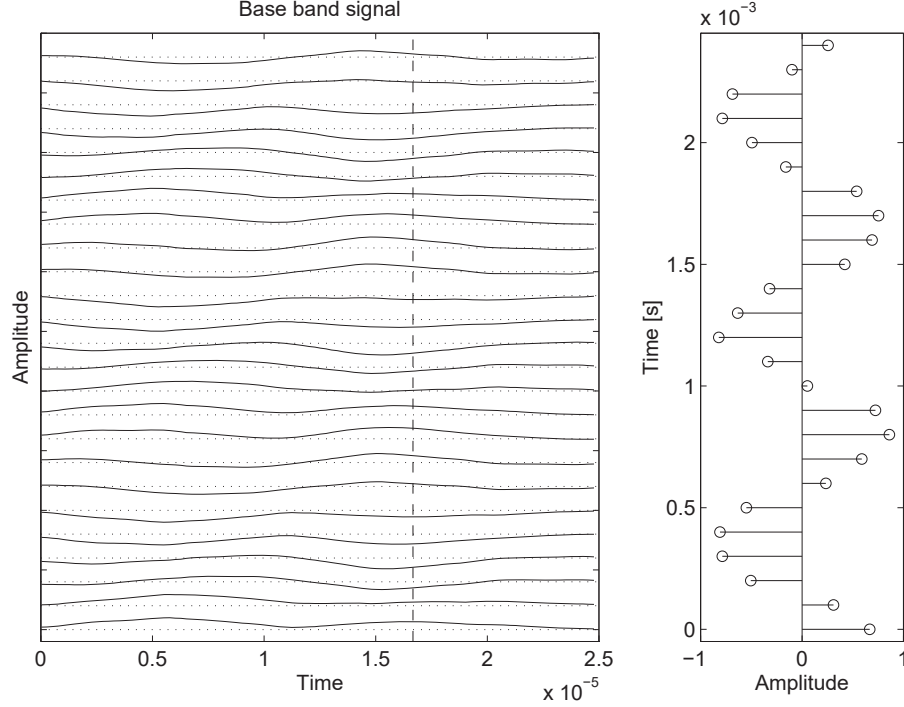


Figure 1.12: Sampling for a gate pulsed wave system with a single range [9]

After the back-scattered signal is received it is multiplied by the centre frequency of the emitted pulse and filtered to remove the sum frequency [9]. A analogue-to-digital converter (*ADC*) quantifies the signal for further signal processing. Referring to displacement fig. 1.12 again, the dashed vertical line represents the sample of each pulse that is taken. If sampling is done T_s after pulse emission, the measurement depth is expressed by eq. (1.26).

$$d_0 = \frac{T_s c}{2} \quad (1.26)$$

Hypothetically, if the velocity of stationary scatterers in blood was measured, a constant amplitude would be measured. A change in the sample value is observed when there is movement. Between two pulses, the scatterer movement is proportional to the velocity v_z in the direction of the ultrasound beam. The time shift of t_s is expressed as eq. (1.27).

$$t_s = \frac{2v_z}{c} \cdot T_{\text{prf}} \quad (1.27)$$

Where c is the speed of sound, and T_{prf} is the timespan between each pulse emission. Taking one sample from each line at a certain depth yields a sampled signal with a frequency proportional to the scatter velocity. Thus, if a sample is taken at the same depth for each line, resulting in a sinusoidal signal proportional in frequency to the scatter velocity [4] and that signal is expressed by eqs. (1.28a) and (1.28b).

$$r(i) = a(i) \sin(2\pi f_p T_{\text{prf}} + \theta) \quad (1.28a)$$

$$f_p = \frac{2v_z}{c} f_0 \quad (1.28b)$$

Where $a(i)$ is the amplitude, f_0 is the emitted frequency, and θ is the phase factor in the depth of interest. This technique improved the accuracy of the investigations of blood vessels and facilitated the display of velocity profiles. Furthermore, by employing two transducers or a multi-element transducer, duplex mode imaging (displaying both a B-mode picture and a blood velocity estimate) became feasible. Two-transducer systems are no longer utilised since it is easier to create a duplex picture with a multi-element transducer.

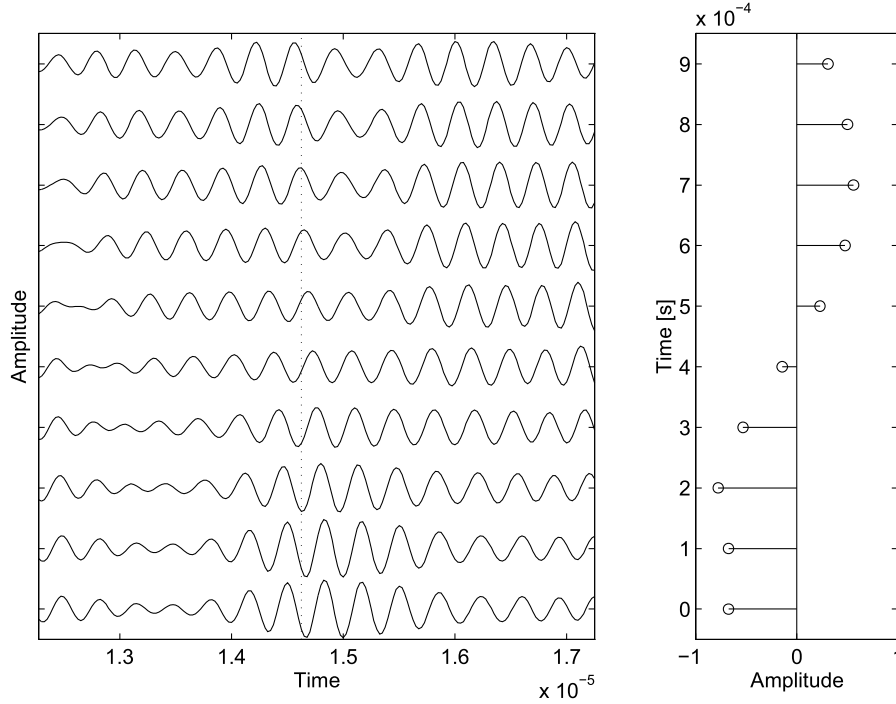


Figure 1.13: Simulated RF sampling of blood vessel with segmented receiver line with a sample interval denoted by a dotted line (left) and the resulting amplitude of the sample (right)

Figure 1.13 displays a signal that has been sampled using RF technology. As the scatterers in the image move away from the transducer, the shift in the pulsed signal is present. The measurement is created by taking one sample at a specific depth (d_0) for each RF line, using a sample/hold circuit. The sampling is performed at a frequency of f_{prf} , as indicated by the dotted line in the figure. Due to the slow movement of the received signals past the sample volume, there is a gradual change in the sampled signal over time. As a result of the slow movement of the signals, the frequency of the sampled signal is much lower than that of the RF signal. It's worth noting that the received signal not only shifts in time from pulse to pulse, but its shape also changes. This is because the signal is constructed by adding up responses from many scatterers that move at different speeds. A stationary structure will result in an identical sample value for all segmented RF lines. The spectrum of this stationary signal is shown in eq. (1.29).

$$|H_s(f)| = \left| a \frac{\sin(\pi f N T_{\text{prf}})}{\sin(\pi f T_{\text{prf}})} \right| \quad (1.29)$$

which for $f = 0$ is equal to aN and has its first zero at f_{prf}/N . The signal spectrum based on eq. (1.29) is shown in fig. 1.14.

When dealing with small blood vessels, the stationary echoes can be significantly stronger

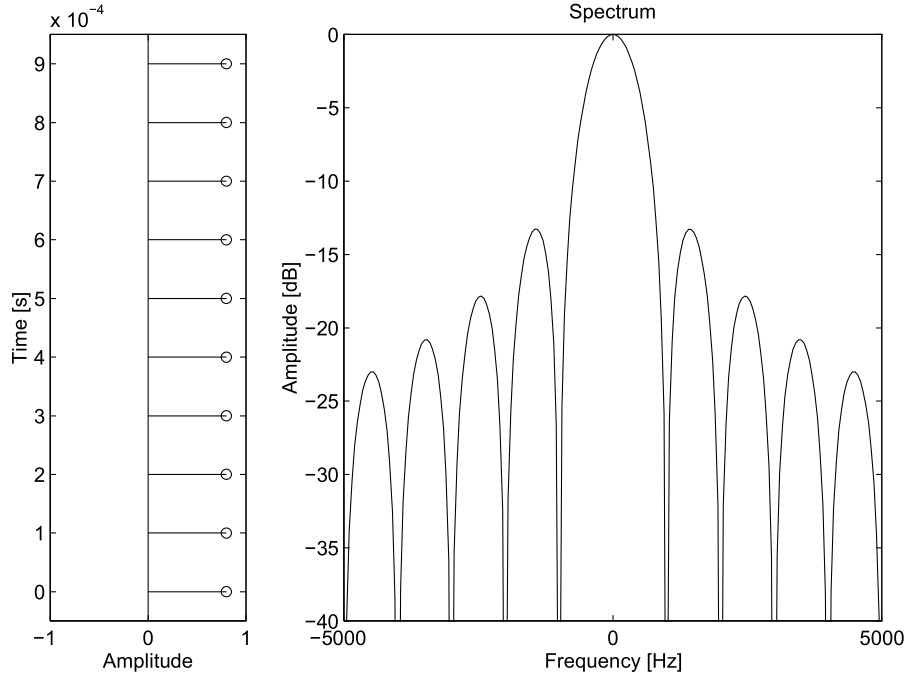


Figure 1.14: Stationary tissue sampled signal (left) and stationary tissue sample spectrum (right) [9]

(up to 40 dB) than the blood signal itself. To properly visualize blood flow details, the stationary signal must be eliminated from the sonogram. This requires setting the cutoff frequency to at least $f_{\text{prf}} = N$, in order to remove the main component. In some cases, a higher cutoff frequency may be necessary, particularly if the stationary echo is strong or the vessel wall is in motion.

1.5 Blood Velocity Estimation

Once a backscattered signal is received and sampled, estimation of velocity can be obtained with multiple methods. In this section the most common methods to estimate blood velocity are mentioned with their strengths and limitations.

1.5.1 Spectral estimation

Given that the frequency volume of the received signal is similar to the blood's velocity distribution, the Fourier transform of the received signal can be used to obtain velocity. The spectrogram, usually erroneously known as the Doppler spectrum, can be created by saving the power spectral density (*PSD*) together. The *PSD* is calculated for each of the components that make up the received signal in order to accomplish this. A quadrature demodulated signal is used to display both positive and negative frequencies. When these spectra are shown side by side, the evolution of the velocity distribution can then be seen. A sonography of an artery is displayed in fig. 1.15.

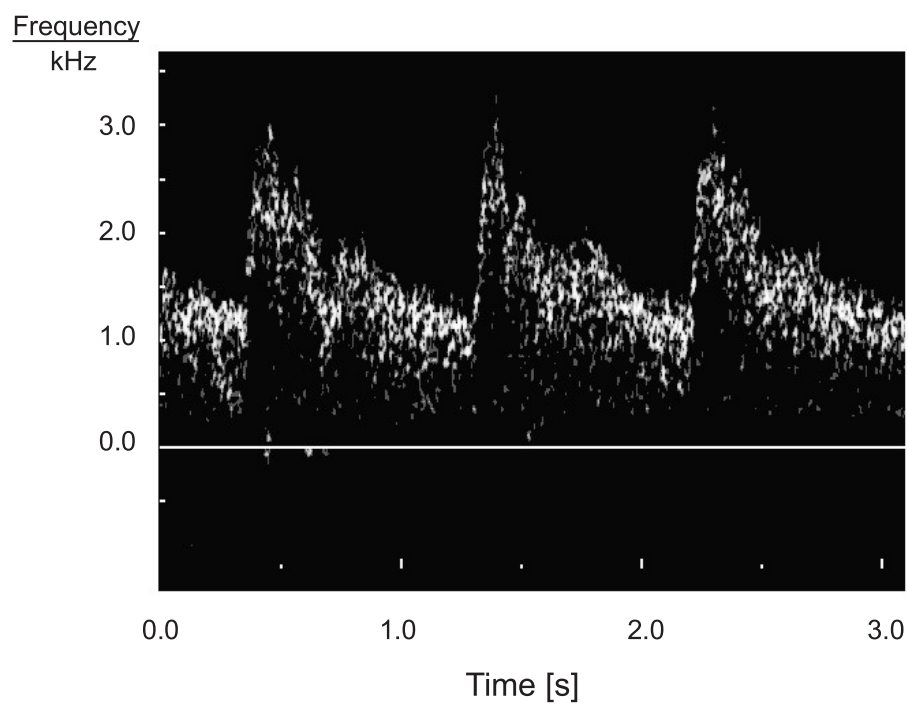


Figure 1.15: Arterial sonogram with time-frequency and Doppler shift [9]

2 Synthesis

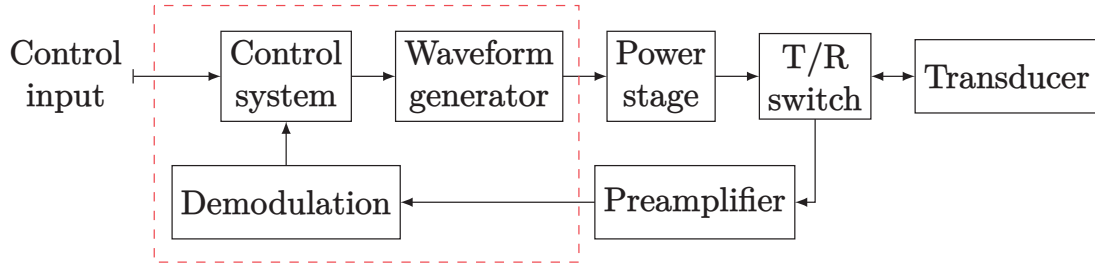


Figure 2.1: Simplified overview of the system with the demodulation and control system indicated with a red dashed rectangle

A simplified overview of the entire system can be seen in fig. 2.1. Each of the various modules will be explained during this chapter of the report. Initially, the control system will be briefly explained and the reasons for its design choice. Secondly, the signal chain in the transmitter will be outlined and how the transducer is driven by the power stage with the added protective switching circuit. Finally, the analogue front-end will be further explained with its various subcircuits for amplifying and demodulating the signal. Lastly, the design of the digital signal processor (*DSP*) within the control system will be explained.

2.1 Control System

The choice of platform for the control system is a microcontroller. A microcontroller is a small computer that is built into a single *IC* chip. It includes a central processing unit (*CPU*), memory, and input/output (*I/O*) peripherals, and it is designed to perform a specific set of tasks. Microcontrollers are used in a wide range of electronic devices, including appliances, automobiles, industrial control systems, and consumer electronics. Microcontrollers are often used in applications where a small, low-power device is needed to perform simple tasks, such as controlling a motor or reading a sensor. They are usually programmed in a high-level language, such as C or C++, and they can be programmed to perform a variety of tasks, depending on the specific application. The chosen microcontroller unit (*MCU*) for this project is STM32F411RE, because it is sufficient for the application and sourcing limitations within the *IC* supply chain. For implementing the control system, a real-time operating system (*RTOS*) can offer multiple benefits for the embedded system development. A *RTOS* is an operating system that is designed to handle real-time applications. Real-time applications are those that require timely processing of data in order to function correctly. This can include tasks such as controlling industrial machinery, monitoring and controlling processes. Real-time operating systems are designed to prioritize certain tasks and ensure that they are completed within a specific timeframe. They do this by allocating a certain amount of processing resources to each task, and by interrupting the execution of lower-priority tasks as needed to ensure that high-priority tasks are completed on time. *RTOS*s typically include features such as preemptive scheduling, real-time communication, and support for multiple processors and hardware architectures. Alternatively, a vendor-locked baremetal implementation is an option, in this case STM32 HAL. Differences between the two options are:

- Multitasking: *RTOS* allows for parallel execution that enable more complex applications.

- Portability: Standard APIs mean that the same code can be easily ported to other devices and even other platforms without modifications.
- Reduced development time: Especially for rapid prototype development, using pre-existing APIs significantly reduces development time by providing many of the low-level tasks such as scheduling, resource management, and timing by the operating system.
- among others.

2.1.1 Development Environment

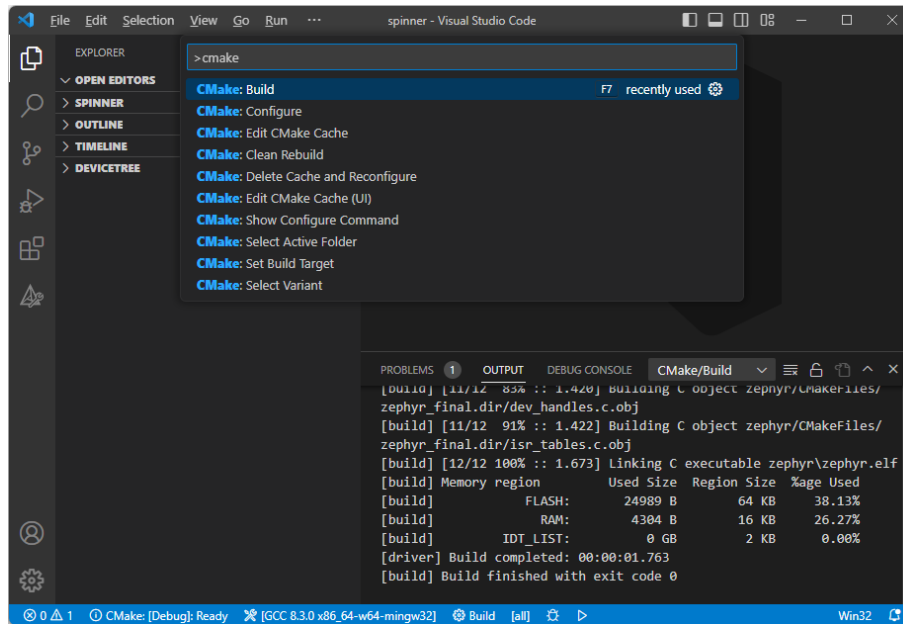


Figure 2.2: VSCode editor with CMake Tools active, displaying available tasks

Visual Studio Code (VSCode) is an open-source code editor developed by Microsoft. It is designed to be highly customizable and efficient, with a wide range of features and extensions that allow developers to customize their workflows and improve their productivity. VSCode works in synergy with CMake through an extension. CMake is a cross-platform build system that helps developers manage the build process for their projects. It is used to generate build files for different platforms and build systems, to build projects on a wide range of platforms. When using CMake with VSCode, the basic idea is to use the CMake extension for VSCode to generate the appropriate build files for the target platform, and then use the VSCode tasks and debugging capabilities to build and debug the project. After setup of VSCode, the CMake Tools [21] extension can be found in the VSCode Marketplace. The CMake Tools extension allows you to create, configure and build CMake projects from within VSCode. Once the extension is installed, you can create a new CMake project and configure it by specifying the path to the `CMakeLists.txt` file and other settings like the target platform and build configuration. After configuring the project, the VSCode tasks are provided to build and run the project. These tasks are defined in the `tasks.json` file, which can be customized to specify the build command and other options. Examples of tasks are build the project, cleaning the build directory, or running tests. The available CMake tasks are shown in fig. 2.2. In addition to building and running the project, VSCode allows for debugging capabilities to debug code.

2.1.2 Zephyr

Zephyr is an open-source *RTOS* designed to be lightweight and run on a wide range of devices, from *MCUs* with as little as 20 kB of random access memory (*RAM*) to more powerful systems with multiple processors. Zephyr is designed to be modular and scalable, with a focus on security and low power consumption. It includes support for a wide range of hardware architectures, including ARM Cortex-M, x86, and RISC-V, and it can be used with a variety of development boards and microcontrollers. One of the key features of Zephyr is its ability to run on very small devices with limited resources. It includes support for various networking protocols, such as bluetooth low energy (*BLE*), IPv4, and IPv6, which makes it well-suited for use in Internet of Things (*IoT*) applications. Zephyr is developed as part of the Linux Foundation's Zephyr Project, and it is widely used in the development of IoT and embedded systems.

Build System

To build an application with the Zephyr kernel, you use CMake which has two phases - configuration and build. During configuration phase, CMake executes the `CMakeLists.txt` build scripts to generate an internal model of the Zephyr build. Starting with device tree source (*DTS*) and device tree source include (*DTSI*) and then using the device-tree nodes and Kconfig to configure the set of build files for ninja. Seen in fig. 2.3 is the

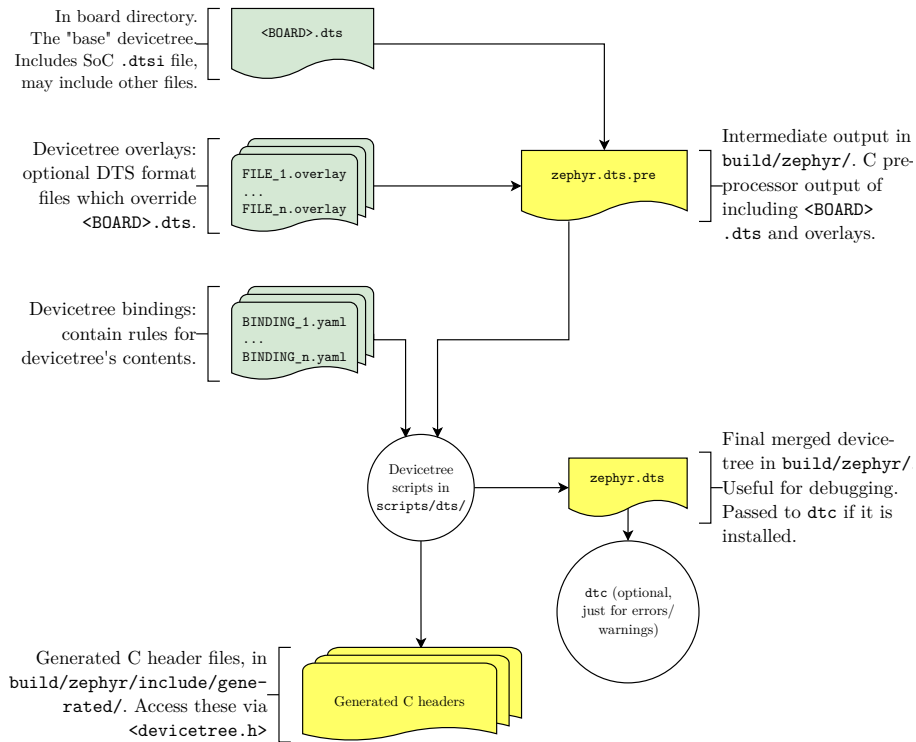


Figure 2.3: Devicetree input files (green) and output files (yellow) [19]

process in which the build system searches out device-trees in certain locations and merges them into the `zephyr.dts` that will be used for configuring and mapping every peripheral. Typically, each supported board has a file called `BOARD.dts` that defines the hardware of the board. The `BOARD.dts` file includes one or more `.dtsi` files that describe the CPU or system-on-chip that Zephyr runs on, and other common hardware features shared by multiple boards. These `.dtsi` files may also include other `.dtsi` files. Additionally, the `BOARD.dts` file provides a description of the specific hardware of the board. After parsing the `BOARD.dts` file, the main point being the merge with the `.overlay` file specific to both the project and the board. This overlay enables the portability feature of Zephyr. A

significant degree of the workload when implementing Zephyr projects are thus in writing hardware devicetrees and then writing as generic firmware implementations as possible. Next, the configuration phase can be seen in fig. 2.4. Once configuration phase is done, CMake generates build scripts that are native to the host platform and initiate the build sequence with the build system Ninja [18]. Afterwards, the generated build scripts are executed to begin the second phase, build. The build scripts can recompile the application without involving CMake after most code changes. Zephyr uses CMake's target concept to organize the build, where a target can be an executable, a library, or a generated file. The final output of Ninja is a binary file ready for flashing using a microcontroller programmer.

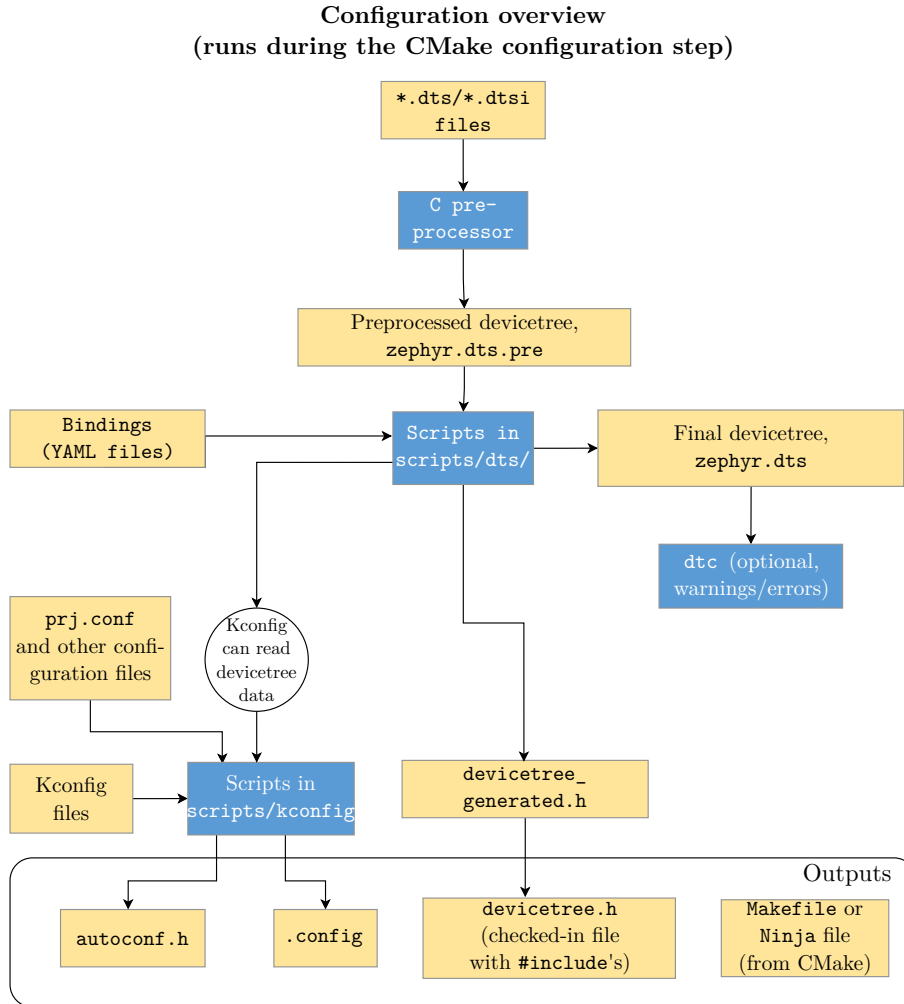


Figure 2.4: Configuration phase of a Zephyr application [19]

After cmake configuration phase has completed, the build phase begins. CMake invokes the build system, which (conceptually) has five (six, one is repeated) stages: (I) pre-build, (II) generation and compilation, (III) first-pass binary (and (IV) second-pass binary), (V) final binary and (VI) post-processing. In fig. 2.5 the build system binds system call functions to implementations. Next, in fig. 2.6 the build system collects source files for various subsystems (decided by the configuration phase) and compiles into archives. The `gen_app_partitions.py` script examines all the archives that are produced and creates linker scripts that organize and align application partitions correctly, based on the memory protection hardware of the target. Then `cpp` process involves merging linker script fragments from various sources, including the target's architecture/system-on-a-chip (SoC), the kernel

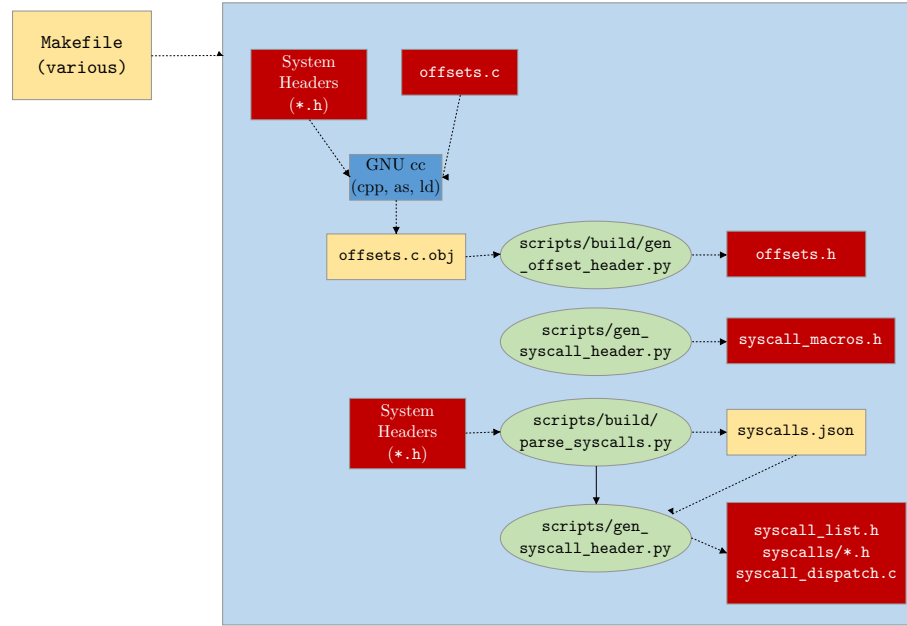


Figure 2.5: Flowchart of build stage I, pre-build

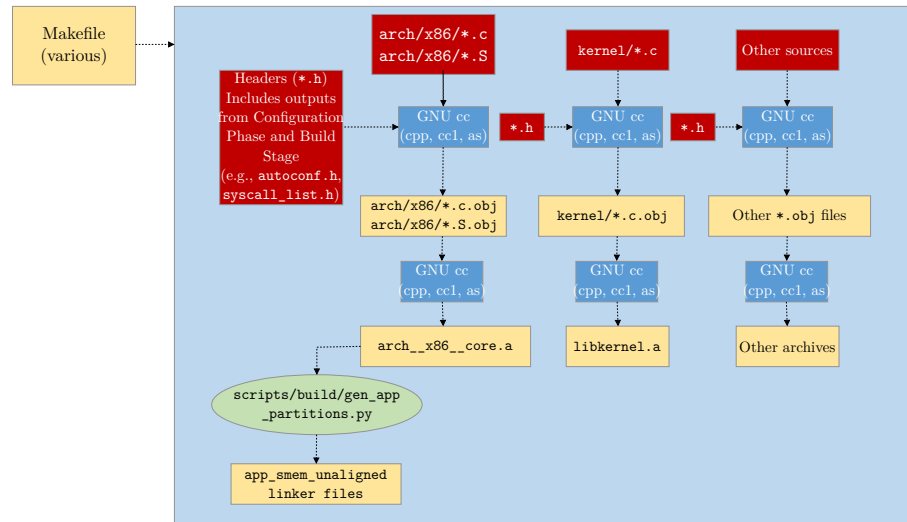


Figure 2.6: Flowchart of build stage II, generation and compilation

tree, partition output (if memory protection is enabled), and any other selected fragments from the configuration process. These are combined into a `linker.cmd` file. The compiled archives are then linked with `ld`, following the specifications in the `linker.cmd` file. Shown

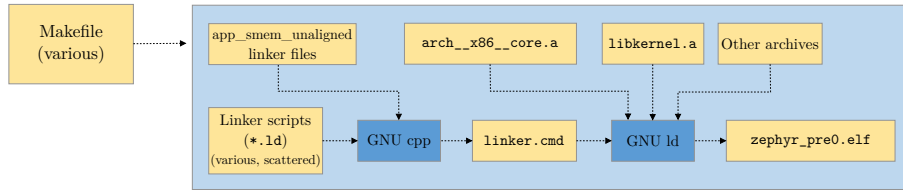


Figure 2.7: Flowchart of build stage III, intermediate binary

in fig. 2.7 is the process, in which an unfixed size intermediate binary is produced. If a devicetree is being used, an intermediate binary is generated that has a variable size. The binary is not fixed in size, which means that it can be modified by post-processing steps that affect the size of the final binary. In Figure 2.8 the fixed size intermediate binary is

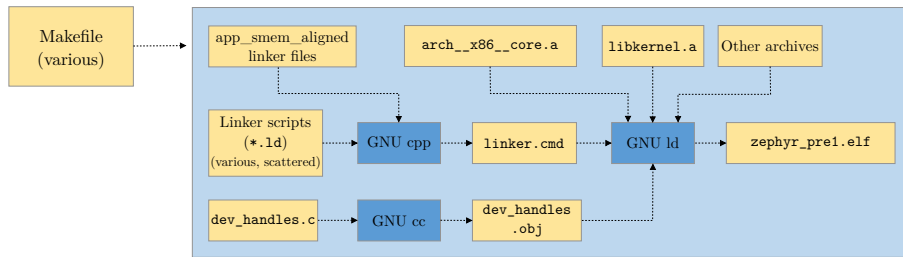


Figure 2.8: Flowchart of build stage IV, second intermediate binary

generated. The previous stage's binaries are not fully formed and contain sections that are empty or marked as placeholders. These sections must be filled in by a process similar to reflection. To finish building, certain scripts are run on the intermediate binaries. These scripts generate the necessary components that are missing from the final binary. Next, in

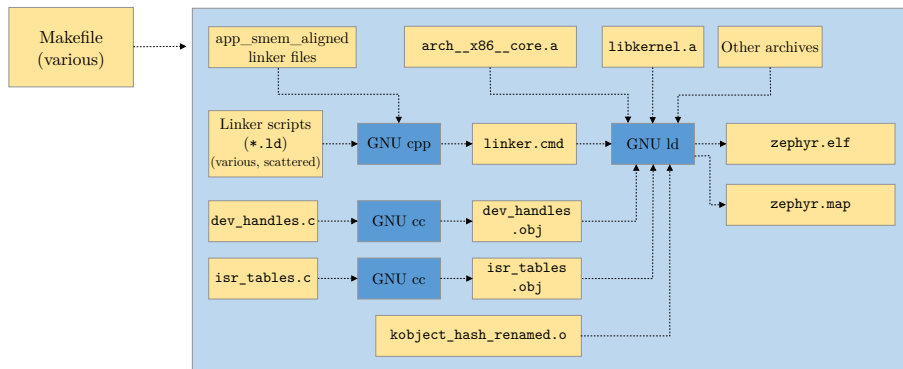


Figure 2.9: Flowchart of build stage V, final binary

fig. 2.9, the final binary is produced by repeating the link from the previous stage, but this time with all the missing pieces populated. Finally, in fig. 2.10, using `GNU objdump`, the completed kernel is converted from an executable and linkable format (*ELF*) file to the hex file that is expected by the flash tool compatible with the target device.

2.1.3 Firmware

A full repository of the revision controlled codebase is available on GitHub at [22].

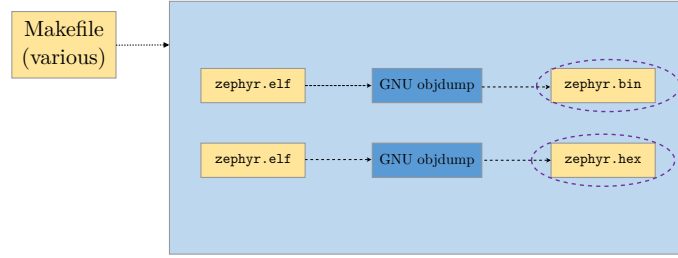


Figure 2.10: Flowchart of build stage VI, post-processing

2.2 Pulse-Width-Modulation Generator

Initially, a waveform generator was designed by using a programmable synthesizer circuit, but due to constraints within generating complementary PWM with dead-time when driving the half-bridge, a timer based PWM generation in the *MCU* is preferable. In a half-bridge power stage, dead-time refers to the amount of time that elapses between the moment when one of the switches in the half-bridge (either the high-side or the low-side switch) turns off and the moment when the other switch turns on. During the dead-time, both switches in the half-bridge are off, which means that there is no current flowing through either switch in the half-bridge. A scenario where both switches are on, can cause problems if the output of the half-bridge is connected to a load, as it may cause the load to behave erratically or even be damaged. To avoid these problems, it is important to carefully consider the amount of dead-time in a half-bridge power stage. In general, a longer dead-time will reduce the risk of damage to the load, but it will also reduce the efficiency of the power stage, as energy will be lost during the dead-time. Therefore, it is important to carefully balance the trade-off between efficiency and safety in order to determine the optimal amount of dead-time for a given half-bridge power stage. Based on discussions during design review, it was decided to change approach and generate the two complementary PWM signals by configuring the PWM module of the microcontroller with the functionality though with a trade-off in resolution. However, for this application there is no need to amplitude modulate the output signal and therefore no downside.

2.3 Power Stage

Several MOSFET drivers were considered, e.g. ISL55111[17], EL7104[6], and MD1213[15]. The MD1213 has an advantage over the ISL55111 or EL7104 for ultrasound MOSFET drivers since it is specifically designed for high-voltage P-channel and N-channel MOSFETs in medical ultrasound and other applications needing a high output current for a capacitive load. It has a high-speed input stage with a logic interface that can function from 1.8 V to 5 V and an ideal operating input signal range of 1.8 V to 3.3 V. The DC-coupled adaptive threshold circuit sets the level translator switch threshold to the average of the input logic LOW and logic HIGH levels. Consequentially, the MD1213 is designed primarily for driving MOSFETs in medical ultrasound applications, whereas the ISL55111 and EL7104 are more general-purpose drivers that may not perform as well in ultrasound applications. The MD1213's output stage has a distinguishing features in that the L and H levels of the output signal may be set independently of the rest of the circuit's supply voltages. The input logic levels, for example, might be 0 V and 1.8 V, whereas the control logic is powered by +5 V to -5 V. The output L and H values, on the other hand, may be changed between -5 V to +5 V. This gives you greater flexibility in adjusting the output signal levels to meet individual needs. The output stage may also provide peak currents of up to

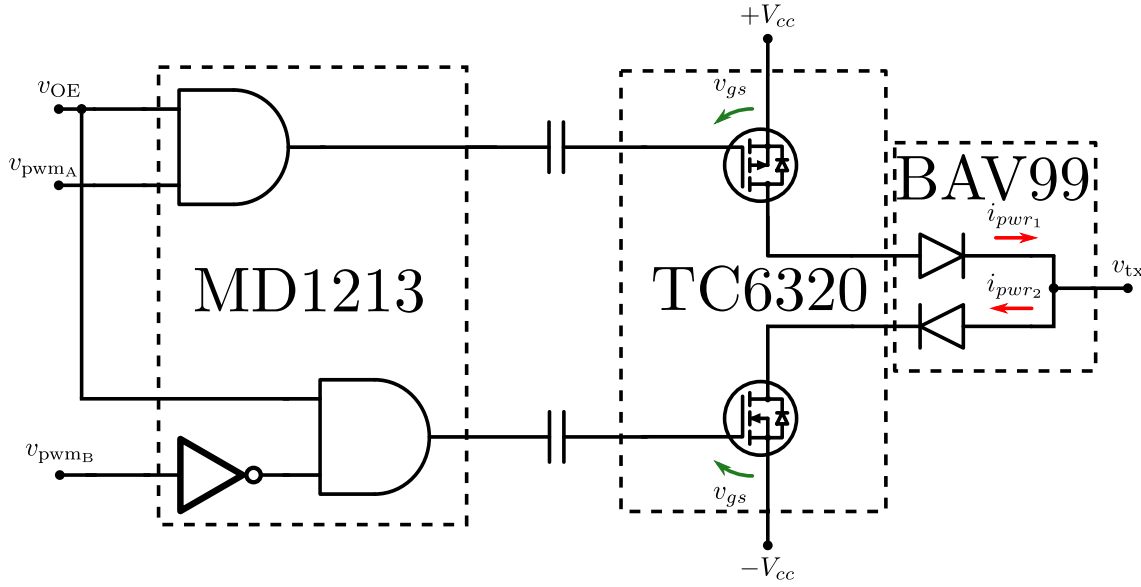


Figure 2.11: Circuit diagram of power stage

2 A, depending on the load capacitance and supply voltages employed.

2.4 Transmit/Receive Switch

Among the design considerations for the transmit and receive switch were the TX810[8] and MD0101[16]. Both ICs are acceptable choices, however the MD0101 is a newer and generally better choice since it has a lower insertion loss, which means that less of the ultrasound signal is lost as it passes through the switch. This results in a higher quality image with better signal-to-noise ratio. Additionally, MD0101 has a wider bandwidth, which means that it can transmit and receive ultrasound signals over a broader range of frequencies. However, since the TX810 is in stock and is also acceptable, it was chosen for the design. TX810 is an IC from Texas Instruments that can be used to switch transmit and receive paths of an ultrasound system. It can switch the transmit and receive paths for up to 8 different transducers (also known as probes) at the same time. The TX810 is programmed to switch the transmit and receive paths at specific times, as determined by the user. For example, the user can program the TX810 to switch the transmit and receive paths of a particular transducer at a specific time during the ultrasound examination. This allows the user to perform multi-channel imaging, where multiple transducers are used simultaneously to capture images from different angles. The IC is typically used in conjunction with an ultrasound system and one or more transducers. Transducers are used to transmit and receive ultrasound waves, which are used to generate images of the body's internal structures. The TX810 is used to switch the transmit and receive paths for each transducer at the appropriate times, allowing the ultrasound system to capture images from multiple angles simultaneously. When high-voltage transmitter signals are applied to the input, the internal diodes limit the output voltage. While in receive mode, the TX810's insertion loss is minimized. The TX810 features a 3-bit interface that may be used to program bias current from 7 mA to 0 mA for varying performance and power requirements, unlike conventional T/R switches. The device is put up in power-down mode when the TX810 bias current is set to 0 mA (high-impedance mode). The TX810 does not put significant load on high-voltage transmitters when operating in the high-impedance

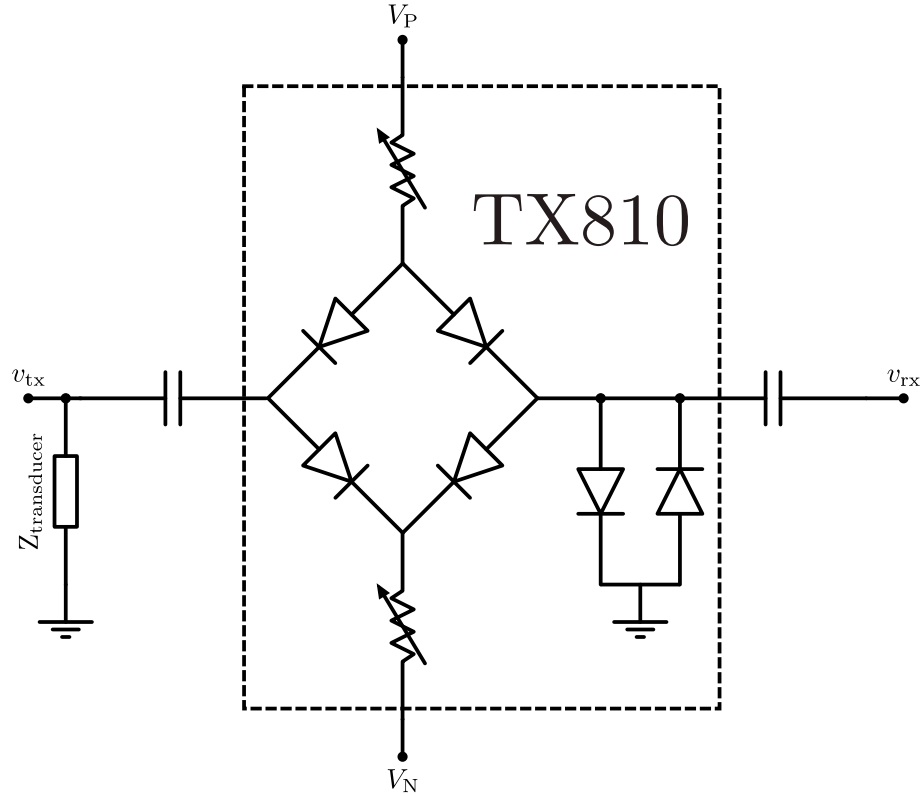


Figure 2.12: Circuit diagram of switch (per channel)

mode. The device can also wake up from power-down mode in less than a μs . A PCB design was implemented in Altium Designer[20] utilising three channels of the maximum eight available channels in the IC. Seen in fig. 2.13 is a 3D render of the designed PCB. The module is designed with three usable channels, either three separate transducers for multi-angle sonography, or a capacitive micromachined ultrasound transducer (*CMUT*) with three channels in a single angle.

2.5 Preamplifier

OPA487

The OPA847[7] is a high-performance, high-speed, voltage feedback amplifier with a bandwidth of over 1 GHz. It has a wide gain range, low distortion, and low noise, making it suitable for a variety of applications including video, RF, and high-speed data acquisition. The OPA847 has a single-ended input and a differential output, which allows it to be used in a variety of circuit configurations. It is available in a surface-mount package and operates over a wide supply voltage range.

AD8332

The AD8332[13] is a fully integrated, single-chip amplifier designed for use in a wide range of RF and microwave applications. It is a low-noise, high-linearity amplifier that can be used in a variety of configurations, including as a stand-alone amplifier or as part of a larger system. The AD8332 is a current-feedback amplifier that can operate over a wide frequency range, from 50 MHz to 4 GHz. It has a high level of integration, with all active components on a single monolithic IC. This makes it suitable for use in small form factor applications where space is at a premium. The AD8332 has a number of features that make it well-suited for use in RF and microwave applications. It has a high level of linearity,

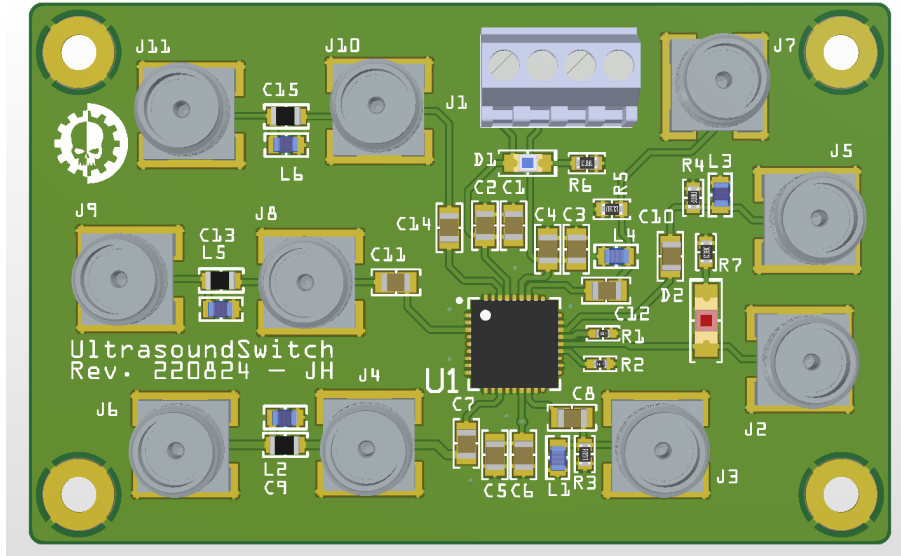


Figure 2.13: 3D Render of PCB in Altium Designer

which allows it to amplify signals without introducing significant distortion. It also has a low noise figure, which makes it well-suited for use in low-noise applications. Additionally, the AD8332 has a wide dynamic range, which makes it capable of handling a wide range of input signals without clipping or saturating. Overall, the AD8332 is a versatile and reliable amplifier that can be used in a wide range of RF and microwave applications. It is well-suited for use in a variety of systems, including communication systems, radar systems, and instrumentation systems.

2.6 Demodulation

To demodulate our signal using the process described in The AD8333[14] can be used to demodulate amplitude modulation (AM) signals. It contains all the necessary circuitry to detect and extract the information contained in an AM signal. In AM, the information is encoded in the amplitude of the carrier wave, which is modulated or varied in some way to convey the information. The AD8333 is able to detect these variations in the carrier wave and extract the original information from the signal. To do this, the AD8333 uses a process called envelope detection. It rectifies the input signal, which removes the negative portions of the waveform, and then filters the resulting signal to remove any remaining high-frequency components. This leaves only the envelope of the original modulated signal, which contains the encoded information. The AD8333 also includes amplifier and buffer stages to amplify the detected envelope and prepare it for further processing or application. It is often used in radio communication systems, industrial control systems, and other applications where an AM signal needs to be demodulated and the information contained in the signal needs to be extracted. Test af git push.

2.7 Sample/Hold

The sample/hold circuit is based on the AD783[10] sample-and-hold amplifier (SHA). It functions by converting an analog input signal into a sequence of quantized samples and holds these samples for a specified time. The SHA is made up of several internal stages, including an input amplifier, sample switch, sample-and-hold capacitor, and output

amplifier. When the sample input of the AD783 is triggered, the input amplifier amplifies the input signal and the sample switch closes, allowing the signal to be stored on the sample-and-hold capacitor. Once the sample is taken, the sample switch opens, and the output amplifier outputs the stored value of the input signal. The hold input of the AD783 maintains the sample on the capacitor until the next sample is taken.

2.8 Pulse-Repetition and Wall Filter

2.9 Amplifier

2.10 Mixer

2.11 Adder

Bibliography

- [1] S. Satomura, T. Yoshida, M. Mori, Y. Nimura, G.-i. Hikita, S. Takagishi, and K. Nakanishi, "Analysis of heart motion with ultrasonic Doppler method and its clinical application," *American Heart Journal*, vol. 61, pp. 61–75, 1 January 1961, ISSN: 00028703. DOI: 10.1016/0002-8703(61)90517-8. [Online]. Available: <https://linkinghub.elsevier.com/retrieve/pii/0002870361905178>.
- [2] D. Baker, "Pulsed Ultrasonic Doppler Blood-Flow Sensing," *IEEE Transactions on Sonics and Ultrasonics*, vol. 17, pp. 170–184, 3 Jul. 1970, ISSN: 0018-9537. DOI: 10.1109/t-su.1970.29558. [Online]. Available: <http://ieeexplore.ieee.org/document/1538563/>.
- [3] K. K. Shung and G. A. Thieme, *Ultrasonic scattering in biological tissues*. CRC Press, 1993, p. 499, ISBN: 9780849365683. [Online]. Available: <https://www.routledge.com/Ultrasonic-Scattering-in-Biological-Tissues/Shung-Thieme/p/book/9780849365683>.
- [4] P. Munk, "Estimation of blood velocity vectors using ultrasound," Technical University of Denmark, 2000. [Online]. Available: <https://findit.dtu.dk/en/catalog/537f0d537401dbcc1200be04>.
- [5] A. Erguri, Y. Huang, X. Zhuang, O. Oralkan, G. Yarahoglu, and B. Khuri-Yakub, "Capacitive micromachined ultrasonic transducers: Fabrication technology," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 52, no. 12, pp. 2242–2258, 2005. DOI: 10.1109/TUFFC.2005.1563267.
- [6] *EL7104 High Speed, Single Channel, Power MOSFET Driver*, Renesas Electronics, Jun. 2006. [Online]. Available: <https://www.renesas.com/us/en/document/dst/el7104-datasheet>.
- [7] *OPA847 Wideband VF Operational Amplifier*, Texas Instruments, Inc., 2008. [Online]. Available: <https://www.ti.com/lit/ds/symlink/opa847.pdf>.
- [8] *TX810 8-Channel, Programmable T/R Switch for Ultrasound*, Texas Instruments, April 2010. [Online]. Available: <https://www.ti.com/lit/gpn/tx810>.
- [9] J. A. Jensen, *Estimation of Blood Velocities Using Ultrasound: A Signal Processing Approach*, Third Edition. Department of Electrical Engineering, Technical University of Denmark, August 2013, ISBN: 9780521464840.
- [10] *AD783 Complete Very High Speed Sample-and-Hold Amplifier*, Analog Devices, October 2014. [Online]. Available: <https://www.analog.com/media/en/technical-documentation/data-sheets/AD783.pdf>.
- [11] T. L. Szabo, *Diagnostic Ultrasound Imaging: Inside Out*, Second Edition. Elsevier, 2014, ISBN: 9780123964878. DOI: 10.1016/c2011-0-07261-7. [Online]. Available: <https://linkinghub.elsevier.com/retrieve/pii/C20110072617>.
- [12] K. K. Shung, *Diagnostic Ultrasound: Imaging and Blood Flow Measurements*, Second Edition. CRC Press, December 2015, ISBN: 978-1-4665-8264-4.
- [13] *AD8332 Ultralow Noise VGAs with Preamplifier and Programmable R_{IN}* , Analog Devices, May 2016. [Online]. Available: https://www.analog.com/media/en/technical-documentation/data-sheets/AD8331_8332_8334.pdf.
- [14] *AD8333 DC to 50 MHz, Dual I/Q Demodulator and Phase Shifter*, Analog Devices, May 2016. [Online]. Available: <https://www.analog.com/media/en/technical-documentation/data-sheets/AD8333.pdf>.

- [15] *MD1213 High-Speed Dual-MOSFET Driver*, Microchip Technology, Inc., Jun. 2017. [Online]. Available: <https://ww1.microchip.com/downloads/en/DeviceDoc/20005713B.pdf>.
- [16] *MD0101 High Voltage Protection T/R Switch with Clamp Diodes*, Microchip Technology, Inc., May 2020. [Online]. Available: <https://ww1.microchip.com/downloads/aemDocuments/documents/APID/ProductDocuments/DataSheets/MD0101-High-Voltage-Protection-TR-Switch-with-Clamp-Diodes-Data-Sheet-20005916A.pdf>.
- [17] *ISL55111 Dual, High Speed MOSFET Driver*, Renesas Electronics, April 2021. [Online]. Available: <https://www.renesas.com/us/en/document/dst/isl55110-isl55111-datasheet>.
- [18] “Ninja, a small build system with a focus on speed.” (August 2022), [Online]. Available: <https://ninja-build.org/> (visited on February 15, 2023).
- [19] “Zephyr Project Documentation.” (Sep. 2022), [Online]. Available: <https://docs.zephyrproject.org/latest/> (visited on February 15, 2023).
- [20] “Altium Designer - PCB design software.” (February 2023), [Online]. Available: <https://www.altium.com/altium-designer>.
- [21] “CMake Tools - Visual Studio Marketplace.” (February 2023), [Online]. Available: <https://marketplace.visualstudio.com/items?itemName=ms-vscode.cmake-tools> (visited on February 15, 2023).
- [22] “Firmware Repository.” (March 2023), [Online]. Available: https://github.com/s163555/doppler_pwm (visited on April 12, 2023).