InBody



InBody260s

Modern

Ergonomic design for
Efficient work flow

Reliable

Proven and reliable
performance

Standard


The archetype of
Body composition test

InBody Technology

InBody uses Bioelectrical Impedance Analysis (BIA) technology to measure human body composition. Impedance is the resistance of the human body generated when a micro alternating current flows through the human body. The human body is made of water that conducts electricity well, and the resistance varies depending on the amount of water. BIA is a technology that quantitatively measures body water through impedance that occurs when an electric current flows through the human body. InBody provides diverse information on body composition based on the measured body water.

Direct Segmental Measurement-BIA

The human body exhibits varying lengths and cross-sectional areas for each body segments. Arms and legs, characterized by narrow cross-sectional areas and length, exhibit higher impedance values and lower muscle mass. Conversely, the trunk, with its broader cross-sectional area, yields lower impedance values and higher muscle mass. Even the slightest change in trunk impedance can significantly influence the total muscle mass. Therefore, it is essential to separately measure trunk impedance for precise total muscle mass assessment. InBody conducts separate measurements for arms, legs, and the trunk, ensuring the utmost accuracy in the analysis.

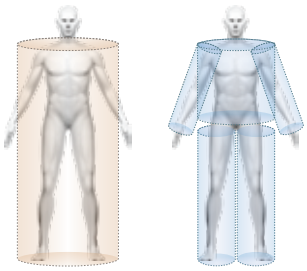


8-Point Tactile Electrodes utilizing Thumb Electrodes

Using the structural features of the human body, InBody pioneered '8-Point Tactile electrode with Thumb Electrodes'. This ensures InBody measurements start at the same location on the wrists and ankles, guaranteeing reliable and reproducible results.




Simultaneous Multi-Frequency Impedance Measurement

InBody introduced a technology in body composition analyzers to transmit multiple frequencies at once, obtaining specific impedance data for each for the first time. This reduces measurement time and error, leading to more accurate body water and fluid balance measurements.




No Estimations or Empirical Equations on Measured Values

InBody does not rely on empirical estimations based on age, gender, and more to ensure the accuracy of the measured data. In the past, empirical estimations were applied to the equations to ensure accuracy due to technological limitations. However, this resulted in lower accuracy when the measured population group changes. InBody overcame these limitations with technological developments such as direct segmental measurement-BIA to measure and analyze accurate body composition without applying empirical estimation. Therefore, InBody devices can provide data regardless of population and can reflect changes in the body with higher sensitivity.



Over 98% Correlation to DEXA on Accuracy

InBody precisely detects changes in body composition using impedance alone, showing a correlation over 0.98 with the gold-standard DEXA device.

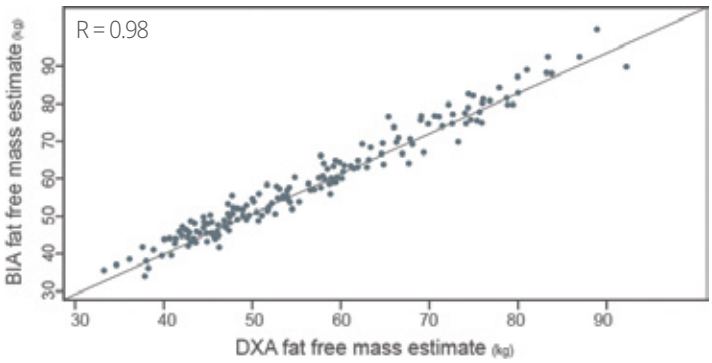

Ryan T Hurt et al., The Comparison of SMF-BIA and DEXA for Estimating Fat Free Mass and Percentage Body Fat in an Ambulatory Population,
J Parenter Enteral Nutr. 2021 Aug;45(6):1231-1238

Portable and Sturdy

Build to last long with accuracy and mobility

Elegant and Timeless style, with notably unique design for efficient space organisation









InBody Result Sheet

Provides reference parameters to thoroughly evaluate patients' conditions across various medical practices.

InBody [InBody260S]

ID	Height	Age	Gender	Test Date & Time
Jane Doe	156.9cm	51	Female	05.30.2024 11:16

7 **Customized Logo**

www.customized.com

1 Body Composition Analysis

Total amount of water in body	Total Body Water	(L)	28.1 (27.0 ~ 33.0)
For building muscles	Protein	(kg)	7.4 (7.2 ~ 8.8)
For strengthening bones	Minerals	(kg)	2.76 (2.49 ~ 3.05)
For storing excess energy	Body Fat Mass	(kg)	20.8 (10.6 ~ 16.9)
Sum of the above	Weight	(kg)	59.1 (45.0 ~ 60.8)

2 Muscle-Fat Analysis


	Under	Normal	Over
Weight (kg)	55 70 85 100 115 130 145 160 175 190 205 %	59.1	
SMM (kg) Skeletal Muscle Mass	70 80 90 100 110 120 130 140 150 160 170 %	20.4	
Body Fat Mass (kg)	40 60 80 100 160 220 280 340 400 460 520 %	20.8	

3 Obesity Analysis

	Under	Normal	Over
BMI (kg/m2) Body Mass Index	10.0 15.0 18.5 21.5 25.0 30.0 35.0 40.0 45.0 50.0 55.0	24.0	
PBF (%) Percent Body Fat	8.0 13.0 18.0 23.0 28.0 33.0 38.0 43.0 48.0 53.0 58.0	35.2	


4 Segmental Lean Analysis

Lean Mass % Evaluation

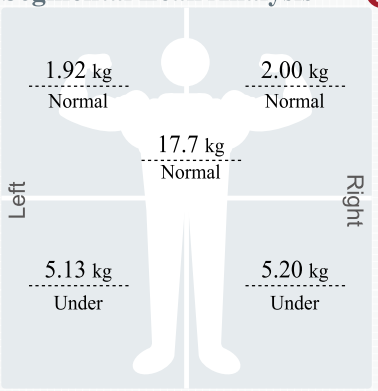

5 Segmental Fat Analysis

Fat Mass % Evaluation

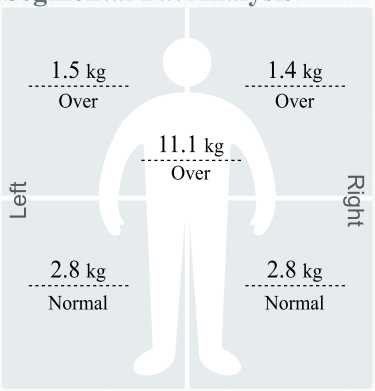

* Segmental fat is estimated.

6 Body Composition History

	01.01.24 09:15	01.30.24 09:40	02.20.24 09:35	03.15.24 11:10	04.12.24 08:33	04.28.24 15:10	05.15.24 08:40	05.30.24 11:16
Weight	65.3	63.9	62.4	61.8	62.3	60.9	60.5	59.1
SMM Skeletal Muscle Mass	20.1	20.0	19.7	19.7	19.8	19.7	19.8	20.4
PBF Percent Body Fat	41.3	40.7	39.2	39.0	39.4	38.6	37.8	35.2

☑ Recent ☐ Total

8 InBody Score

69 / 100 Points

* Total score that reflects the evaluation of body composition. A muscular person may score over 100 points.

9 Weight Control

Target Weight	53.0 kg
Weight Control	- 6.1 kg
Fat Control	- 8.6 kg
Muscle Control	+ 2.5 kg

10 Obesity Evaluation

BMI	☑ Normal	☐ Under	☐ Slightly Over ☐ Over
PBF	☐ Normal	☐ Slightly Over	☑ Over

11 Waist-Hip Ratio

0.96 (0.75 0.85)

12 Visceral Fat Level

11 (Low 10 High)

13 Reasearch Parameters


Fat Free Mass	38.3 kg	(36.7 ~ 44.8)
Basal Metabolic Rate	1197 kcal	(1255 ~ 1451)
Obesity Degree	112 %	(90 ~ 110)
SMI	5.8 kg/m²	
Recommended calorie intake per day	1397 kcal	

Calorie Expenditure of Exercise

Golf	104	Gateball	112
Walking	118	Yoga	118
Badminton	134	Table Tennis	134
Tennis	177	Bicycling	177
Boxing	177	Racketball	177
Mountain Climbing	193	Jumping Rope	207
Aerobics	207	Jogging	207
Soccer	207	Swimming	207
Japanese Fencing	295	Racketball	295
Squash	295	Taekwondo	295

*Based on your current weight
*Based on 30 minute duration

14 Impedance

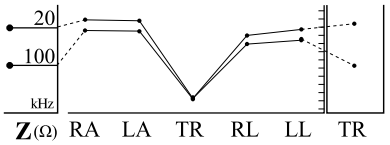

Copyright ©1996~by InBody Co.,Ltd. All rights reserved.

Result Sheet Interpretation

1 Body Composition Analysis
Body weight is the sum of Total Body Water, Protein, Minerals, and Body Fat Mass. Maintain a balanced body composition to stay healthy.

2 Muscle-Fat Analysis
Compare the bar lengths of Skeletal Muscle Mass and Body Fat Mass. The longer the Skeletal Muscle Mass bar is compared to the Body Fat Mass bar, the better health status you are in.

3 Obesity Analysis
BMI is an index used to determine obesity by using height and weight. PBF is the percentage of body fat compared to body weight.

4 Segmental Lean Analysis
Analyze to evaluate if the muscles are adequately developed in the body segments. A balanced distribution between the arms, legs, upper, and lower body is considered ideal.

5 Segmental Fat Analysis
Evaluate whether the amount of fat is adequately distributed in segments of the body.

6 Body Composition History
Measure your body composition periodically to monitor your progress.

7 Logo Customization
The Customized Logo can be applied on the Result Sheet. URL can also be applied at the bottom of the Result Sheet as well.

8 InBody Score
InBody Score is your score after evaluating your body composition.

9 Weight Control
Use the Target Weight, Weight Control, Fat Control, Muscle Control to set your own goal.

10 Obesity Evaluation
Evaluate obesity based on BMI and Percent Body Fat.

11 Waist-Hip Ratio (WHR)
Waist-Hip Ratio is the ratio of waist circumference to hip circumference.

12 Visceral Fat Level
Visceral Fat Level is an indicator based on the estimated amount of fat surrounding internal organs in the abdomen.

13 Research Parameters
Various research parameters such as Basal Metabolic Rate, Waist-Hip Ratio, Obesity Degree, Skeletal Muscle Mass Index (SMI), Body Cell Mass, and more are provided.

14 Impedance
Impedance is the resistance value measured when electrical currents are applied to the body. Based on the measured data, key body composition outputs can be analyzed. Impedance is also used for many research purposes.

***Additional InBody Results Sheet**
InBody Result Sheet for Children, Thermal Result Sheet

Optional Results Sheet

1 InBody Result Sheet for Children

With the InBody Result Sheet for Children, you can assess and track a child's growth progress.

1

InBody

[InBody260S]

InBody
inbody.com

ID	Height	Age	Gender	Test Date / Time
Jane Doe C	139.4cm	10	Male	06.21.2024 16 : 40

Body Composition Analysis

Total amount of water in my body	Total Body Water	(L)	19.2 (18.0 ~ 22.0)
What I need to build muscles	Protein	(kg)	5.1 (4.9 ~ 5.9)
What I need for strong bones	Minerals	(kg)	1.91 (1.66 ~ 2.04)
Where my excess energy is stored	Body Fat Mass	(kg)	8.8 (3.8 ~ 7.7)
Sum of the above	Weight	(kg)	35.0 (27.3 ~ 36.9)

Muscle-Fat Analysis

	Under	Normal	Over
Weight (kg)	55 70 85 100 115 130 145 160 175 190 205 %	35.0	
SMM Skeletal Muscle Mass (kg)	70 80 90 100 110 120 130 140 150 160 170 %	13.4	
Body Fat Mass (kg)	40 60 80 100 160 220 280 340 400 460 520 %	8.8	


Obesity Analysis

	Under	Normal	Over
BMI Body Mass Index (kg/m²)	7.9 10.9 13.9 16.4 18.6 20.2 22.2 24.2 26.2 28.2 30.2	18.0	
PBF Percent Body Fat (%)	0.0 5.0 10.0 15.0 20.0 25.0 30.0 35.0 40.0 45.0 50.0	25.2	

Growth Graph


Height : 50 ~ 75%

Height(cm)

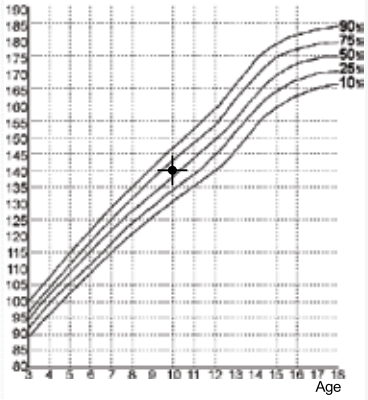

Weight : 50 ~ 75%

Weight(kg)

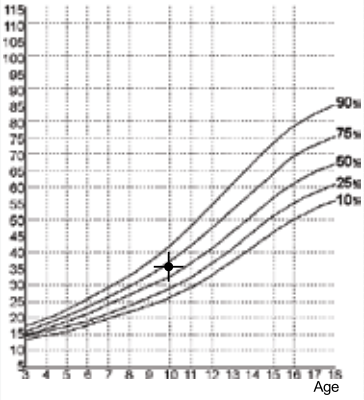

Body Composition History

Height (cm)	136.5	137.2	138.6	139.4
Weight (kg)	35.1	35.6	37.3	35.0
SMM Skeletal Muscle Mass (kg)	13.3	13.0	12.9	13.4
PBF Percent Body Fat (%)	26.2	26.5	26.0	25.2
☐ Recent ☑ Total	09.10.23 09:15	11.30.23 09:40	01.02.24 09:35	06.21.24 16:40

Growth Score

86 / 100 Points

* If tall and within great body comparison standards, the growth score may surpass 100 points.

Obesity Evaluation

BMI	☑ Normal	☐ Under	☐ Slightly Over ☐ Over
PBF	☐ Normal	☐ Slightly Over	☑ Over

Research Parameters

Basal Metabolic Rate	936 kcal	(948 ~ 1077)
Child Obesity Degree	109 %	(90 ~ 110)

Results Interpretation


Growth Graph

Compares the height and weight among peers of the same age group.

Results Interpretation QR Code

Scan the QR Code to see results interpretation in more detail.

Impedance

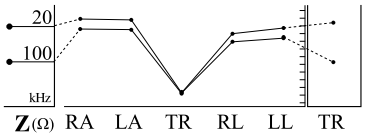


[000/000/000]

Copyright ©1996~by InBody Co.,Ltd. All rights reserved.

InBody Application

InBody Test results can be used as an indicator for proper prescription by monitoring your health status in
many areas such as obesity, nutrition, rehabilitation etc.


Providing a smart healthcare service with high technology and helping everyone live a healthier life,
thats the great mission of InBody.

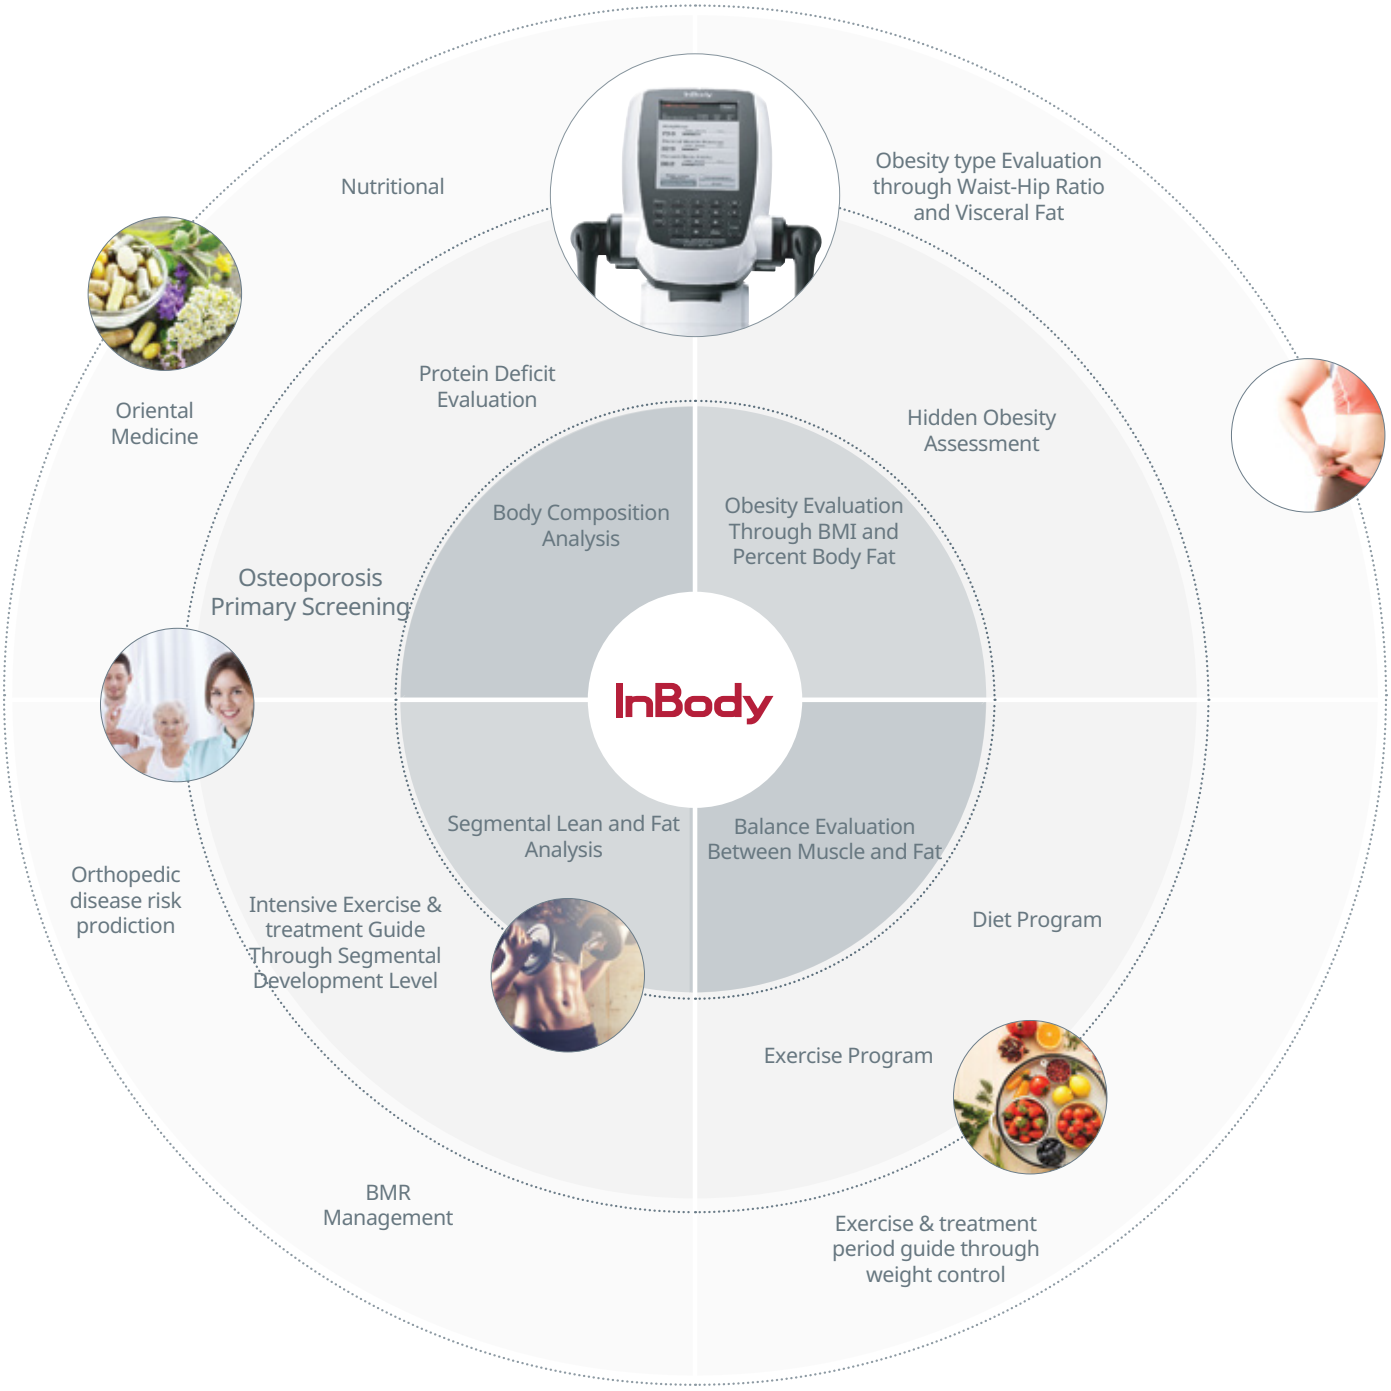

Specifications

InBody260S Body Composition Analyzer

Bioelectrical Impedance Analysis (BIA) Measurement Items	Impedance (Z)	10 Impedance measurements by using 2 different frequencies (20 kHz, 100 kHz) at each 5 segments of the body (Right Arm, Left Arm, Trunk, Right Leg, Left Leg)
Electrode Method	4 electric poles 8 Points Touch type electrode measurement	
Measurement Method	Direct Segmental Multi-frequency Bioelectrical Impedance Analysis Method, DSM-BIA Method	
Body Composition Calculation	No use of Empirical Estimation	
Logo Display	Name, Address, and Contact Information can be shown on the InBody Results Sheet.	
Digital Results	LCD Monitor	
Type of Results Sheets	InBody Results Sheet, InBody Results Sheet for Children, InBody Thermal Results Sheet	
Data Storage	Test results can be saved if the member ID is utilized. The InBody can save up to 100,000 results.	
Test Mode	Self Mode, Professional Mode	
Administrator Menu	· Setup: Configure settings and manage data · Troubleshooting: Additional information to help use the InBody	
USB Thumb Drive	Copy, Backup or restore the InBody test data (data can be viewed on Excel or LookinBody data management software)	
Barcode Reader	The member ID will be automatically inputted when the barcode ID is scanned.	
Backup data	Backup data saved in the InBody by using a USB Thumb Drive, Restore results on the InBody from a backup file.	
Applied Rating Current	300 μA (± 30 μA)	
Adapter ② (DELTA)	Power Input	AC 100 - 240 V, 50 - 60 Hz, 1.5 A - 0.75 A
	Power Output	DC 12 V, 5.0 A
Adapter ① (MEAN WELL)	Power Input	AC 100 - 240 V, 50 / 60 Hz, 1.0 A - 0.5 A
	Power Output	DC 12 V, 3.34 A
Display Type	480 × 800 7 inch Color TFT LCD	
Internal Interface	Touchscreen, Keypad	
External Interface	RS-232C 1EA, USB HOST 2EA, USB SLAVE 1EA, LAN (10/100T) 1EA, Bluetooth 1EA, Wi-Fi(2.4G/5G) 1EA	
Compatible Printer	Laser/Inkjet PCL 3 or above and SPL	
Dimension	356 (W) X 796 (L) X 995 (H) : mm 14.0 (W) X 31.3 (L) X 39.2 (H) : inch	
Device Weight	13.4 kg (29.5 lb)	
Testing Duration	About 30 Seconds *Test duration may vary depending on the measurement posture or external environment.	
Operation Environment	10 - 40 °C (50 - 104 °F), 30 - 75 % RH, 70 - 106 kPa	
Storage Environment	−10 - 70 °C (14 - 158 °F), 10 - 80 % RH, 50 - 106 kPa (No Condensation)	
Testing Weight Range	2 - 250 kg (4.4 - 551.2 lbs)	

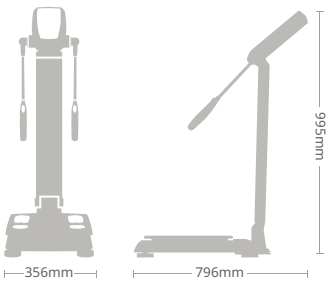

Age Range	3+ years
Height Range	95 - 220 cm (3 ft 1.4 in - 7 ft 2.6 in)
Language Support	InBody supports over 30 languages.
Outputs (InBody Result Sheet)	Results and Interpretations · Body Composition Analysis (Total Body Water, Protein, Minerals, Body Fat Mass, Weight) · Muscle-Fat Analysis (Weight, Skeletal Muscle Mass, Body Fat Mass) · Obesity Analysis (Body Mass Index, Percent Body Fat) · Segmental Lean Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg) · Segmental Fat Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg) · Body Composition History (Weight, Skeletal Muscle Mass, Percent Body Fat) · InBody Score · Weight Control (Target Weight, Weight Control, Fat Control, Muscle Control) · Obesity Evaluation (BMI, Percent Body Fat) · Waist-Hip Ratio (Graph) · Visceral Fat Level (Graph) · Research Parameters (Fat Free Mass, Basal Metabolic Rate, Obesity Degree, SMI) · Recommended calorie intake per day · Calorie Expenditure of Exercise · Impedance (Each segment and each frequency)
Outputs (InBody Result Sheet for Children)	Results and Interpretations · Body Composition Analysis (Total Body Water, Protein, Minerals, Body Fat Mass, Weight) · Muscle-Fat Analysis (Weight, Skeletal Muscle Mass, Body Fat Mass) · Obesity Analysis (Body Mass Index, Percent Body Fat) · Growth Graph (Height, Weight, SMI) · Body Composition History (Height, Weight, Skeletal Muscle Mass, Percent Body Fat) · Growth Score · Obesity Evaluation (BMI, Percent Body Fat) · Research Parameters (Basal Metabolic Rate, Child Obesity Degree) · QR Code · Results Interpretation QR Code · Impedance (Each segment and each frequency)
Outputs (InBody Thermal Result Sheet)	Weight, Muscle Mass, Body Fat Mass, Percent Body Fat, BMI, Basal Metabolic Rate, Waist-Hip Ratio, Visceral Fat Level, Segmental Lean Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg), Segmental Fat Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg), InBody Score, Fat Control, Muscle Control, Impedance (Each segment and each frequency)

* Specifications may change without prior notice.
* "QR Code" is registered trademark of DENSO WAVE INCORPORATED.

InBody

InBody HQ [KOREA]
InBody Bldg., 625, Eonju-ro, Gangnam-gu, Seoul 06106 Republic of Korea
TEL: +82-2-501-3939 FAX: +82-2-6919-2417
Website: inbody.com E-mail: info@inbody.com

InBody USA [USA]
13850 Cerritos Corporate Dr. Unit C Cerritos, CA 90703 USA
TEL: +1-323-932-6503 FAX: +1-323-952-5009
Website: inbodyusa.com E-mail: info.us@inbody.com

InBody China [CHINA]
Room 306b、307a、307b、308, MT2 Office Building, No. 3999 Hongxin Road, Minhang District, Shanghai
TEL: +86-21-6443-9705 FAX: +86-21-6443-9706
Website: inbodychina.com E-mail: info@inbodychina.com

InBody Japan [JAPAN]
Tani Bldg., 1-28-6, Kameido, Koto-ku, Tokyo 136-0071 Japan
TEL: +81-3-5875-5780 FAX: +81-3-5875-5781
Website: inbody.co.jp E-mail: inbody@inbody.co.jp

InBody Europe B.V. [NETHERLANDS]
Gyroscoopweg 122, 1042 AZ, Amsterdam, The Netherlands
TEL: +31-20-238-6080 FAX: +31-6-5734-1858
Website: nl.inbody.com E-mail: info.eu@inbody.com

InBody BWA Inc. [USA]
2550 Eisenhower Avenue, Suite C 209, Audubon, PA 19403
TEL: +1-610-348-7745
Website: inbodybwa.com E-mail: bwainquiries@inbody.com

InBody Europe B.V. Niederlassung Deutschland [GERMANY]
Mergenthalerallee 15-21, 65760 Eschborn, Germany
TEL: +49-6196-76-916-62 FAX: +49-6196-76-916-11
Webseite: de.inbody.com E-mail: erfolg@inbody.com

InBody UK [UNITED KINGDOM]
Orega, Belmont Road, Uxbridge, UB8 1HE, United Kingdom
TEL: +44-1530-569620
Website: uk.inbody.com E-mail: uk@inbody.com

Biospace Latin America [MÉXICO]
Insurgentes Sur 1457, Piso 15 Int.2. Col. Insurgentes Mixcoac, Alcaldia Benito Juarez, C.P. 03920, Ciudad de México, México
TEL: +52-55-5025-0147
Website: inbodymexico.com E-mail: info.mx@inbody.com

InBody Oceania [AUSTRALIA]
U2/82-86 Minnie Street, Southport, Queensland
TEL: +61-7-5681-1900
Website: au.inbody.com Email: oceania@inbody.com

InBody Asia [MALAYSIA & SINGAPORE]
Unit 3A-11, Oval Damansara, 685 Jalan Damansara Kuala Lumpur, WP KL 60000 Malaysia
TEL: +60-3-7732-0790 FAX: +60-3-7733-0790
Website: inbodyasia.com E-mail: info@inbodyasia.com

InBody India [INDIA]
57/57 A,1st Floor, Raj Industrial Complex, Military Road, Marol, Andheri (East). Mumbai- 400059, Maharashtra, India
TEL: +91-22-6223-1911
Website: inbody.inE-mail: india@inbody.com

InBody Vietnam [VIETNAM]
11th Floor, COBI TOWER II, 2-4 Street 8, Tan Phu Ward, District 7, HSMC, 70000 Vietnam
TEL: +84-096-983-6595
Website: inbodyvietnam.com E-mail: info.vn@inbody.com

Certificates

CE1639 NAWI ISO13485 ISO9001 MDSAP GMP

Awards

iF Design Award

For more details about the patents that we acquired, please visit our website or refer to the patent gazette of intellectual property office of each country. (Korea, U.S, China, Japan)

ⓒ2025 InBody Co., Ltd. All rights reserved. IC-ENG-V6-A-250626