


Analyst
Date

Administrator
Tuesday, April 30, 2024 5:17 PM

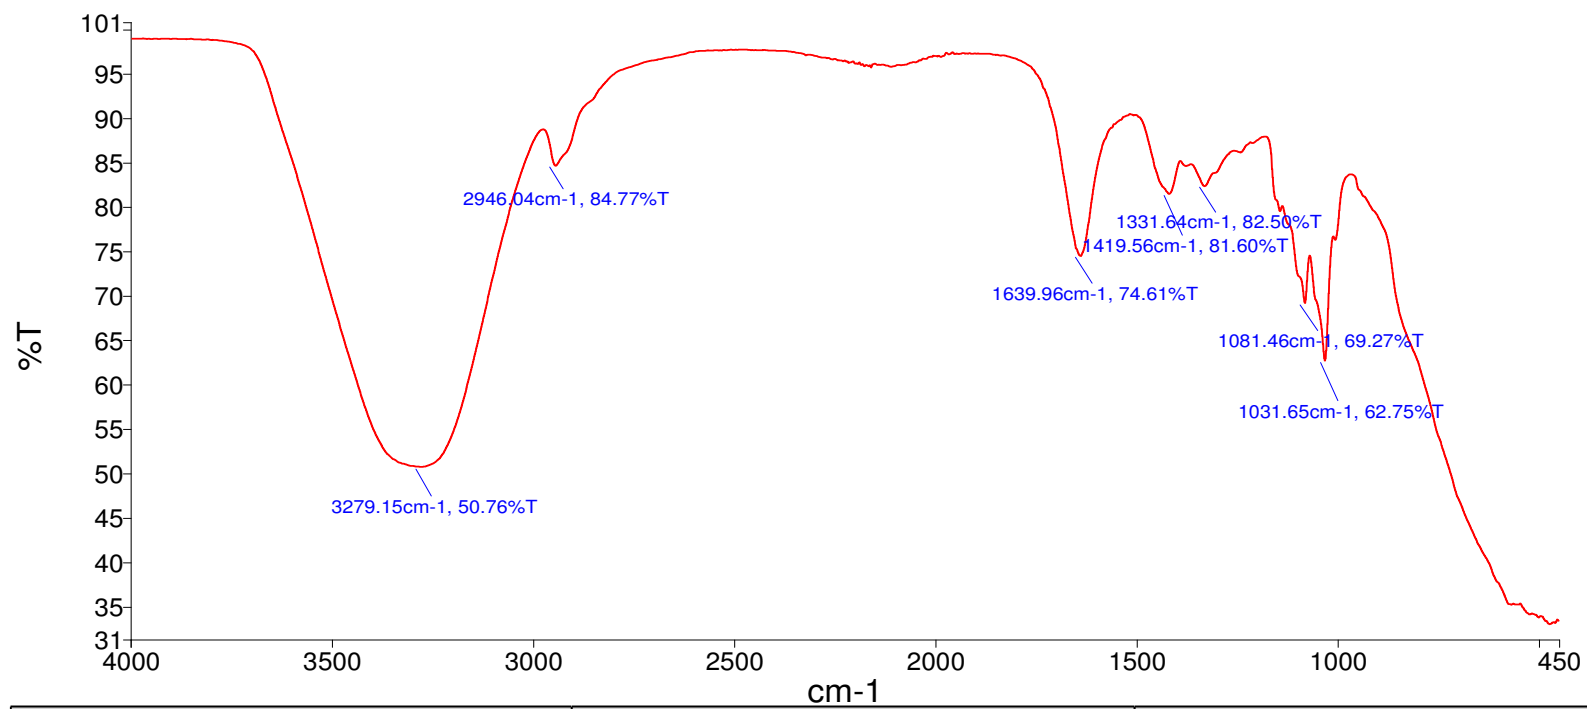

Sample Name	Description	Quality Checks
21PVA-CA-BCD_O1wet	Sample 006 By Administrator Date Tuesday, April 30 2024	The Quality Checks do not report any warnings for the sample.