


Analyst
Date

Administrator
Tuesday, April 30, 2024 5:18 PM

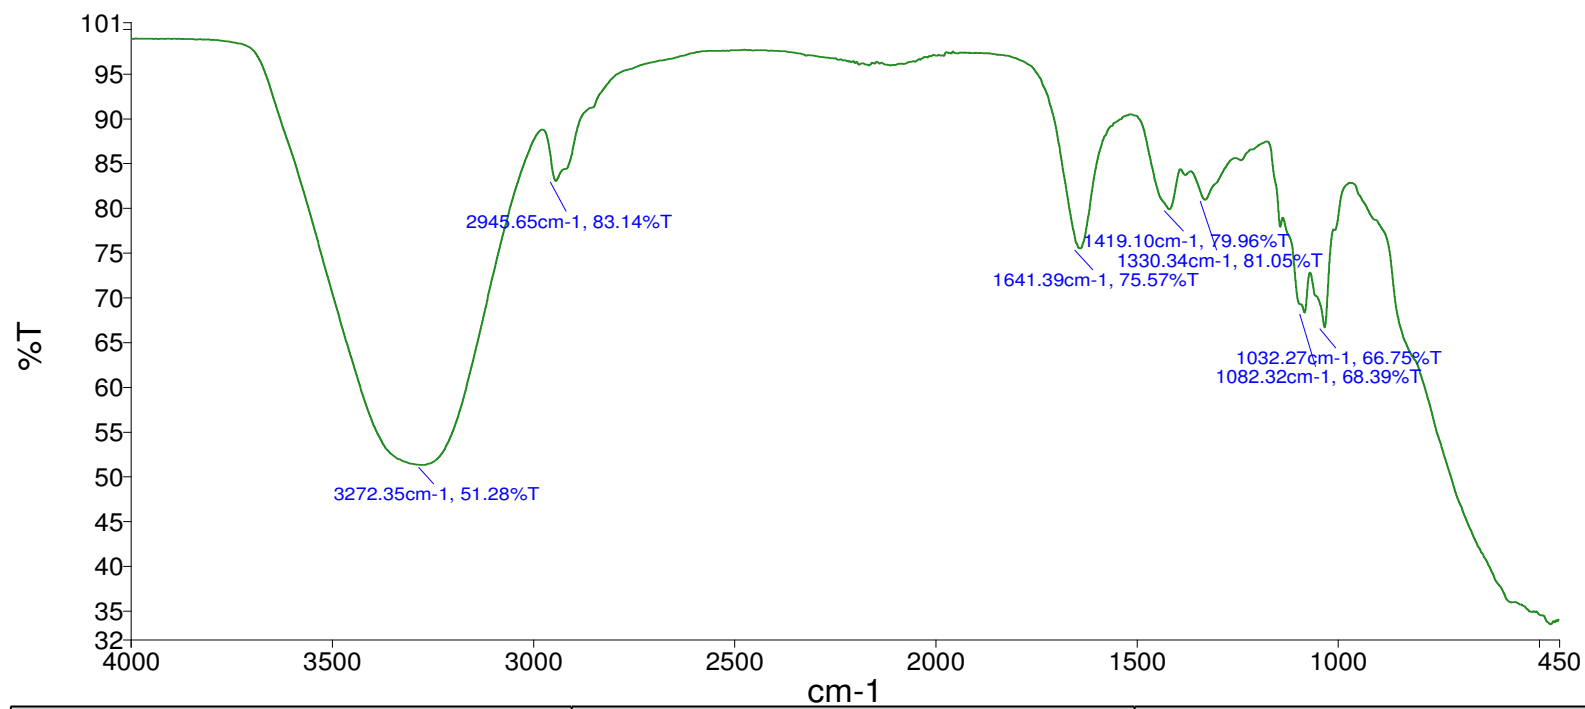

Sample Name	Description	Quality Checks
41PVA-CA-BCD_02wet	Sample 008 By Administrator Date Tuesday, April 30 2024	The Quality Checks do not report any warnings for the sample.