

M.J. Biopharm Private Limited

Plot No. 18, International Biotech Park, Hinjawadi, Phase II, Pune 411057.



Format for Attachment

Title: Weight Print Sheet.

Test Name: system suitability

A.R No.: NR125/0438

For Hypothesis (system suitability)

Text 1 Material Name

114 Benzoquinone

Text 2 Batch No. :

RS1002/23-003

Text 3 A.R. No. :

NR125/0438

21/03/2026 18:51:43

Text 4

M.J. Biopharm Pvt.
Ltd.

Manuf. Sartorius

Model MCA6.6S-20IN-M

Ser.no 0043901273

ID 1 I/QC/013

N	*	7.508 mg
N		0.000 mg
n		2
s		5.3090 mg
Sum		7.508 mg
Min		0.000 mg
Max		7.508 mg
Diff		7.508 mg

21/03/2026 18:55:14

Login 952

Displa

Dhananjay Ibhad

Signat.

21/03/26

21/03/26

M.J. Biopharm Private Limited

Plot No. 18, International Biotech Park, Hinjawadi, Phase II, Pune 411057.



Format for Attachment

Test Name: 2 point calibration of system suitability A.R No.: HR/25/0438

Text 1 Material Name

Sucrose

Text 2 Batch No. :

PS/009/001

Text 3 A.R. No. :

HR/25/0438

21/03/2026 20:14:38

Text 4

M.J. Biopharm Pvt.

Ltd.

Manuf. Sartorius

Model MCA6.6S-20IN-M

Ser. no 0043901273

ID 1 I/QC/013

N + 11.893 mg

N + 0.001 mg

n 2

s 8.4089 mg

Sum 11.894 mg

Min 0.001 mg

Max 11.893 mg

Diff 11.892 mg

21/03/2026 20:16:35

Login 952

Displa

Dhananjay Ibhad

Signat.

21/03/26

Text 1 Material Name

1,4 Benzocaine

Text 2 Batch No. :

NA

Text 3 A.R. No. :

HR/25/0438

21/03/2026 21:08:12

Text 4

M.J. Biopharm Pvt.

Ltd.

Manuf. Sartorius

Model MCA6.6S-20IN-M

Ser. no 0043901273

ID 1 I/QC/013

N + 7.526 mg

N + 0.016 mg

n 2

s 5.3104 mg

Sum 7.542 mg

Min 0.016 mg

Max 7.526 mg

Diff 7.510 mg

21/03/2026 21:10:03

Login 952

Displa

Dhananjay Ibhad

Signat.

21/03/26

21/03/26

Prepared By (User)
(Sign & Date)

21/03/26

Reviewed By (User)
(Sign & Date)

21/03/26

Reference SOP No.: SOP/DP/QC/007

Unit- Drug Product

M.J. Biopharm Private Limited Plot No. 18, International Biotech Park, Hinjawadi, Phase II, Pune 411057.	
Blank Data Sheet	

Product Name: <u>NA</u>	A. R. No./ <u>NR/25/0438</u> Batch No: <u>NA</u>
Test	<u>2 point calibration and system suitability.</u>
Reference Document	<u>SOP/DP/QC/045</u>

Instrument details :-

Name of instrument <u>Ultra micro Balance</u>	Instrument ID <u>ILAC/013</u>	calibration due date <u>22/03/26</u>
Standard details <u>Sucrose</u>	<u>E-1001009</u>	<u>07/05/26</u>
Name of standard <u>Sucrose</u>	Batch no. <u>PS10091001</u>	use before date <u>17/02/27</u>
<u>1,4-Benzquinone</u>	<u>RS1002123-003</u>	current lot

Preparation details :- sucrose weight 11.892 mg dissolved in 100ml purified water. pipetted 1 ml of 50000ppb sucrose stock solution & diluted to 100 ml with purified water (500ppb). sonicated for 30 sec & vortex.

Preparation details of 1,4 Benzquinone :- Benzquinone weight 7.570 mg dissolved in 100 ml purified water. pipetted out 1 ml of 50000ppb Benzquinone solution & diluted to 100 ml with purified water (500ppb). sonicated for 30 sec & vortex.

Result :-

TOC of Blank water in ppb = $\frac{SD \times Area \text{ of Blank}}{Area \text{ of sucrose} - Area \text{ of Blank}}$

= $\frac{SD \times 4.431}{36.82 - 4.431} = 68.40285 \approx 68 \text{ ppb.}$

Recovery of Benzquinone = $\frac{Area \text{ of Benzquinone} - Area \text{ of Blank} \times 100}{Area \text{ of sucrose} - Area \text{ of Blank}}$

= $\frac{36.41 - 4.431}{36.82 - 4.431} \times 100 = 98.73413 \approx 98.73$

Name of solution	SD Area	CV Area	Acceptance criteria's
Blank	0.08021	1.81 %	standard deviation: Not more than 0.50 % or CV Not more than 5.0 %
sucrose (500ppb)	0.8698	2.36 %	
1,4 Benzquinone	0.5314	1.46 %	

Conclusion: complies / Does not complies

Analysed By: Sign & Date: <u>21/03/26</u>	Checked By: Sign & Date: <u>21/03/26</u>
--	---

21-03-2026 21:46:11(+05:30) : Confirm[Dhananjay Ibhad]Other CommentData Submitted For Reviewed

21-03-2026 21:49:23(+05:30) : Review[Nilesh Dushing]Other CommentData Reviewed

Date of creation 2026/03/21 21:12:00
Sample Run TOC_I-QC-018_2026 - 5-572-4 - CAL_21032026_03.tlx
User Dhananjay Ibhad
Object ID 0L-H54436004105-13525E131B60-0000
System TOC-L + ASI-L
Origin TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald

Cal. Curve


Sample Name: Sucrose
Sample ID: Standard
Object ID 0L-H54436004105-13525E131B60-0000
Cal. Curve: TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald
Status Completed
Comment:

Type	Anal.
Standard	NPOC

Conc: 0.000ppb

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	4.523	816uL	1.000	*****		2026/03/21 20:46:45
2	4.374	816uL	1.000	*****		2026/03/21 20:50:29
3	4.397	816uL	1.000	*****		2026/03/21 20:54:17


Acid Add. 0.000%
Spurge Gas Flow 80mL/min
Sp. Time 60.00sec
Mean Area 4.431
SD Area 0.08021
CV Area 1.81%
Vial 7
No Washes 2

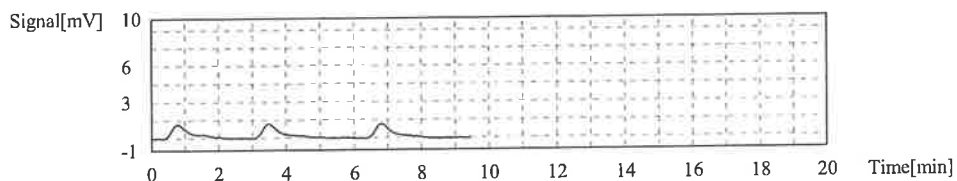


Conc: 500.0ppb

No.	Area	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Date / Time
1	35.86	816uL	1.000	*****		2026/03/21 21:03:32
2	37.03	816uL	1.000	*****		2026/03/21 21:07:40
3	37.56	816uL	1.000	*****		2026/03/21 21:11:58

Acid Add. 0.000%
Spurge Gas Flow 80mL/min
Sp. Time 60.00sec
Mean Area 36.82
SD Area 0.8698
CV Area 2.36%
Vial 8
No Washes 2

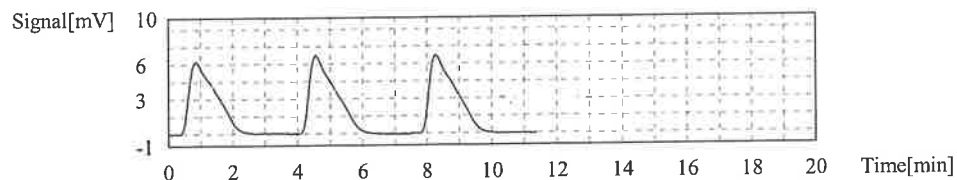

Slope: N/A
Intercept N/A
 r^2 N/A
 r N/A
RSE(%)
Zero Shift Yes

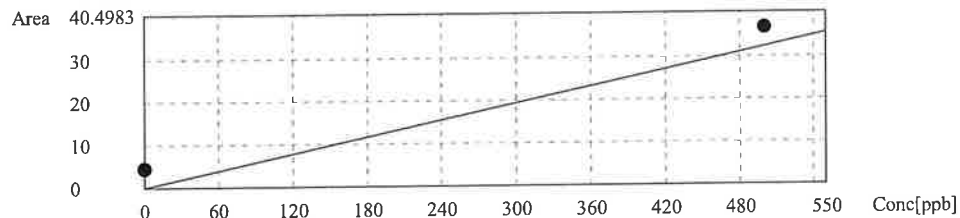**History**

No. 1
Date & Time 2026/03/21 20:32:37(+0530)
User Name Dhananjay Ibhad
Changes New
Contents
Reason for change

21-03-2026 21:46:53(+05:30) : Confirm[Dhananjay Ibhad]Other CommentData Submitted For Review

21-03-2026 21:49:23(+05:30) : Review[Nilesh Dushing]Other CommentData Reviewed

Date of creation 2026/03/21 21:41:06
Sample Run TOC_I-QC-018_2026 - 5-572-7 - CAL_21032026_03.txl
User Dhananjay Ibhad
Object ID 0L-H54436004105-13525E133CBD-0000
System TOC-L + ASI-L
Origin TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald

Sample

Sample Name: 1,4-Benzoquinone
Sample ID: Std SST
Object ID 0L-H54436004105-13525E133CBD-0000
Origin: TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald
Status Completed
Chk. Result 98.73% : USP/EP system suitability test: Pass
Comment

Type	Anal.	Manual Dilution	Result
Unknown	NPOC	1.000	NPOC:562.1ppb


1. Det

Anal.: NPOC

No.	Area	Conc.	Inj. Vol.	Aut. Dil.	Rem.	Ex.	Cal. Curve	Date / Time
1	35.95	555.0ppb	816uL	1.000	**h****		TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald	2026/03/21 21:32:42
2	36.28	560.1ppb	816uL	1.000	**h****		TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald	2026/03/21 21:36:49
3	36.99	571.1ppb	816uL	1.000	**h****		TOC_I-QC-018_2026 - CAL_21032026_01.2026_03_21_20_39_03.cald	2026/03/21 21:41:05

Acid Add. 0.000%
Spurge Gas Flow 80mL/min
Sp. Time 60.00sec
Mean Area 36.41
Mean Conc. 562.1ppb
SD Area 0.5314
CV Area 1.46%
SD Conc 8.205
CV Conc 1.46%
Vial 9
No Washes 2

Signal[mV]

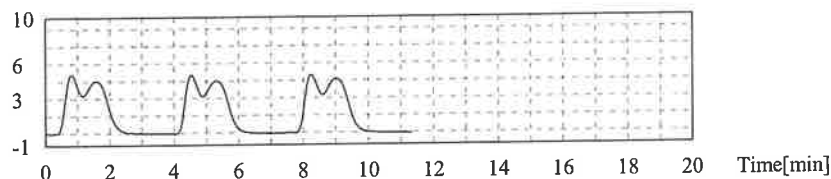**History**