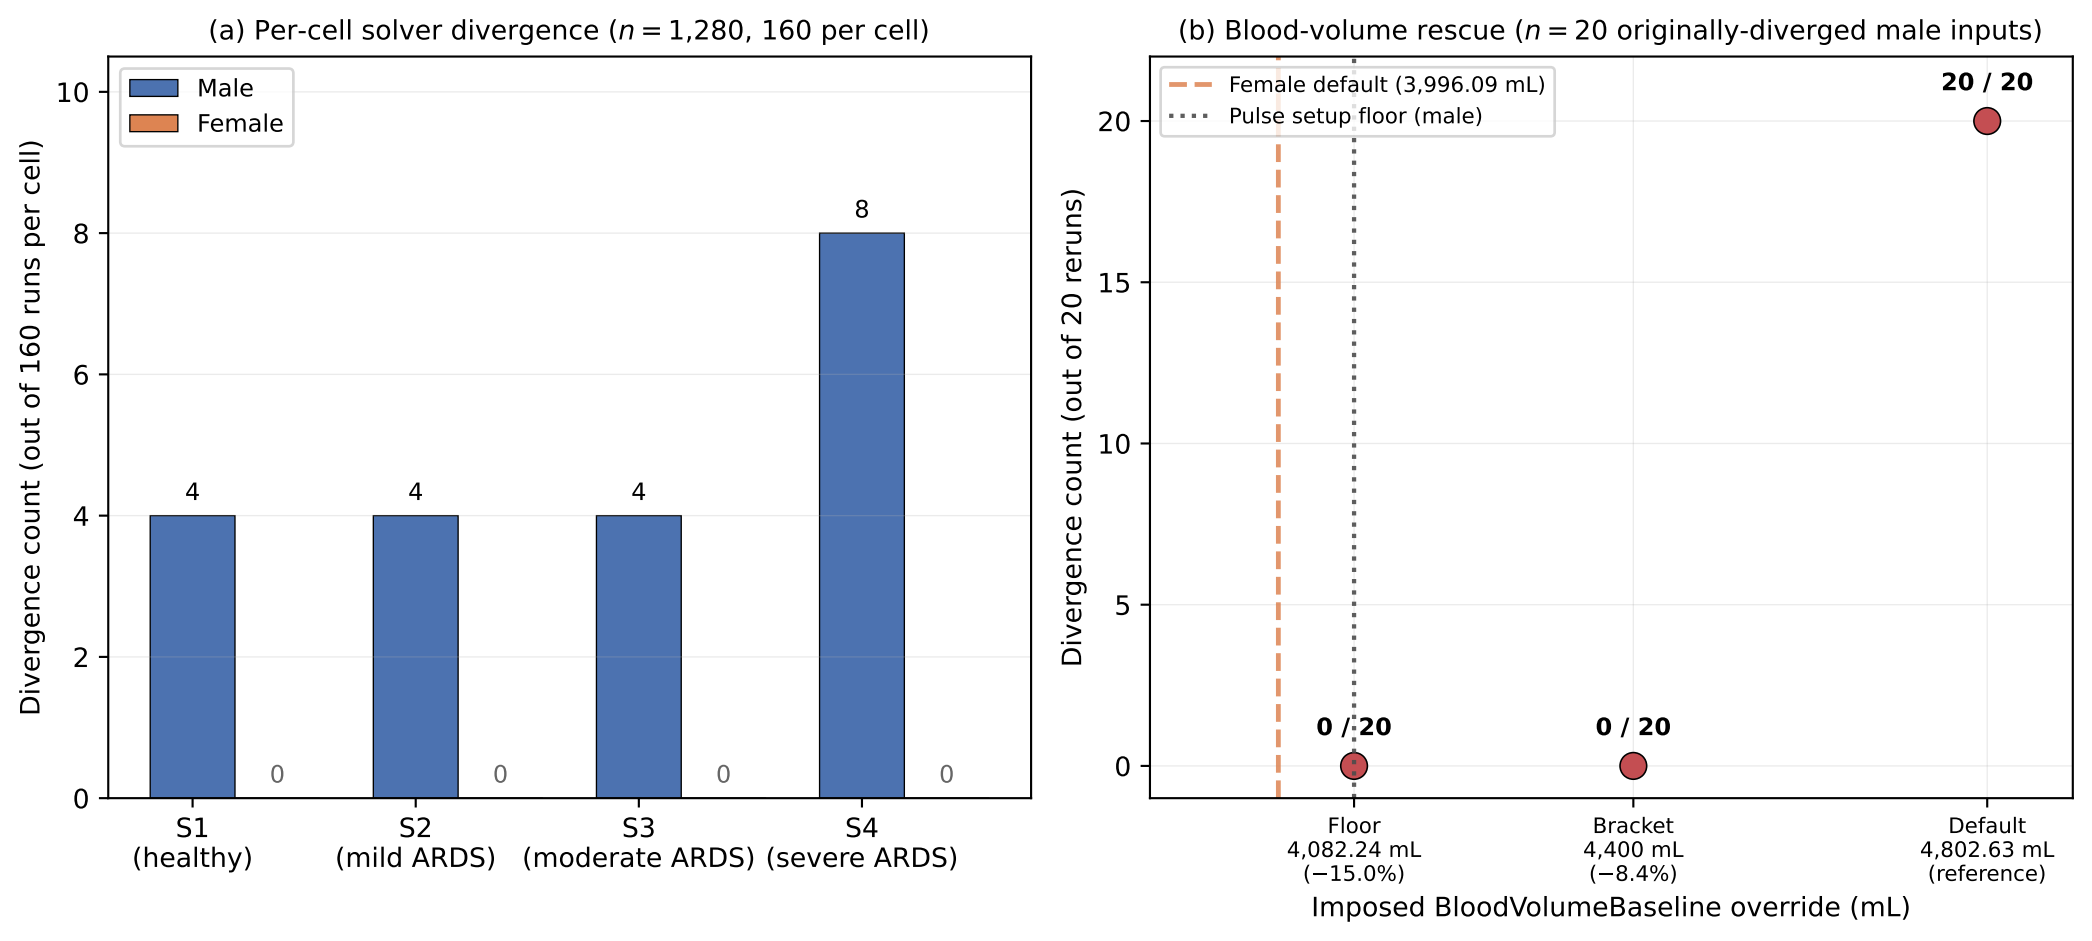
(a) Per-cell solver divergence ($n = 1{,}280$, 160 per cell)
Male
Female
Divergence count (out of 160 runs per cell)
0
2
4
6
8
10
4
0
4
0
4
0
8
0
S1
(healthy)
S2
(mild ARDS)
S3
(moderate ARDS)
S4
(severe ARDS)
(b) Blood-volume rescue ($n = 20$ originally-diverged male inputs)
Female default (3,996.09 mL)
Pulse setup floor (male)
Divergence count (out of 20 reruns)
0
5
10
15
20
0 / 20
0 / 20
20 / 20
Floor
4,082.24 mL
(−15.0%)
Bracket
4,400 mL
(−8.4%)
Default
4,802.63 mL
(reference)
Imposed BloodVolumeBaseline override (mL)