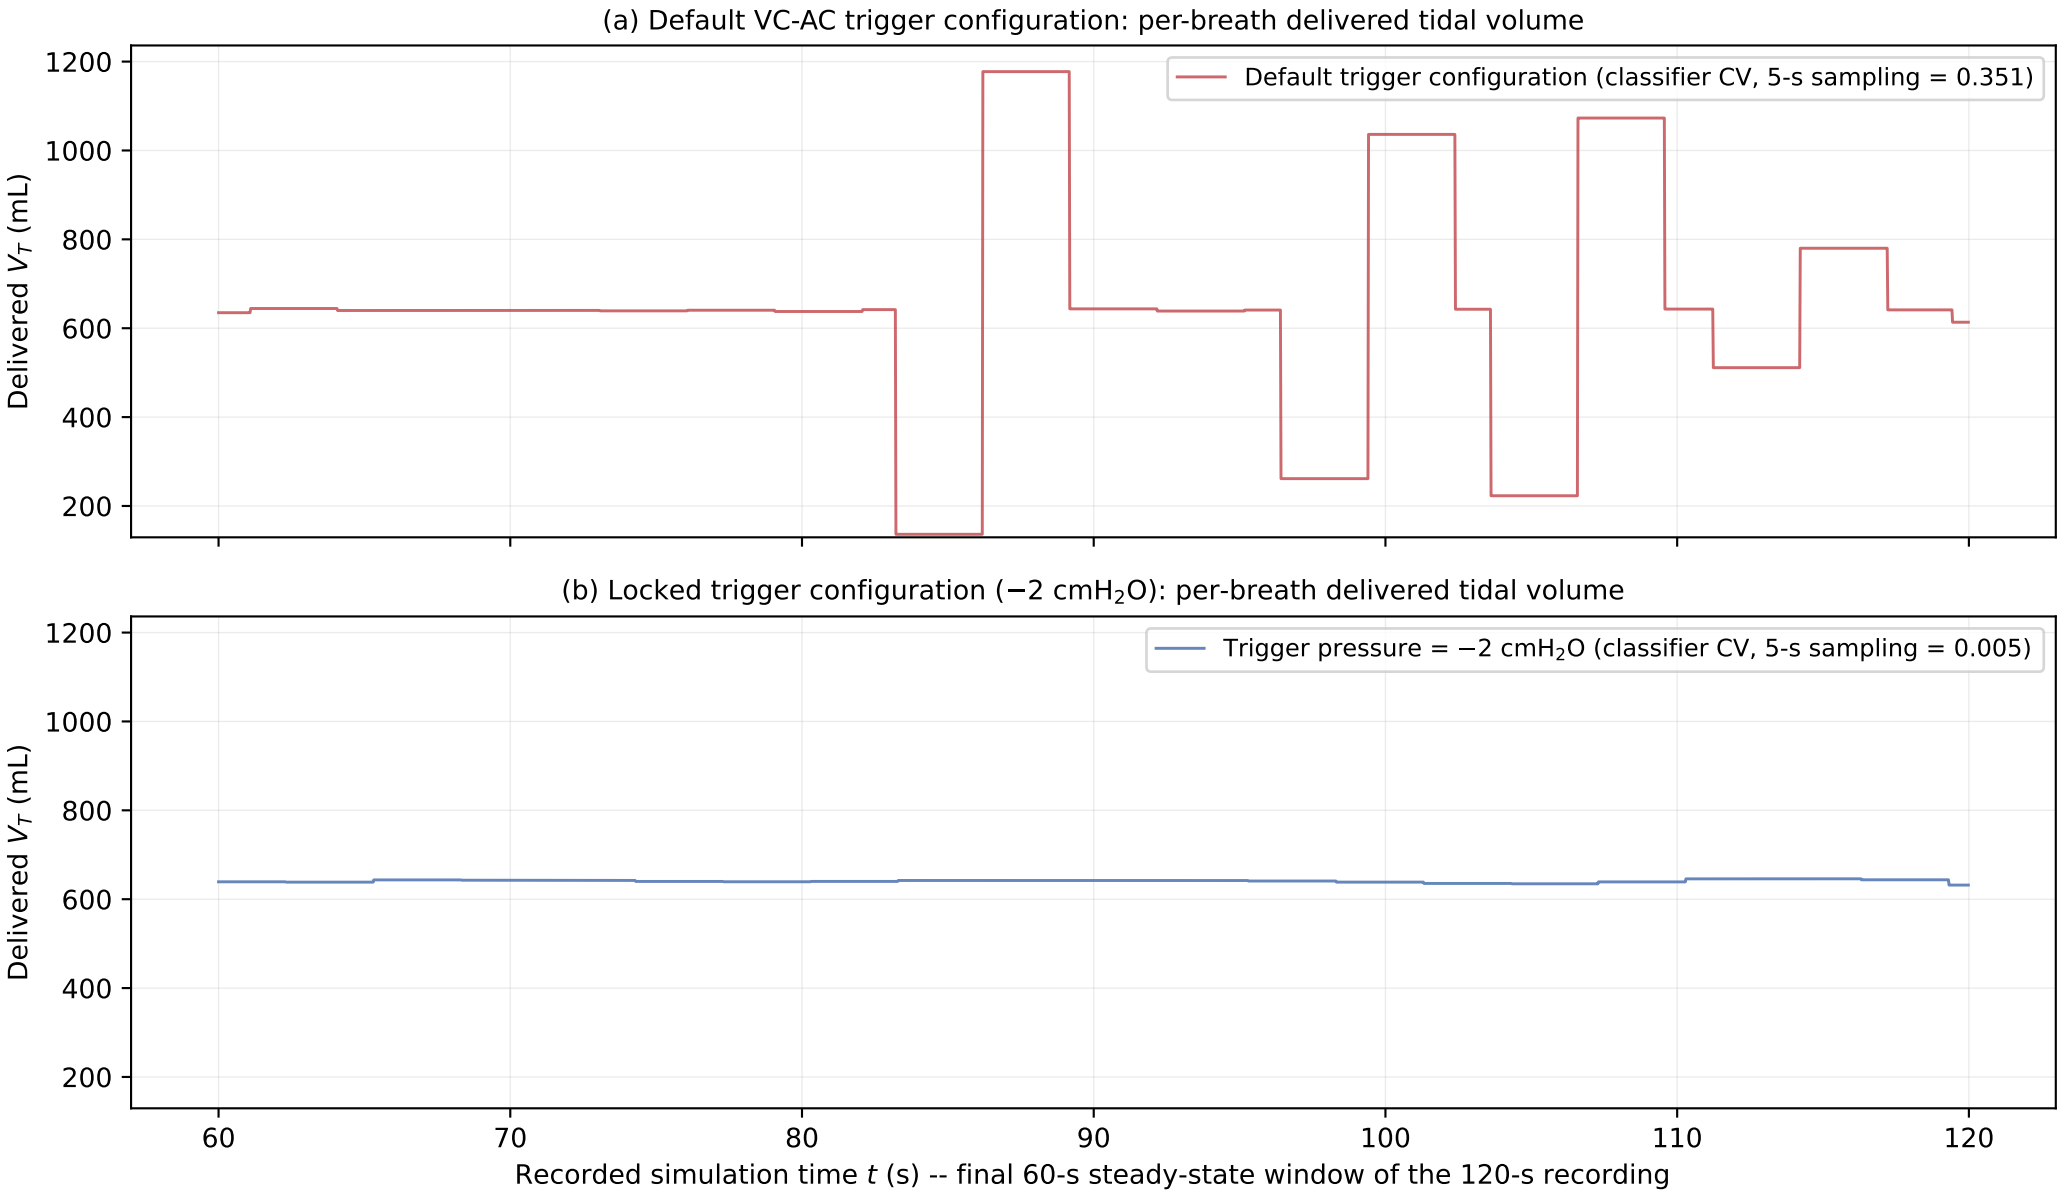
(a) Default VC-AC trigger configuration: per-breath delivered tidal volume
Default trigger configuration (classifier CV, 5-s sampling = 0.351)
Delivered V_T (mL)
1200
1000
800
600
400
200
(b) Locked trigger configuration (−2 cmH$_2$O): per-breath delivered tidal volume
Trigger pressure = −2 cmH$_2$O (classifier CV, 5-s sampling = 0.005)
Delivered V_T (mL)
1200
1000
800
600
400
200
60
70
80
90
100
110
120
Recorded simulation time t (s) -- final 60-s steady-state window of the 120-s recording