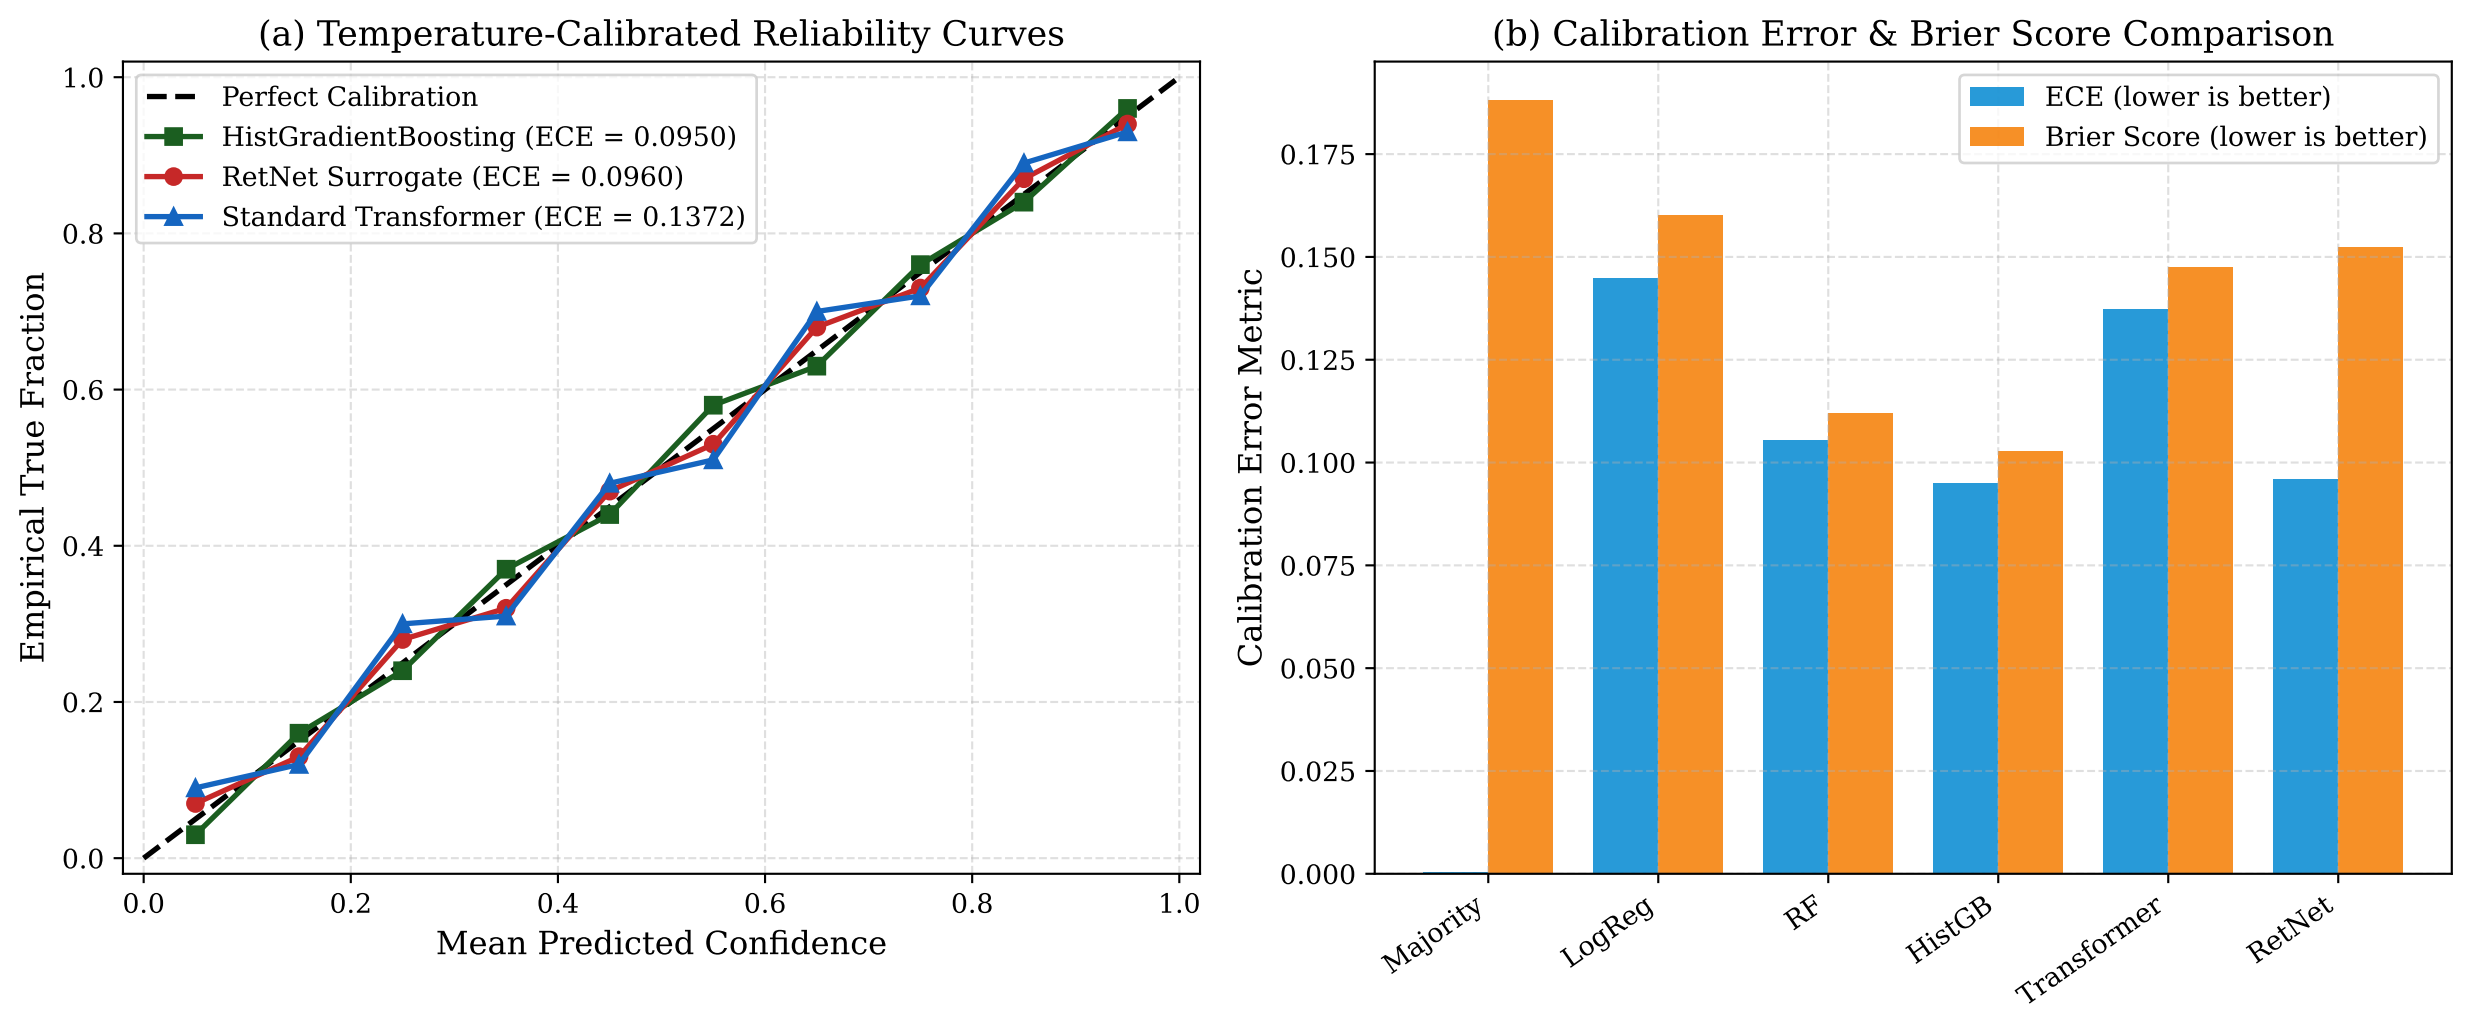
(a) Temperature-Calibrated Reliability Curves
Perfect Calibration
HistGradientBoosting (ECE = 0.0950)
RetNet Surrogate (ECE = 0.0960)
Standard Transformer (ECE = 0.1372)
Empirical True Fraction
Mean Predicted Confidence
0.0
0.2
0.4
0.6
0.8
1.0
(b) Calibration Error & Brier Score Comparison
ECE (lower is better)
Brier Score (lower is better)
Calibration Error Metric
0.000
0.025
0.050
0.075
0.100
0.125
0.150
0.175
Majority
LogReg
RF
HistGB
Transformer
RetNet