ProntoDx

Where Accuracy Meets Urgency

"Touching Human Lives Through Innovation"

SG1

Blood Gas & Electrolyte Analyzer



A handheld blood analyzer that delivers lab-quality, diagnostic results in minutes.

MATRIX LABS
DIAGNOCARE PVT. LTD.

Scanned with OKEN Scanner

Product features

Easy to use

Testing can be performed in 3 simple steps at the patient's side with only 2 or 3 drops of whole blood.

Handheld portability

Lightweight with build-in battery allowing diagnosis at the point of care, patient side, out in the field or exam room.

Fast results

Get accurate results in 4 minutes at the patient's side to enable rapid decision-making, and optimize patient-care.

Multi-parameter cartridge

Single-use test cartridges a broad menu of tests on a single, portable platform. Each test card has a unique combination of biosensors to suit a wide range of clinical needs.

Use Cases



Emergency Treatment



ICU



Oncology



Anesthesiology Department



Gynecology and Obstetrics



Clinical Laboratory


Test Cartridges


Sample	Whole blood / Capillary
Test Time	50s
Display	4.3 IPS touch screen
Weight	600g
Battery	3.7V, 5000mAh Up to 55 samples in a row


Sample volume	100 µl
Connectors	Type c
Printer	Built-in thermal printer
Connection	WIFI, Direction LIS (HL7)
Operating temperature	Temperature: 5 - 32℃; Relative humidity ≤85%;


Scanned with OKEN Scanner

Reagent performance analysis

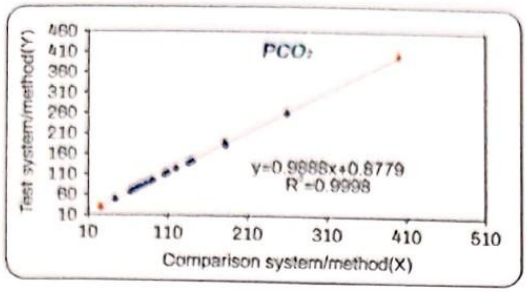

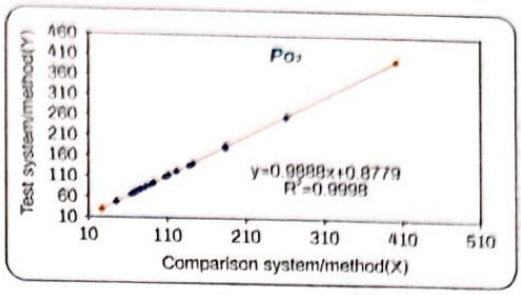

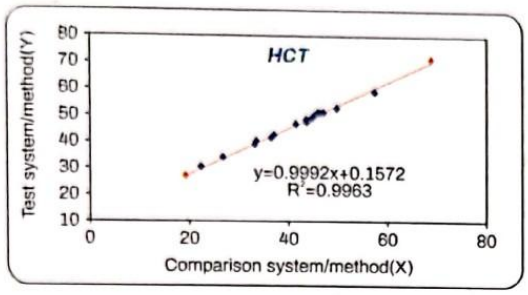

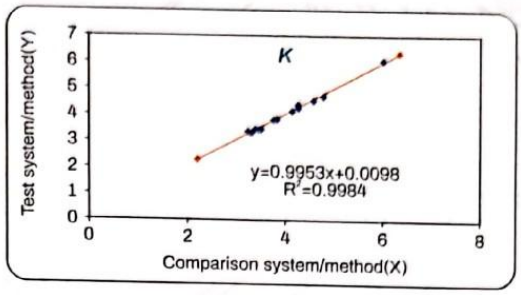

Easy 3 steps operation

Regular Test Cartridge



Add sample

Add 2 or 3 drops of whole blood into cartridge



Insert cartridge

Insert the cartridge into the analyzer



Read result

Read the test report in 4 minutes

Auto Aspiration Cartridge




Insert syringe

Flat insert the syringe into the fill port of test cartridge



Insert cartridge

Insert cartridge into the analyzer

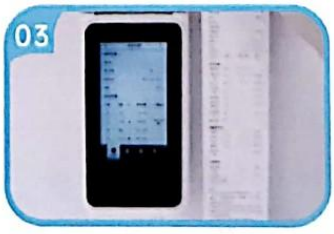

Read result

Read the test report in 4 minutes

Test Cartridges

Parameter	· BG3	· BG3-N	· BG8	· BG8-N	· BG10	· BG10-N	· BE5
pH	●	●	●	●	●	●	●
pO_2	●	●	●	●	●	●	
pCO_2	●	●	●	●	●	●	
K^+			●	●	●	●	●
Na^+			●	●	●	●	●
Cl^-			●	●	●	●	●
Ca^{2+}			●	●	●	●	●
Hct			●	●	●	●	
Glu					●	●	
Lac					●	●	
tCO_2*	●	●	●	●	●	●	
cHgb*	●	●	●	●	●	●	
$cHCO_3^-$*	●	●	●	●	●	●	
BE(ecf)*	●	●	●	●	●	●	
BE(b)*	●	●	●	●	●	●	
cSO_2*	●	●	●	●	●	●	
AG*	●	●	●	●	●	●	

* Calculated parameter

Measured Parameter

Parameter

Na^+	pCO_2
K^+	pO_2
Cl^-	Hct
Ca^{2+}	Glu
pH	Lac
Li #	Mg #
tCO_2 #	.....

Under development

Calculated Parameter

pH(T)	cH^+	cH^+(T)
pCO_2(T)	$cHCO_3^-$	cBase(B)$_c$
cBase(Ecf)$_c$	cBase(Ecf,ox)$_c$ #	$cHCO_3^-$(P, st)$_c$ #
cBase(B,ox)$_c$ #	$ctCO_2$(B)	$ctCO_2$(P)
pO_2(T)	pO_2(A)	pO_2(A-a)
pO_2(a/A)	ctO_2(B)	RI
cHgb	pO_2(a)/FO_2(I) #	pO_2(a/A,T)
pO_2(A-a,T) #	pO_2(a,T)/FO_2(I) #	RI(T)
cCa^{2+}(7.4)	Anion Gap(K^+)$_c$	cSO_2
AG	FO_2(I) #	.....

Under development

Samarth Agency

'Moreshwar', Plot No.10,
Abhiyantanagar, Islampur
Pin -415 409 Tal.Walwa,
Dist. Sangli, Maharastra

ph-
+918329160577 +919699637355
+918412821206 +919699627366

email-
sharadmore7517@gmail.com