Final image errors: median and interquartile range (logarithmic error axis)

1% noise, CT: 30 samples per resolution

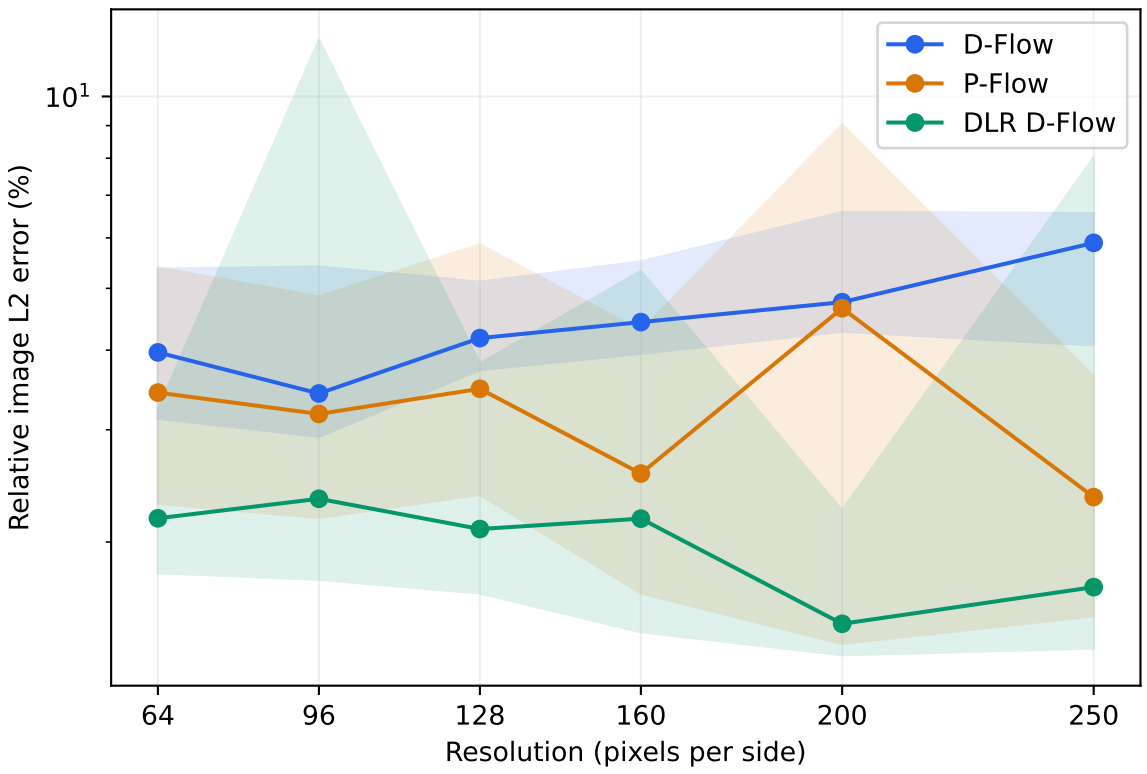

1% noise, MRI: 30 samples per resolution

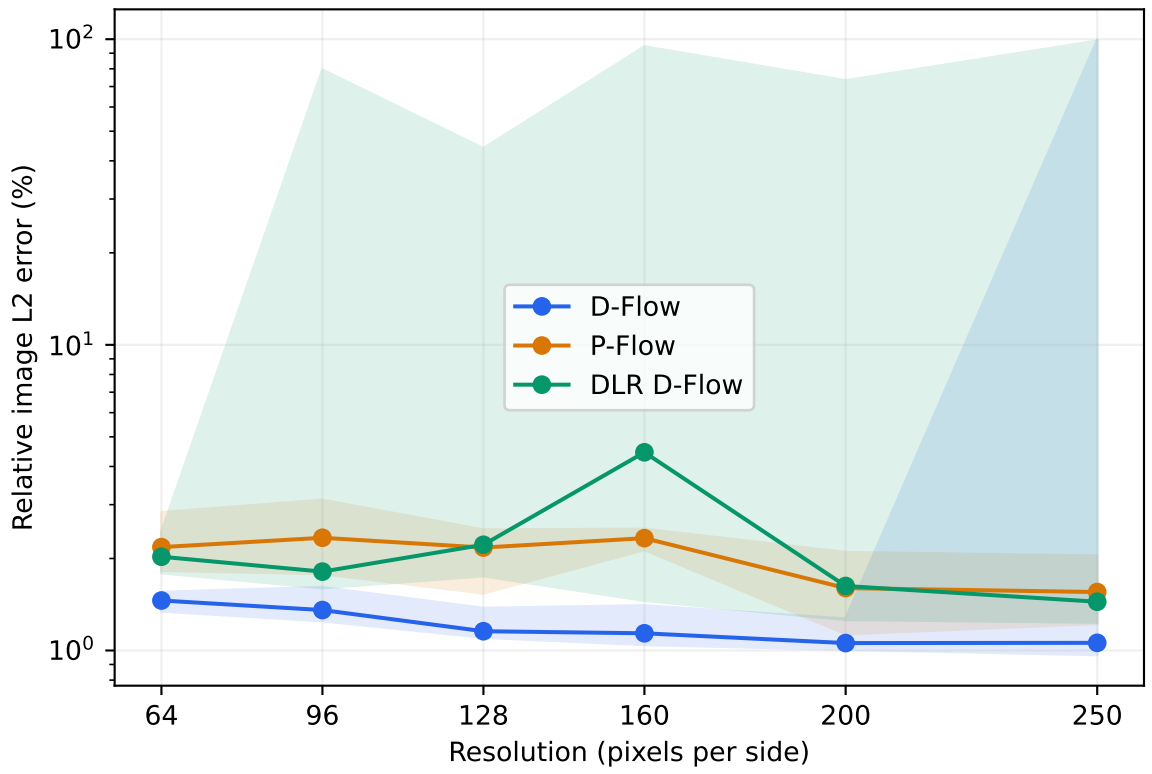

5% noise, CT: 30 samples per resolution

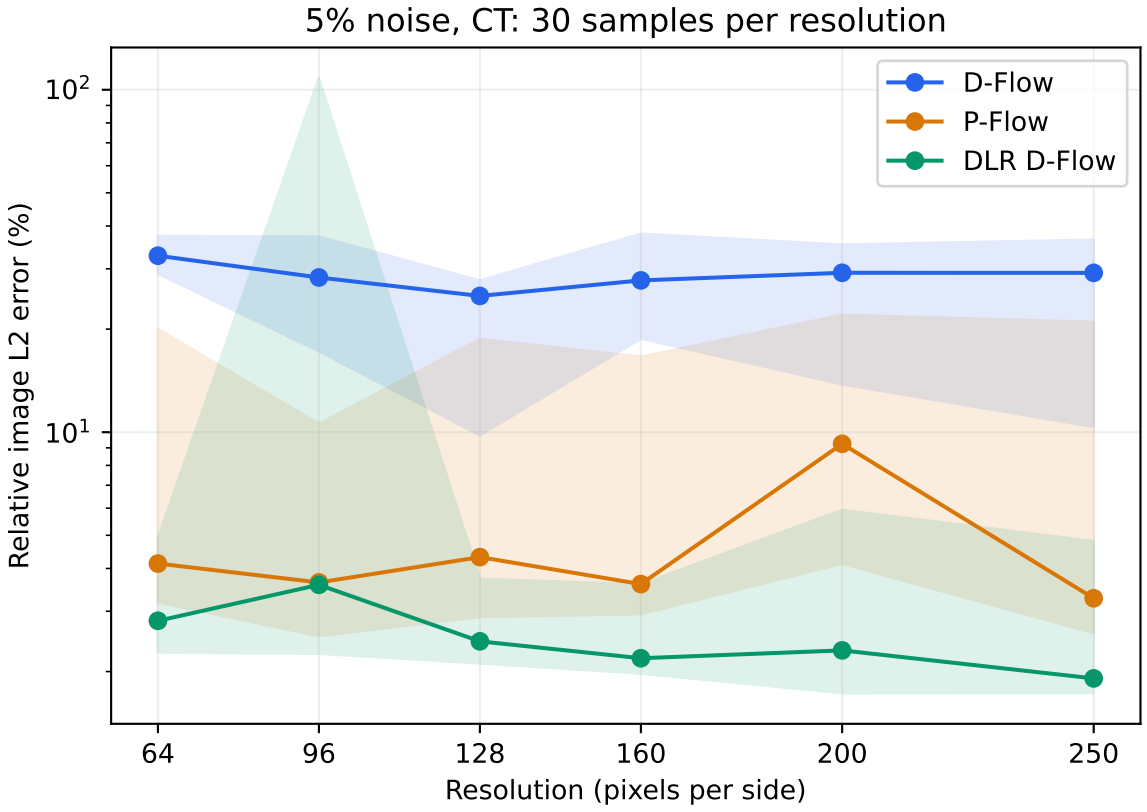

5% noise, MRI: 30 samples per resolution

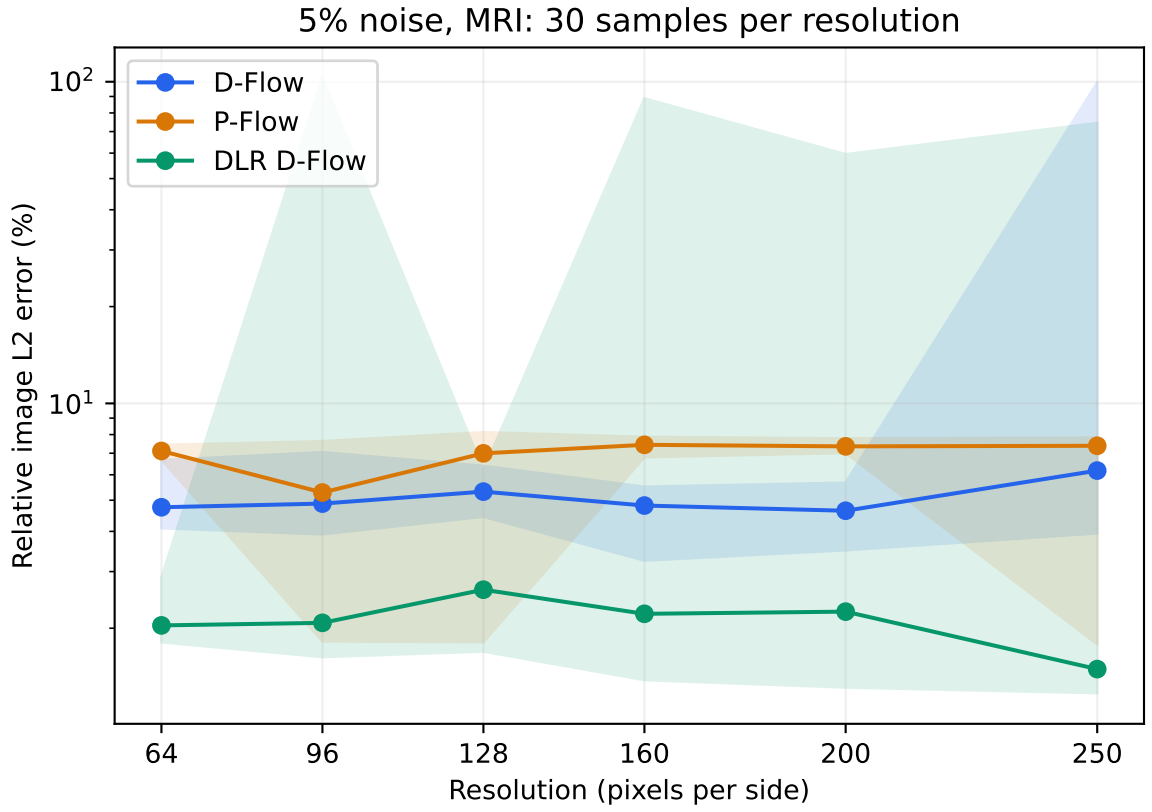

10% noise, CT: 30 samples per resolution

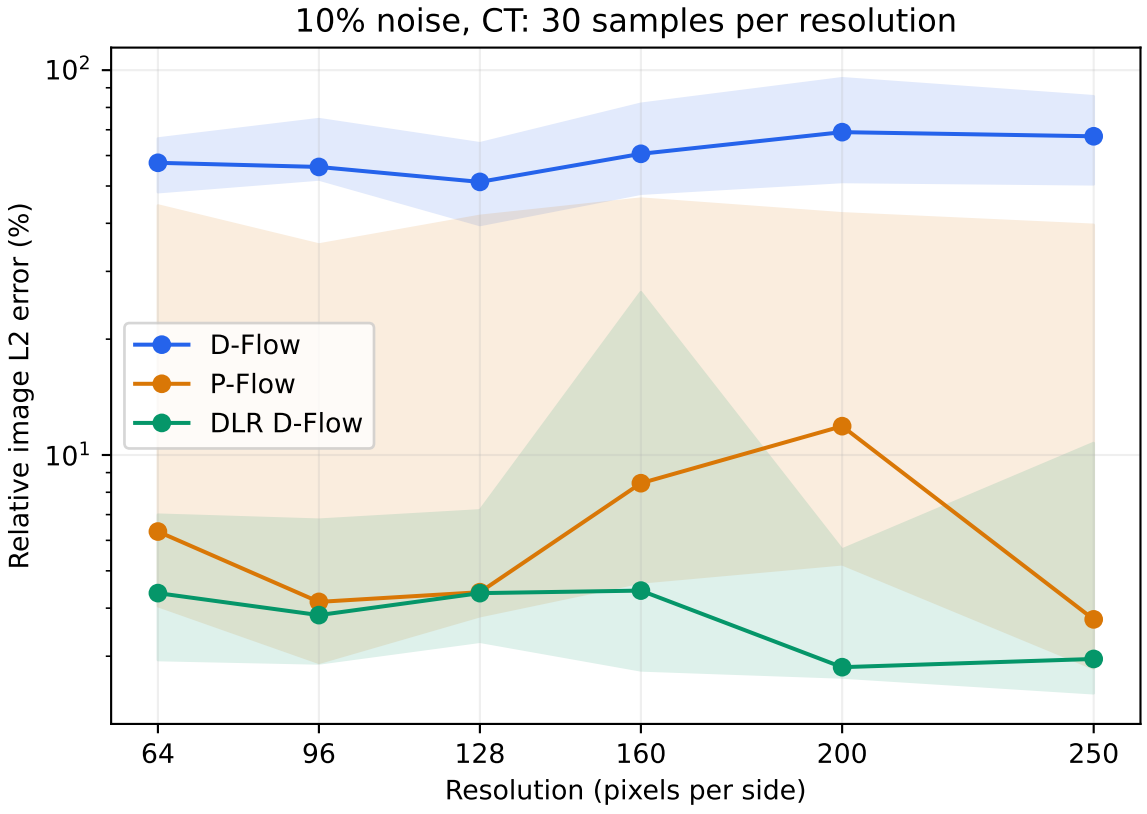

10% noise, MRI: 30 samples per resolution

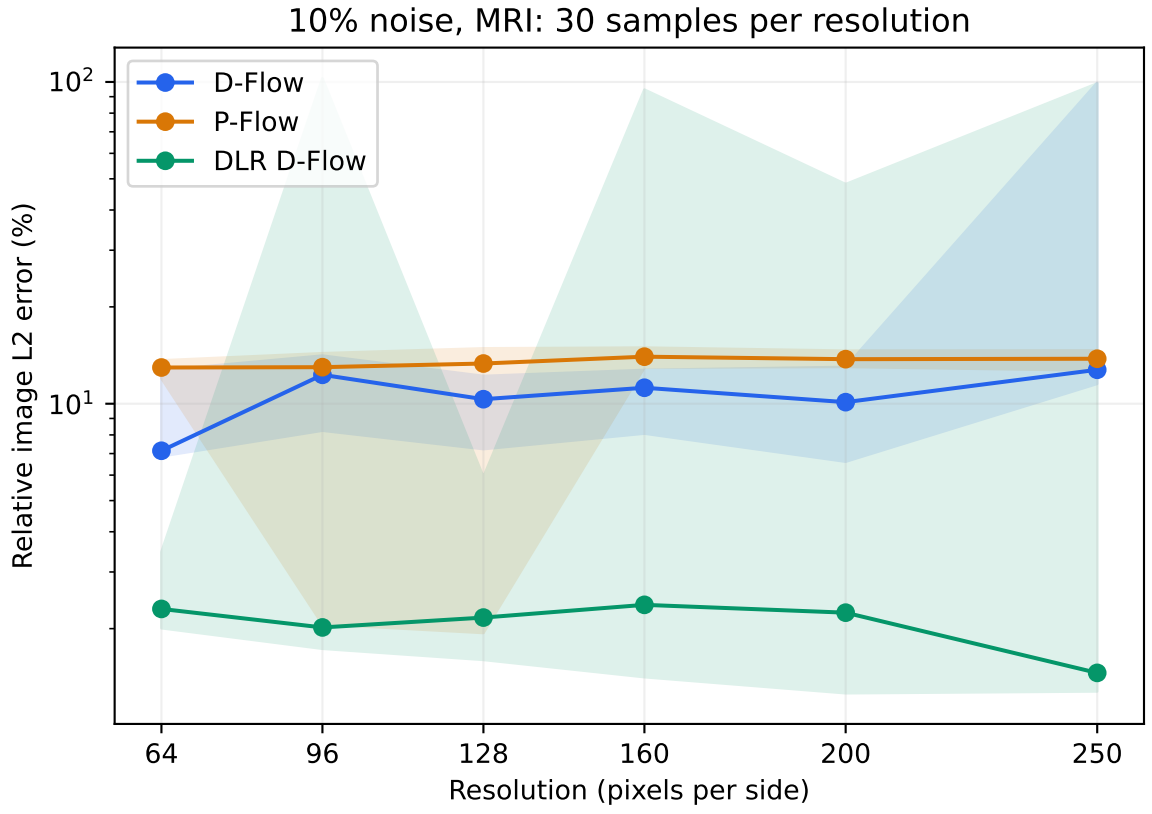

20% noise, CT: 30 samples per resolution

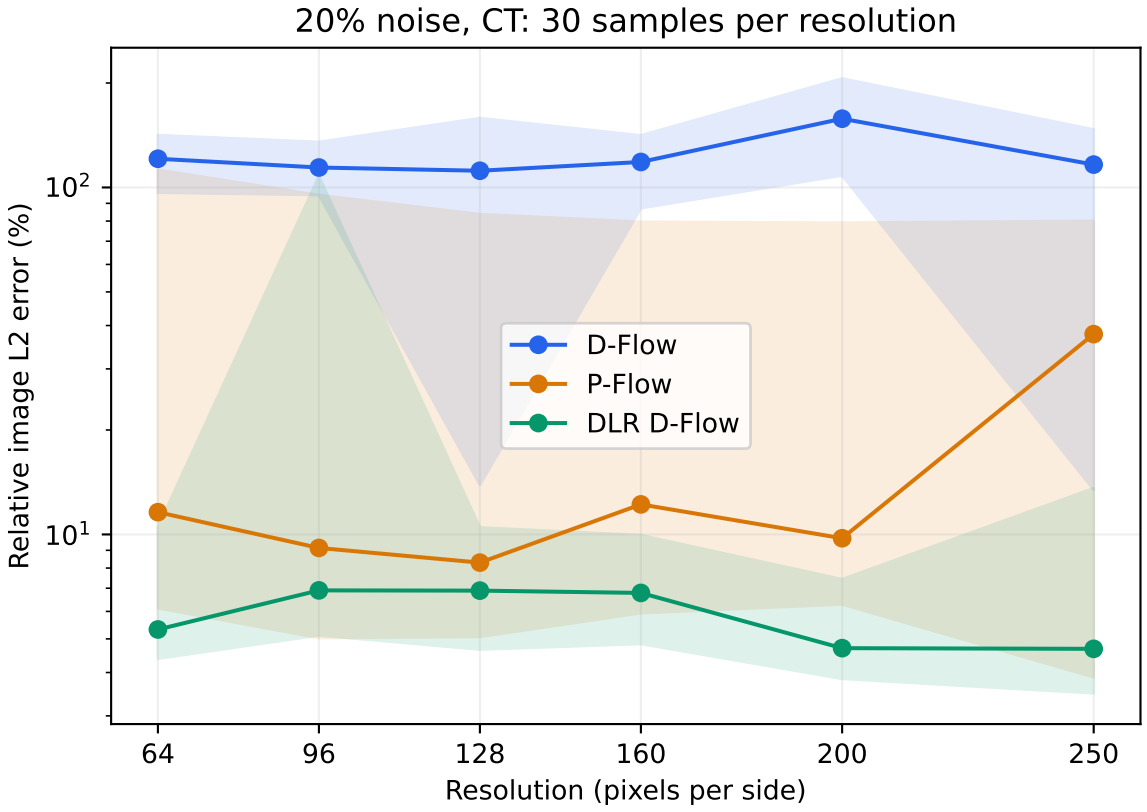
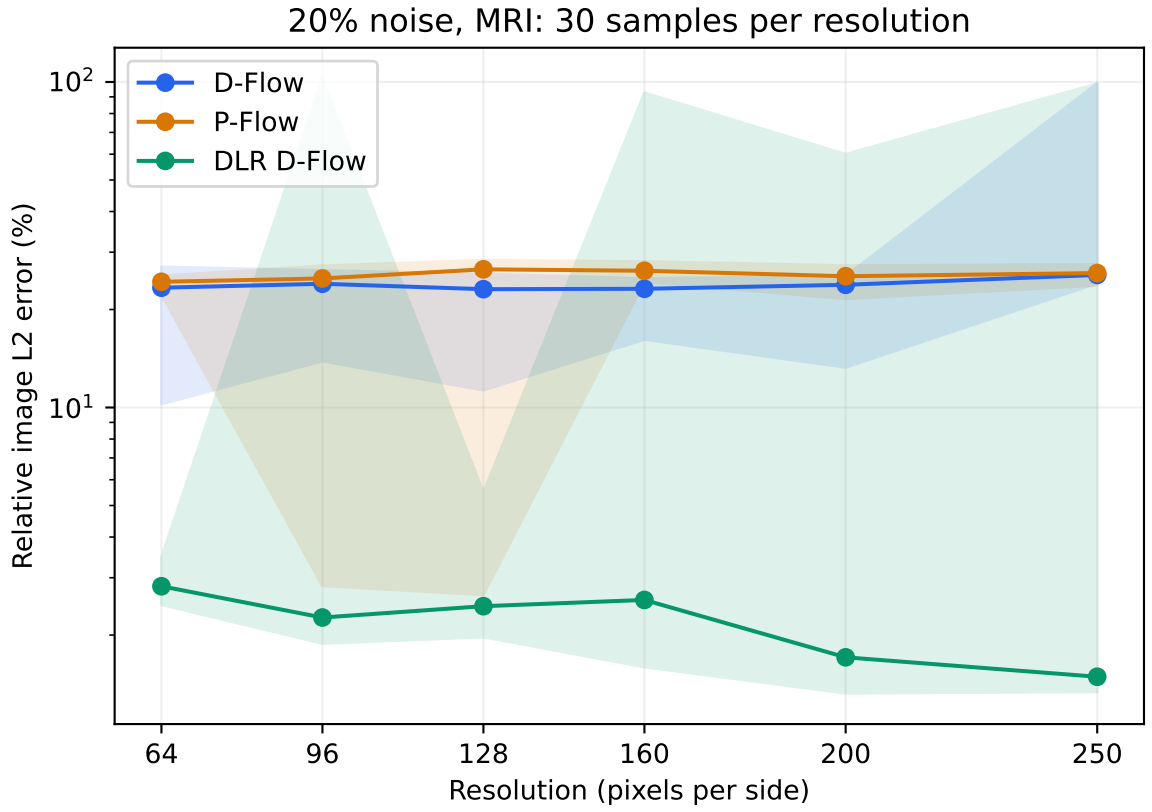
20% noise, MRI: 30 samples per resolution