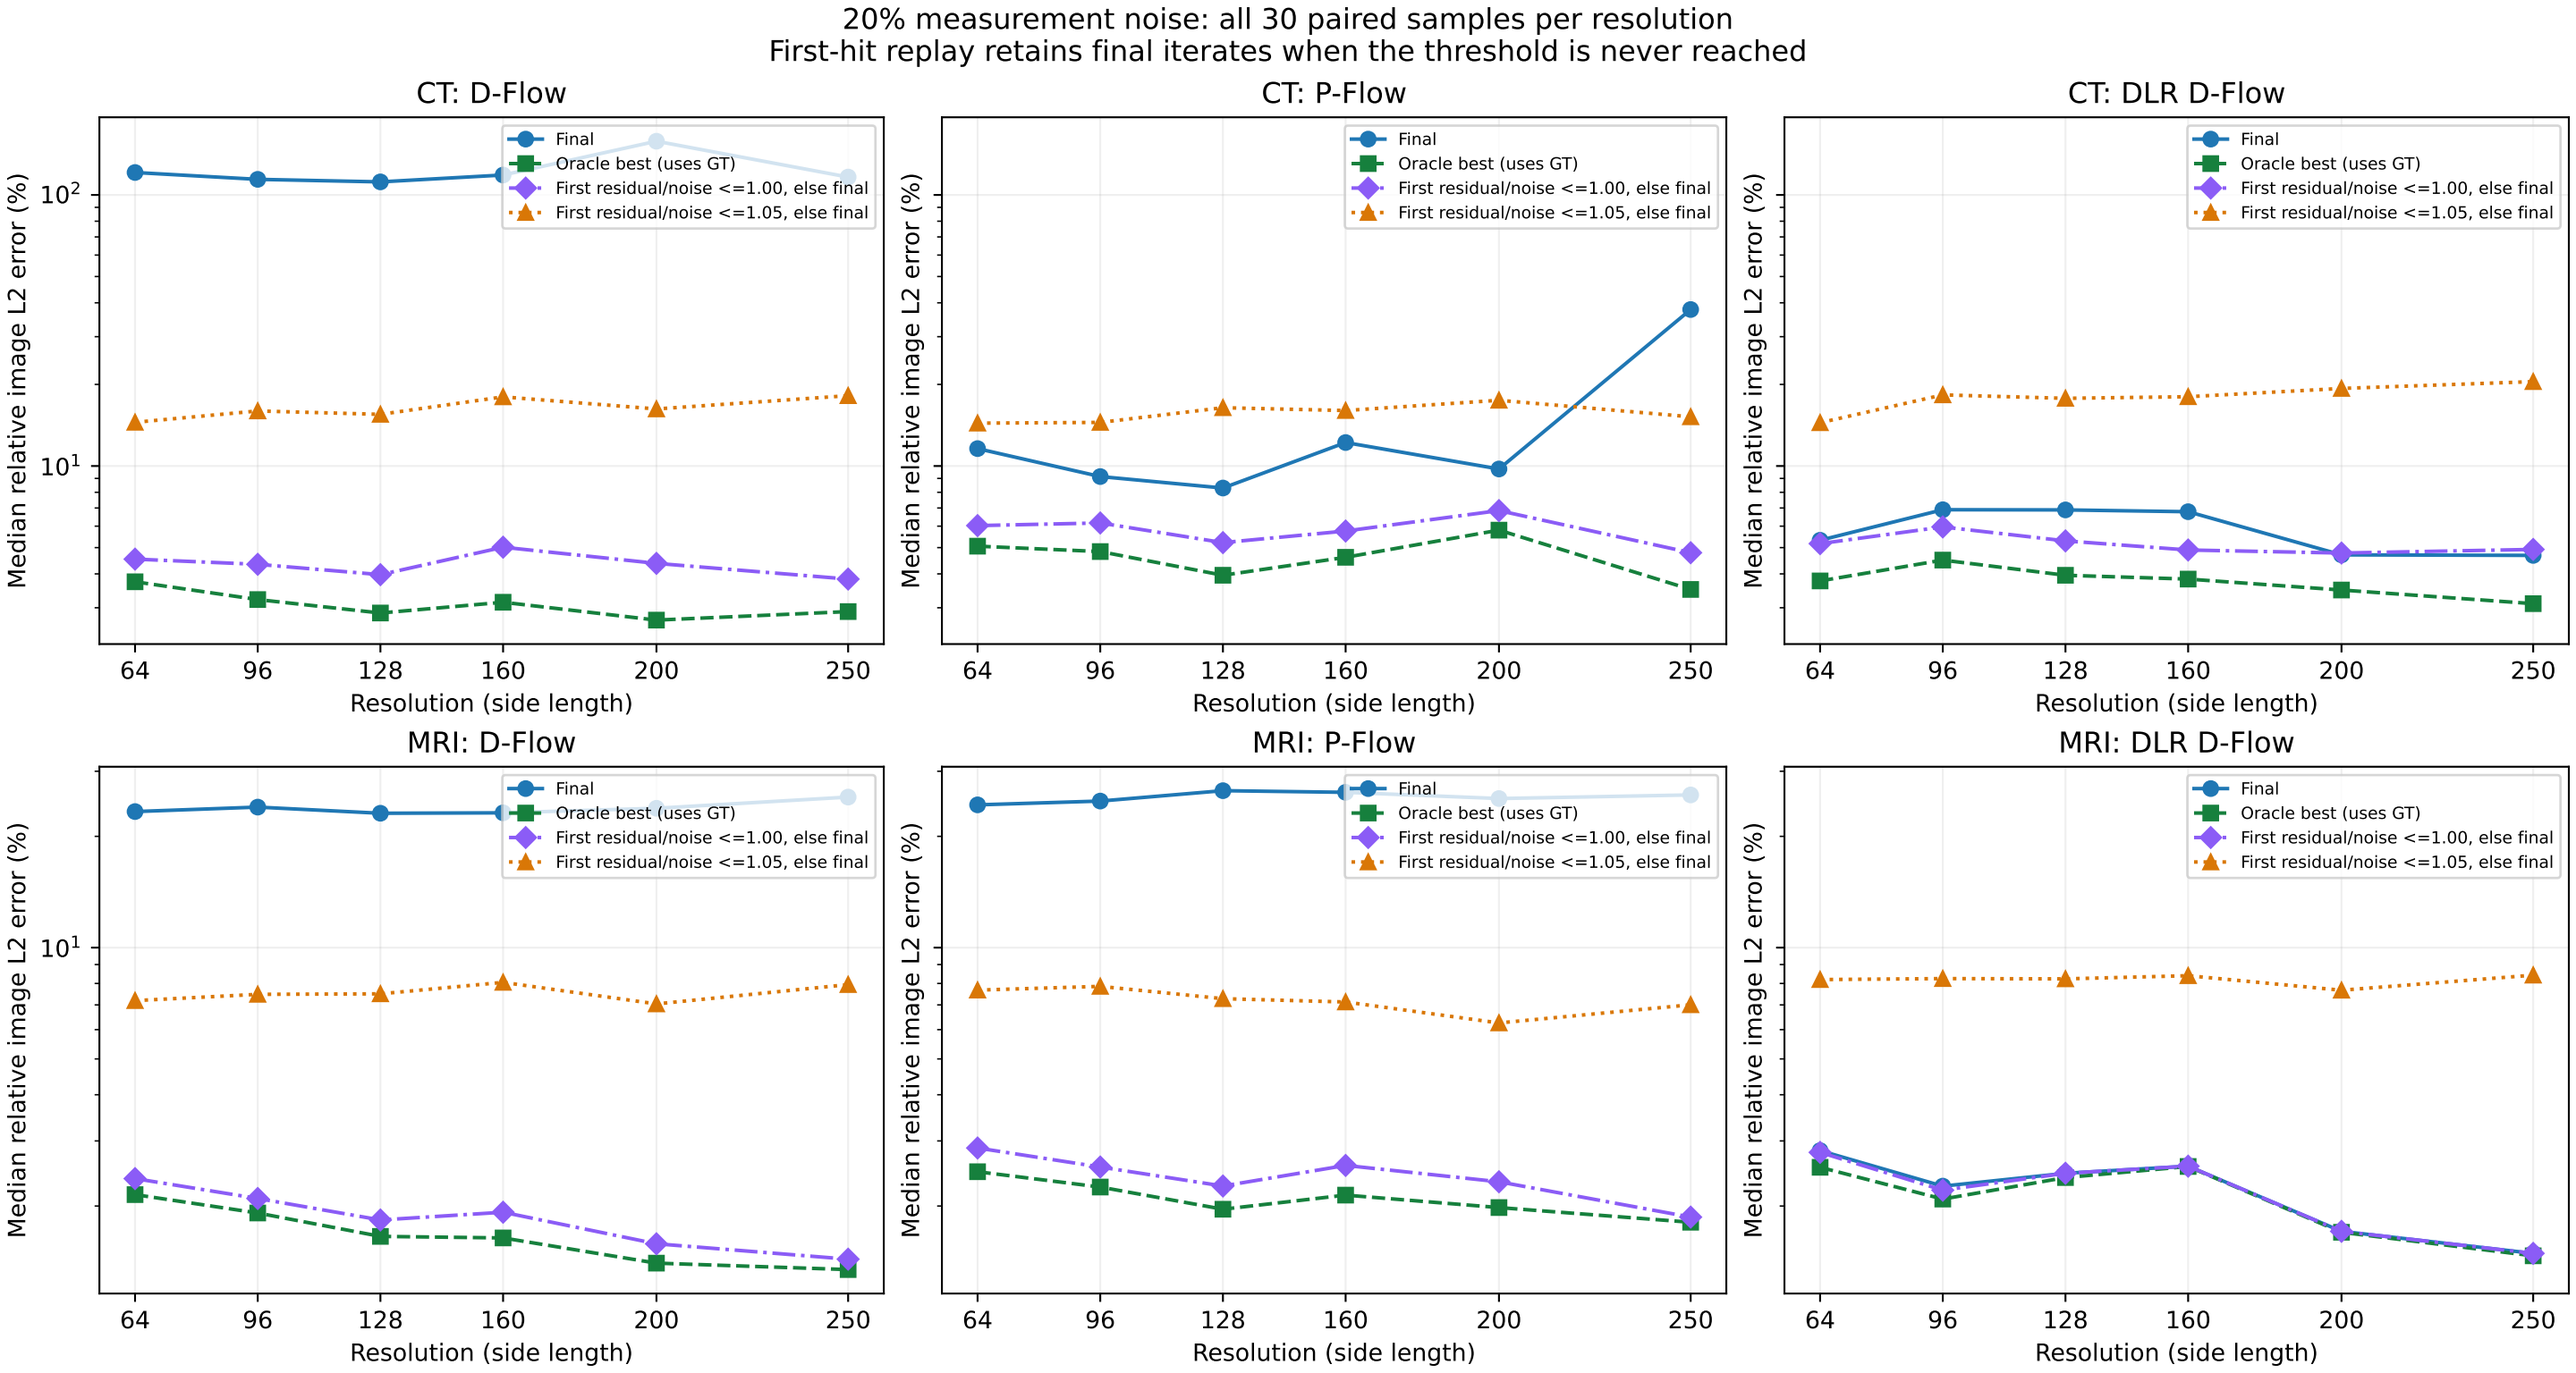
20% measurement noise: all 30 paired samples per resolution
First-hit replay retains final iterates when the threshold is never reached
CT: D-Flow
CT: P-Flow
CT: DLR D-Flow
MRI: D-Flow
MRI: P-Flow
MRI: DLR D-Flow
Median relative image L2 error (%)
Resolution (side length)
Final
Oracle best (uses GT)
First residual/noise <=1.00, else final
First residual/noise <=1.05, else final