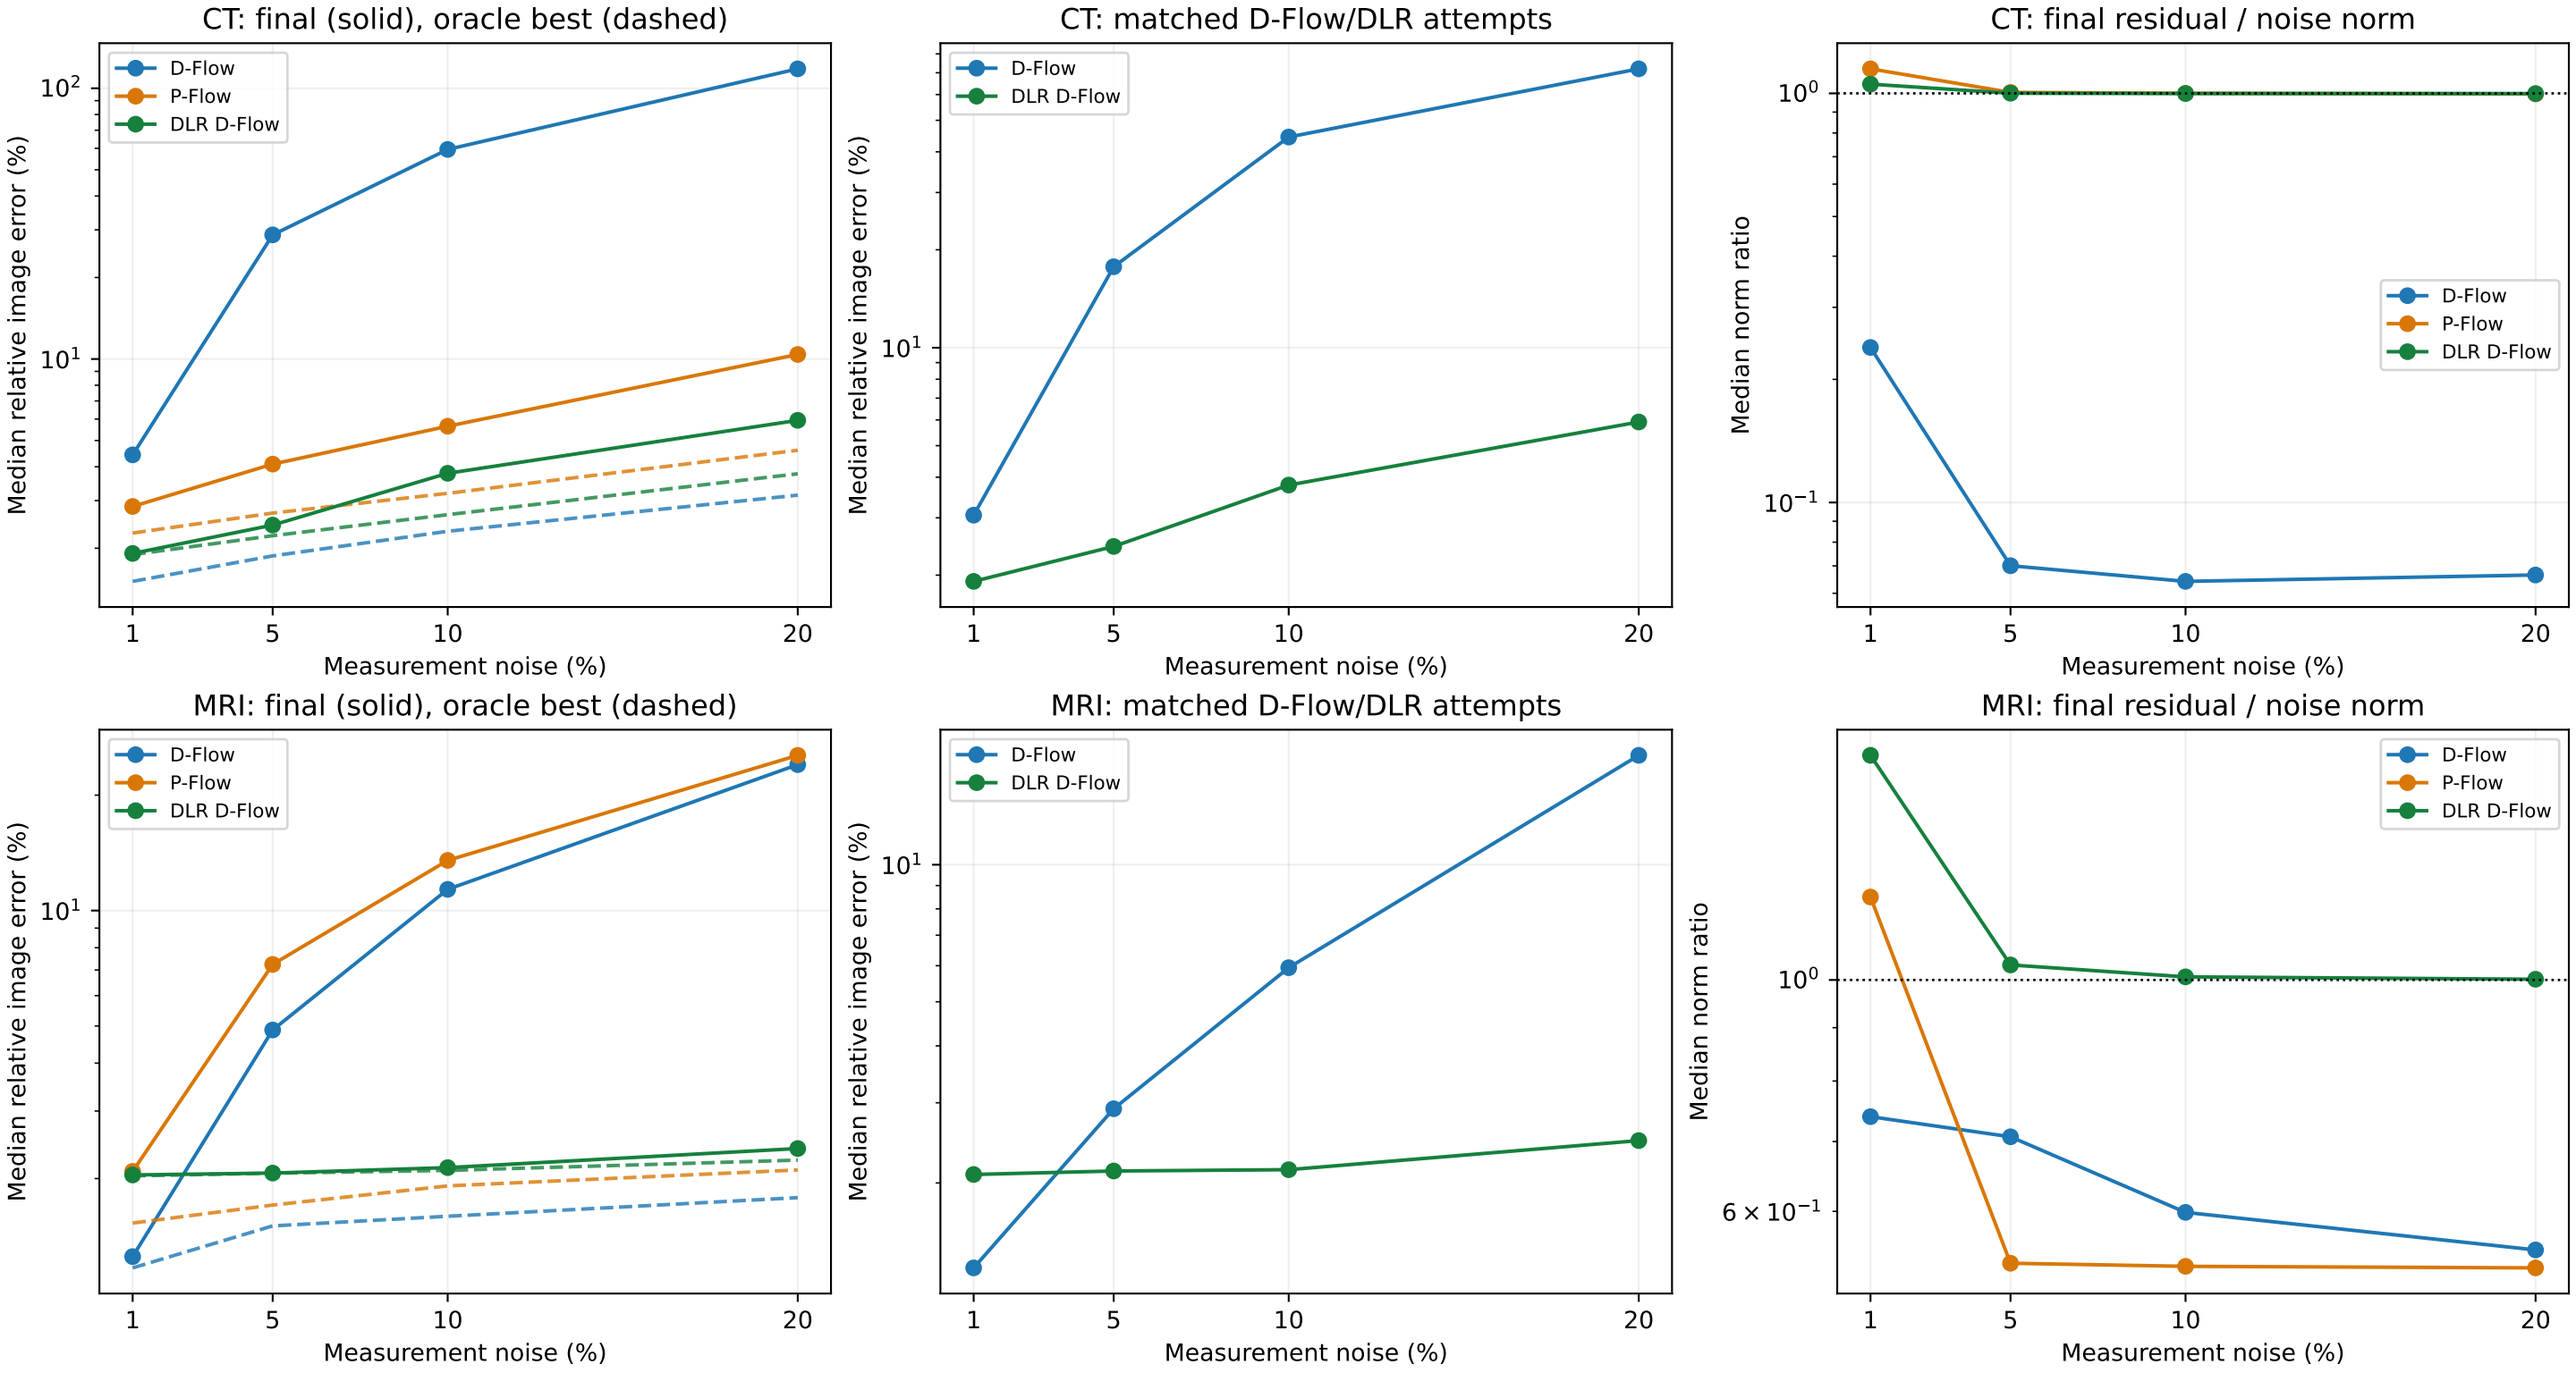
CT: final (solid), oracle best (dashed)
CT: matched D-Flow/DLR attempts
CT: final residual / noise norm
MRI: final (solid), oracle best (dashed)
MRI: matched D-Flow/DLR attempts
MRI: final residual / noise norm
D-Flow
P-Flow
DLR D-Flow
Median relative image error (%)
Median norm ratio
Measurement noise (%)
1
5
10
20
10^2
10^1
10^0
10^{-1}
6×10^{-1}