


Test No:	000031	Tested Date:	2024-01-03
Patient Name :	dfsdf sdf sdfsd	Age:	44
Doctors Name:	Default-Unknown	Gender:	Male

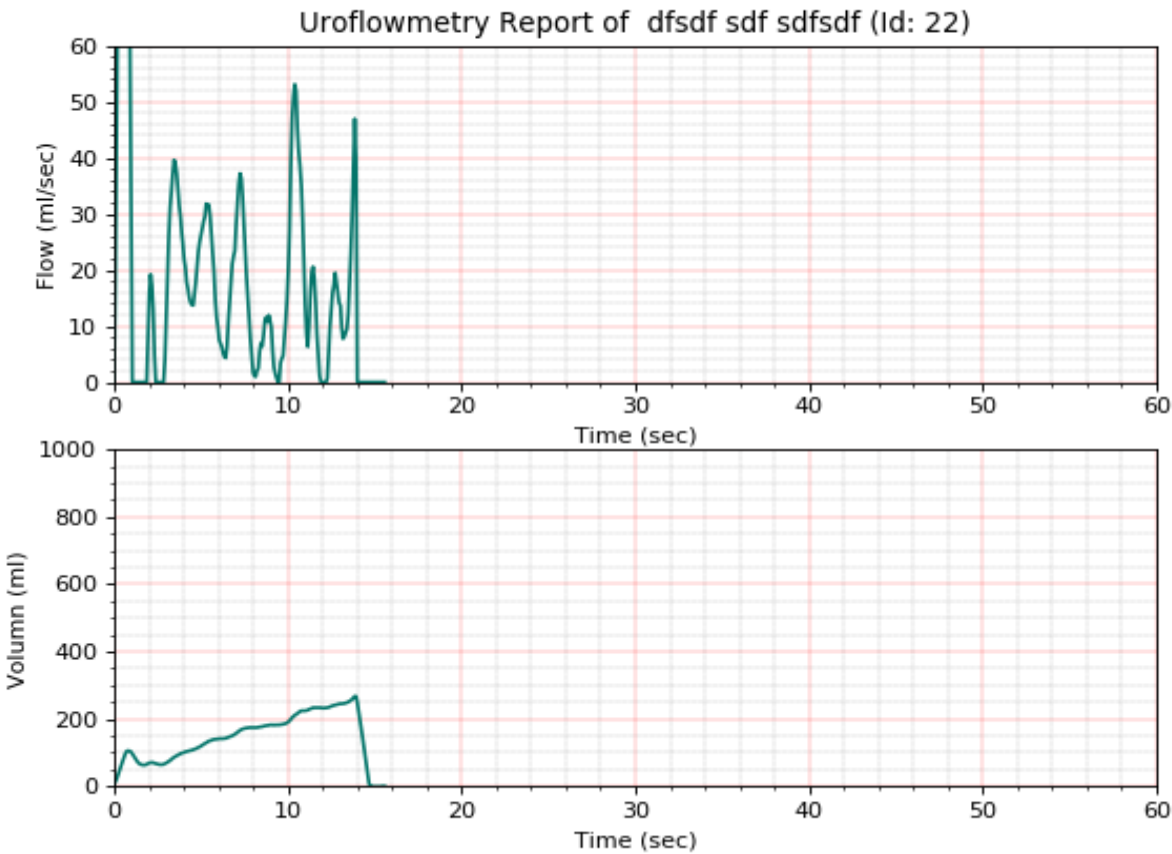

Parameters	Value	Standard Deviation %
Voided Vol (ml)	267.0	Vol SD (%): 72.87
Max. Flow (ml/sec)	154.04	Flow SD (%): 27.22
Avg. Flow (ml/sec)	25.23	--
Flow Time (sec)	11.97	--
Voiding Time(sec)	13.85	--
Time to Max Flow(sec)	0.6	--
Flow at 2 sec.	2.02	--
Accelaration	0.0	--
Hesitancy Time (sec)	4.65	--

Remark : -----

Ark medico software division