


Test No:	000002	Tested Date:	2023-04-04
Patient Name :	sdfdsfsdf dsfsdf dsf	Age:	44
Doctors Name:	Default-Unknown	Gender:	Male

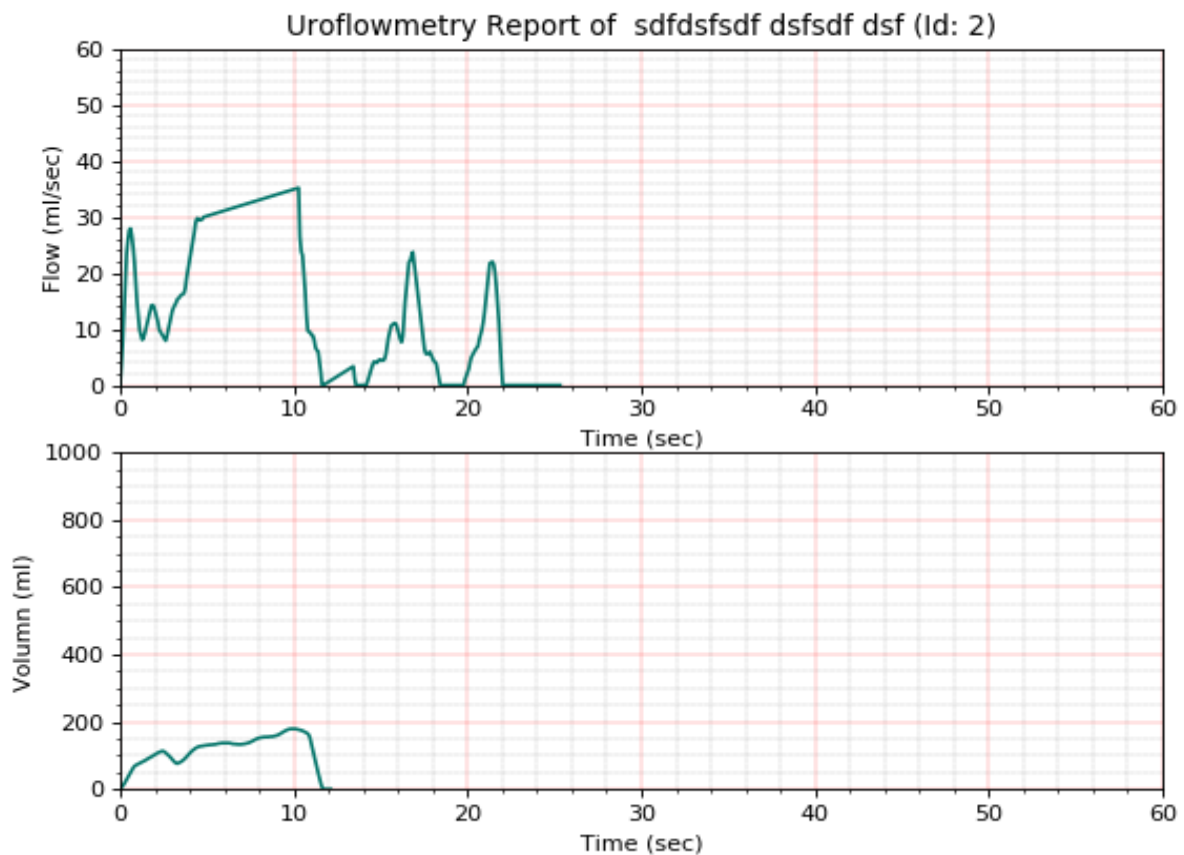

Parameters	Value	Standard Deviation %
Voided Vol (ml)	209.0	Vol SD (%): 74.07
Max. Flow (ml/sec)	35.16	Flow SD (%): 8.76
Avg. Flow (ml/sec)	12.17	--
Flow Time (sec)	18.05	--
Voiding Time(sec)	21.87	--
Time to Max Flow(sec)	10.28	--
Flow at 2 sec.	1.95	--
Accelaration	3.52	--
Hesitancy Time (sec)	2.325	--

Remark : -----