
Thornmouth Borough Council, Environmental Protection. To: Marc Bevan, Ashcroft Air Quality Services (QA/QC audit). From: Conor Robinson. 28 March 2028.

Three PM10 stations take the data-capture note for 2027

Three stations cannot be reported as meeting the PM10 24-hour objective for 2027: North Gate (TBT1), Harbour Walk (TH3) and South Yard (TBT4). Each counted 35 or fewer days above 50 µg/m³ among its valid daily means (22, 17 and 19) but more than 35 over the whole year once its days without a valid daily mean are counted (57, 51 and 51), so under AQ-QP-04 section 5.2 their results go into the ASR with the data-capture note. The other nine stations carry no note.

The days these three lost are not like the days they reported. Their TEOMs stopped as the terminal's dust reached them and stayed down until the next round: the wind blew from the terminal for six hours or more on 103 of their 229 lost days, against 72 of their 866 valid days, and on those valid days they averaged 53.9, 82.1 and 63.0 µg/m³ against a network median of 19.9, 22.2 and 21.0. The lost hours are rebuilt from the other stations' median that hour plus each station's own response to the wind (sector, speed, wet or dry day) on its valid hours; every usual variant of that rebuild keeps all three above 35 (lowest 40) and every other station at or under 35.

Scaling the valid-day count by data capture would put Market Street and Westholme Avenue over 35 (37.8 and 41.9) and none of the three: those two lost long stretches in quiet spells (the Market Street resurfacing works, the Westholme Avenue analyser away for repair), and rebuilt they reach 30 and 30.

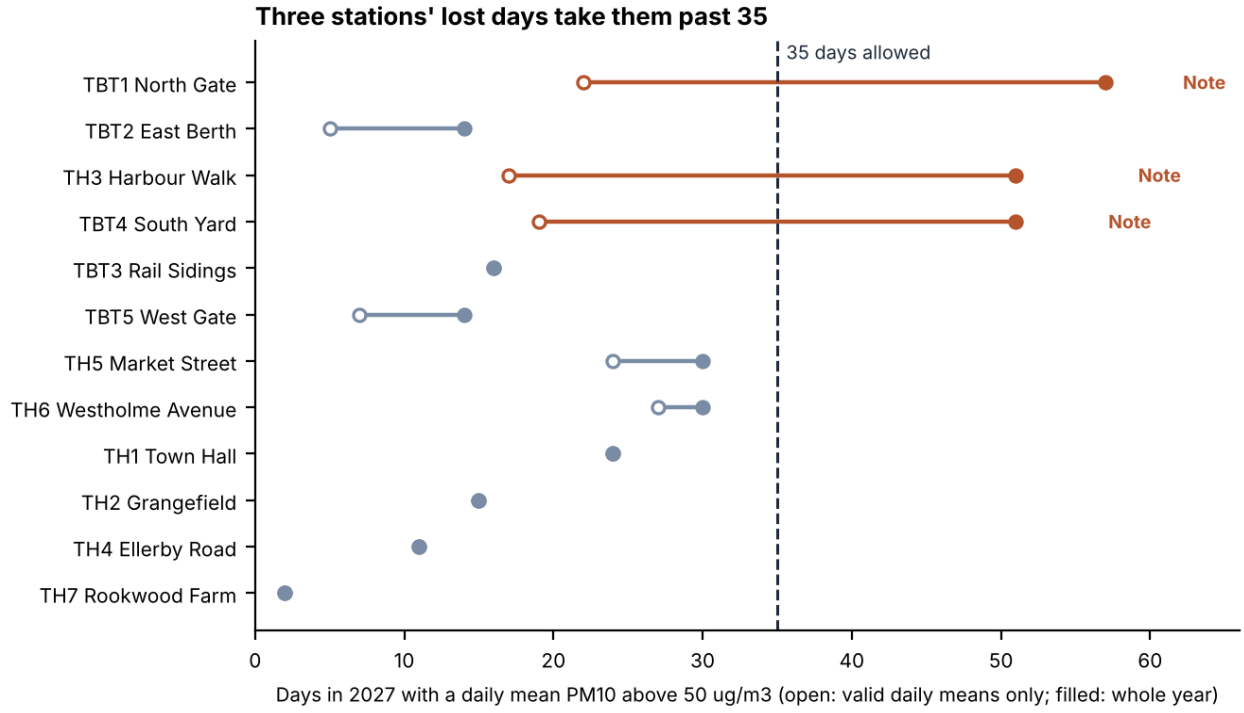

Whole year: lost days rebuilt from the network's median and each station's own response to the wind (AQ-QP-04 v4, 5.1 and 5.2).
Source: network database (ratified 2027), terminal PM10 workbook, port met mast.

Days above 50: valid daily means (18 or more valid hours, GMT days). Whole year: the same days plus the rebuilt days without a valid daily mean (section 5.1); ranges in the workbook. NO2 and deposition figures for the audit are in the workbook.