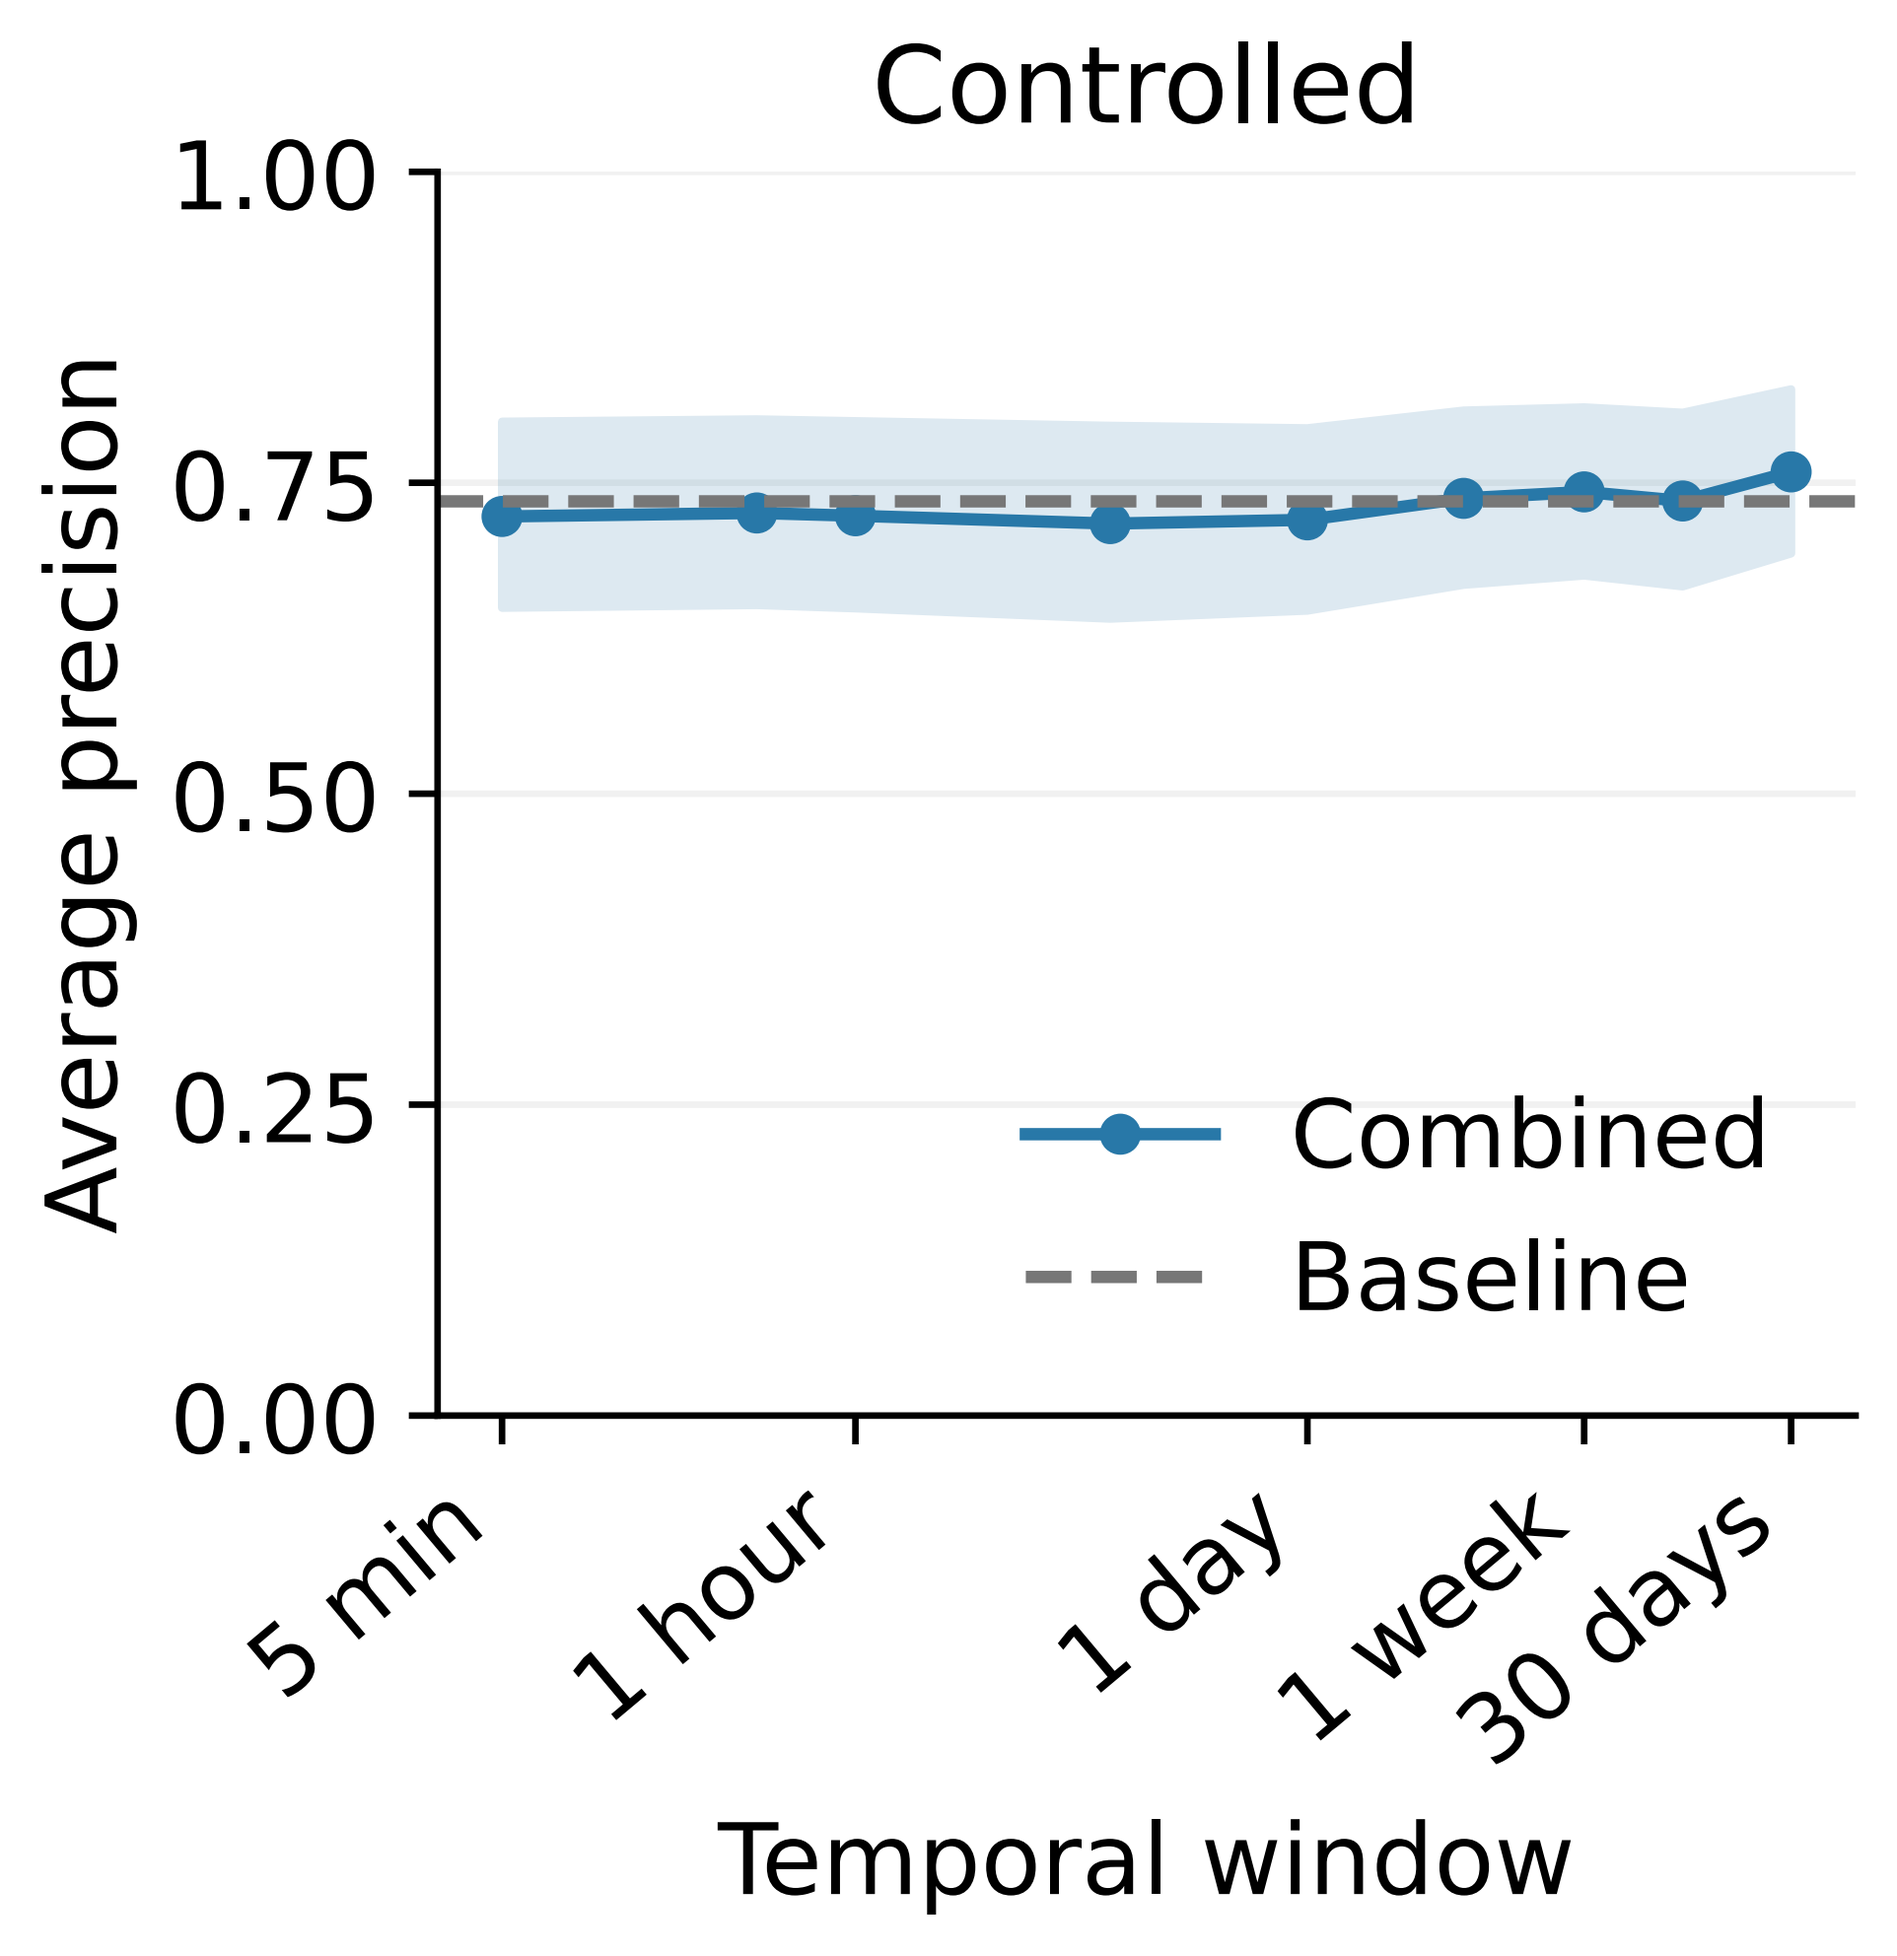
Controlled
1.00
0.75
0.50
0.25
0.00
Average precision
Combined
Baseline
5 min
1 hour
1 day
1 week
30 days
Temporal window